


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD100518\
Data File : VD060133.D
Acq On : 5 Oct 2018 10:05
Operator : VA/AP
Sample : BFB
Misc : 5.00µl/5ml/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D100118S.M
Title : SW846 8260
Last Update : Tue Oct 02 06:56:35 2018

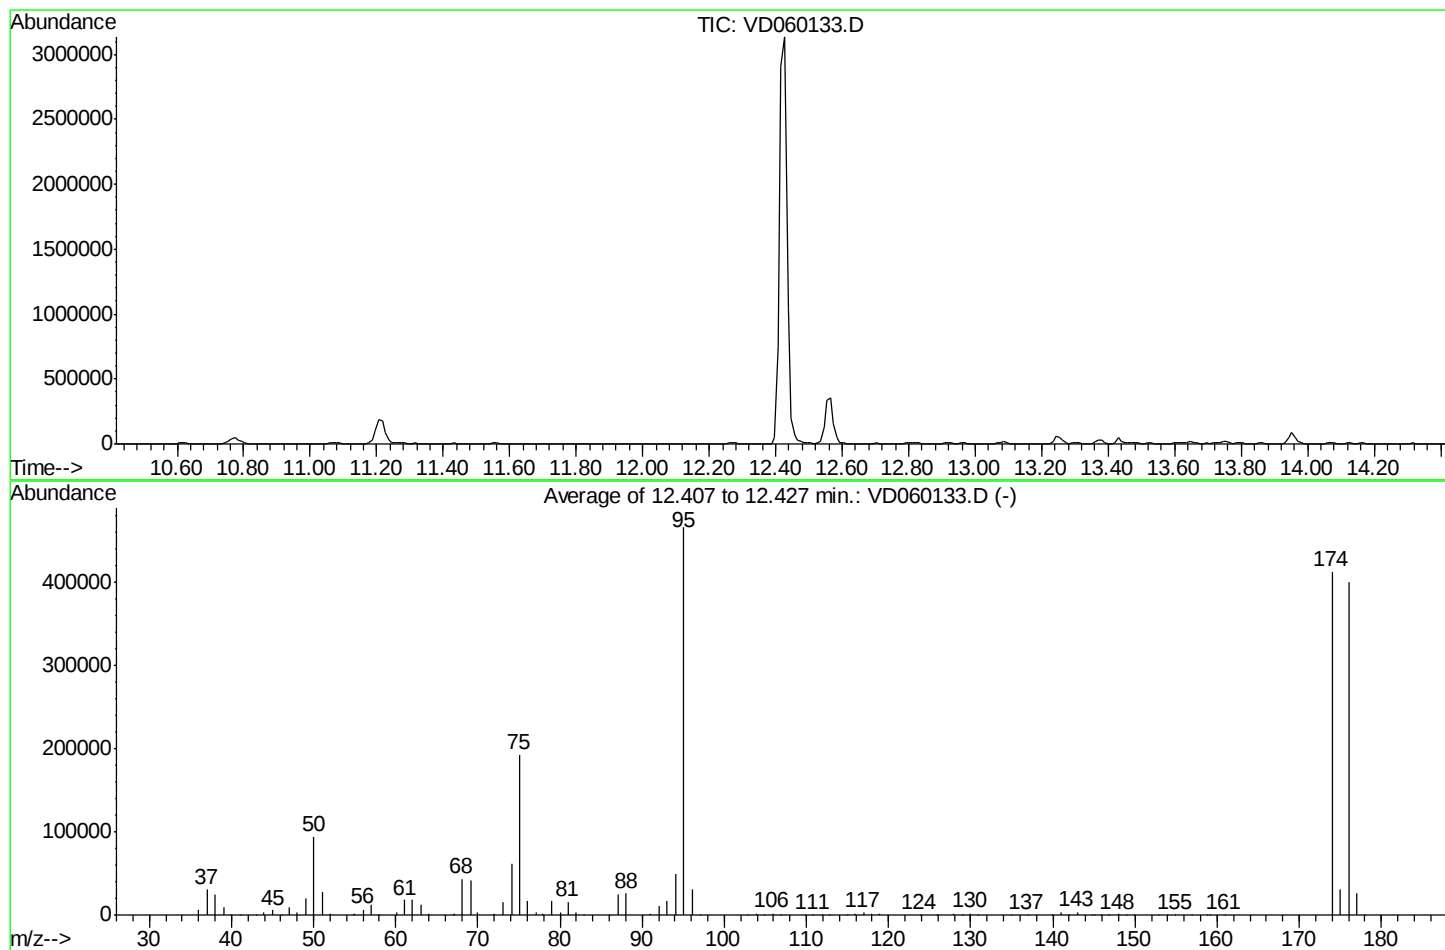

AutoFind: Scans 1106, 1107, 1108; Background Corrected with Scan 1101

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.2	93957	PASS
75	95	30	60	41.4	193136	PASS
95	95	100	100	100.0	465984	PASS
96	95	5	9	6.5	30214	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	88.6	412770	PASS
175	174	5	9	7.3	30332	PASS
176	174	95	101	97.0	400568	PASS
177	176	5	9	6.6	26323	PASS