


Bromomethane

Response Ratio

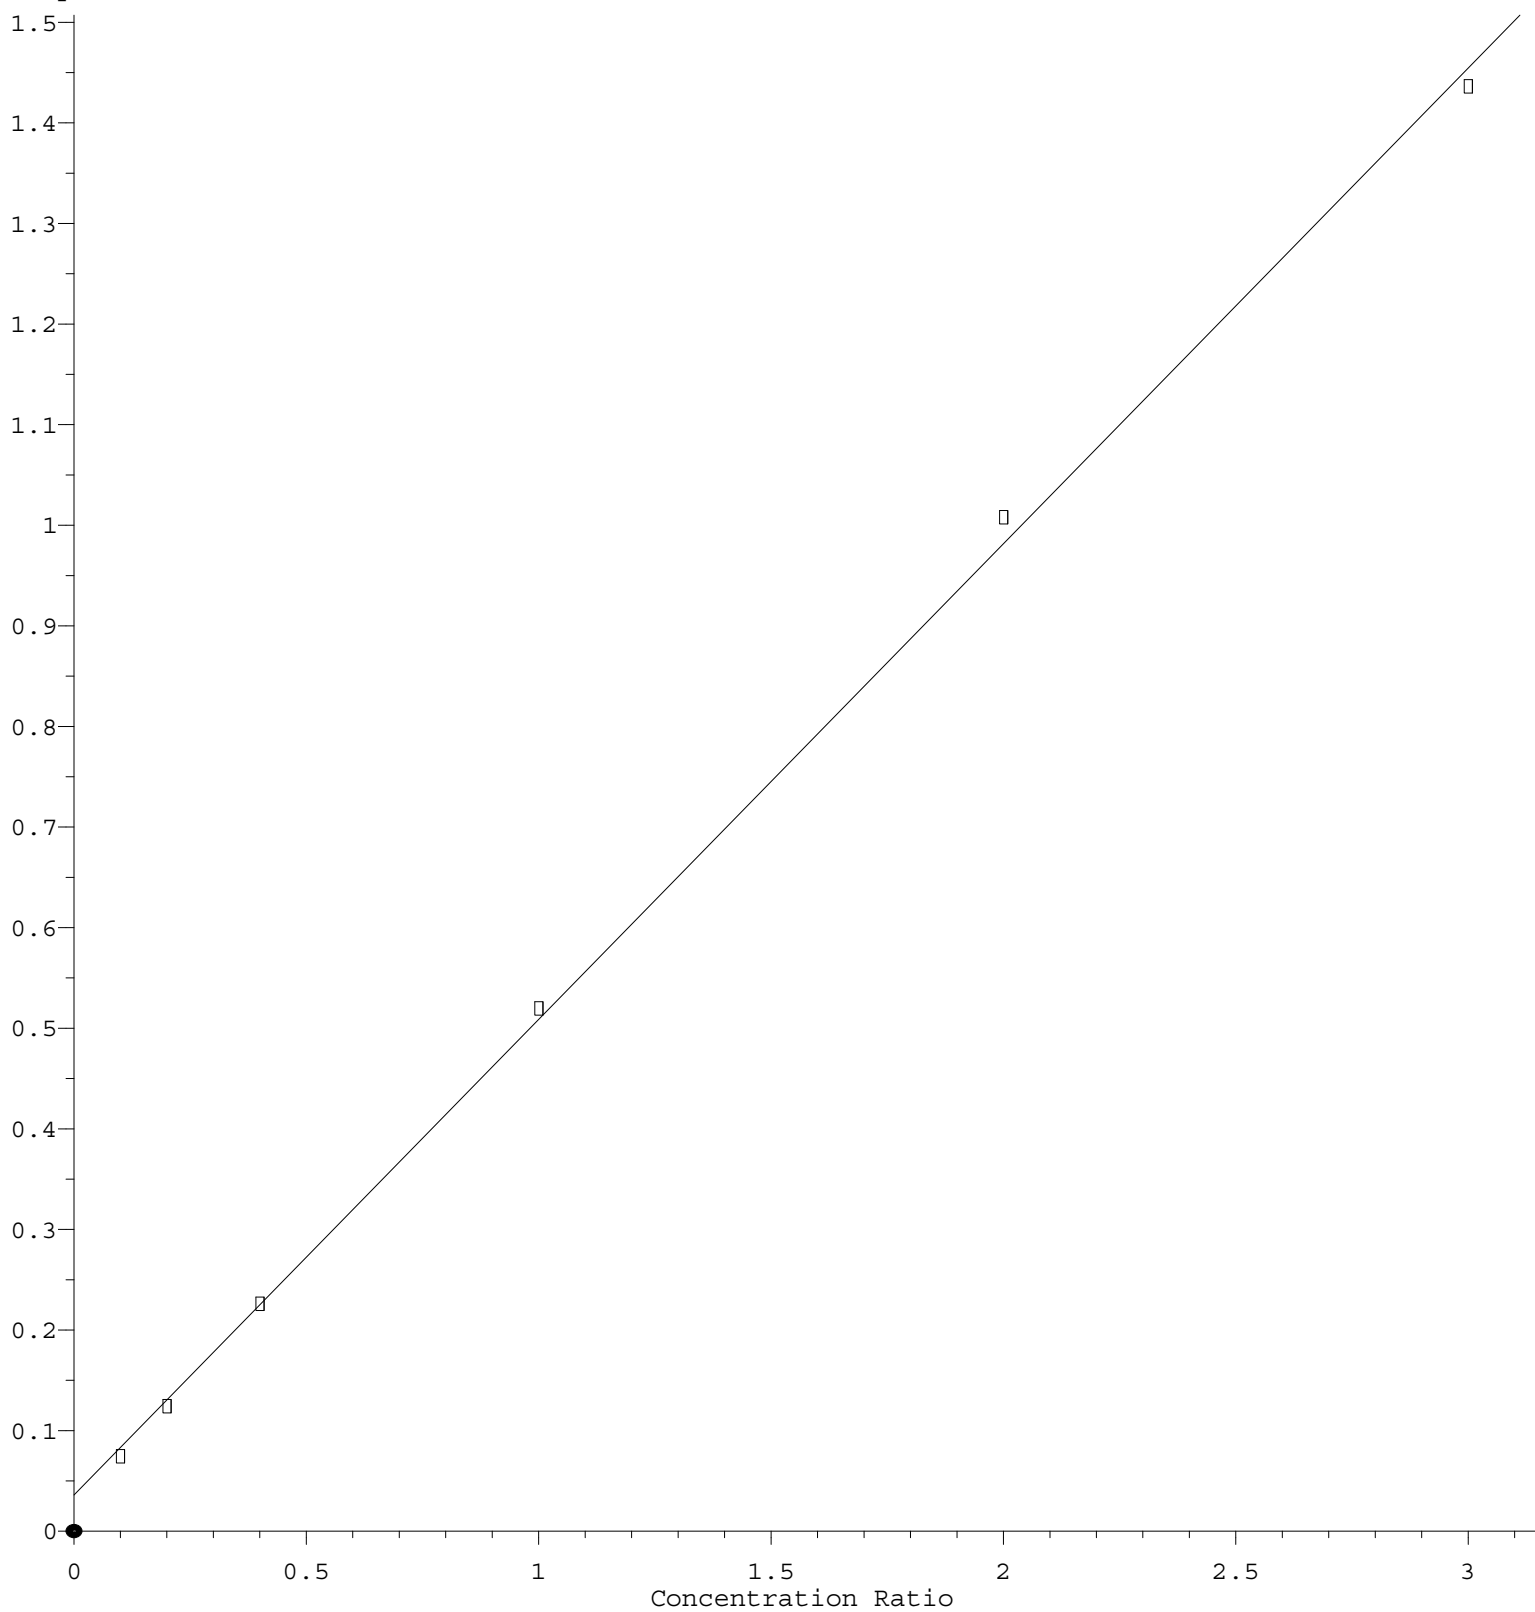

$$\text{Response} = 4.731\text{e-}001 * \text{Amt} + 3.644\text{e-}002$$


Coef of Det (r^2) = 0.999166 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D100521S.M

Calibration Table Last Updated: Wed Oct 06 09:10:31 2021

Methyl Iodide

Response Ratio

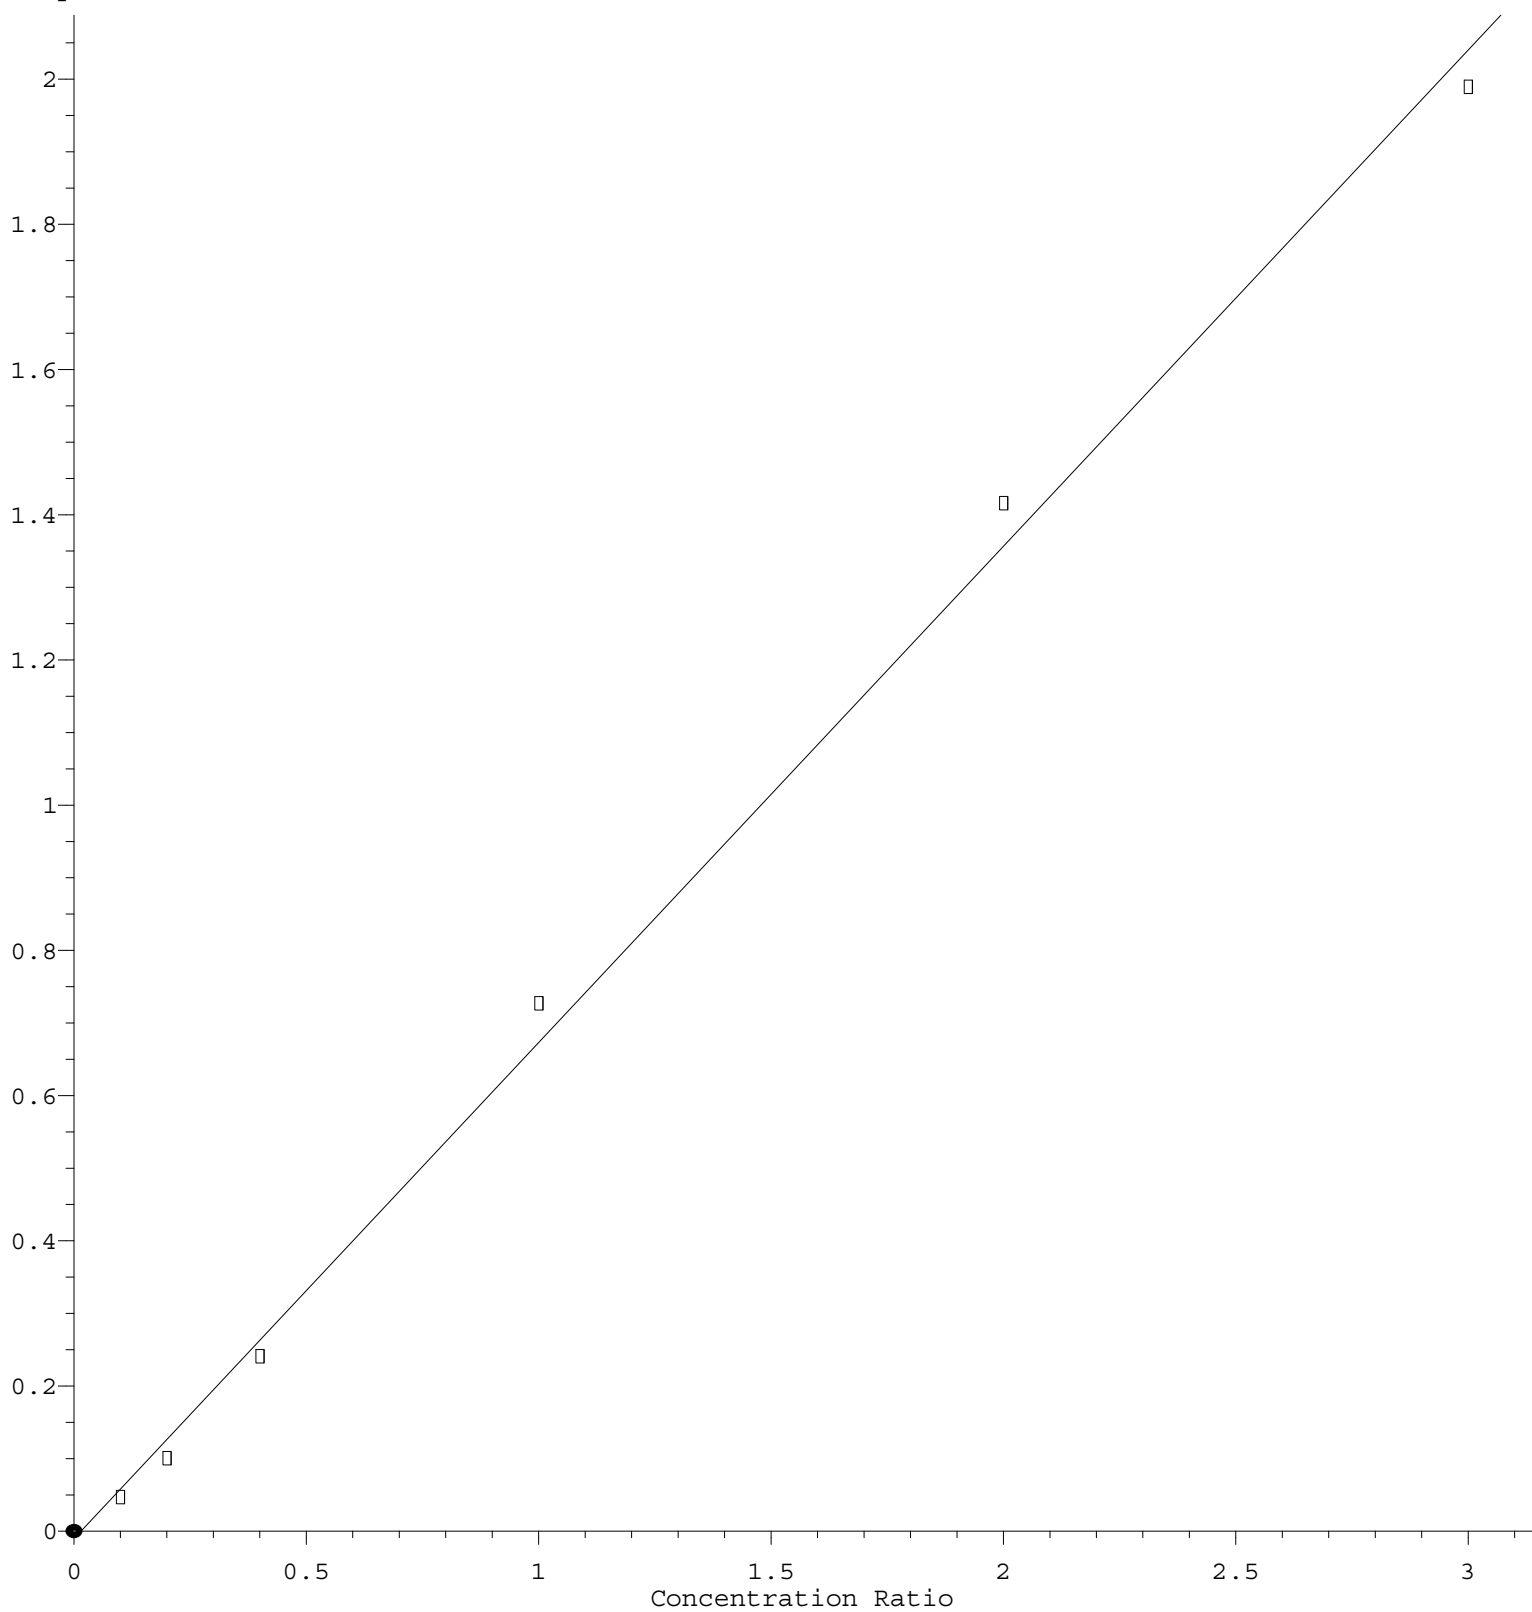

$$\text{Response} = 6.837\text{e-}001 * \text{Amt} - 1.002\text{e-}002$$


Coef of Det (r^2) = 0.996738 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D100521S.M

Calibration Table Last Updated: Wed Oct 06 09:10:31 2021

Methylene Chloride

Response Ratio

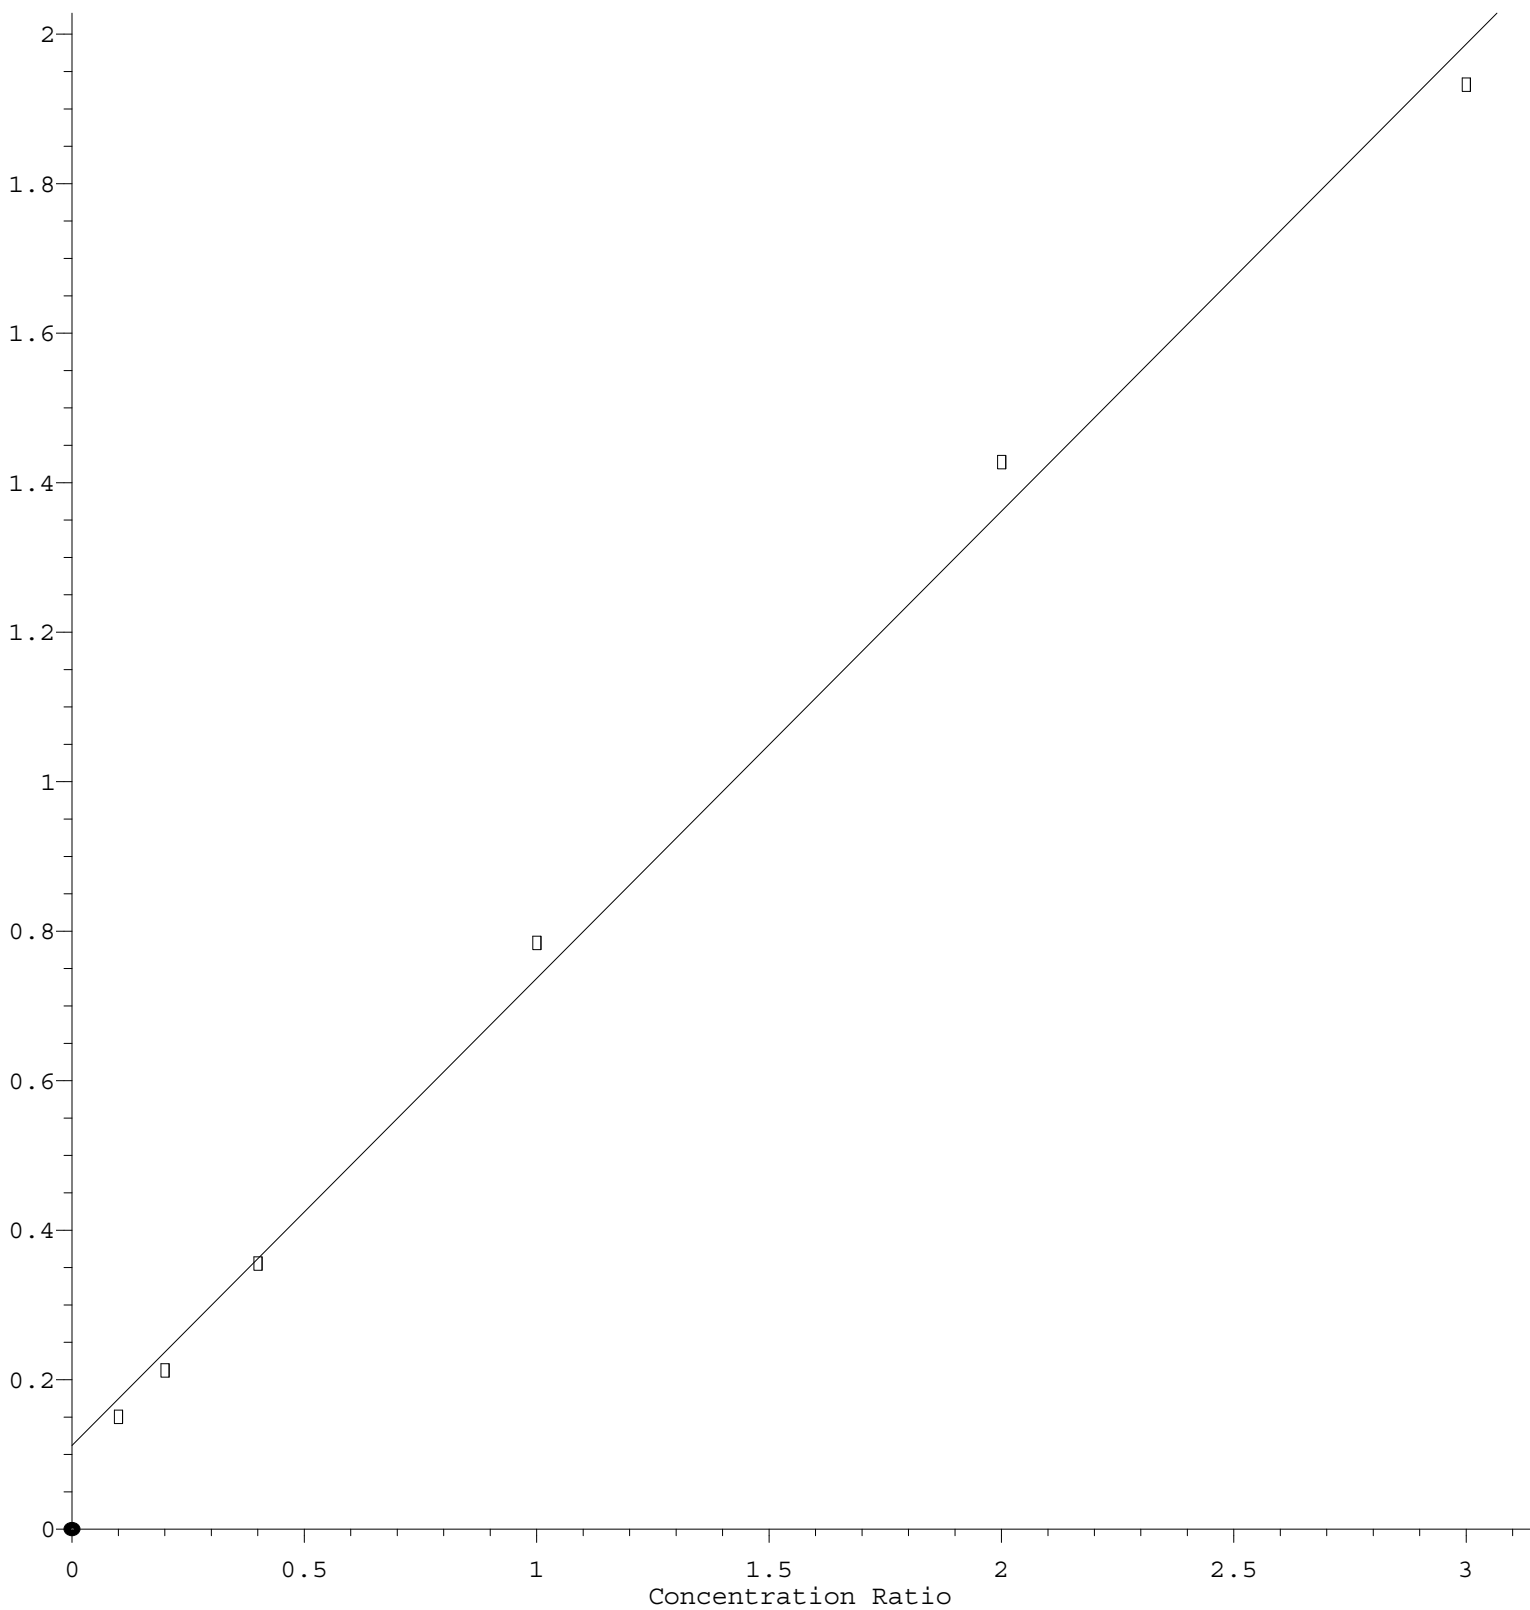

$$\text{Response} = 6.252\text{e-}001 * \text{Amt} + 1.122\text{e-}001$$


Coef of Det (r^2) = 0.995936 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D100521S.M

Calibration Table Last Updated: Wed Oct 06 09:10:31 2021

Ethyl methacrylate

Response Ratio

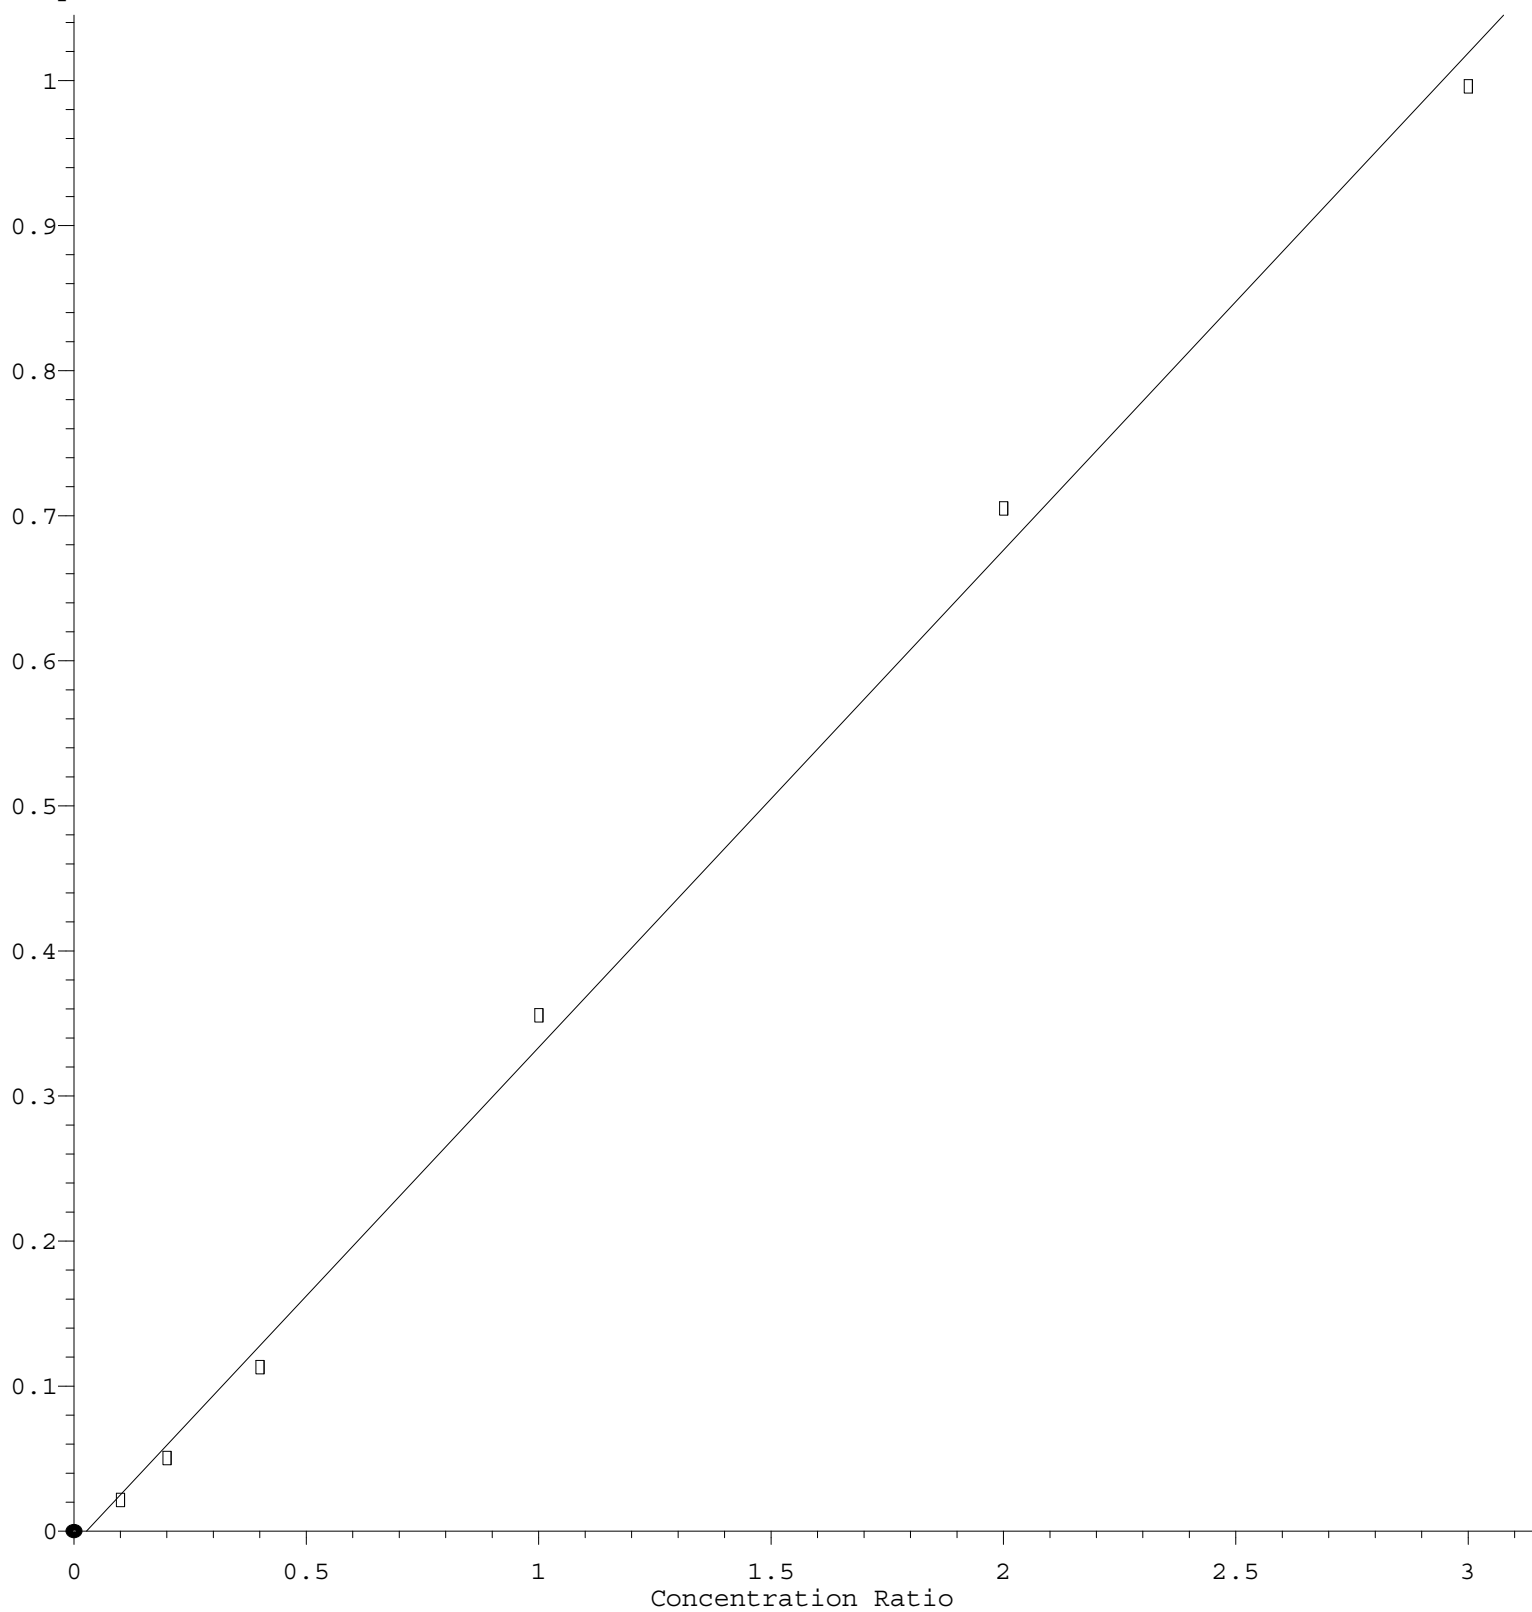

$$\text{Response} = 3.430\text{e-}001 * \text{Amt} - 9.423\text{e-}003$$


Coef of Det (r^2) = 0.997282 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D100521S.M

Calibration Table Last Updated: Wed Oct 06 09:10:31 2021

2-Hexanone

Response Ratio

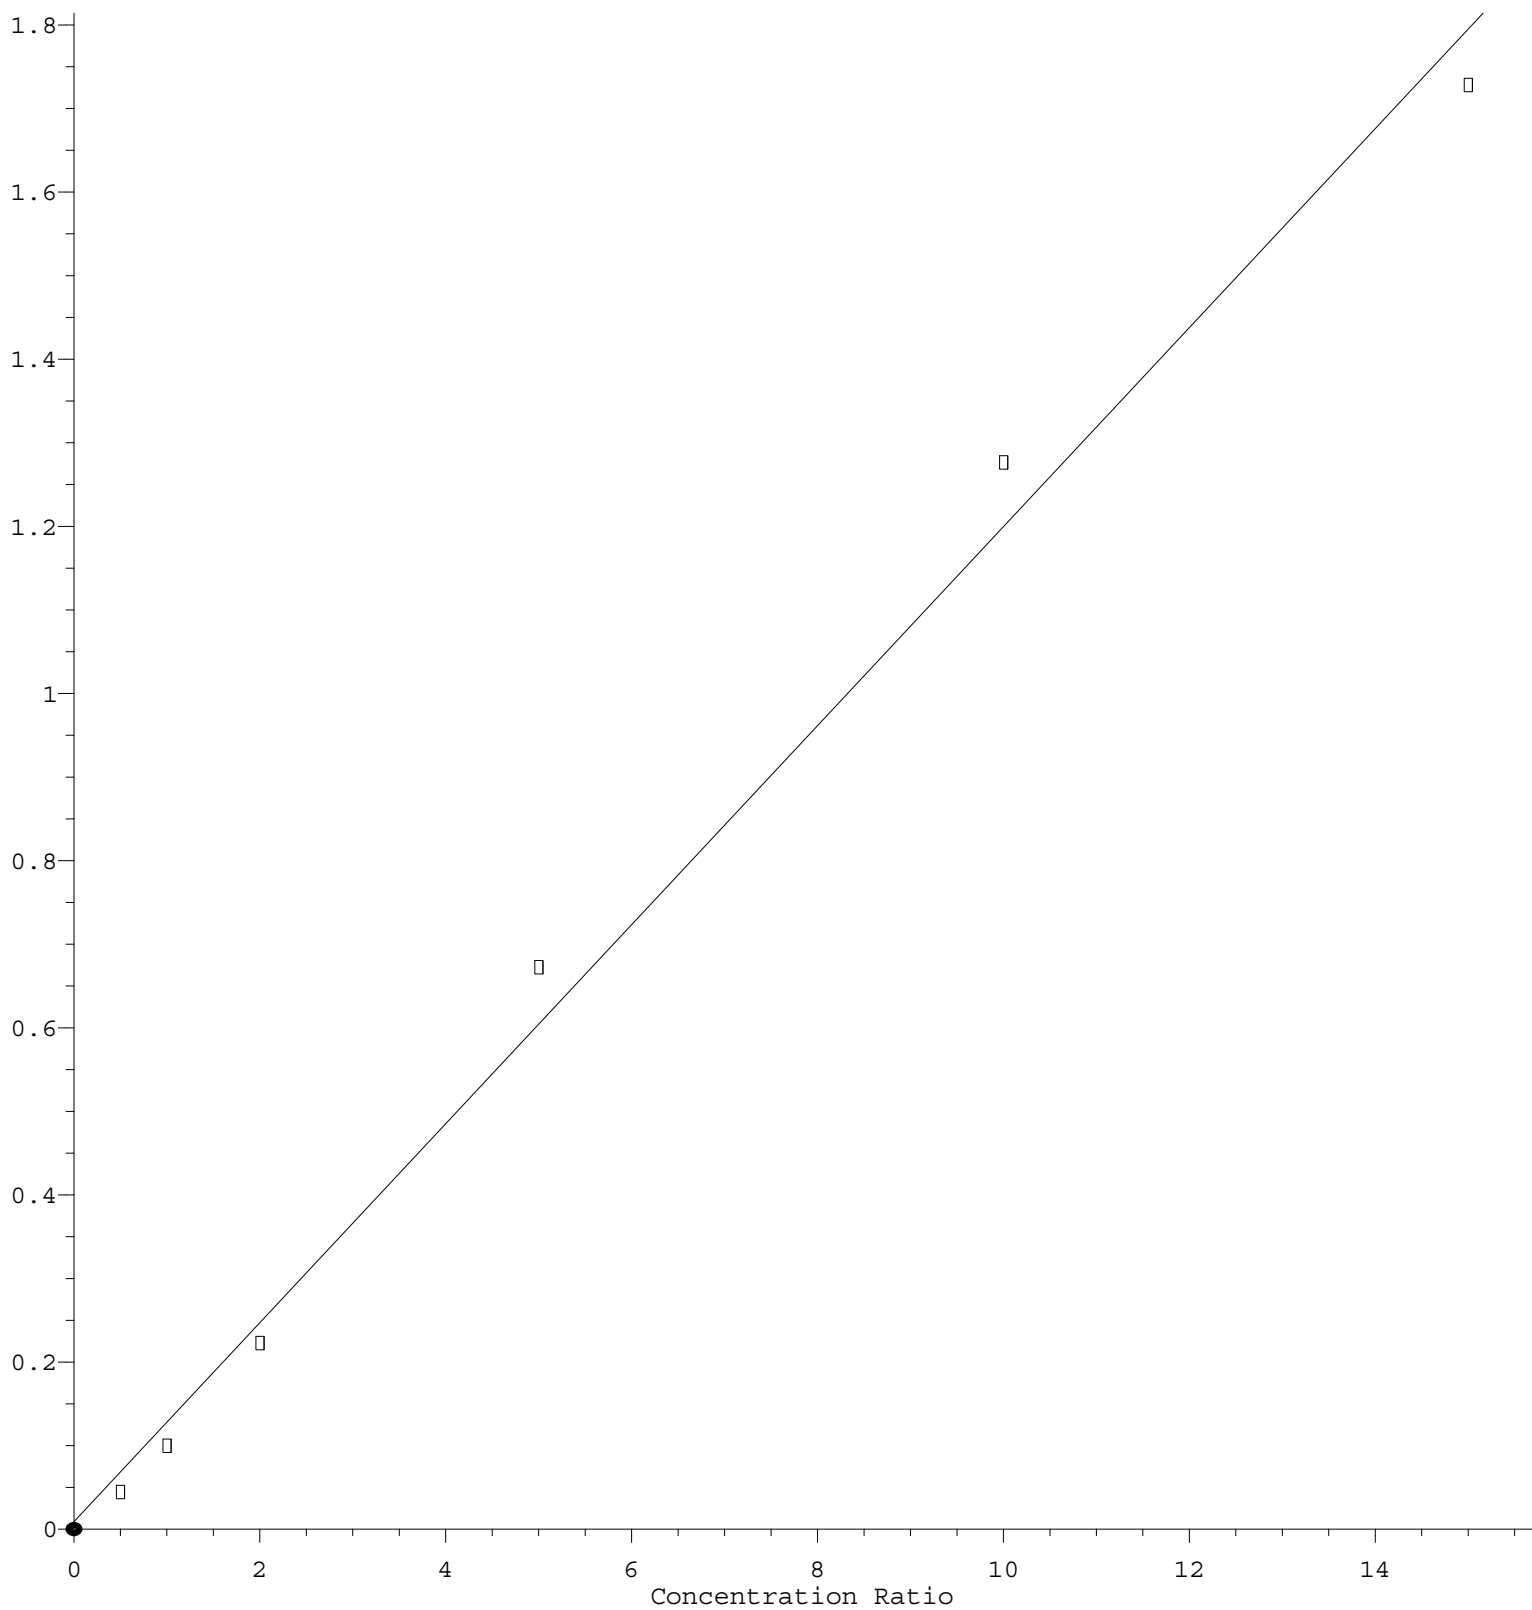

$$\text{Response} = 1.191\text{e-}001 * \text{Amt} + 8.834\text{e-}003$$


Coef of Det (r^2) = 0.992937 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D100521S.M

Calibration Table Last Updated: Wed Oct 06 09:10:31 2021

Naphthalene

Response Ratio

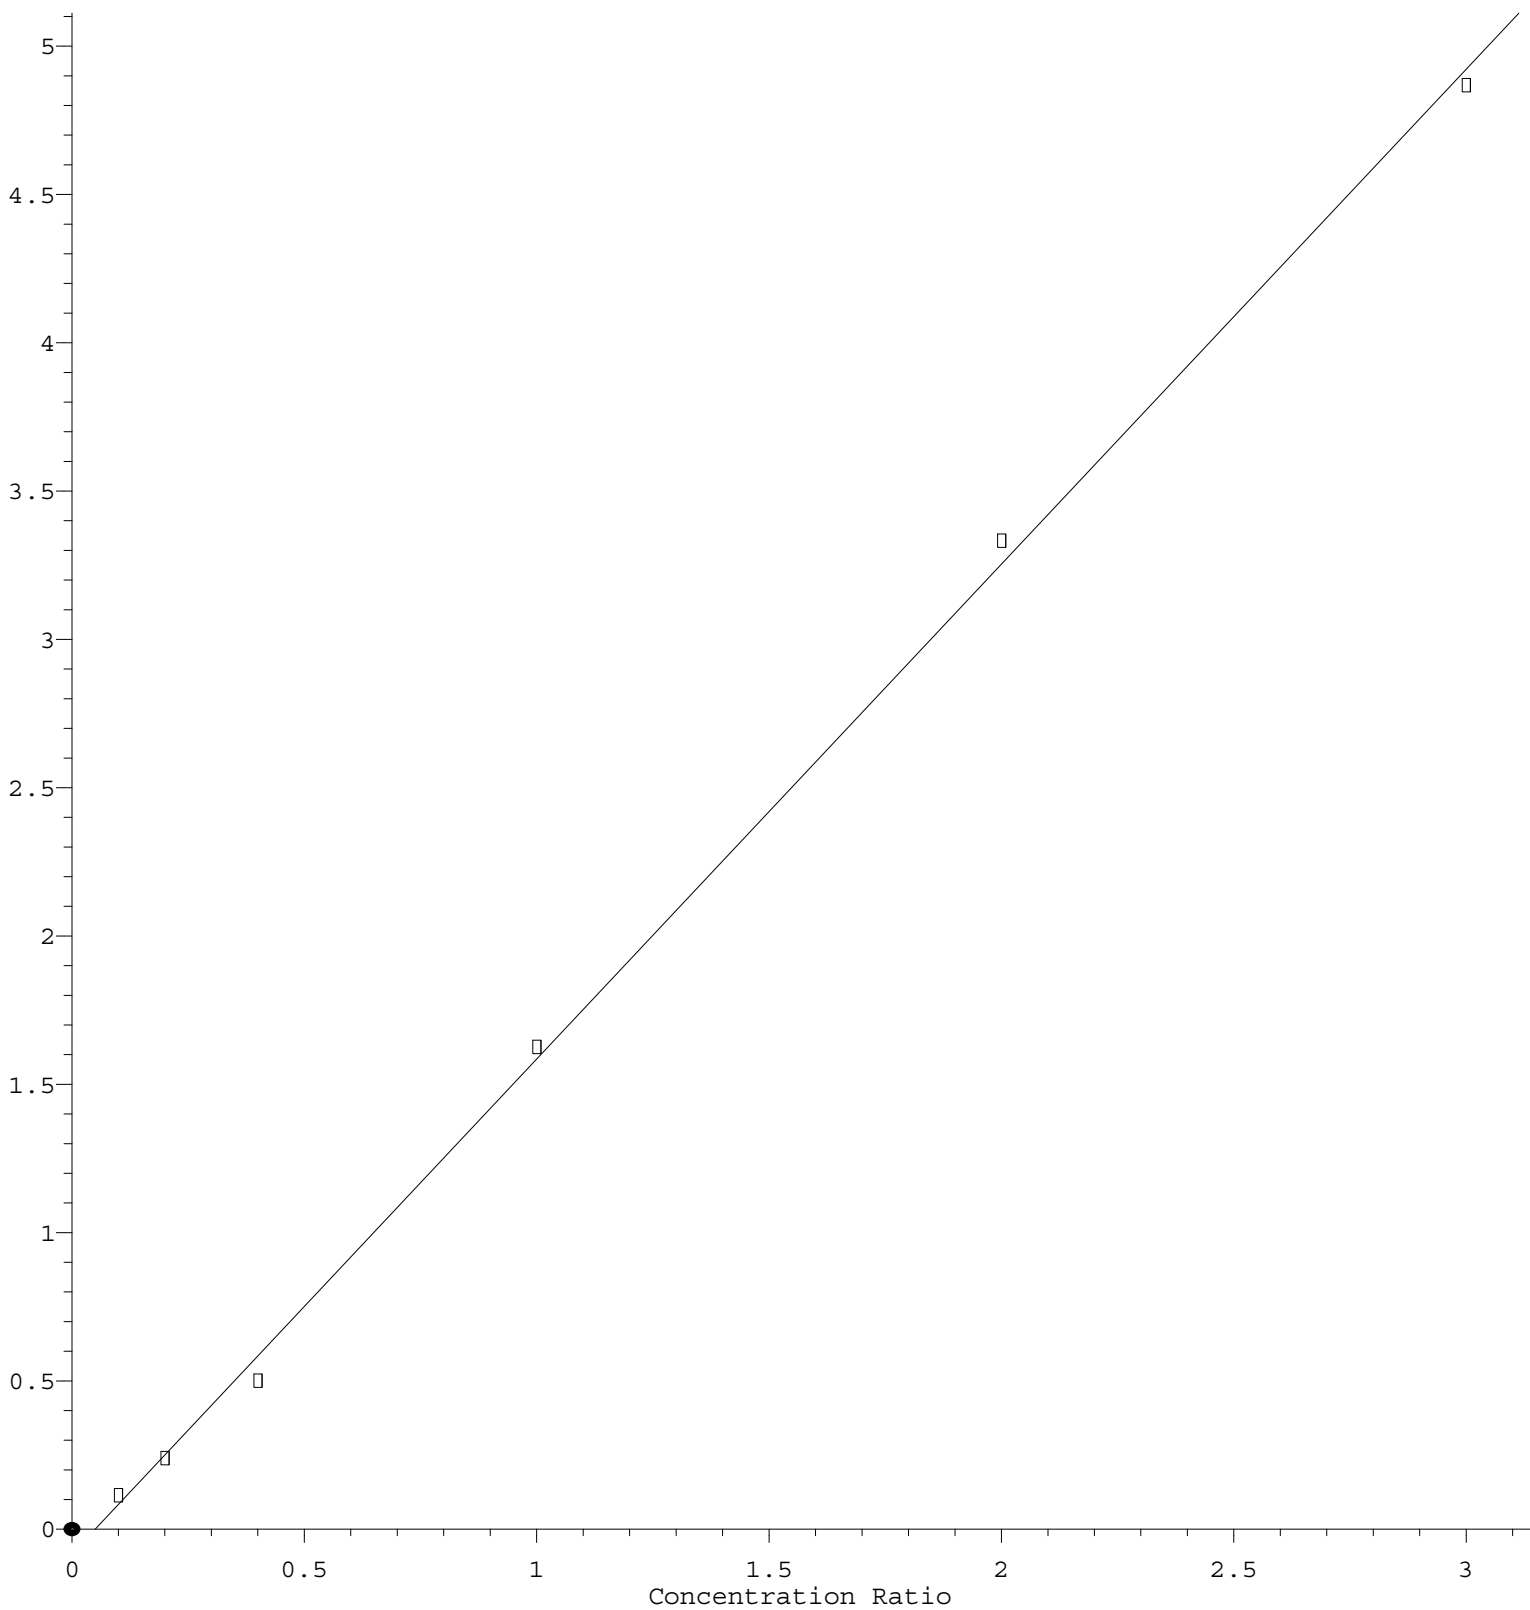

$$\text{Response} = 1.669\text{e}+000 * \text{Amt} - 8.309\text{e}-002$$

Coef of Det (r^2) = 0.998993 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D100521S.M

Calibration Table Last Updated: Wed Oct 06 09:10:31 2021