
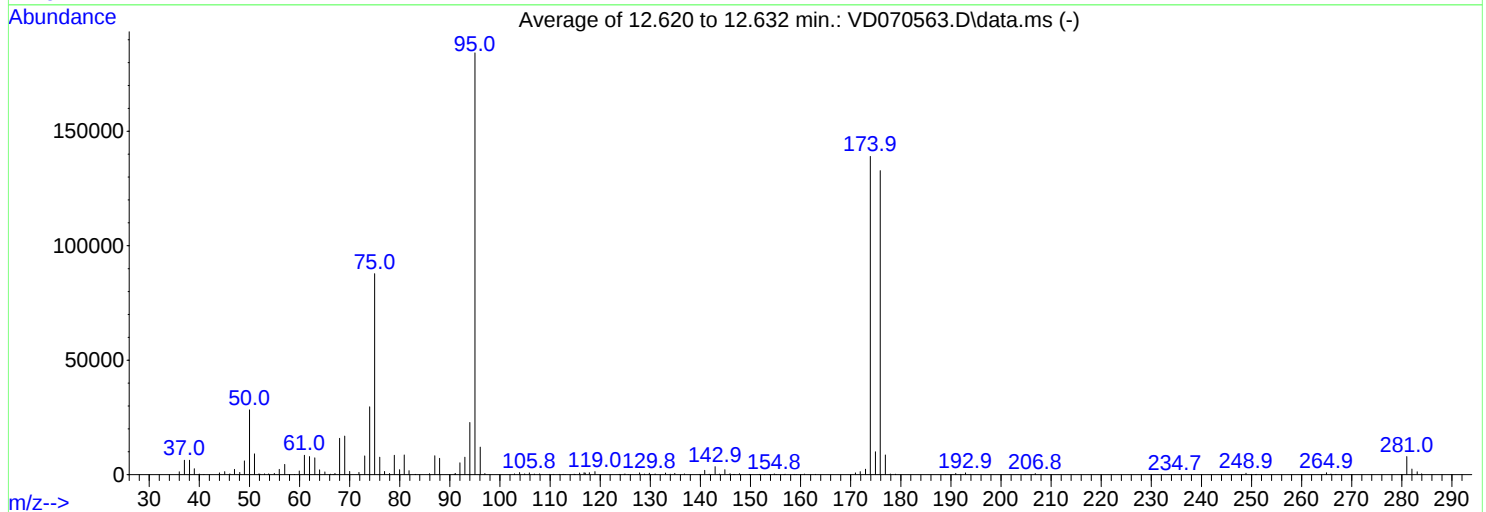


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_D\Data\VD100521\  
Data File : VD070563.D  
Acq On : 05 Oct 2021 10:05  
Operator : VA/SY  
Sample : BFB  
Misc : 5.00G/5.00ml/MSVOA\_D/SOIL  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_D  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_D\Method\82D100521S.M  
Title : SW846 8260  
Last Update : Wed Oct 06 09:10:31 2021

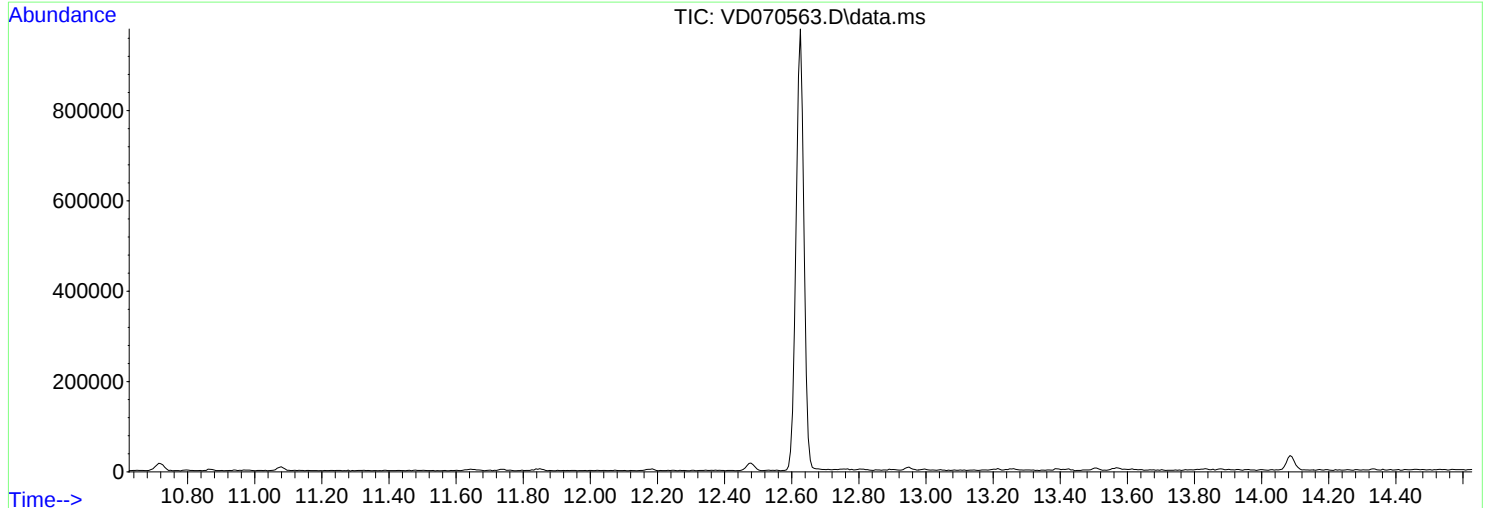

AutoFind: Scans 1819, 1820, 1821; Background Corrected with Scan 1810

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 15.4         | 28325      | PASS                |
| 75             | 95              | 30              | 60              | 47.6         | 87768      | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 184277     | PASS                |
| 96             | 95              | 5               | 9               | 6.5          | 12024      | PASS                |
| 173            | 174             | 0.00            | 2               | 1.7          | 2358       | PASS                |
| 174            | 95              | 50              | 100             | 75.5         | 139064     | PASS                |
| 175            | 174             | 5               | 9               | 7.2          | 10024      | PASS                |
| 176            | 174             | 95              | 101             | 95.5         | 132811     | PASS                |
| 177            | 176             | 5               | 9               | 6.5          | 8618       | PASS                |