


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD100620\
 Data File : VD067119.D
 Acq On : 06 Oct 2020 20:51
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA D/SOIL
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D100120S.M
 Title : SW846 8260
 Last Update : Thu Oct 01 15:19:17 2020

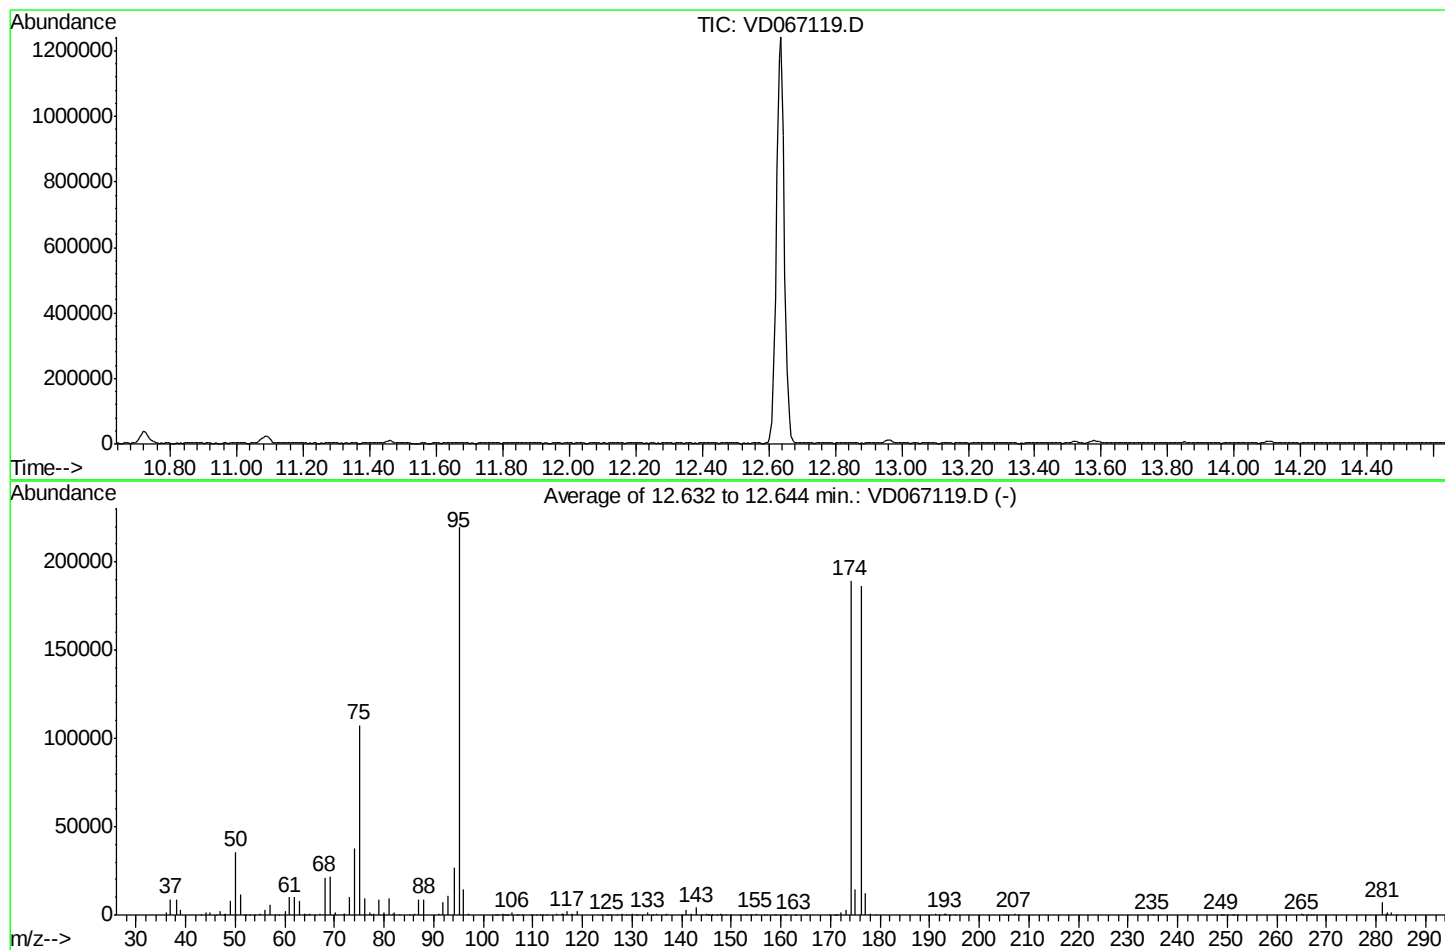

AutoFind: Scans 1821, 1822, 1823; Background Corrected with Scan 1811

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.3	35885	PASS
75	95	30	60	49.0	107549	PASS
95	95	100	100	100.0	219520	PASS
96	95	5	9	6.6	14387	PASS
173	174	0.00	2	1.4	2582	PASS
174	95	50	100	86.2	189184	PASS
175	174	5	9	7.6	14428	PASS
176	174	95	101	98.3	186005	PASS
177	176	5	9	6.6	12297	PASS