
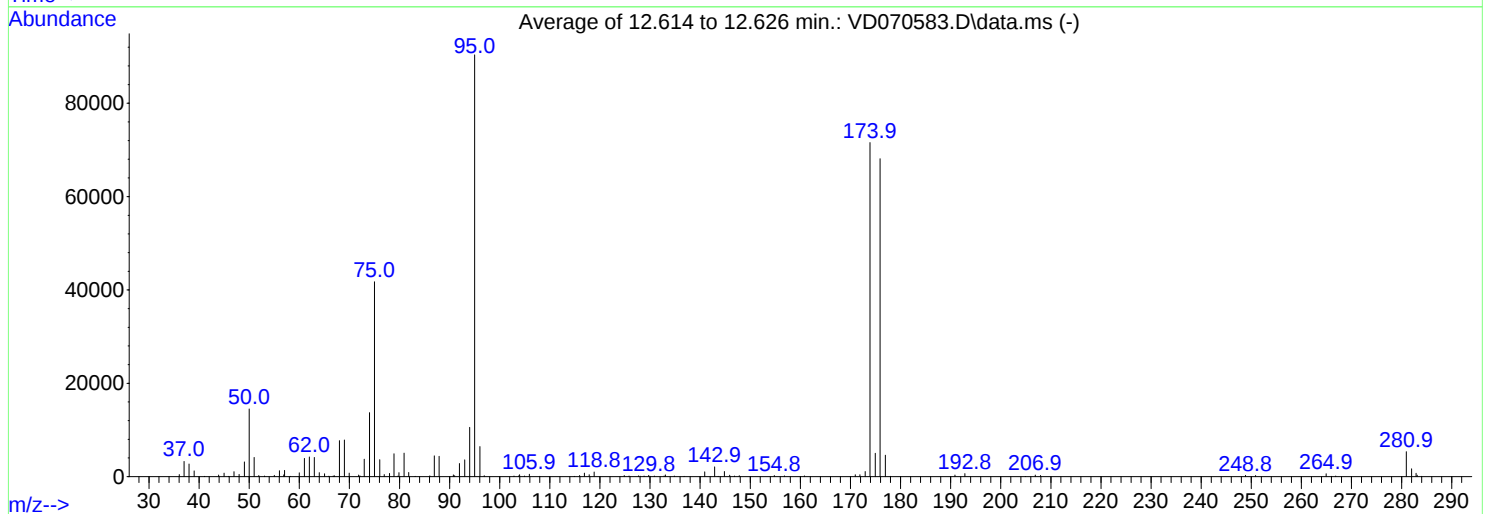


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD100621\
Data File : VD070583.D
Acq On : 06 Oct 2021 10:19
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D100521S.M
Title : SW846 8260
Last Update : Wed Oct 06 09:10:31 2021

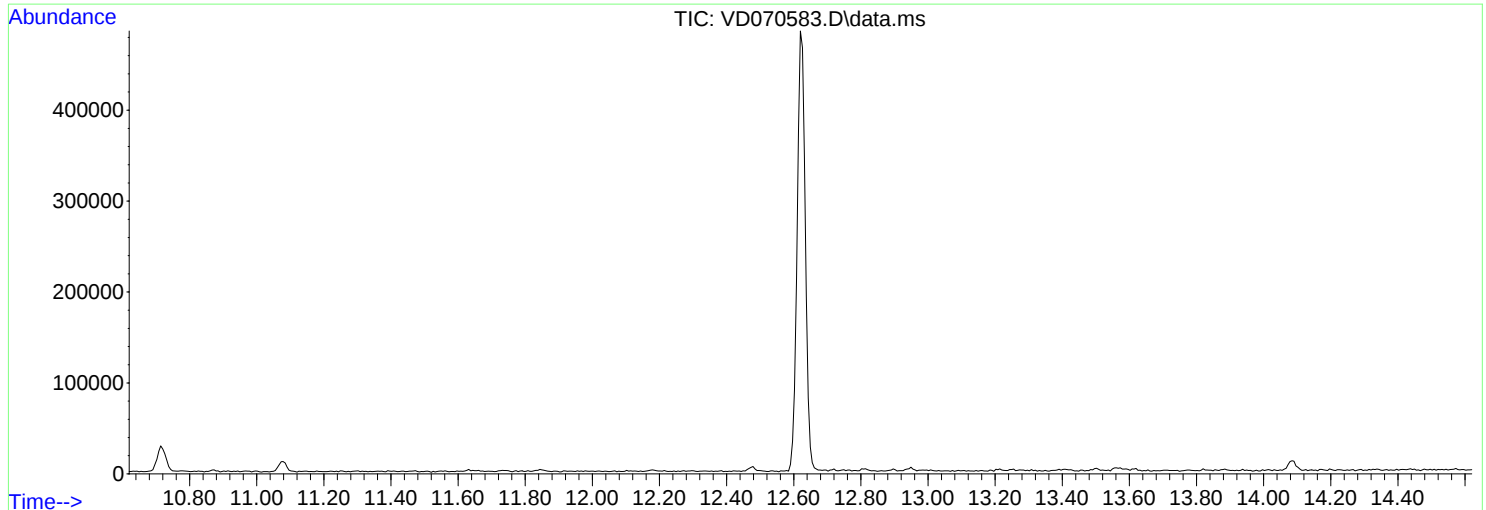

AutoFind: Scans 1818, 1819, 1820; Background Corrected with Scan 1811

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.1	14510	PASS
75	95	30	60	46.2	41749	PASS
95	95	100	100	100.0	90376	PASS
96	95	5	9	7.1	6452	PASS
173	174	0.00	2	1.5	1104	PASS
174	95	50	100	79.2	71571	PASS
175	174	5	9	7.0	5007	PASS
176	174	95	101	95.2	68109	PASS
177	176	5	9	6.8	4598	PASS