
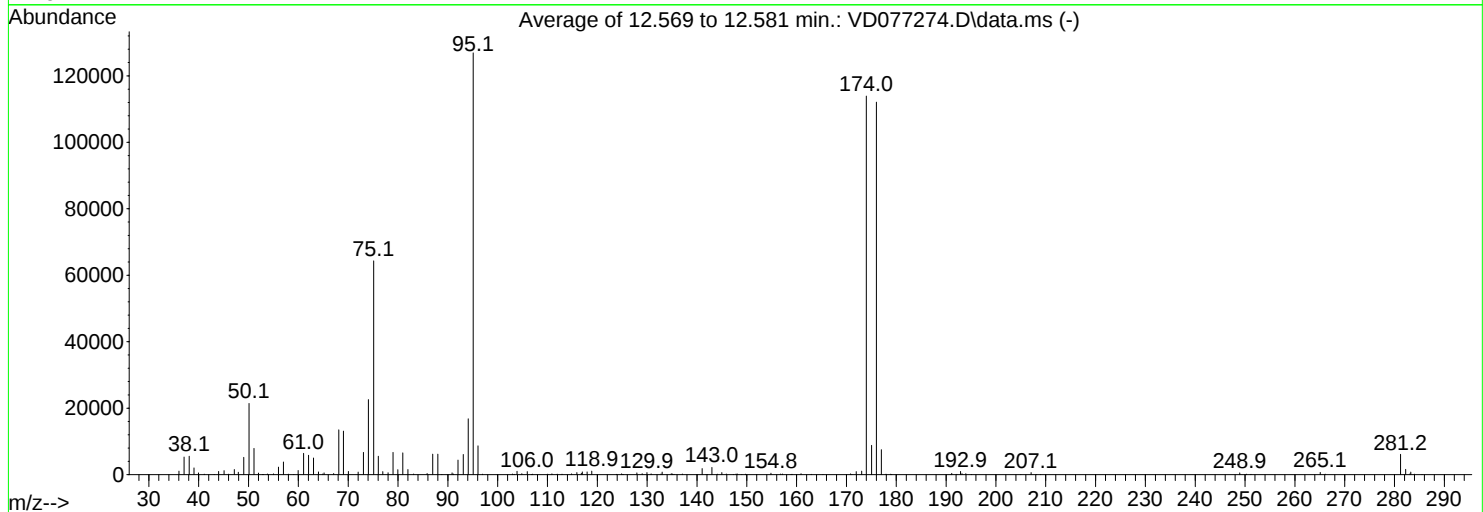


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD100623\
Data File : VD077274.D
Acq On : 05 Oct 2023 12:15
Operator : JC/SY
Sample : BFB
Misc : 5.00G/5.0ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D100623S.M
Title : SW846 8260
Last Update : Mon Oct 09 09:52:06 2023

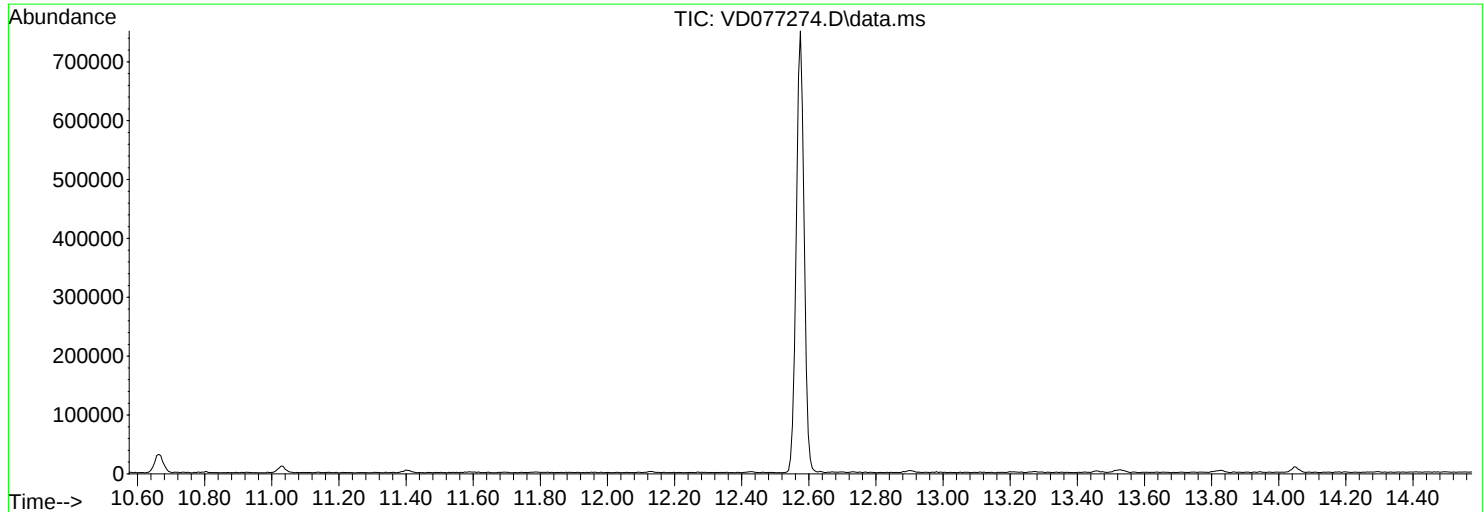

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1858

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	21437	PASS
75	95	30	60	50.7	64304	PASS
95	95	100	100	100.0	126925	PASS
96	95	5	9	6.8	8691	PASS
173	174	0.00	2	0.9	1050	PASS
174	95	50	100	89.8	113928	PASS
175	174	5	9	7.7	8807	PASS
176	174	95	101	98.4	112067	PASS
177	176	5	9	6.7	7542	PASS