

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD100721\
 Data File : VD070622.D
 Acq On : 07 Oct 2021 17:40
 Operator : VA/SY
 Sample : M4117-03
 Misc : 4.21G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 SB-1(6.5-7.0)

Quant Time: Oct 08 04:54:01 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D100521S.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 06 09:10:31 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.979	168	364584	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.861	114	706134	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.638	117	661972	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.567	152	275167	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.326	65	220062	51.29	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	102.58%
35) Dibromofluoromethane	7.908	113	234178	49.88	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	99.76%
50) Toluene-d8	10.338	98	901580	50.23	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	100.46%
62) 4-Bromofluorobenzene	12.626	95	266926	44.50	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	89.00%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD100721\
Data File : VD070622.D
Acq On : 07 Oct 2021 17:40
Operator : VA/SY
Sample : M4117-03
Misc : 4.21G/5.00ml/MSVOA_D/SOIL
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
SB-1(6.5-7.0)

Quant Time: Oct 08 04:54:01 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D100521S.M
Quant Title : SW846 8260
QLast Update : Wed Oct 06 09:10:31 2021
Response via : Initial Calibration




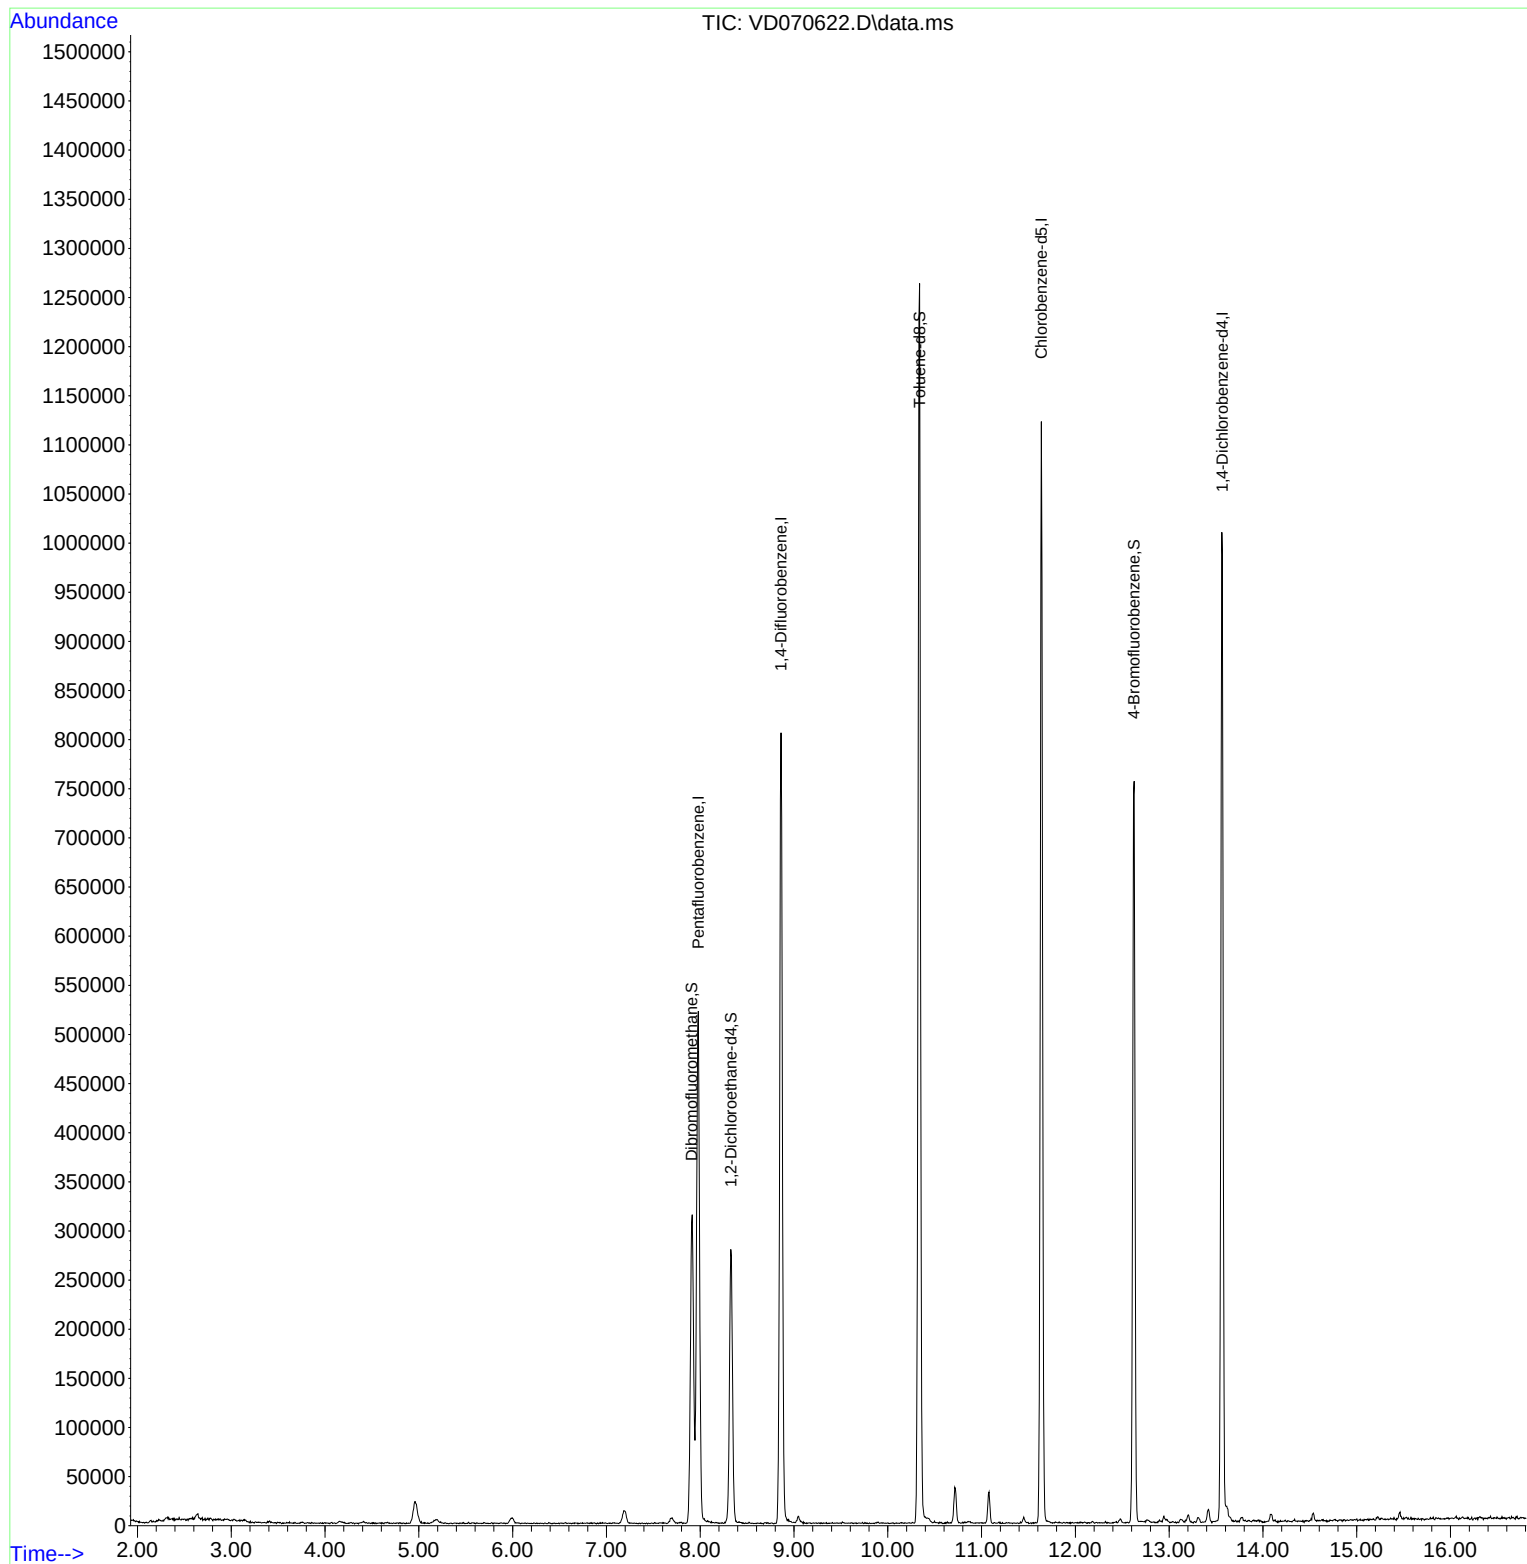


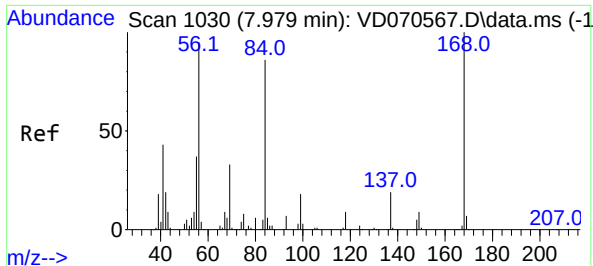

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.979 min Scan# 1030
Delta R.T. 0.000 min
Lab File: VD070622.D
Acq: 07 Oct 2021 17:40




Instrument :
MSVOA_D
ClientSampleId :
SB-1(6.5-7.0)


Tgt Ion:168 Resp: 364584
Ion Ratio Lower Upper
168 100
99 63.0 51.4 77.0

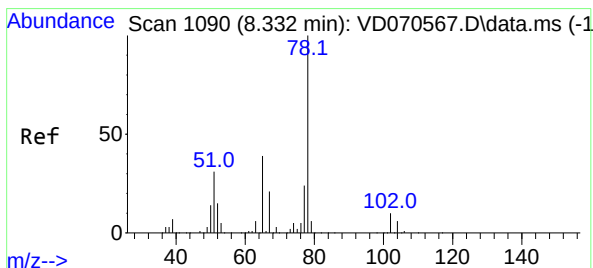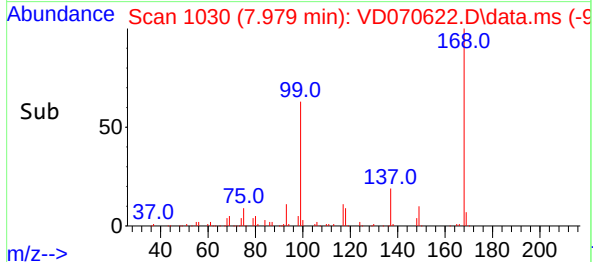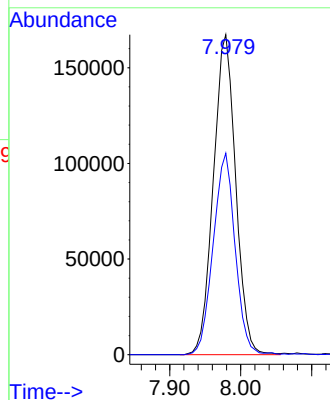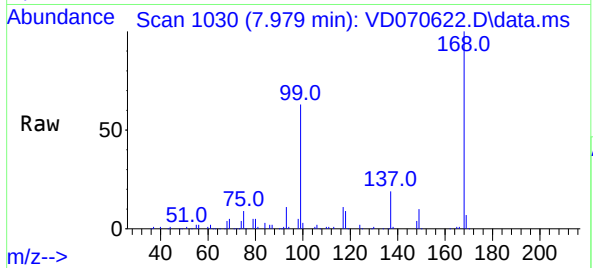

#33
1,2-Dichloroethane-d4
Concen: 51.29 ug/l
RT: 8.326 min Scan# 1089
Delta R.T. -0.006 min
Lab File: VD070622.D
Acq: 07 Oct 2021 17:40

Tgt Ion: 65 Resp: 220062
Ion Ratio Lower Upper
65 100
67 55.4 0.0 110.2

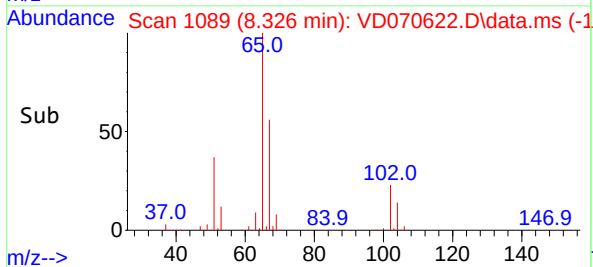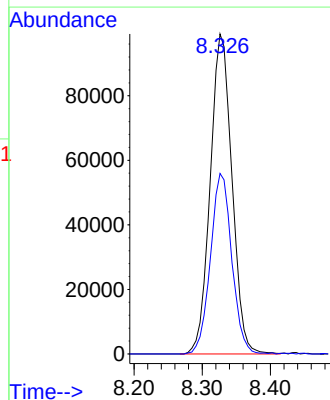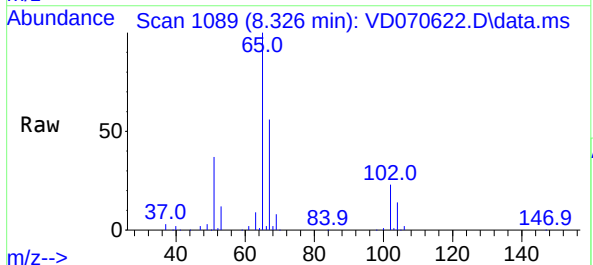

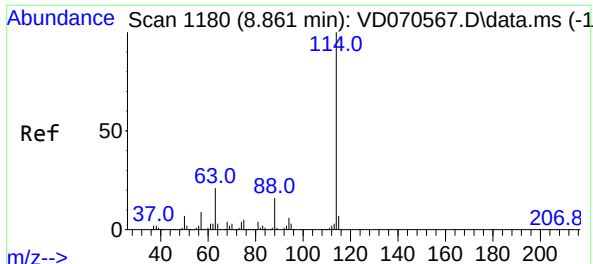





#34

1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.861 min Scan# 1180
Delta R.T. -0.000 min
Lab File: VD070622.D
Acq: 07 Oct 2021 17:40

Instrument :
MSVOA_D
ClientSampleId :
SB-1(6.5-7.0)

Tgt Ion:114 Resp: 706134

Ion	Ratio	Lower	Upper
114	100		
63	19.6	0.0	41.8
88	15.8	0.0	32.6

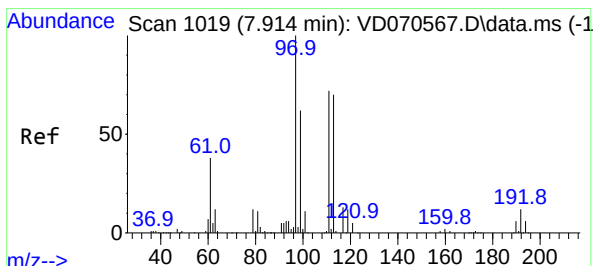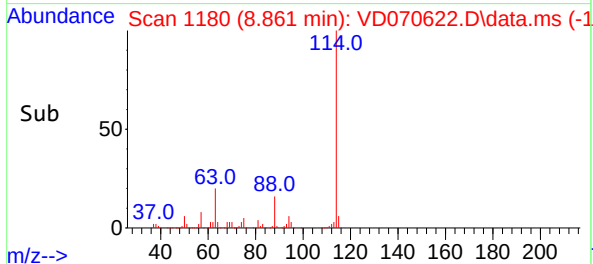
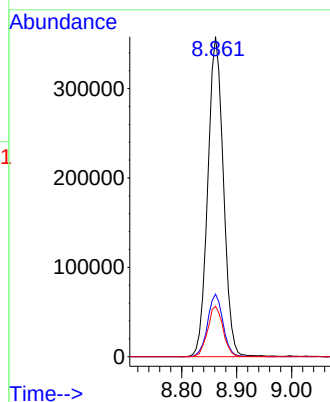
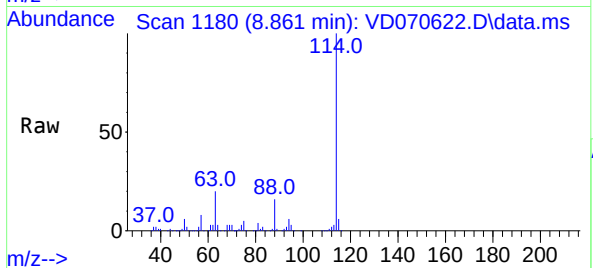



#35

Dibromofluoromethane
Concen: 49.88 ug/l
RT: 7.908 min Scan# 1018
Delta R.T. -0.006 min
Lab File: VD070622.D
Acq: 07 Oct 2021 17:40

Tgt Ion:113 Resp: 234178

Ion	Ratio	Lower	Upper
113	100		
111	103.2	83.1	124.7
192	17.2	12.7	19.1


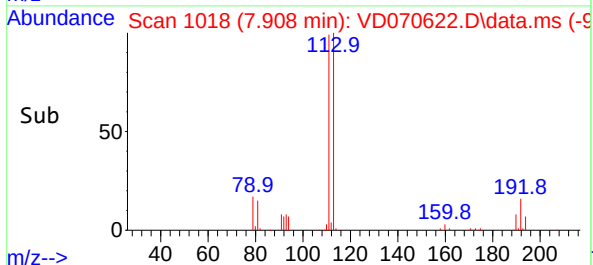
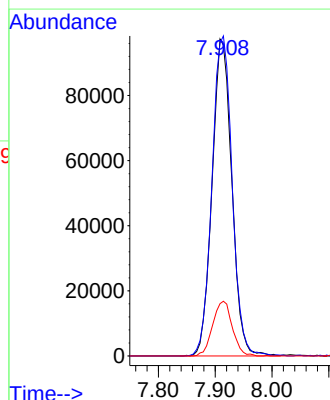
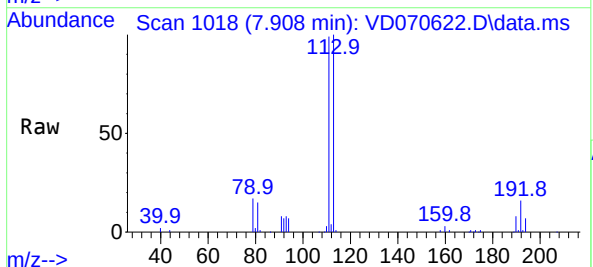


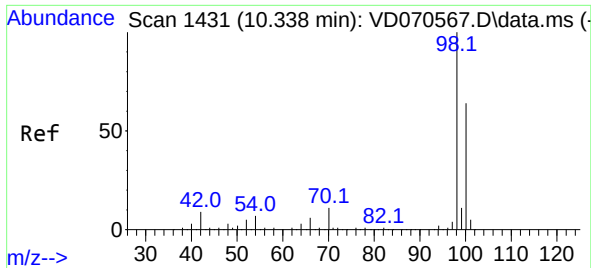

#50
Toluene-d8
Concen: 50.23 ug/l
RT: 10.338 min Scan# 1431
Delta R.T. 0.000 min
Lab File: VD070622.D
Acq: 07 Oct 2021 17:40




Instrument :
MSVOA_D
ClientSampleId :
SB-1(6.5-7.0)


Tgt Ion: 98 Resp: 901580
Ion Ratio Lower Upper
98 100
100 65.6 52.2 78.4

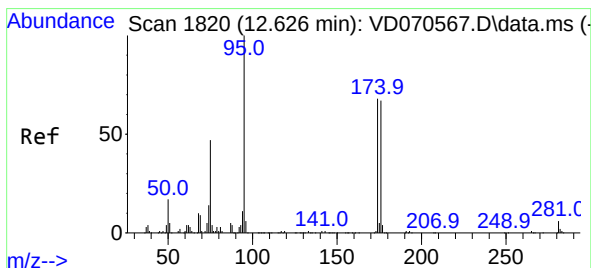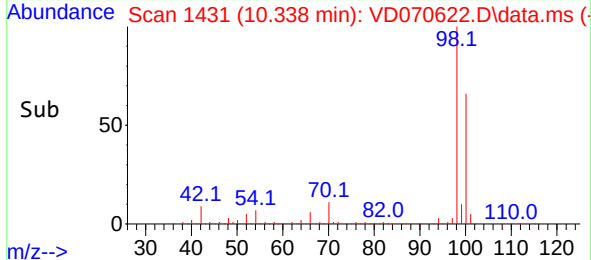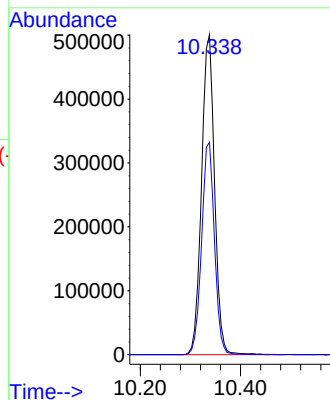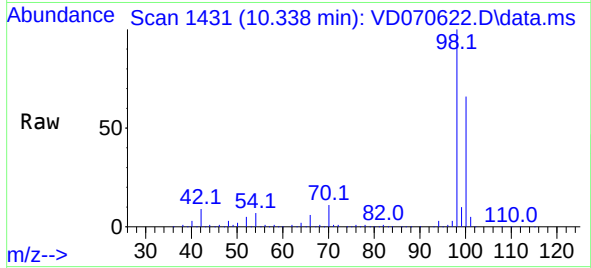

#62
4-Bromofluorobenzene
Concen: 44.50 ug/l
RT: 12.626 min Scan# 1820
Delta R.T. 0.000 min
Lab File: VD070622.D
Acq: 07 Oct 2021 17:40

Tgt Ion: 95 Resp: 266926
Ion Ratio Lower Upper
95 100
174 75.8 0.0 138.0
176 71.7 0.0 135.6


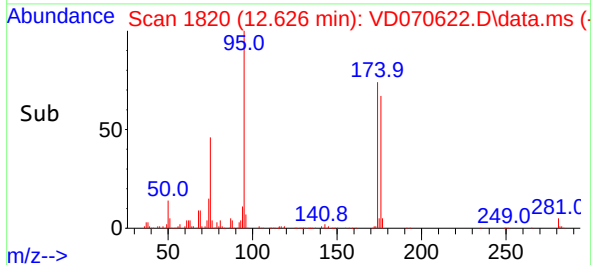
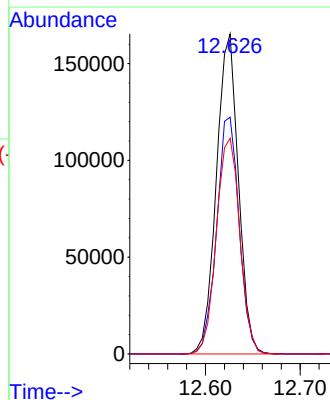
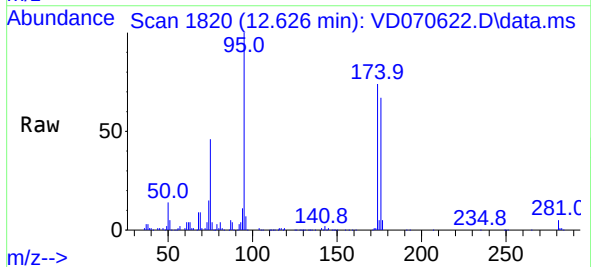


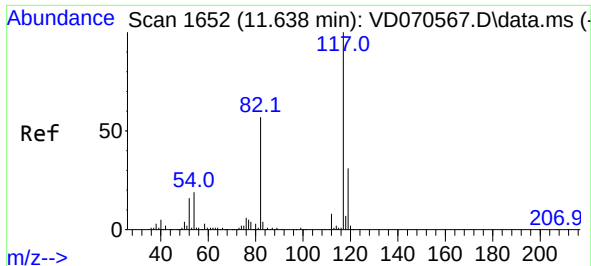

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.638 min Scan# 1652
Delta R.T. 0.000 min
Lab File: VD070622.D
Acq: 07 Oct 2021 17:40

Instrument :
MSVOA_D
ClientSampleId :
SB-1(6.5-7.0)

Tgt Ion:	117	Resp:	661972
Ion	Ratio	Lower	Upper
117	100		
82	55.5	45.4	68.2
119	32.1	24.7	37.1

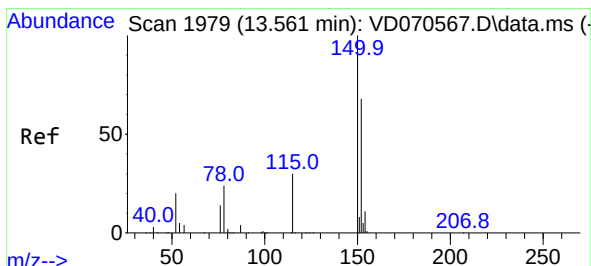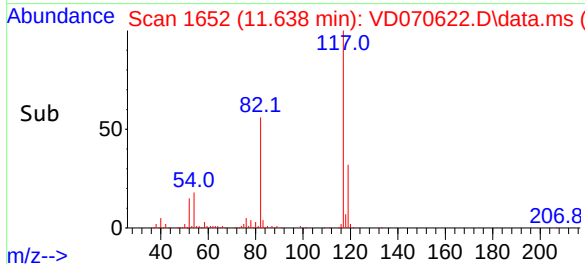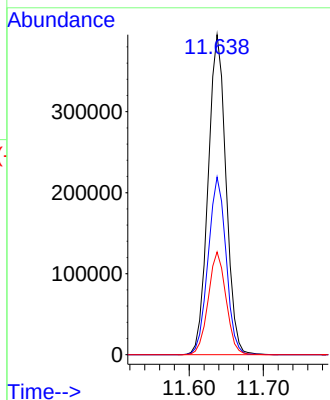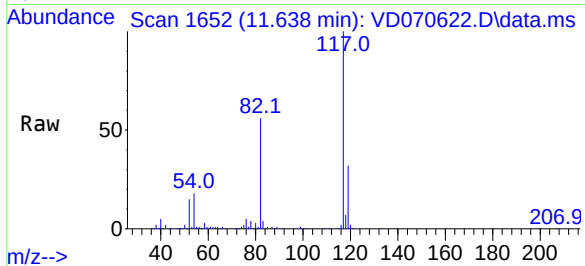

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.567 min Scan# 1980
Delta R.T. 0.006 min
Lab File: VD070622.D
Acq: 07 Oct 2021 17:40

Tgt Ion:	152	Resp:	275167
Ion	Ratio	Lower	Upper
152	100		
115	61.9	31.9	95.7
150	155.3	0.0	350.0

