

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD100721\
 Data File : VD070618.D
 Acq On : 07 Oct 2021 15:47
 Operator : VA/SY
 Sample : M4113-05
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 TP-3

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D100521S.M
 Title : SW846 8260

Signal : TIC: VD070618.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.209	47	49	50	rBV2	1548	1362	2.17%	0.288%
2	2.379	76	78	81	rVB	1534	1306	2.08%	0.276%
3	2.403	81	82	85	rBV3	1968	1698	2.71%	0.359%
4	2.509	99	100	102	rVB	2136	991	1.58%	0.209%
5	2.638	120	122	125	rVV	1114	1309	2.09%	0.277%
6	2.668	125	127	130	rVV2	1139	1472	2.35%	0.311%
7	2.862	156	160	164	rVB2	1187	1414	2.25%	0.299%
8	3.003	183	184	187	rVB2	1241	1040	1.66%	0.220%
9	3.044	187	191	193	rBV2	1386	1926	3.07%	0.407%
10	3.368	244	246	252	rBV2	939	1711	2.73%	0.361%
11	3.479	261	265	268	rBV2	1282	2591	4.13%	0.547%
12	3.597	283	285	287	rBV	1630	1074	1.71%	0.227%
13	3.732	303	308	309	rBV2	1506	2113	3.37%	0.446%
14	3.832	322	325	328	rVB2	978	1209	1.93%	0.255%
15	4.162	378	381	384	rBV2	944	1248	1.99%	0.264%
16	4.350	410	413	416	rVB2	830	963	1.53%	0.203%
17	4.397	420	421	426	rBV2	739	1069	1.70%	0.226%
18	4.644	459	463	465	rBV2	1059	1470	2.34%	0.311%
19	4.903	505	507	511	rBV2	923	1154	1.84%	0.244%
20	4.950	513	515	517	rBV2	1190	1434	2.28%	0.303%
21	4.991	520	522	526	rVB2	979	1308	2.08%	0.276%
22	5.114	541	543	546	rBV2	959	1156	1.84%	0.244%
23	5.173	549	553	555	rBV	758	996	1.59%	0.210%
24	5.332	579	580	585	rVB2	872	1193	1.90%	0.252%
25	5.697	640	642	645	rVB	1222	1182	1.88%	0.250%
26	5.732	645	648	650	rBV2	800	1131	1.80%	0.239%
27	6.056	702	703	707	rVV2	1104	1110	1.77%	0.234%
28	6.279	740	741	743	rBV	2348	1204	1.92%	0.254%
29	6.403	759	762	764	rVB2	1086	1396	2.22%	0.295%
30	6.432	764	767	769	rBV2	948	1015	1.62%	0.214%
31	6.797	827	829	832	rVV2	1140	1285	2.05%	0.271%
32	6.826	832	834	839	rVV2	1293	1202	1.92%	0.254%
33	6.914	847	849	853	rVB2	922	1191	1.90%	0.252%
34	6.956	853	856	859	rVB2	795	971	1.55%	0.205%
35	7.526	948	953	955	rVV	827	1085	1.73%	0.229%
36	7.620	967	969	972	rVB	1467	1200	1.91%	0.254%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD100721\
 Data File : VD070618.D
 Acq On : 07 Oct 2021 15:47
 Operator : VA/SY
 Sample : M4113-05
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 TP-3

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D100521S.M
 Title : SW846 8260

37	7.908	1009	1018	1024	rBV2	11569	24971	39.78%	5.275%
38	7.973	1024	1029	1038	rVB3	17567	36449	58.07%	7.700%
39	8.326	1081	1089	1096	rBV4	14612	33705	53.70%	7.120%
40	8.444	1105	1109	1111	rVB	1191	1347	2.15%	0.285%
41	8.473	1111	1114	1117	rVV2	1121	1341	2.14%	0.283%
42	8.855	1173	1179	1188	rBV2	22266	45759	72.90%	9.667%
43	8.944	1193	1194	1199	rVB2	1078	991	1.58%	0.209%
44	9.502	1287	1289	1295	rVB2	1040	1269	2.02%	0.268%
45	9.838	1343	1346	1348	rBV	1461	1726	2.75%	0.365%
46	9.861	1348	1350	1353	rVB2	1359	1096	1.75%	0.232%
47	9.891	1353	1355	1358	rBV2	1049	1082	1.72%	0.229%
48	10.232	1410	1413	1416	rVB	1060	1315	2.10%	0.278%
49	10.332	1424	1430	1439	rVB	34119	62767	100.00%	13.260%
50	10.620	1477	1479	1482	rVV	962	1065	1.70%	0.225%
51	10.673	1484	1488	1489	rBV2	873	973	1.55%	0.206%
52	11.191	1574	1576	1579	rVB2	1068	1000	1.59%	0.211%
53	11.391	1607	1610	1612	rBV2	1095	1233	1.96%	0.260%
54	11.426	1614	1616	1620	rBV2	1049	1061	1.69%	0.224%
55	11.638	1646	1652	1660	rVB2	29322	53761	85.65%	11.358%
56	11.696	1660	1662	1665	rBV2	1110	1101	1.75%	0.233%
57	11.767	1672	1674	1678	rVB3	1619	1865	2.97%	0.394%
58	11.802	1678	1680	1681	rBV	1830	1443	2.30%	0.305%
59	12.020	1715	1717	1719	rBV	992	997	1.59%	0.211%
60	12.073	1725	1726	1728	rBV2	1646	1308	2.08%	0.276%
61	12.161	1736	1741	1742	rBV2	1303	1823	2.90%	0.385%
62	12.420	1783	1785	1790	rVV2	853	1049	1.67%	0.222%
63	12.626	1813	1820	1829	rVB3	19766	34294	54.64%	7.245%
64	12.702	1829	1833	1836	rBV	1599	2444	3.89%	0.516%
65	12.791	1844	1848	1850	rBV2	1324	1878	2.99%	0.397%
66	12.926	1870	1871	1875	rVV3	1200	1251	1.99%	0.264%
67	12.973	1875	1879	1882	rVV	1248	1549	2.47%	0.327%
68	13.026	1886	1888	1891	rBV	1645	1825	2.91%	0.386%
69	13.096	1898	1900	1902	rVB2	1810	1349	2.15%	0.285%
70	13.132	1902	1906	1907	rBV3	1293	1387	2.21%	0.293%
71	13.373	1944	1947	1949	rBV2	738	968	1.54%	0.204%
72	13.438	1957	1958	1964	rVB2	1368	1796	2.86%	0.379%
73	13.561	1973	1979	1986	rVB2	28656	45515	72.51%	9.615%
74	13.702	2002	2003	2005	rBV	1448	1156	1.84%	0.244%
75	13.726	2005	2007	2010	rVB2	1411	1207	1.92%	0.255%
76	13.843	2024	2027	2028	rBV2	1282	1177	1.88%	0.249%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD100721\
 Data File : VD070618.D
 Acq On : 07 Oct 2021 15:47
 Operator : VA/SY
 Sample : M4113-05
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 TP-3

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D100521S.M
 Title : SW846 8260

77	13.990	2049	2052	2053	rBV3	1216	1363	2.17%	0.288%
78	14.002	2053	2054	2058	rVB3	1647	1441	2.30%	0.304%
79	14.038	2058	2060	2063	rBV2	1148	1412	2.25%	0.298%
80	14.096	2066	2070	2072	rBV2	1751	2320	3.70%	0.490%
81	14.167	2080	2082	2083	rVB	1752	997	1.59%	0.211%
82	14.196	2083	2087	2088	rVB3	1706	1805	2.88%	0.381%
83	14.232	2088	2093	2094	rBV3	1129	1677	2.67%	0.354%
84	14.338	2110	2111	2114	rVB2	1838	1197	1.91%	0.253%
85	14.396	2117	2121	2122	rBV3	1752	2158	3.44%	0.456%
86	14.620	2152	2159	2160	rBV4	2028	2884	4.59%	0.609%
87	15.055	2230	2233	2235	rBV3	2324	2439	3.89%	0.515%
88	15.102	2239	2241	2244	rVV	2641	1813	2.89%	0.383%
89	15.143	2246	2248	2249	rBV2	1572	1217	1.94%	0.257%
90	15.379	2285	2288	2289	rBV3	2002	2246	3.58%	0.474%
91	15.426	2294	2296	2298	rBV	2086	1670	2.66%	0.353%
92	15.555	2316	2318	2319	rBV2	2153	1466	2.34%	0.310%
93	15.590	2323	2324	2326	rVB	2160	1159	1.85%	0.245%
94	15.832	2363	2365	2366	rBV2	1795	1335	2.13%	0.282%
95	15.949	2383	2385	2387	rBV3	1841	1595	2.54%	0.337%
96	15.973	2387	2389	2392	rVV3	2202	1722	2.74%	0.364%
97	16.390	2457	2460	2462	rBV3	2317	2815	4.48%	0.595%
98	16.414	2462	2464	2466	rVV2	2607	2615	4.17%	0.552%
99	16.461	2470	2472	2477	rVB5	3585	3604	5.74%	0.761%
100	16.767	2522	2524	2527	rBV2	2169	2930	4.67%	0.619%


Sum of corrected areas: 473352

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD100721\
Data File : VD070618.D
Acq On : 07 Oct 2021 15:47
Operator : VA/SY
Sample : M4113-05
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
TP-3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D100521S.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

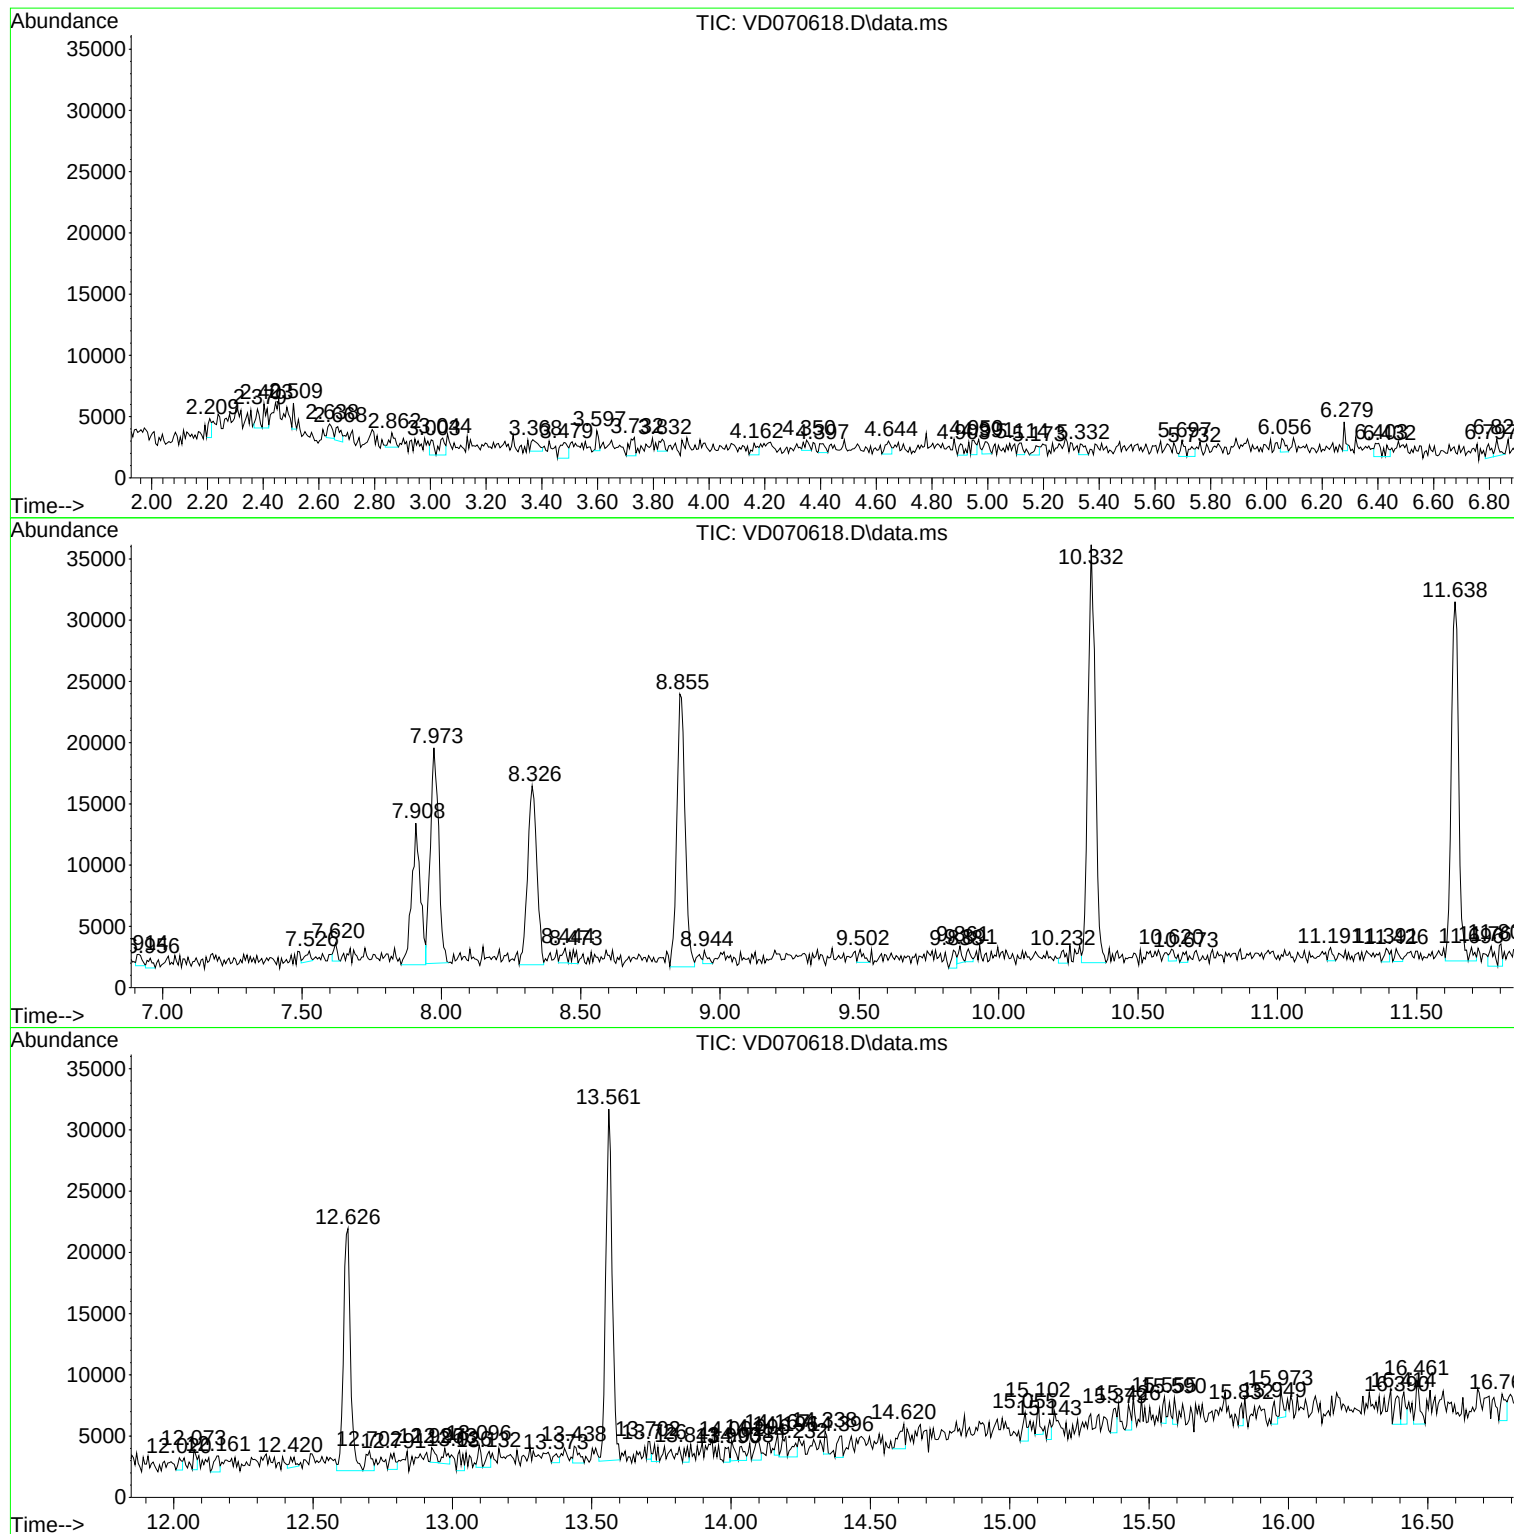

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD100721\
Data File : VD070618.D
Acq On : 07 Oct 2021 15:47
Operator : VA/SY
Sample : M4113-05
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
TP-3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D100521S.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD100721\
Data File : VD070618.D
Acq On : 07 Oct 2021 15:47
Operator : VA/SY
Sample : M4113-05
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
TP-3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D100521S.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
