
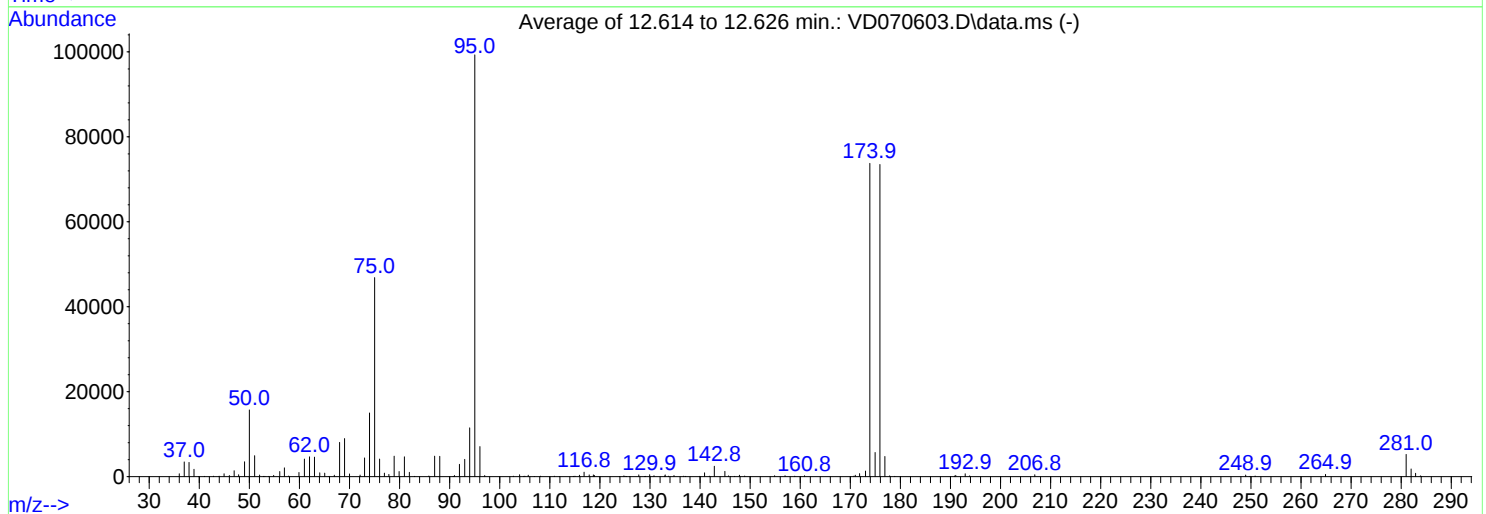


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD100721\
Data File : VD070603.D
Acq On : 07 Oct 2021 08:20
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D100521S.M
Title : SW846 8260
Last Update : Wed Oct 06 09:10:31 2021

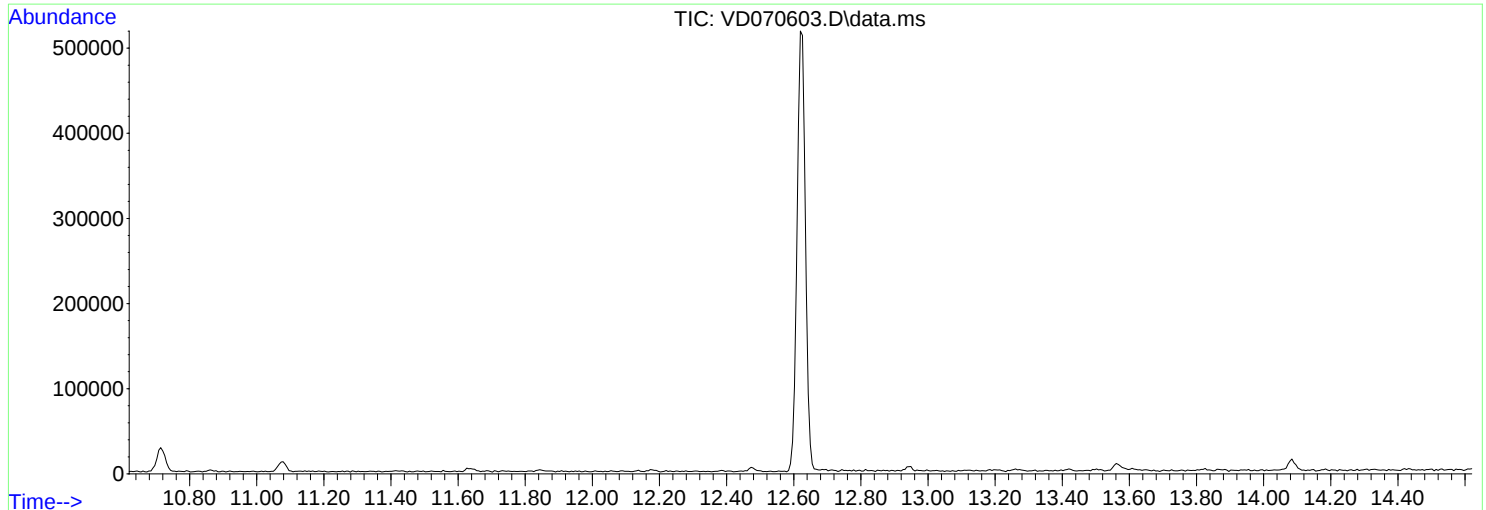

AutoFind: Scans 1818, 1819, 1820; Background Corrected with Scan 1810

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.8	15724	PASS
75	95	30	60	47.2	46851	PASS
95	95	100	100	100.0	99309	PASS
96	95	5	9	7.1	7094	PASS
173	174	0.00	2	1.8	1317	PASS
174	95	50	100	74.3	73763	PASS
175	174	5	9	7.7	5672	PASS
176	174	95	101	99.6	73501	PASS
177	176	5	9	6.4	4740	PASS