

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD100722\
 Data File : VD074492.D
 Acq On : 07 Oct 2022 15:52
 Operator : VA/SY
 Sample : N5014-13
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 SB-01-0-2.0

Quant Time: Oct 08 02:25:08 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D100522S.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 06 01:54:40 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.875	168	109564	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.775	114	197854	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.581	117	173756	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.510	152	71375	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.234	65	50678	52.061	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	104.120%
35) Dibromofluoromethane	7.804	113	60654	46.490	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	92.980%
50) Toluene-d8	10.269	98	236568	49.655	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	99.300%
62) 4-Bromofluorobenzene	12.569	95	60501	39.825	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	79.660%
Target Compounds						
16) Acetone	4.016	43	3520	24.511	ug/l	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD100722\
Data File : VD074492.D
Acq On : 07 Oct 2022 15:52
Operator : VA/SY
Sample : N5014-13
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
SB-01-0-2.0

Quant Time: Oct 08 02:25:08 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D100522S.M
Quant Title : SW846 8260
QLast Update : Thu Oct 06 01:54:40 2022
Response via : Initial Calibration




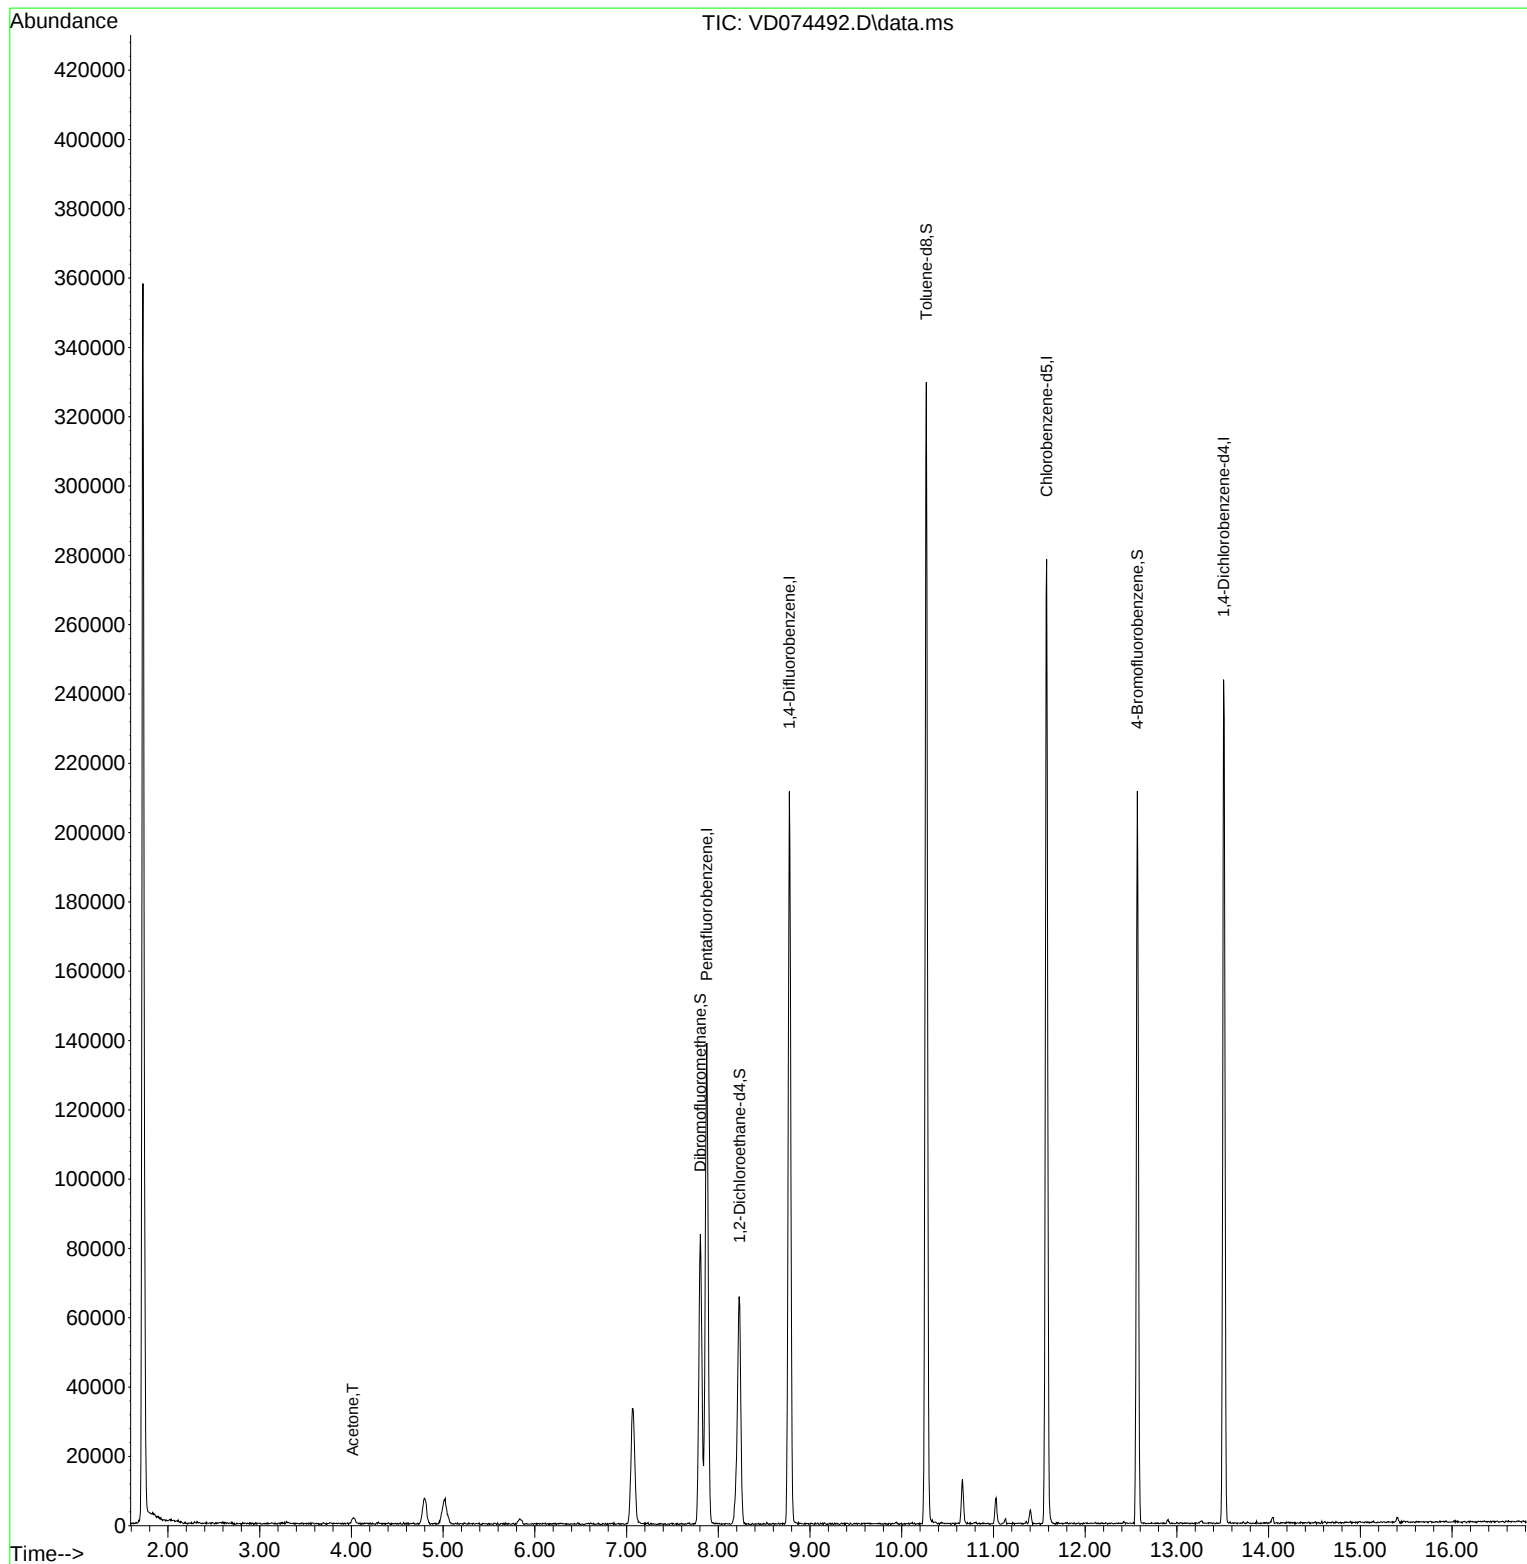


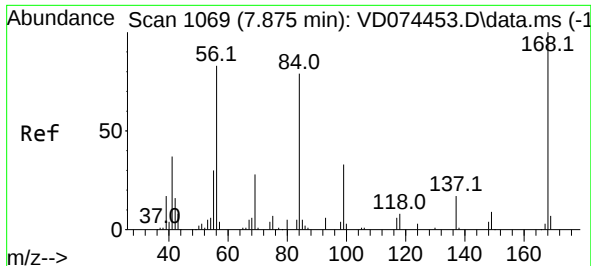

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.875 min Scan# 1069
Delta R.T. 0.000 min
Lab File: VD074492.D
Acq: 07 Oct 2022 15:52




Instrument :
MSVOA_D
ClientSampleId :
SB-01-0-2.0


Tgt Ion:168 Resp: 109564
Ion Ratio Lower Upper
168 100
99 51.8 40.9 61.3

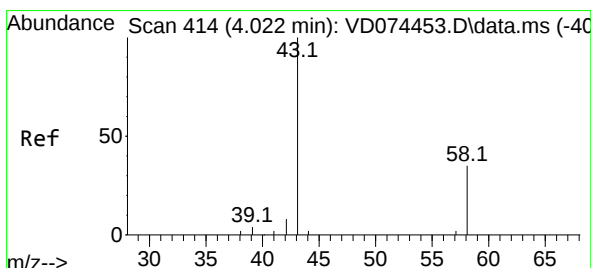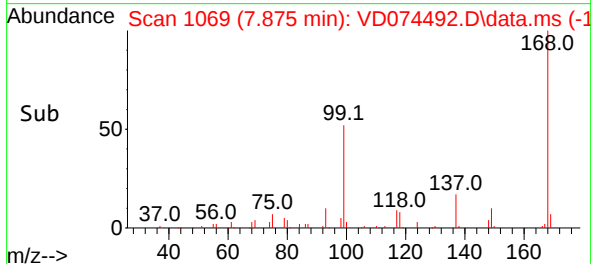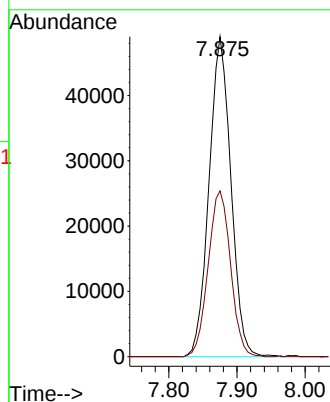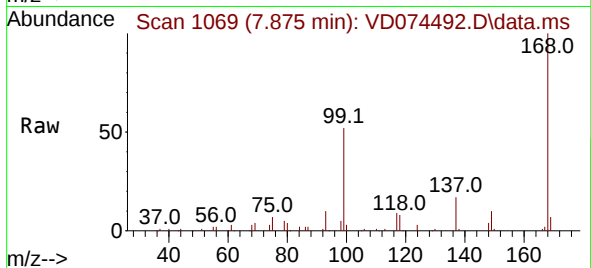

#16
Acetone
Concen: 24.511 ug/l
RT: 4.016 min Scan# 413
Delta R.T. -0.006 min
Lab File: VD074492.D
Acq: 07 Oct 2022 15:52

Tgt Ion: 43 Resp: 3520
Ion Ratio Lower Upper
43 100
58 35.5 30.2 45.2

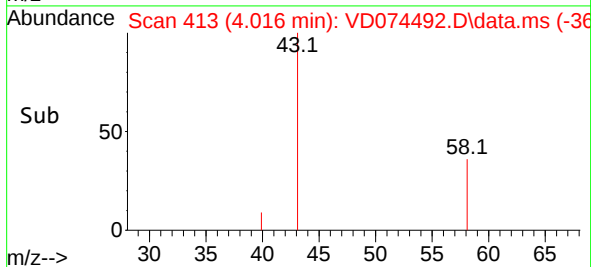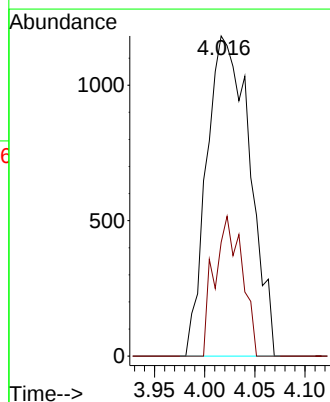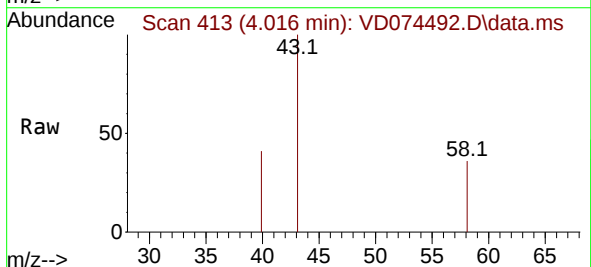

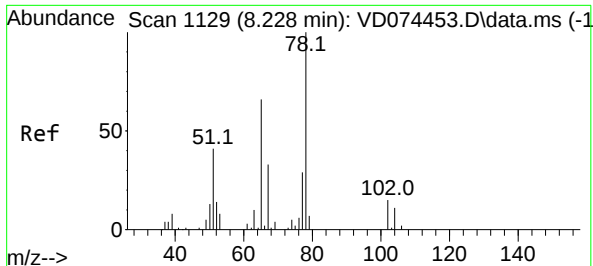

#33

1,2-Dichloroethane-d4

Concen: 52.061 ug/l

RT: 8.234 min Scan# 1129

Delta R.T. 0.006 min

Lab File: VD074492.D

Acq: 07 Oct 2022 15:52

Instrument :

MSVOA_D

ClientSampleId :





SB-01-0-2.0

Tgt Ion: 65 Resp: 50678

Ion Ratio Lower Upper

65 100

67 53.2 0.0 110.2

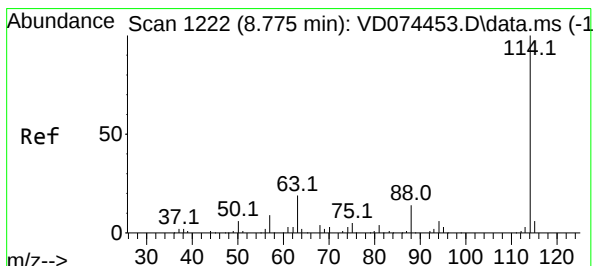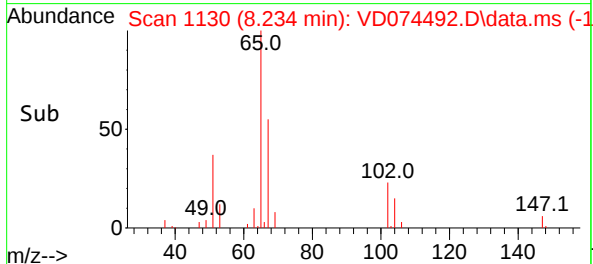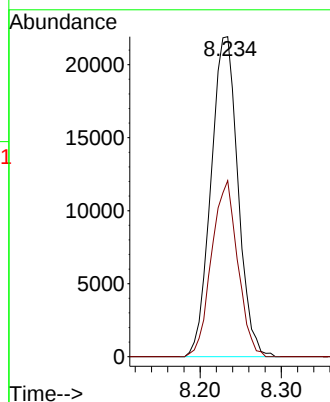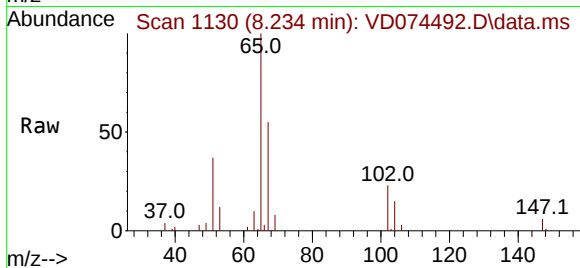

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.775 min Scan# 1222

Delta R.T. -0.000 min

Lab File: VD074492.D

Acq: 07 Oct 2022 15:52




Tgt Ion: 114 Resp: 197854


Ion Ratio Lower Upper

114 100

63 16.8 0.0 33.2

88 13.6 0.0 28.2

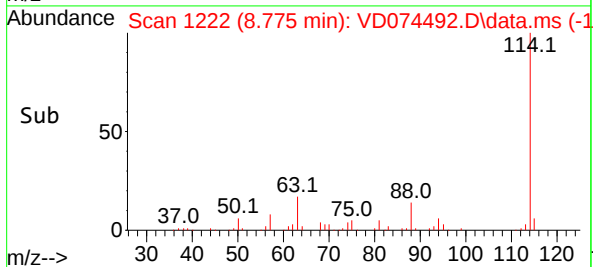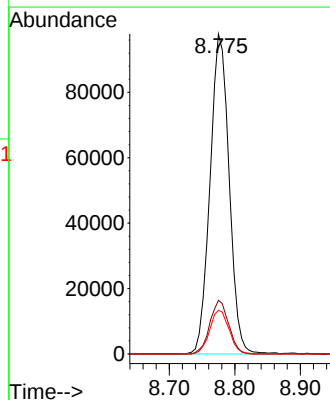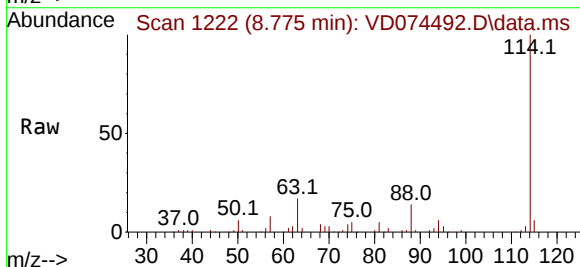

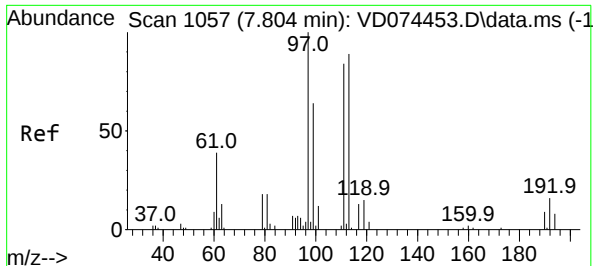

#35

Dibromofluoromethane

Concen: 46.490 ug/l

RT: 7.804 min Scan# 1057

Delta R.T. -0.000 min

Lab File: VD074492.D

Acq: 07 Oct 2022 15:52

Instrument :

MSVOA_D

ClientSampleId :

SB-01-0-2.0





Tgt Ion:113 Resp: 60654

Ion Ratio Lower Upper

113 100

111 103.7 82.3 123.5

192 18.4 16.4 24.6

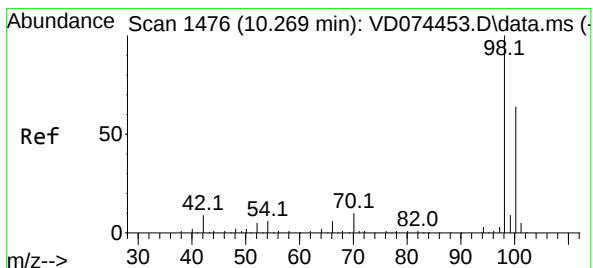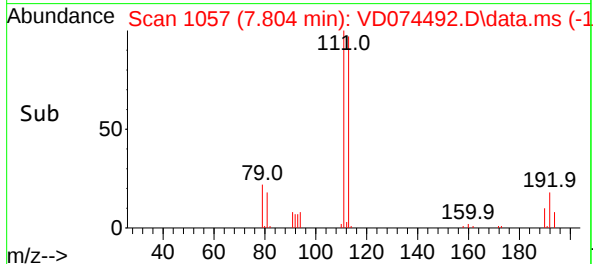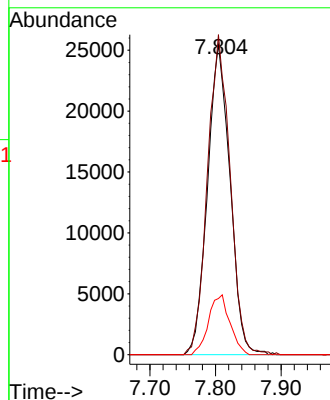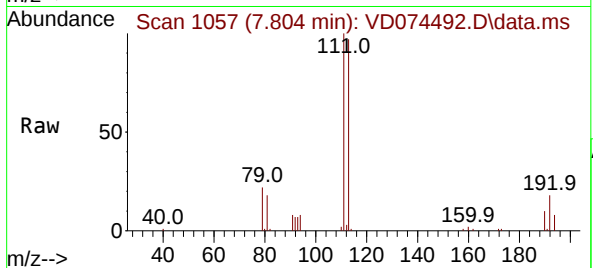

#50

Toluene-d8

Concen: 49.655 ug/l

RT: 10.269 min Scan# 1476

Delta R.T. 0.000 min

Lab File: VD074492.D




Acq: 07 Oct 2022 15:52


Tgt Ion: 98 Resp: 236568

Ion Ratio Lower Upper

98 100

100 64.1 51.4 77.0


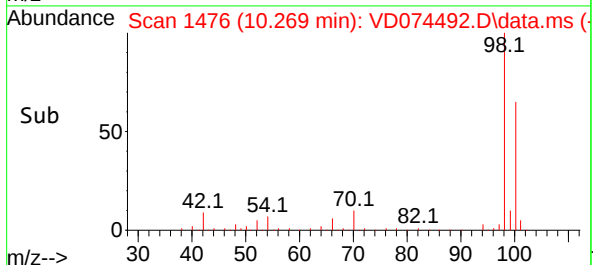
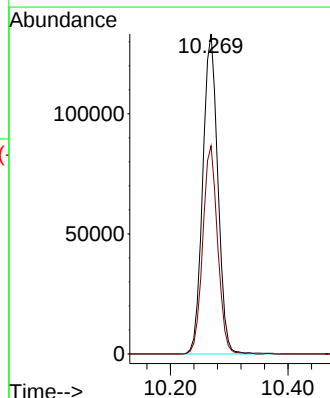
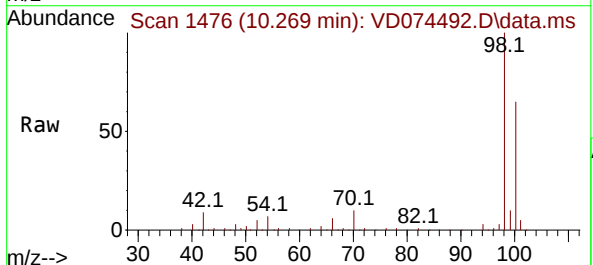


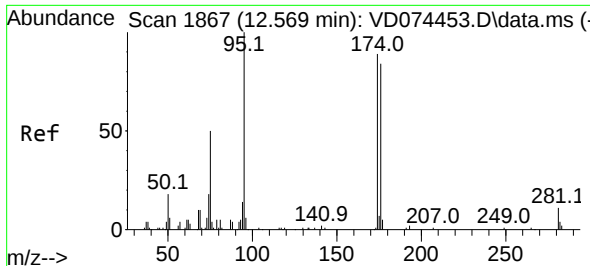

#62
4-Bromofluorobenzene
Concen: 39.825 ug/l
RT: 12.569 min Scan# 1867
Delta R.T. -0.000 min
Lab File: VD074492.D
Acq: 07 Oct 2022 15:52




Instrument :
MSVOA_D
ClientSampleId :
SB-01-0-2.0


Tgt Ion: 95 Resp: 60501
Ion Ratio Lower Upper
95 100
174 94.9 0.0 197.0
176 91.5 0.0 182.6

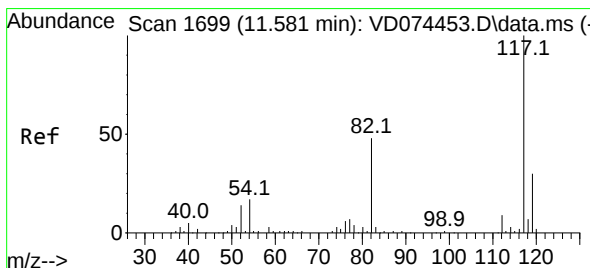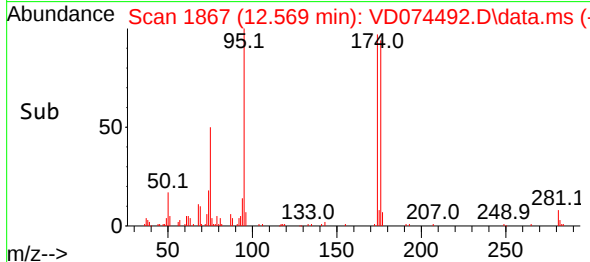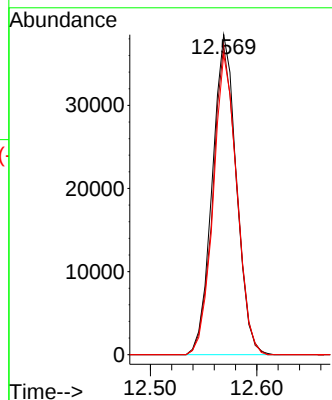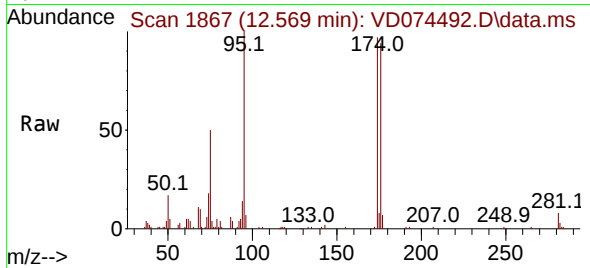

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.581 min Scan# 1699
Delta R.T. -0.000 min
Lab File: VD074492.D
Acq: 07 Oct 2022 15:52

Tgt Ion: 117 Resp: 173756
Ion Ratio Lower Upper
117 100
82 50.4 41.6 62.4
119 29.8 25.2 37.8

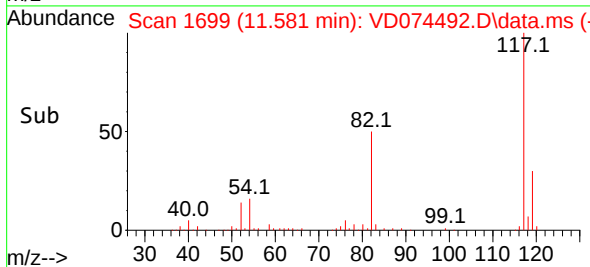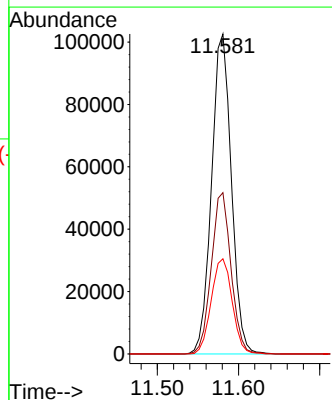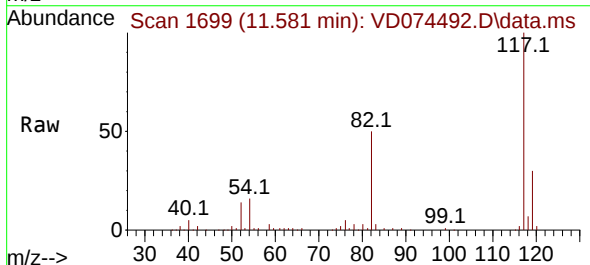

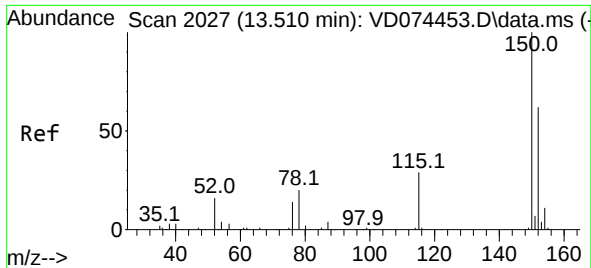

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.510 min Scan# 20

Delta R.T. -0.000 min

Lab File: VD074492.D


Acq: 07 Oct 2022 15:52

Instrument :

MSVOA_D

ClientSampleId :

SB-01-0-2.0

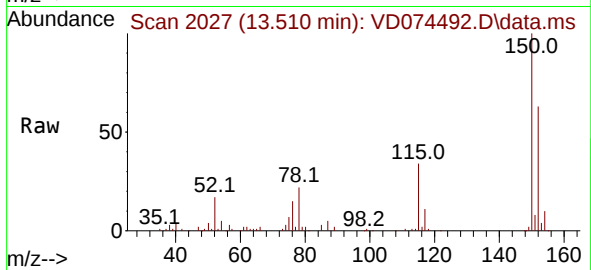

Tgt Ion:152 Resp: 71375

Ion Ratio Lower Upper

152 100

115 53.8 26.8 80.4

150 156.0 0.0 348.2

