


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD101018\
Data File : VD060166.D
Acq On : 10 Oct 2018 10:17
Operator : VA/AP
Sample : BFB
Misc : 5.00µl/5ml/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D100118S.M
Title : SW846 8260
Last Update : Tue Oct 02 06:56:35 2018

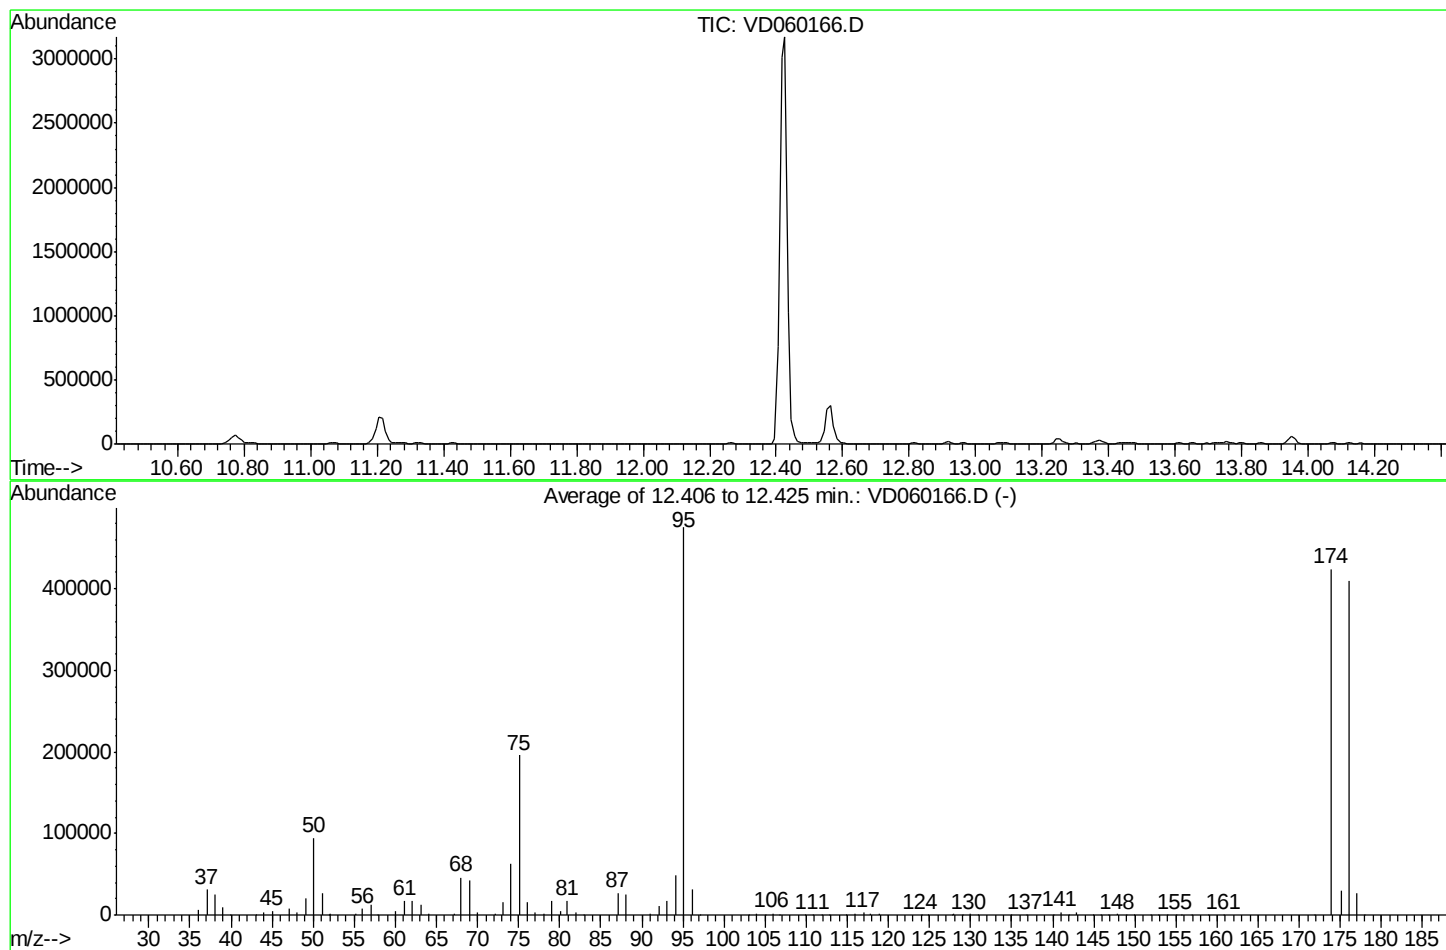

AutoFind: Scans 1106, 1107, 1108; Background Corrected with Scan 1102

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.9	94557	PASS
75	95	30	60	41.2	195685	PASS
95	95	100	100	100.0	475370	PASS
96	95	5	9	6.6	31456	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	89.2	423840	PASS
175	174	5	9	7.2	30617	PASS
176	174	95	101	96.7	410045	PASS
177	176	5	9	6.5	26588	PASS