

Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD101019\
 Data File : VD063913.D
 Acq On : 10 Oct 2019 16:38
 Operator : VA/SY
 Sample : K5285-13
 Misc : 4.90G/MSVOA D/SOIL
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :

Quant Time: Oct 11 07:39:53 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D100219S.M
 Quant Title : SW846 8260
 QLast Update : Sat Oct 05 03:51:17 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.98	168	10798	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.86	114	19084	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.65	117	17933	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.58	152	8433	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.34	65	6768	64.38	ug/l	0.00
Spiked Amount	50.000		Recovery	=	128.76%	
35) Dibromofluoromethane	7.91	113	6551	56.17	ug/l	0.00
Spiked Amount	50.000		Recovery	=	112.34%	
50) Toluene-d8	10.34	98	22099	46.68	ug/l	0.00
Spiked Amount	50.000		Recovery	=	93.36%	
62) 4-Bromofluorobenzene	12.63	95	8241	50.10	ug/l	0.00
Spiked Amount	50.000		Recovery	=	100.20%	
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	2.24	85	154	2.011 ug/l #		47
3) Chloromethane	2.20	50	343	Below Cal #		40
5) Bromomethane	2.78	94	600	3.771 ug/l		95
8) Diethyl Ether	3.88	74	55	1.047 ug/l #		1
11) Tert butyl alcohol	5.24	59	58	Below Cal #		1
13) Acrolein	3.93	56	54	5.751 ug/l #		17
15) Acrylonitrile	5.54	53	149	6.435 ug/l #		17
16) Acetone	4.15	43	480	17.537 ug/l #		42
18) Methyl Acetate	4.74	43	132	2.466 ug/l #		49
20) Methylene Chloride	4.97	84	158	Below Cal #		7
25) 2-Butanone	7.21	43	81	2.497 ug/l #		51
28) Bromochloromethane	7.70	49	166	4.085 ug/l #		10
29) Tetrahydrofuran	7.57	42	59	3.116 ug/l #		25
31) Cyclohexane	7.98	56	204	Below Cal #		13
36) 1,1-Dichloropropene	8.02	75	201	1.152 ug/l #		64
37) Ethyl Acetate	7.28	43	70	Below Cal #		68
38) Carbon Tetrachloride	7.98	117	728	4.129 ug/l #		15
41) Methacrylonitrile	7.53	41	68	1.681 ug/l #		4
46) Dibromomethane	9.54	93	71	1.019 ug/l #		3
49) 1,4-Dioxane	9.65	88	69	72.521 ug/l #		14
51) 4-Methyl-2-Pentanone	10.35	43	130	1.713 ug/l #		1
53) t-1,3-Dichloropropene	10.52	75	219	1.251 ug/l #		1
55) 1,1,2-Trichloroethane	10.78	97	142	1.443 ug/l #		14
59) 2-Hexanone	10.99	43	119	2.168 ug/l #		24
76) 1,2,3-Trichloropropane	12.78	75	183	3.240 ug/l #		100
81) trans-1,4-Dichloro-2-buten	12.63	75	4002	125.384 ug/l #		13
92) 1,2-Dibromo-3-Chloropropan	14.48	75	66	1.944 ug/l #		1
96) 1,2,3-Trichlorobenzene	15.58	180	174	1.087 ug/l #		13


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD101019\
Data File : VD063913.D
Acq On : 10 Oct 2019 16:38
Operator : VA/SY
Sample : K5285-13
Misc : 4.90G/MSVOA D/SOIL
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :

Quant Time: Oct 11 07:39:53 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D100219S.M
Quant Title : SW846 8260
QLast Update : Sat Oct 05 03:51:17 2019
Response via : Initial Calibration

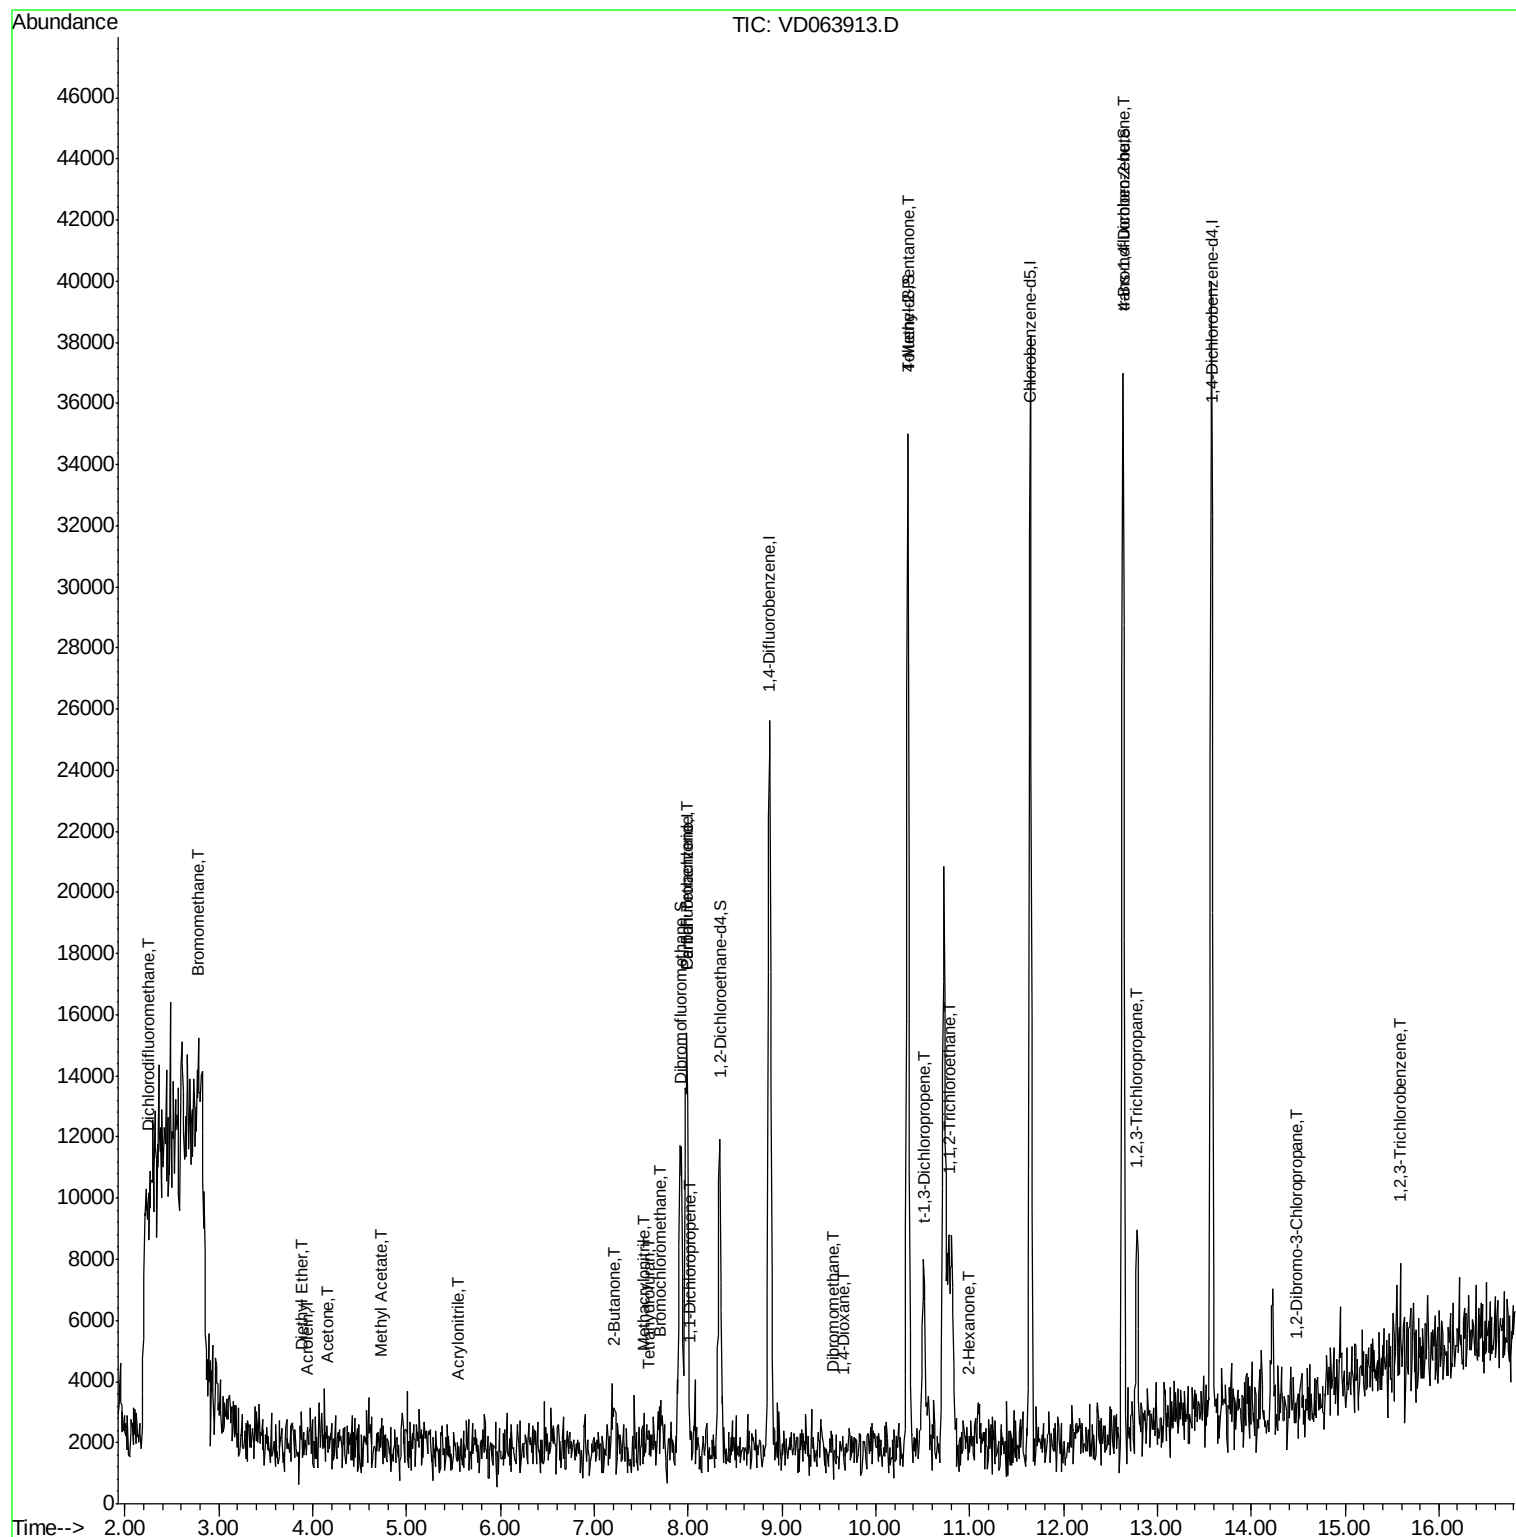


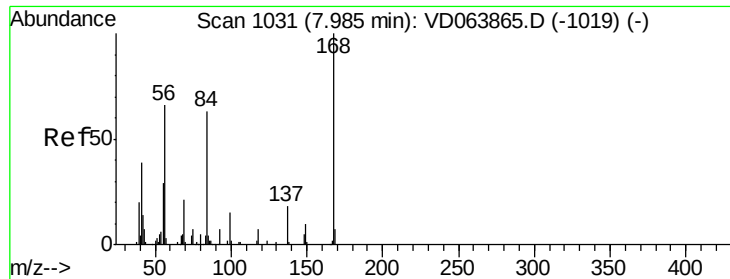




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.98 min Scan# 1031
Delta R.T. -0.00 min
Lab File: VD063913.D
Acq: 10 Oct 2019 16:38

Instrument :
MSVOA_D
ClientSampleId :

Tot Ion:168 Resp: 10798
Ion Ratio Lower Upper
168 100
99 60.6 43.0 64.4




Abundance Ion 167.90 (167.60 to 168.60): V
Ion 98.90 (98.60 to 99.60): VDC

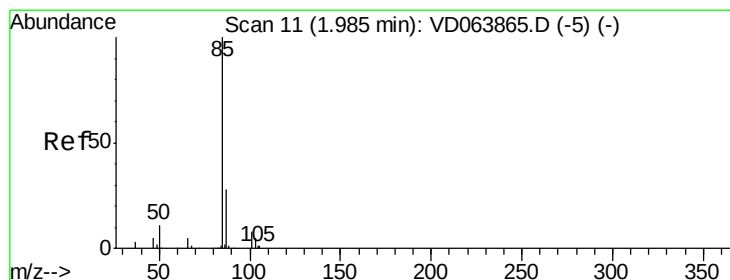
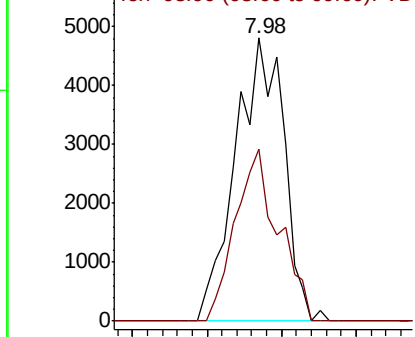



#2
Dichlorodifluoromethane
Concen: 2.011 ug/l
RT: 2.24 min Scan# 55
Delta R.T. 0.26 min
Lab File: VD063913.D
Acq: 10 Oct 2019 16:38

Tgt Ion: 85 Resp: 154
Ion Ratio Lower Upper
85 100
87 0.0 14.0 42.0#



Abundance Ion 84.90 (84.60 to 85.60): VDC
Ion 86.90 (86.60 to 87.60): VDC

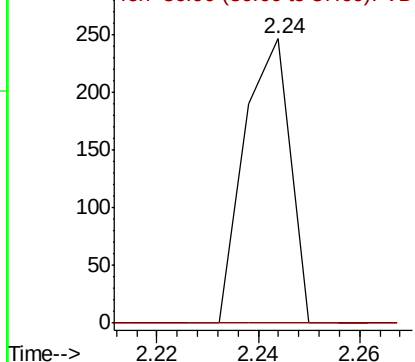



#3

Chloromethane

Concen: Below Cal

RT: 2.20 min Scan# 48

Delta R.T. -0.01 min

Lab File: VD063913.D

Acq: 10 Oct 2019 16:38

Instrument :

MSVOA_D





ClientSampled :

Tot Ion: 50 Resp: 343

Ion Ratio Lower Upper

50 100

52 0.0 27.5 41.3#

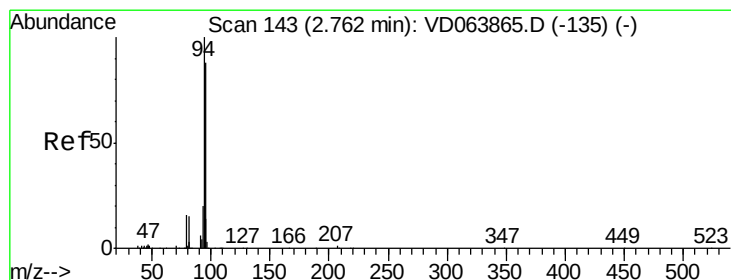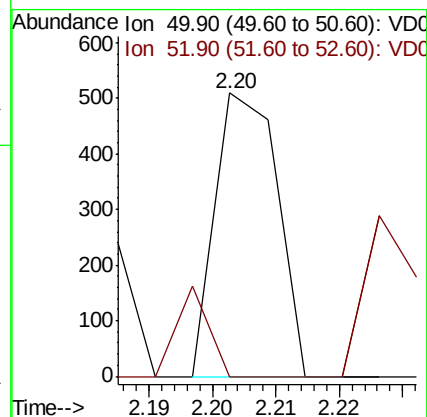

#5

Bromomethane

Concen: 3.771 ug/l

RT: 2.78 min Scan# 146

Delta R.T. 0.02 min

Lab File: VD063913.D




Acq: 10 Oct 2019 16:38


Tgt Ion: 94 Resp: 600

Ion Ratio Lower Upper

94 100

96 92.9 70.8 106.2

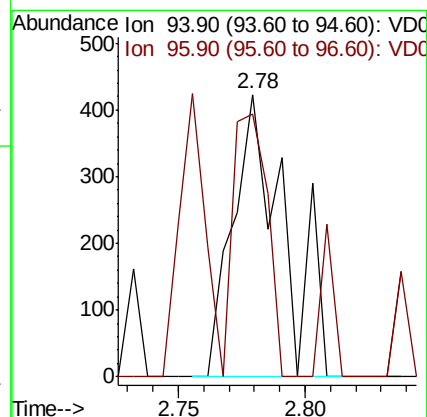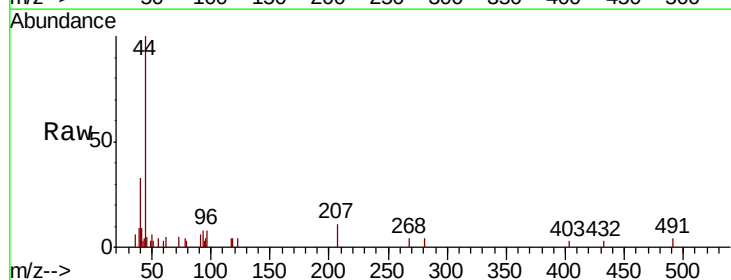



#8

Diethyl Ether

Concen: 1.047 ug/l

RT: 3.88 min Scan# 333

Delta R.T. 0.17 min

Lab File: VD063913.D

Acq: 10 Oct 2019 16:38

Instrument :

MSVOA_D


ClientSampled :

Tot Ion: 74 Resp: 55

Ion Ratio Lower Upper




74 100

45 396.4 48.1 144.4#



Abundance Ion 74.00 (73.70 to 74.70): VDC

Ion 45.00 (44.70 to 45.70): VDC

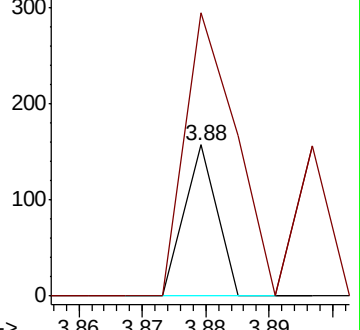

#13

Acrolein

Concen: 5.751 ug/l

RT: 3.93 min Scan# 342

Delta R.T. 0.01 min

Lab File: VD063913.D


Acq: 10 Oct 2019 16:38

Tgt Ion: 56 Resp: 54

Ion Ratio Lower Upper



56 100


55 0.0 53.0 79.6#



Abundance Ion 56.00 (55.70 to 56.70): VDC

Ion 55.00 (54.70 to 55.70): VDC

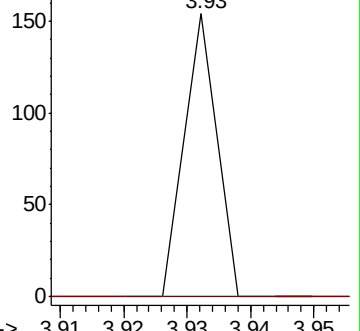



#15

Acrylonitrile

Concen: 6.435 ug/l

RT: 5.54 min Scan# 616

Delta R.T. 0.11 min

Lab File: VD063913.D

Acq: 10 Oct 2019 16:38

Instrument :

MSVOA_D

ClientSampleId :


Tot Ion: 53 Resp: 149

Ion Ratio Lower Upper

53 100

52 0.0 67.3 100.9#




51 0.0 30.5 45.7#

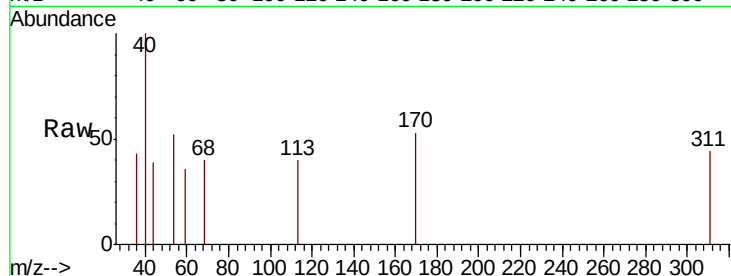

Abundance Ion 53.00 (52.70 to 53.70): VDC

Ion 52.00 (51.70 to 52.70): VDC

Ion 51.00 (50.70 to 51.70): VDC

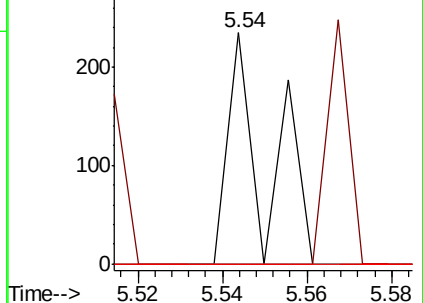

#16

Acetone

Concen: 17.537 ug/l

RT: 4.15 min Scan# 379

Delta R.T. -0.02 min

Lab File: VD063913.D


Acq: 10 Oct 2019 16:38

Tgt Ion: 43 Resp: 480

Ion Ratio Lower Upper



43 100


58 0.0 26.2 39.4#



Abundance Ion 43.00 (42.70 to 43.70): VDC

Ion 58.00 (57.70 to 58.70): VDC



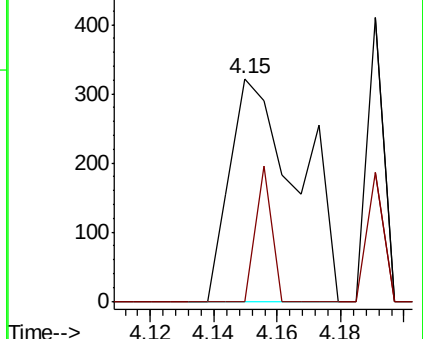





#18
Methyl Acetate
Concen: 2.466 ug/l
RT: 4.74 min Scan# 479
Delta R.T. 0.02 min
Lab File: VD063913.D
Acq: 10 Oct 2019 16:38




Instrument :
MSVOA_D
ClientSampled :


Tot Ion: 43 Resp: 132
Ion Ratio Lower Upper
43 100
74 0.0 20.8 31.2#

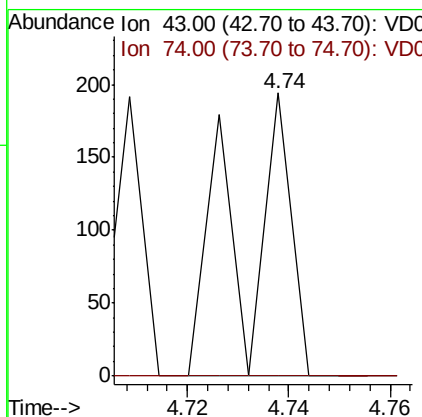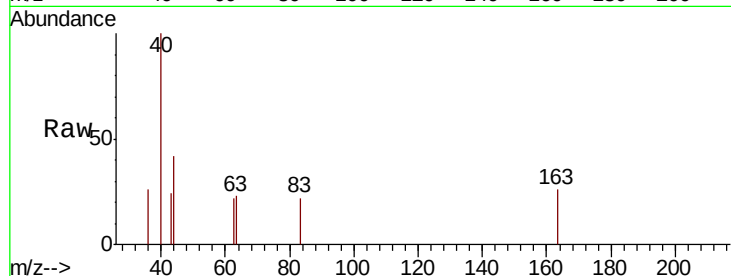

#20
Methylene Chloride
Concen: Below Cal
RT: 4.97 min Scan# 519
Delta R.T. 0.01 min
Lab File: VD063913.D
Acq: 10 Oct 2019 16:38

Tgt Ion: 84 Resp: 158
Ion Ratio Lower Upper
84 100
49 0.0 97.3 145.9#
51 0.0 30.1 45.1#
86 0.0 51.4 77.2#



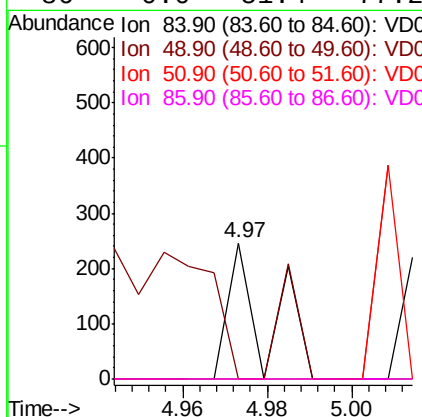



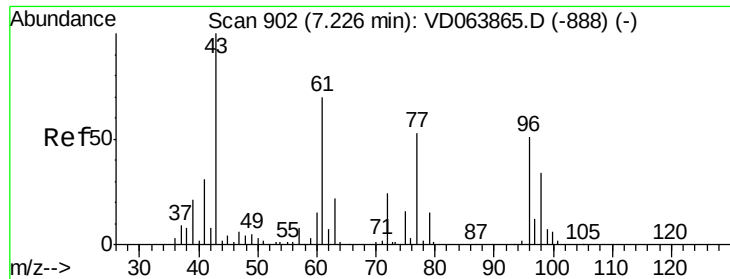

#25
 2-Butanone
 Concen: 2.497 ug/l
 RT: 7.21 min Scan# 900
 Delta R.T. -0.01 min
 Lab File: VD063913.D
 Acq: 10 Oct 2019 16:38




Instrument :
 MSVOA_D
 ClientSampled :


Tot Ion: 43 Resp: 81
 Ion Ratio Lower Upper
 43 100
 72 0.0 19.2 28.8#

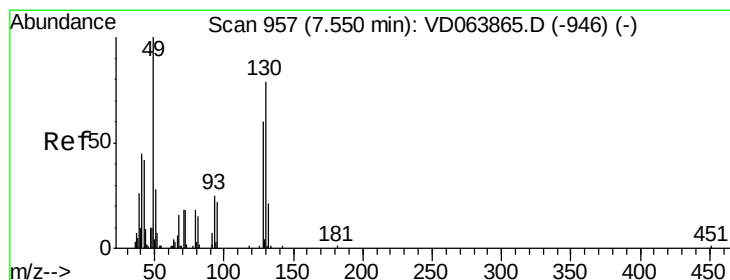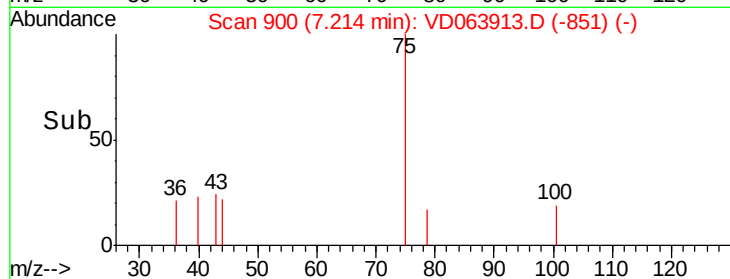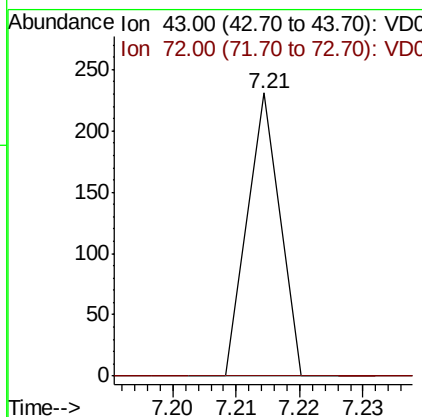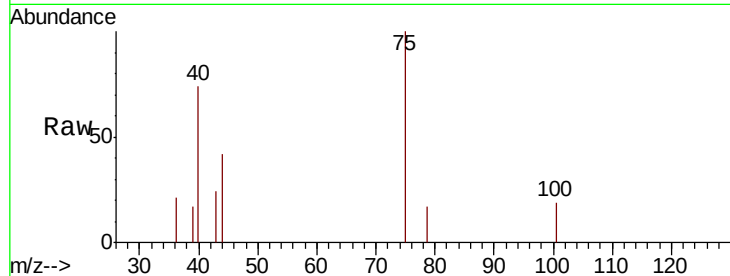

#28
 Bromochloromethane
 Concen: 4.085 ug/l
 RT: 7.70 min Scan# 983
 Delta R.T. 0.15 min
 Lab File: VD063913.D
 Acq: 10 Oct 2019 16:38

Tgt Ion: 49 Resp: 166
 Ion Ratio Lower Upper
 49 100
 129 0.0 0.0 5.6
 130 0.0 66.8 100.2#

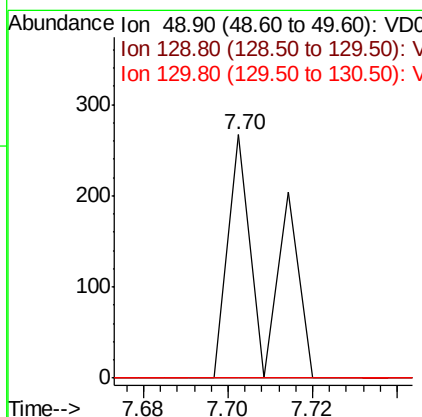


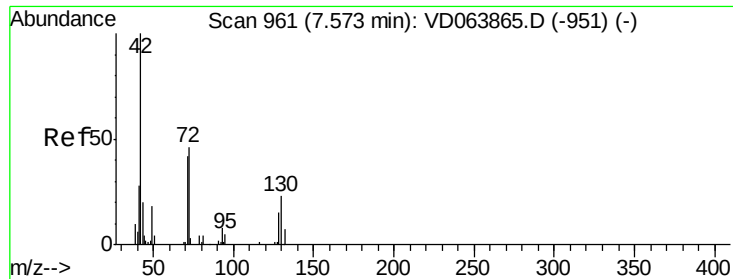




#29
Tetrahydrofuran
Concen: 3.116 ug/l
RT: 7.57 min Scan# 961
Delta R.T. -0.00 min
Lab File: VD063913.D
Acq: 10 Oct 2019 16:38

Instrument :
MSVOA_D
ClientSampled :

Tot Ion: 42 Resp: 59
Ion Ratio Lower Upper
42 100
72 0.0 37.6 56.4#
71 94.9 35.0 52.6#

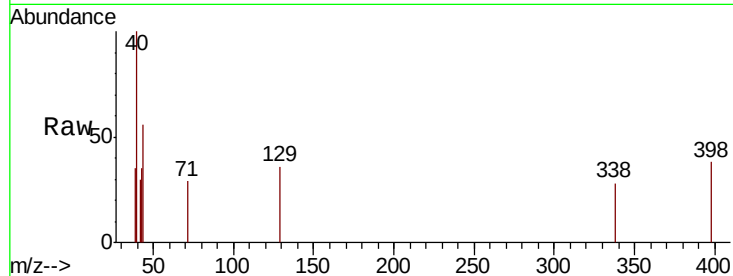


Abundance Ion 42.00 (41.70 to 42.70): VDC
Ion 72.00 (71.70 to 72.70): VDC
Ion 71.00 (70.70 to 71.70): VDC

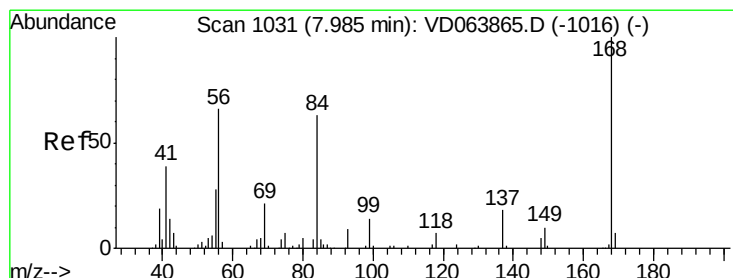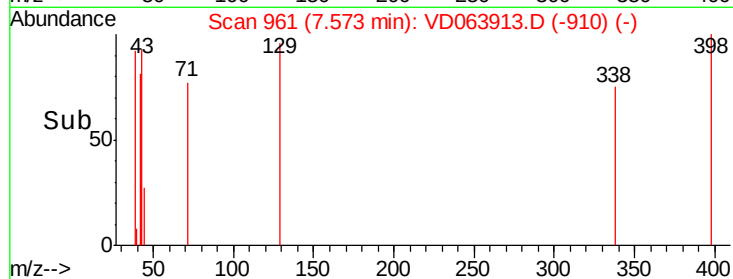
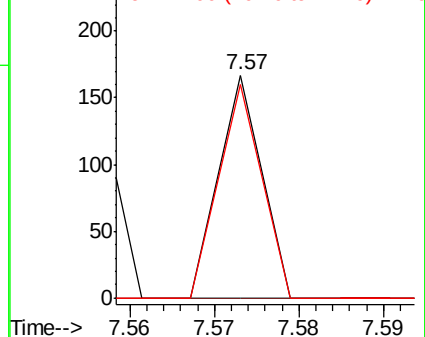



#31
Cyclohexane
Concen: Below Cal
RT: 7.98 min Scan# 1030
Delta R.T. -0.01 min
Lab File: VD063913.D
Acq: 10 Oct 2019 16:38

Tgt Ion: 56 Resp: 204
Ion Ratio Lower Upper
56 100
69 60.1 25.0 37.4#
84 0.0 76.3 114.5#

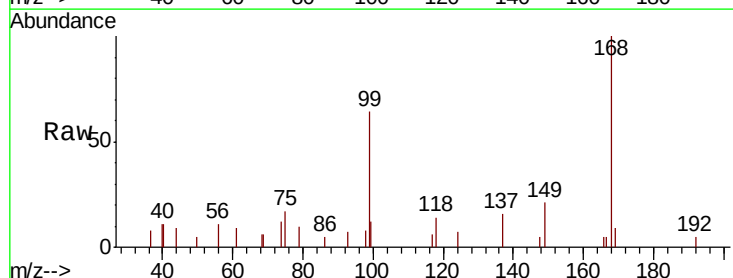

Abundance Ion 56.00 (55.70 to 56.70): VDC
Ion 69.00 (68.70 to 69.70): VDC
Ion 84.00 (83.70 to 84.70): VDC



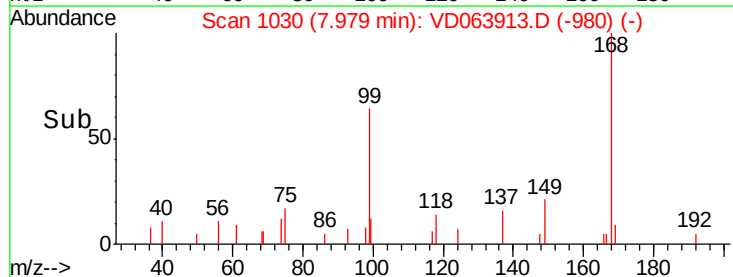
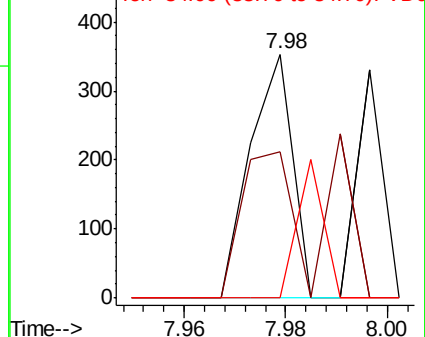




#33
 1,2-Dichloroethane-d4
 Concen: 64.379 ug/l
 RT: 8.34 min Scan# 1091
 Delta R.T. 0.01 min
 Lab File: VD063913.D
 Acq: 10 Oct 2019 16:38




Instrument :
 MSVOA_D
 ClientSampleId :


Tot Ion: 65 Resp: 6768
 Ion Ratio Lower Upper
 65 100
 67 62.4 0.0 106.4

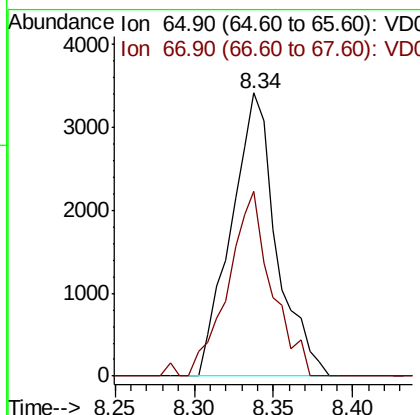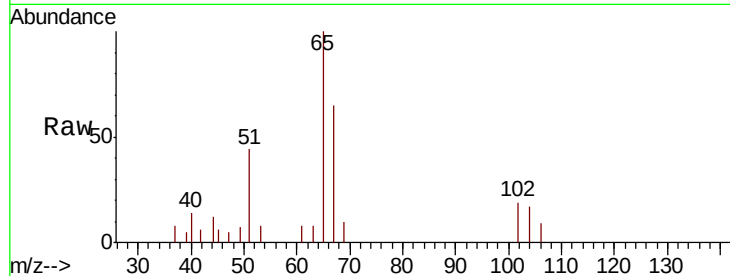

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.86 min Scan# 1180
 Delta R.T. -0.01 min
 Lab File: VD063913.D
 Acq: 10 Oct 2019 16:38

Tgt Ion: 114 Resp: 19084
 Ion Ratio Lower Upper
 114 100
 63 14.5 0.0 38.4
 88 15.3 0.0 27.4

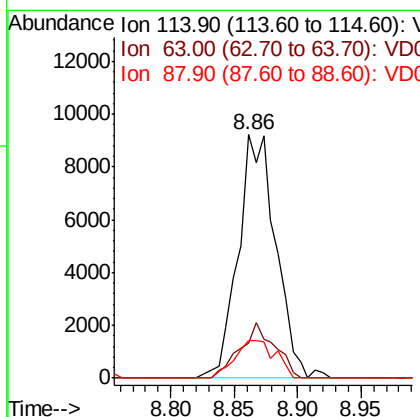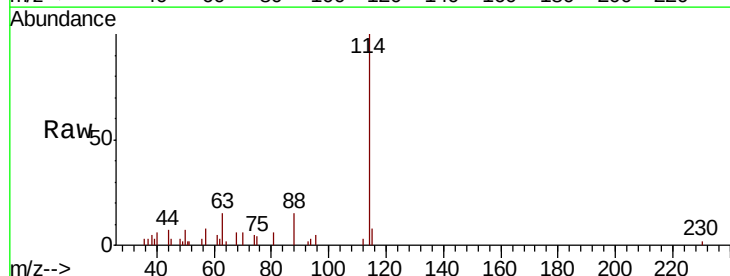



#35

Dibromofluoromethane

Concen: 56.170 ug/l

RT: 7.91 min Scan# 1019

Delta R.T. -0.00 min

Lab File: VD063913.D

Acq: 10 Oct 2019 16:38

Instrument :
MSVOA_D
ClientSampleId :


Tot Ion:113 Resp: 6551

Ion Ratio Lower Upper




113 100

111 101.4 82.6 123.8

192 27.7 17.1 25.7#

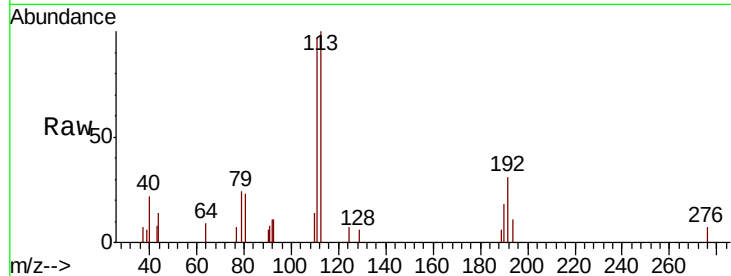

Abundance Ion 112.80 (112.50 to 113.50): V
Ion 110.80 (110.50 to 111.50): V
Ion 191.70 (191.40 to 192.40): V

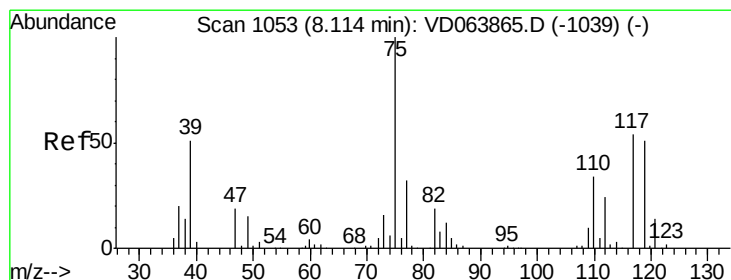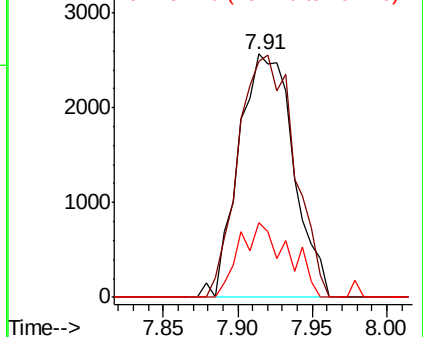

#36

1,1-Dichloropropene

Concen: 1.152 ug/l

RT: 8.02 min Scan# 1037

Delta R.T. -0.09 min

Lab File: VD063913.D

Acq: 10 Oct 2019 16:38


Tgt Ion: 75 Resp: 201

Ion Ratio Lower Upper



75 100


110 0.0 17.4 52.3#

77 36.3 25.4 38.0



Abundance Ion 74.90 (74.60 to 75.60): V
Ion 109.90 (109.60 to 110.60): V
Ion 76.90 (76.60 to 77.60): V




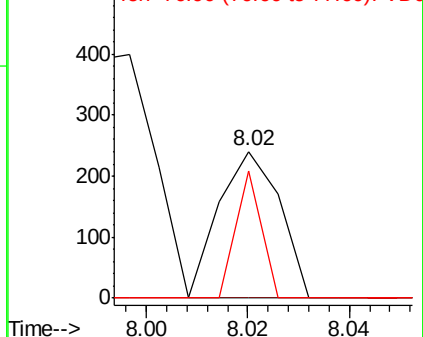




#37
Ethyl Acetate
Concen: Below Cal
RT: 7.28 min Scan# 912
Delta R.T. -0.01 min
Lab File: VD063913.D
Acq: 10 Oct 2019 16:38




Instrument :
MSVOA_D
ClientSampled :


Tot Ion: 43 Resp: 70
Ion Ratio Lower Upper
43 100
61 0.0 11.5 17.3#
70 0.0 8.2 12.4#

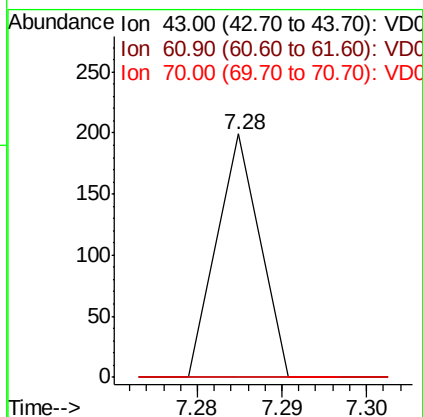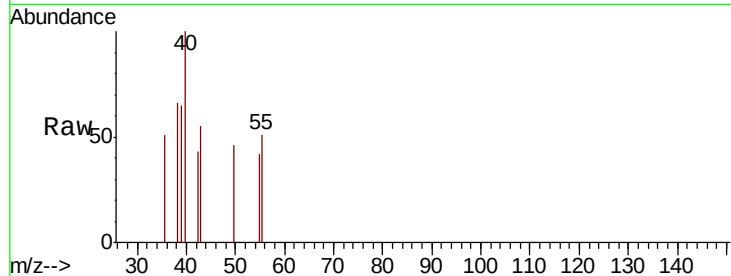

#38
Carbon Tetrachloride
Concen: 4.129 ug/l
RT: 7.98 min Scan# 1031
Delta R.T. -0.11 min
Lab File: VD063913.D
Acq: 10 Oct 2019 16:38

Tgt Ion: 117 Resp: 728
Ion Ratio Lower Upper
117 100
119 0.0 70.8 106.2#
121 0.0 21.4 32.0#


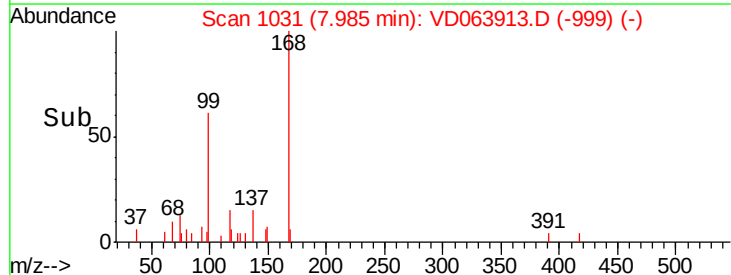
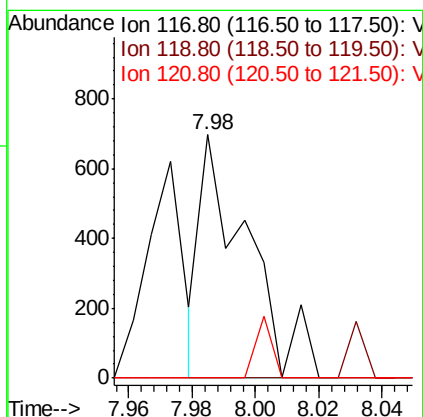





#41
Methacrylonitrile
Concen: 1.681 ug/l
RT: 7.53 min Scan# 954
Delta R.T. 0.01 min
Lab File: VD063913.D
Acq: 10 Oct 2019 16:38




Instrument :
MSVOA_D
ClientSampleId :


Tot Ion: 41 Resp: 68
Ion Ratio Lower Upper
41 100
39 155.9 52.6 78.8#
67 0.0 74.2 111.2#
52 0.0 34.0 51.0#

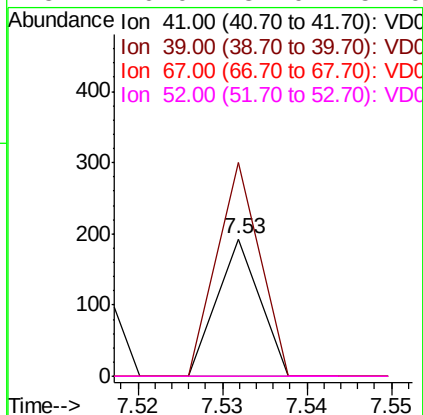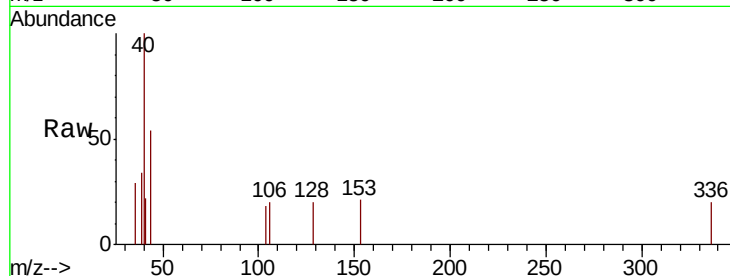

#46
Dibromomethane
Concen: 1.019 ug/l
RT: 9.54 min Scan# 1295
Delta R.T. 0.06 min
Lab File: VD063913.D
Acq: 10 Oct 2019 16:38

Tgt Ion: 93 Resp: 71
Ion Ratio Lower Upper
93 100
95 0.0 66.0 99.0#
174 0.0 83.4 125.0#

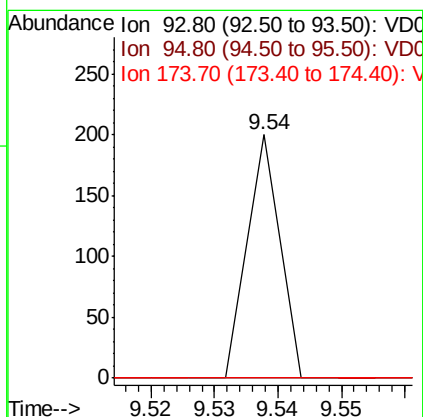







#49
1,4-Dioxane
Concen: 72.521 ug/l
RT: 9.65 min Scan# 1314
Delta R.T. 0.18 min
Lab File: VD063913.D
Acq: 10 Oct 2019 16:38

Instrument :
MSVOA_D
ClientSampleId :

Tot Ion: 88 Resp: 69
Ion Ratio Lower Upper
88 100
43 87.0 27.6 41.4#
58 0.0 54.1 81.1#




Abundance Ion 88.00 (87.70 to 88.70): VDC
Ion 43.00 (42.70 to 43.70): VDC
Ion 58.00 (57.70 to 58.70): VDC


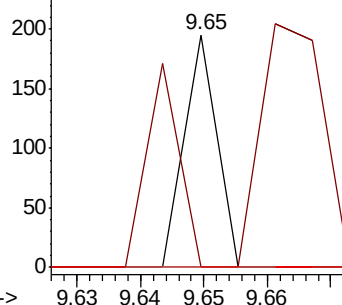



#50
Toluene-d8
Concen: 46.684 ug/l
RT: 10.34 min Scan# 1432
Delta R.T. 0.01 min
Lab File: VD063913.D
Acq: 10 Oct 2019 16:38

Tgt Ion: 98 Resp: 22099
Ion Ratio Lower Upper
98 100
100 66.9 52.1 78.1



Abundance Ion 98.00 (97.70 to 98.70): VDC
Ion 100.00 (99.70 to 100.70): VDC




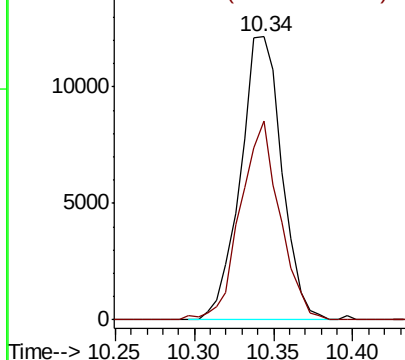




#51
 4-Methyl-2-Pentanone
 Concen: 1.713 ug/l
 RT: 10.35 min Scan# 1433
 Delta R.T. 0.12 min
 Lab File: VD063913.D
 Acq: 10 Oct 2019 16:38




Instrument :
 MSVOA_D
 ClientSampleID :


Tot Ion: 43 Resp: 130
 Ion Ratio Lower Upper
 43 100
 58 145.4 33.0 49.4#

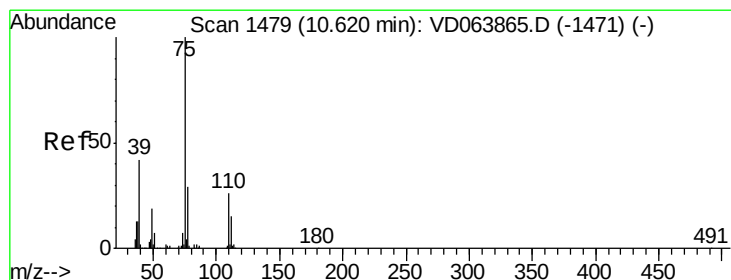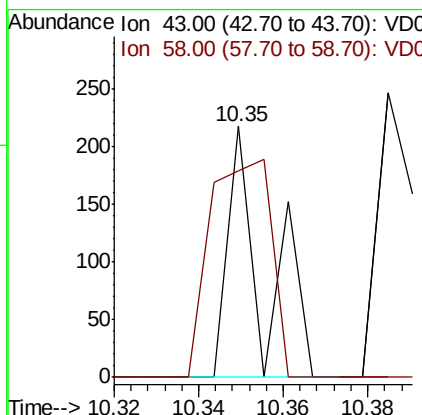

#53
 t-1,3-Dichloropropene
 Concen: 1.251 ug/l
 RT: 10.52 min Scan# 1462
 Delta R.T. -0.10 min
 Lab File: VD063913.D
 Acq: 10 Oct 2019 16:38

Tgt Ion: 75 Resp: 219
 Ion Ratio Lower Upper
 75 100
 77 652.7 22.8 34.2#

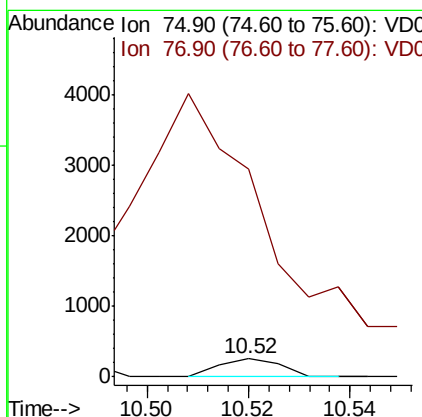


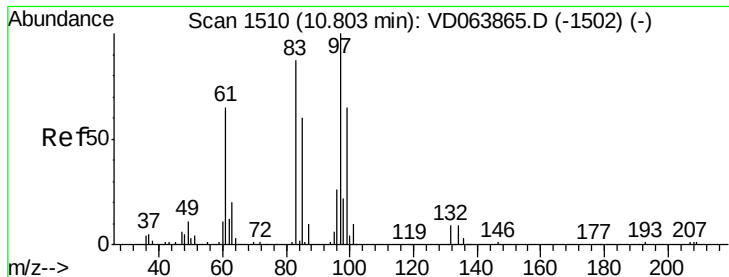




#55
 1,1,2-Trichloroethane
 Concen: 1.443 ug/l
 RT: 10.78 min Scan# 1506
 Delta R.T. -0.02 min
 Lab File: VD063913.D
 Acq: 10 Oct 2019 16:38

Instrument :
 MSVOA_D
 ClientSampleId :

Tot Ion: 97 Resp: 142
 Ion Ratio Lower Upper
 97 100
 83 0.0 69.7 104.5#
 85 0.0 48.1 72.1#
 99 0.0 51.9 77.9#

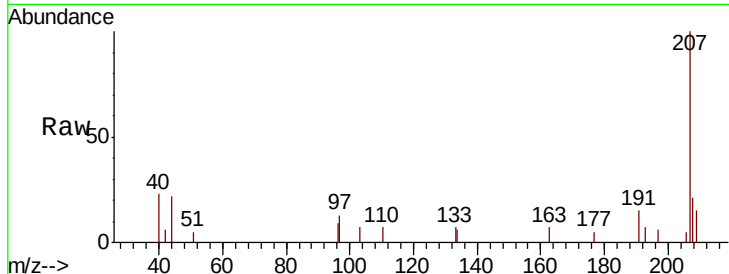


Abundance Ion 96.90 (96.60 to 97.60): VDC
 Ion 82.90 (82.60 to 83.60): VDC
 Ion 84.90 (84.60 to 85.60): VDC
 Ion 98.90 (98.60 to 99.60): VDC

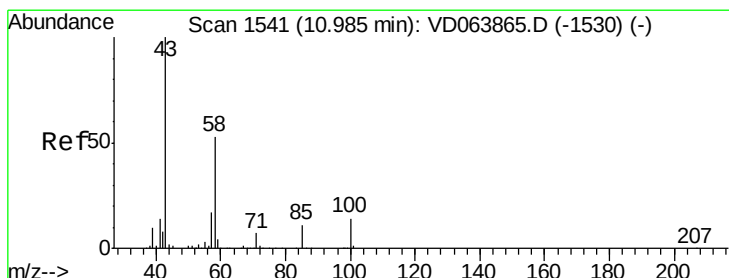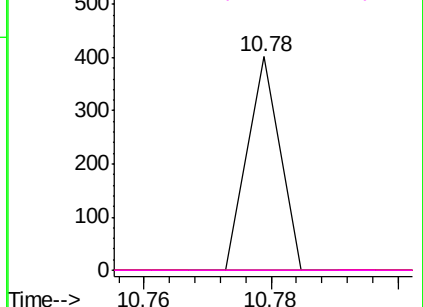
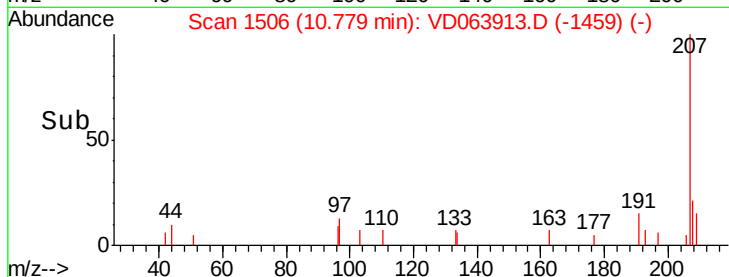



#59
 2-Hexanone
 Concen: 2.168 ug/l
 RT: 10.99 min Scan# 1542
 Delta R.T. 0.01 min
 Lab File: VD063913.D
 Acq: 10 Oct 2019 16:38

Tgt Ion: 43 Resp: 119
 Ion Ratio Lower Upper
 43 100
 58 0.0 27.7 83.0#

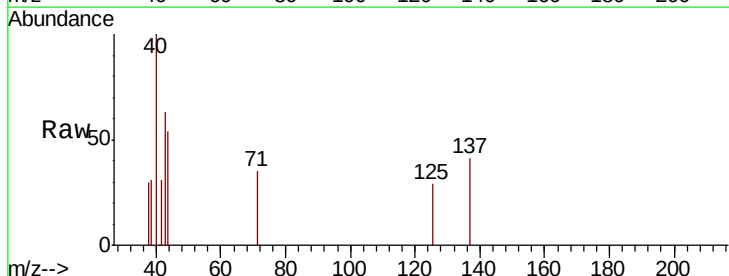

Abundance Ion 43.00 (42.70 to 43.70): VDC
 Ion 58.00 (57.70 to 58.70): VDC



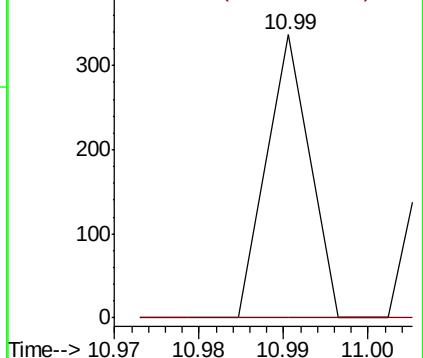
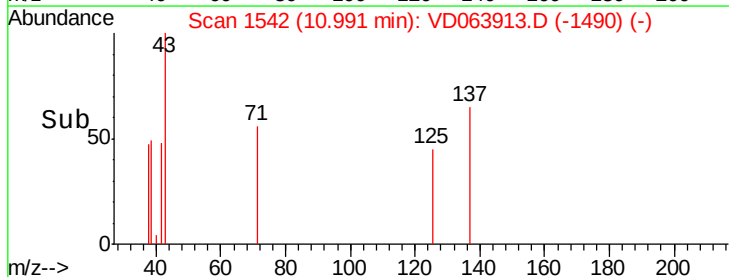




#62
4-Bromofluorobenzene
Concen: 50.098 ug/l
RT: 12.63 min Scan# 1821
Delta R.T. -0.00 min
Lab File: VD063913.D
Acq: 10 Oct 2019 16:38




Instrument :
MSVOA_D
ClientSampleId :


Tot Ion: 95 Resp: 8241
Ion Ratio Lower Upper
95 100
174 94.0 0.0 186.4
176 82.0 0.0 184.2

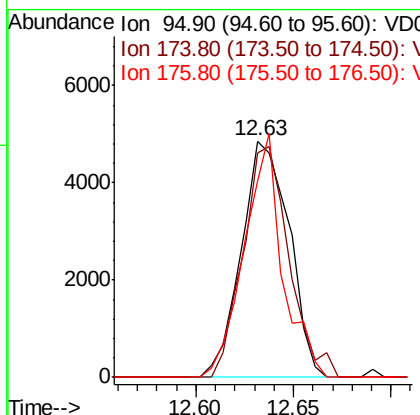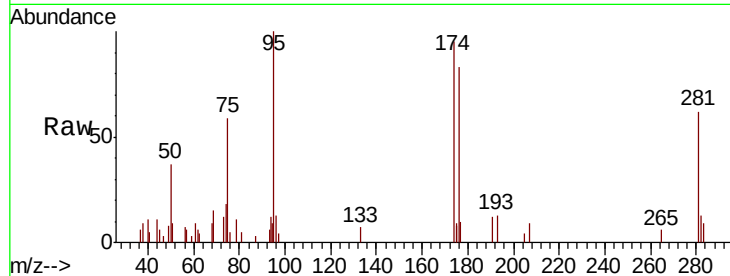

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.65 min Scan# 1654
Delta R.T. 0.01 min
Lab File: VD063913.D
Acq: 10 Oct 2019 16:38

Tgt Ion: 117 Resp: 17933
Ion Ratio Lower Upper
117 100
82 59.2 42.8 64.2
119 40.0 24.4 36.6#

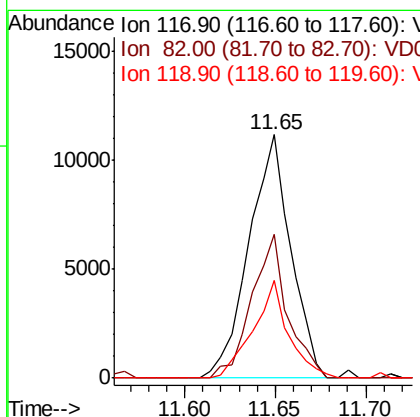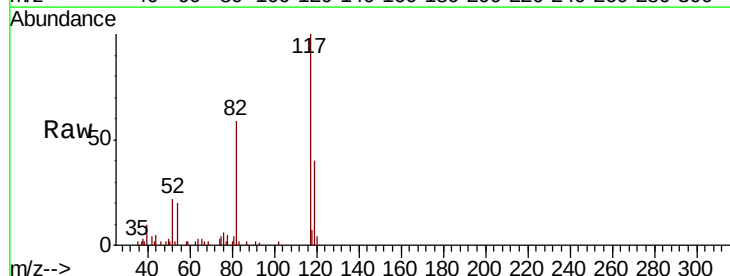

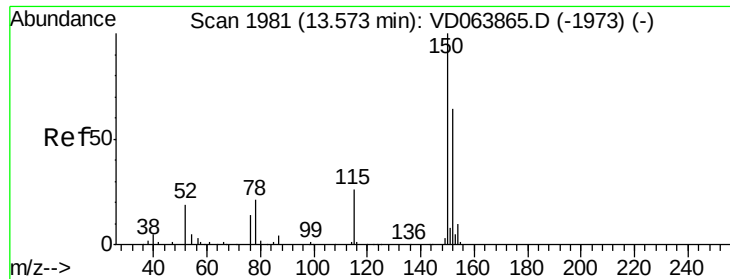

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.58 min Scan# 1982

Delta R.T. 0.01 min

Lab File: VD063913.D

Acq: 10 Oct 2019 16:38

Instrument :

MSVOA_D

ClientSampleId :


Tot Ion:152 Resp: 8433

Ion Ratio Lower Upper

152 100

115 63.5 25.9 77.7




150 162.7 0.0 344.2

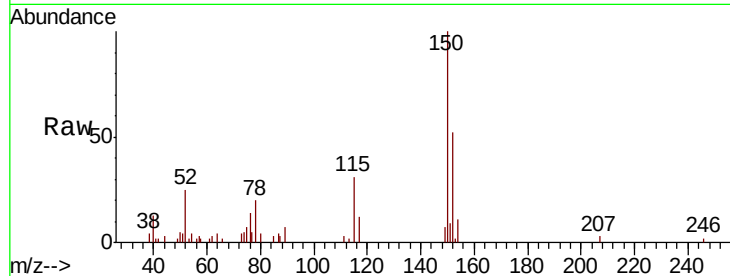

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

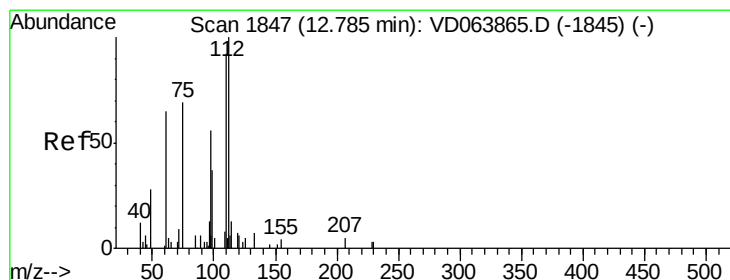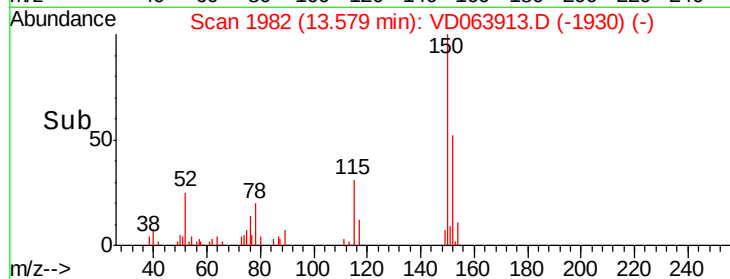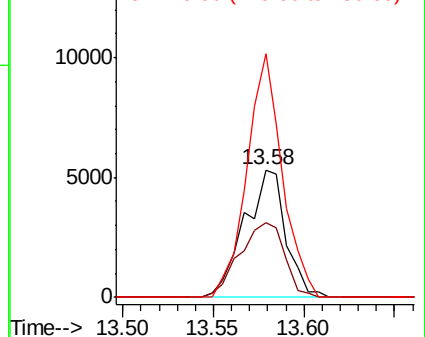

#76

1,2,3-Trichloropropane

Concen: 3.240 ug/l

RT: 12.78 min Scan# 1846

Delta R.T. -0.01 min

Lab File: VD063913.D


Acq: 10 Oct 2019 16:38

Tgt Ion: 75 Resp: 183

Ion Ratio Lower Upper



75 100


77 492.9 0.0 0.0#



Abundance Ion 74.90 (74.60 to 75.60): V

Ion 77.00 (76.70 to 77.70): V

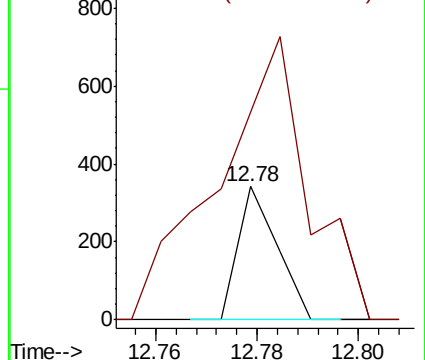



#81

trans-1,4-Dichloro-2-butene

Concen: 125.384 ug/l

RT: 12.63 min Scan# 1821

Delta R.T. 0.10 min

Lab File: VD063913.D

Acq: 10 Oct 2019 16:38

Instrument :

MSVOA_D

ClientSampleId :


Tot Ion: 75 Resp: 4002

Ion Ratio Lower Upper




75 100

53 1.4 75.0 112.6#

89 0.0 38.2 57.4#



Abundance Ion 74.90 (74.60 to 75.60): VDC
Ion 53.00 (52.70 to 53.70): VDC
Ion 88.90 (88.60 to 89.60): VDC

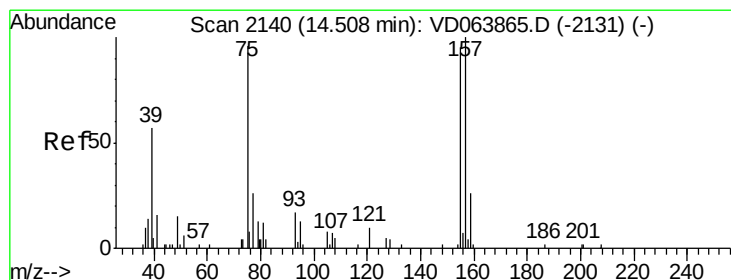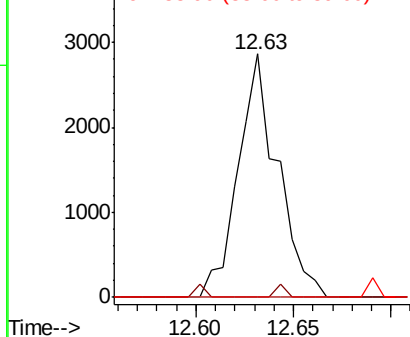

#92

1,2-Dibromo-3-Chloropropane

Concen: 1.944 ug/l

RT: 14.48 min Scan# 2136

Delta R.T. -0.02 min

Lab File: VD063913.D

Acq: 10 Oct 2019 16:38


Tgt Ion: 75 Resp: 66

Ion Ratio Lower Upper



75 100


155 0.0 43.9 131.6#

157 0.0 56.0 167.9#

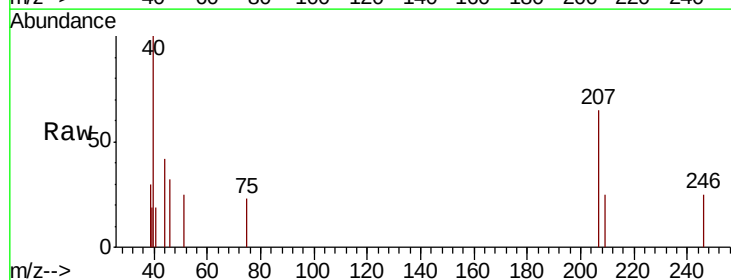

Abundance Ion 74.90 (74.60 to 75.60): VDC
Ion 154.80 (154.50 to 155.50): V
Ion 156.80 (156.50 to 157.50): V

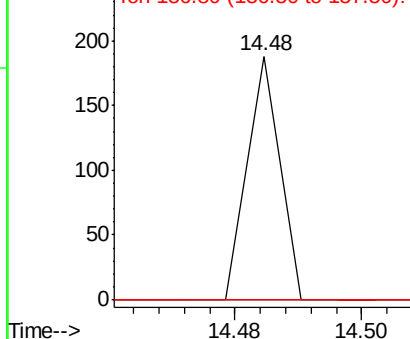



#96
 1,2,3-Trichlorobenzene
 Concen: 1.087 ug/l
 RT: 15.58 min Scan# 2323
 Delta R.T. -0.01 min
 Lab File: VD063913.D
 Acq: 10 Oct 2019 16:38

Instrument :
 MSVOA_D
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
180	100		
182	0.0	47.0	141.0#
145	0.0	15.3	45.9#

