


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD101019\  
 Data File : VD063900.D  
 Acq On : 10 Oct 2019 10:10  
 Operator : VA/SY  
 Sample : BFB  
 Misc : 5.00G/MSVOA D/SOIL  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_D  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_D\METHOD\82D100219S.M  
 Title : SW846 8260  
 Last Update : Sat Oct 05 03:51:17 2019

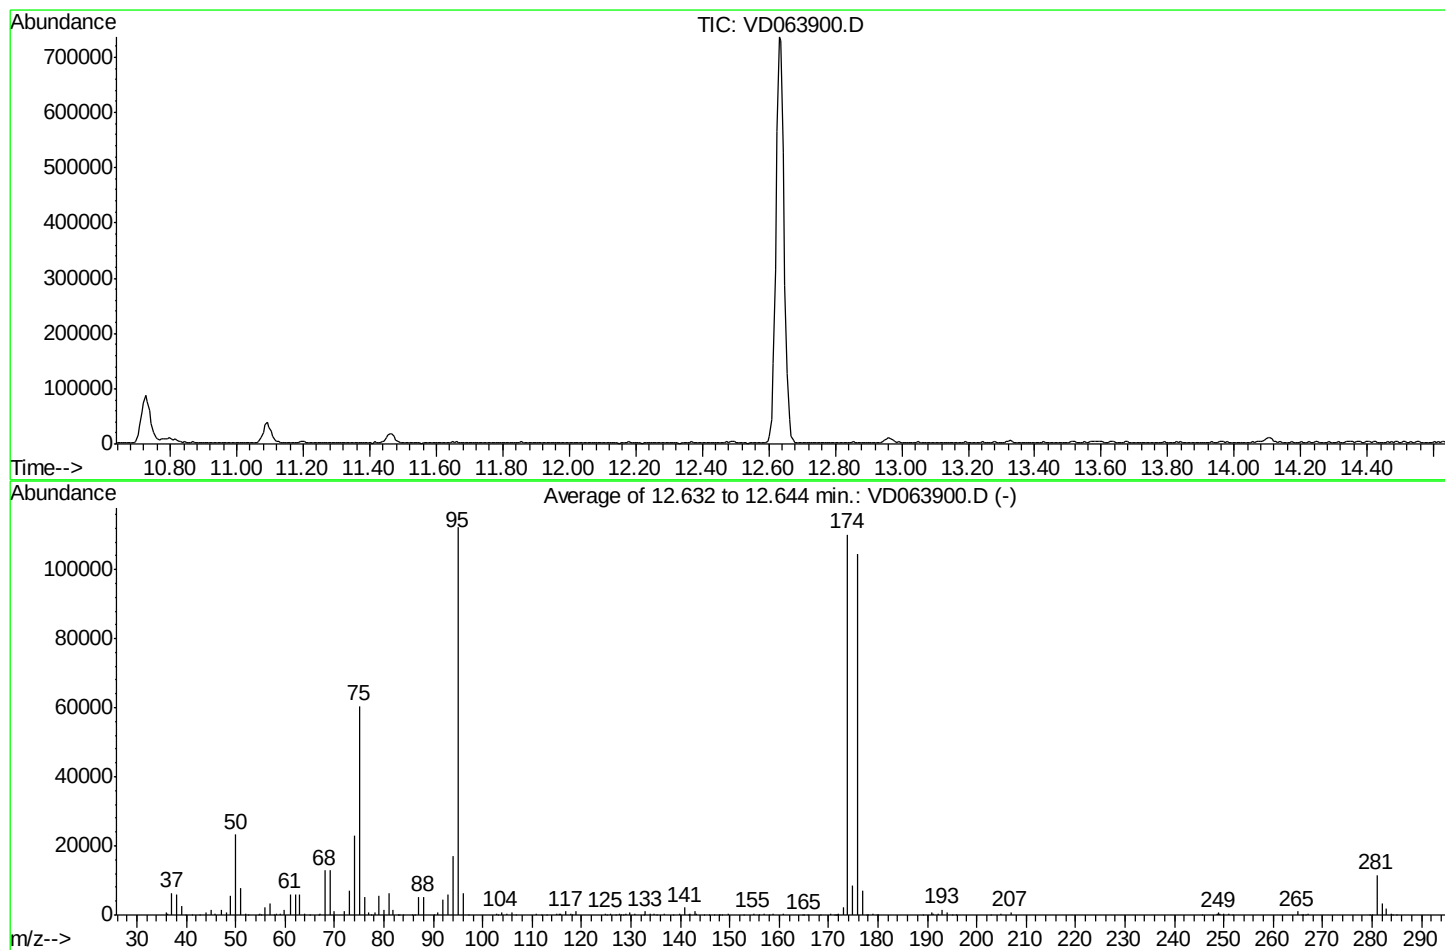

AutoFind: Scans 1821, 1822, 1823; Background Corrected with Scan 1812

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 20.8      | 23309   | PASS             |
| 75          | 95           | 30           | 60           | 54.0      | 60573   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 112202  | PASS             |
| 96          | 95           | 5            | 9            | 5.6       | 6291    | PASS             |
| 173         | 174          | 0.00         | 2            | 1.9       | 2142    | PASS             |
| 174         | 95           | 50           | 100          | 98.1      | 110064  | PASS             |
| 175         | 174          | 5            | 9            | 7.9       | 8653    | PASS             |
| 176         | 174          | 95           | 101          | 95.0      | 104560  | PASS             |
| 177         | 176          | 5            | 9            | 6.8       | 7124    | PASS             |