
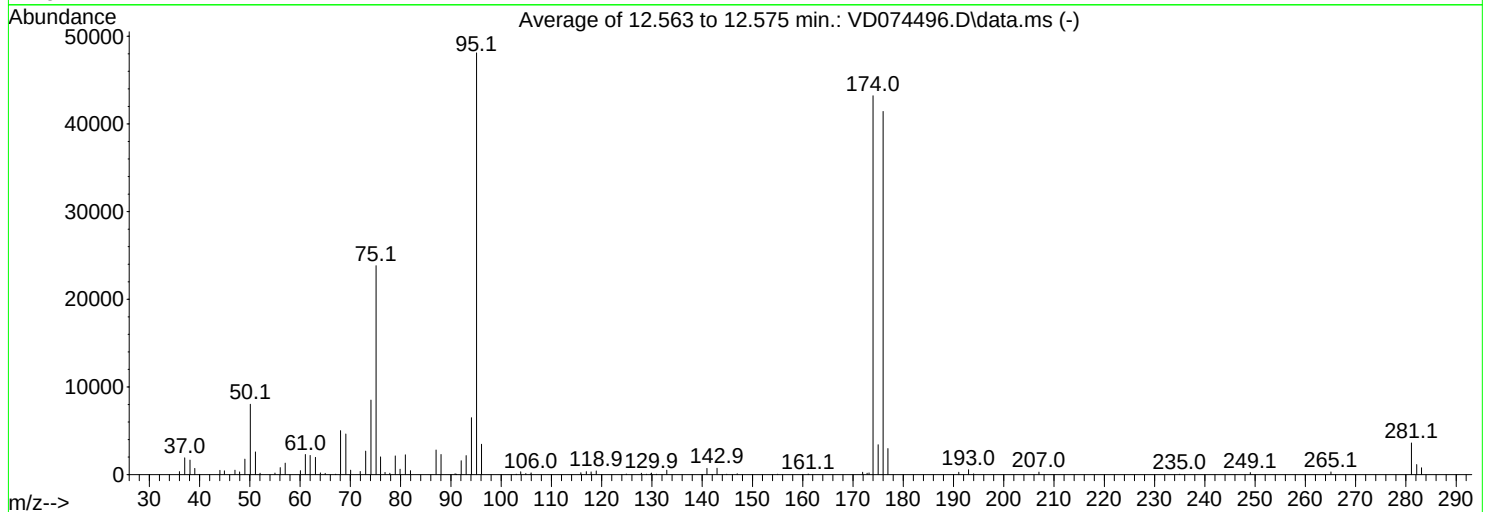


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD101022\
Data File : VD074496.D
Acq On : 10 Oct 2022 10:59
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D100522S.M
Title : SW846 8260
Last Update : Thu Oct 06 01:54:40 2022

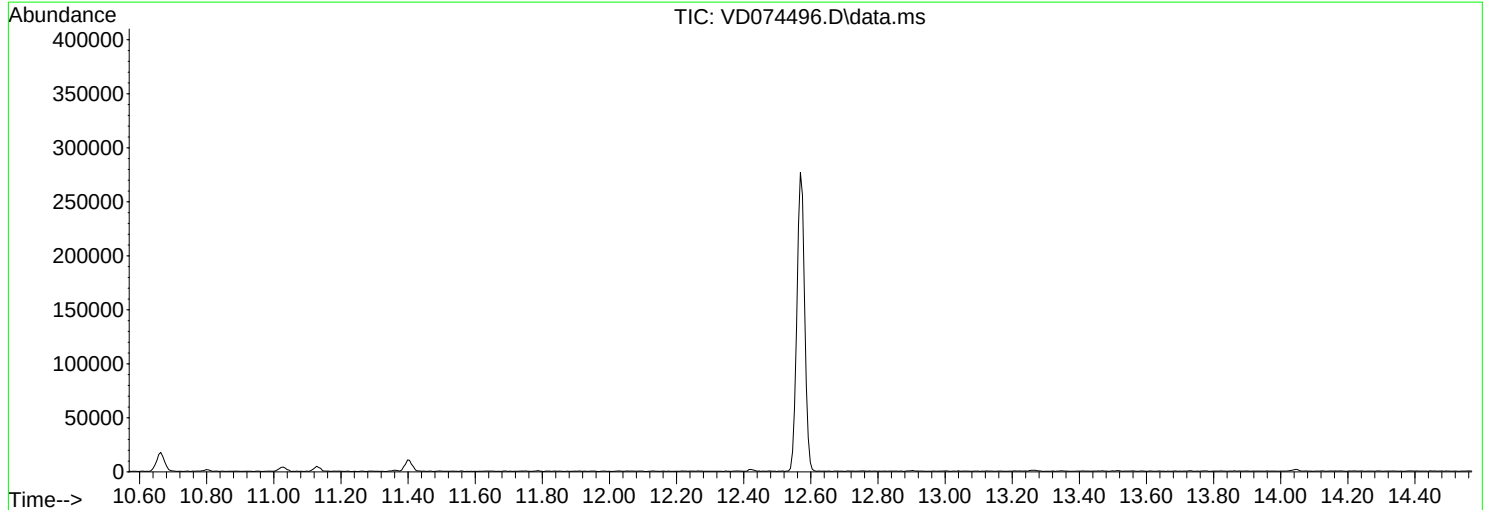

AutoFind: Scans 1866, 1867, 1868; Background Corrected with Scan 1859

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	8027	PASS
75	95	30	60	49.5	23827	PASS
95	95	100	100	100.0	48109	PASS
96	95	5	9	7.2	3467	PASS
173	174	0.00	2	0.5	206	PASS
174	95	50	100	89.8	43221	PASS
175	174	5	9	7.9	3423	PASS
176	174	95	101	95.8	41424	PASS
177	176	5	9	7.2	2985	PASS