
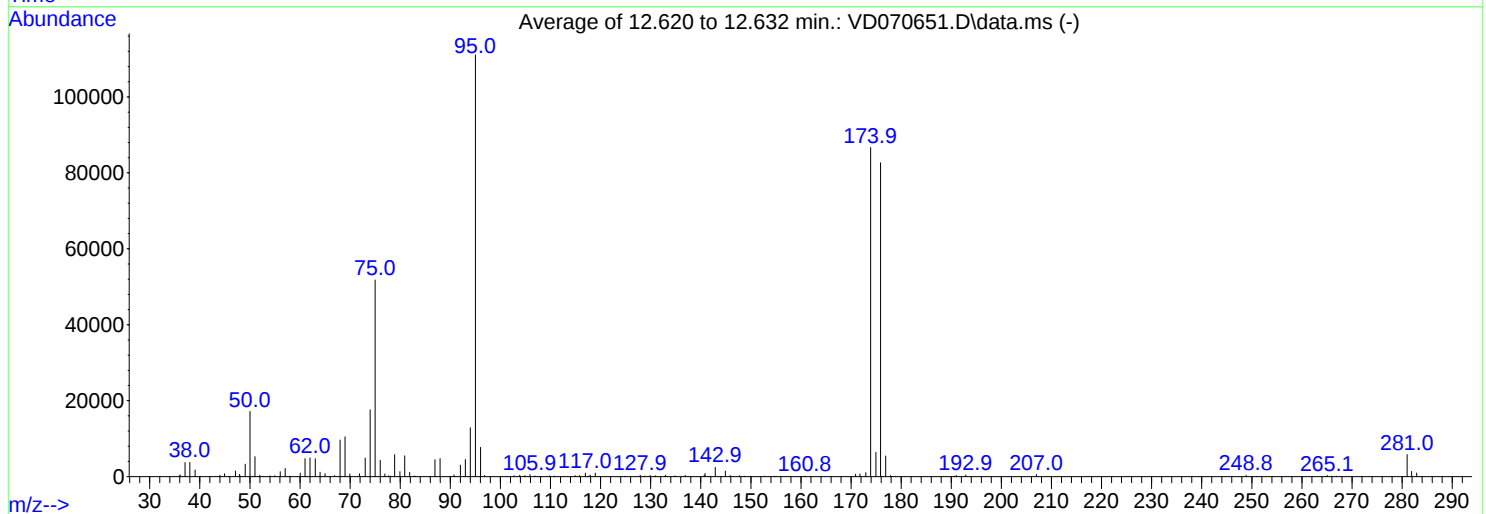


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD101121\
Data File : VD070651.D
Acq On : 11 Oct 2021 08:23
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D100521S.M
Title : SW846 8260
Last Update : Wed Oct 06 09:10:31 2021

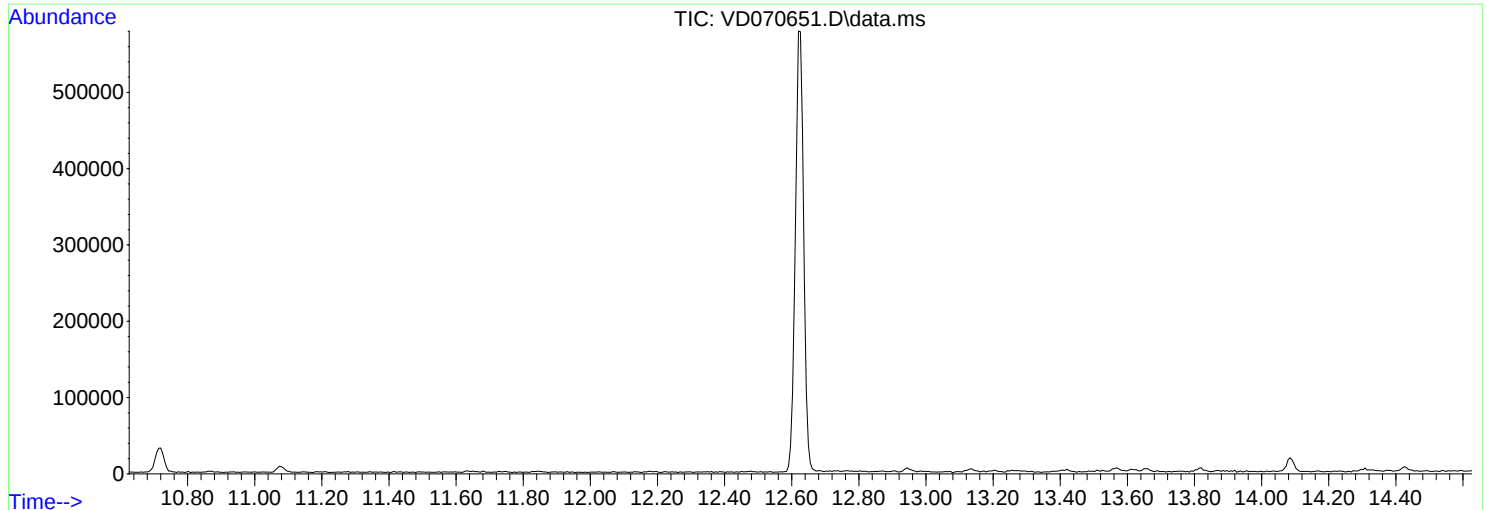

AutoFind: Scans 1819, 1820, 1821; Background Corrected with Scan 1810

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.5	17192	PASS
75	95	30	60	46.6	51800	PASS
95	95	100	100	100.0	111083	PASS
96	95	5	9	7.0	7726	PASS
173	174	0.00	2	1.2	1054	PASS
174	95	50	100	78.0	86661	PASS
175	174	5	9	7.4	6407	PASS
176	174	95	101	95.4	82677	PASS
177	176	5	9	6.6	5439	PASS