
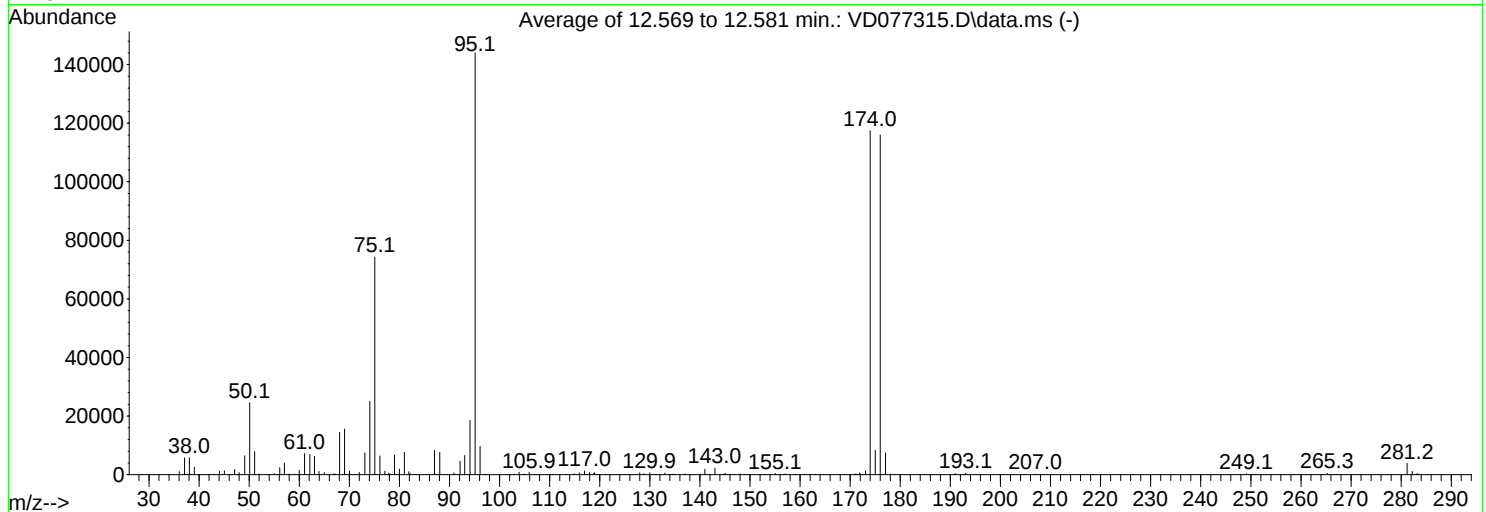


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD101223\
Data File : VD077315.D
Acq On : 12 Oct 2023 11:24
Operator : JC/SY
Sample : BFB
Misc : 5.00G/5.0ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D101123S.M
Title : SW846 8260
Last Update : Fri Oct 13 17:30:18 2023

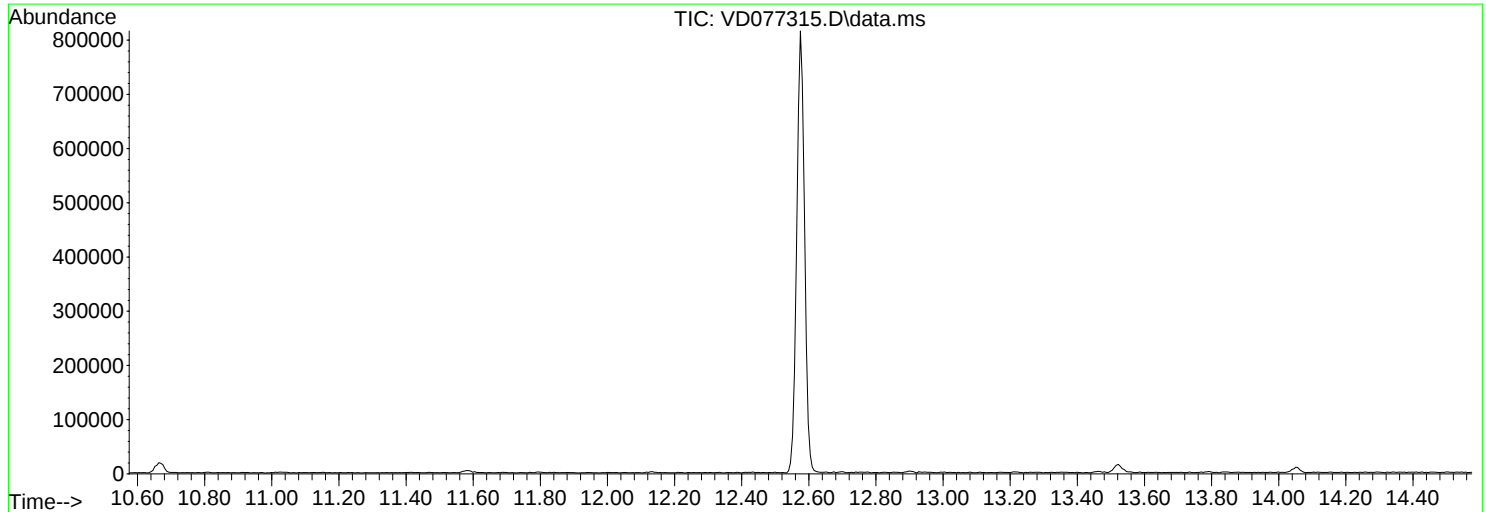

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1859

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.1	24573	PASS
75	95	30	60	51.5	74237	PASS
95	95	100	100	100.0	144013	PASS
96	95	5	9	6.7	9652	PASS
173	174	0.00	2	1.2	1378	PASS
174	95	50	100	81.6	117448	PASS
175	174	5	9	7.1	8337	PASS
176	174	95	101	98.7	115965	PASS
177	176	5	9	6.4	7409	PASS