



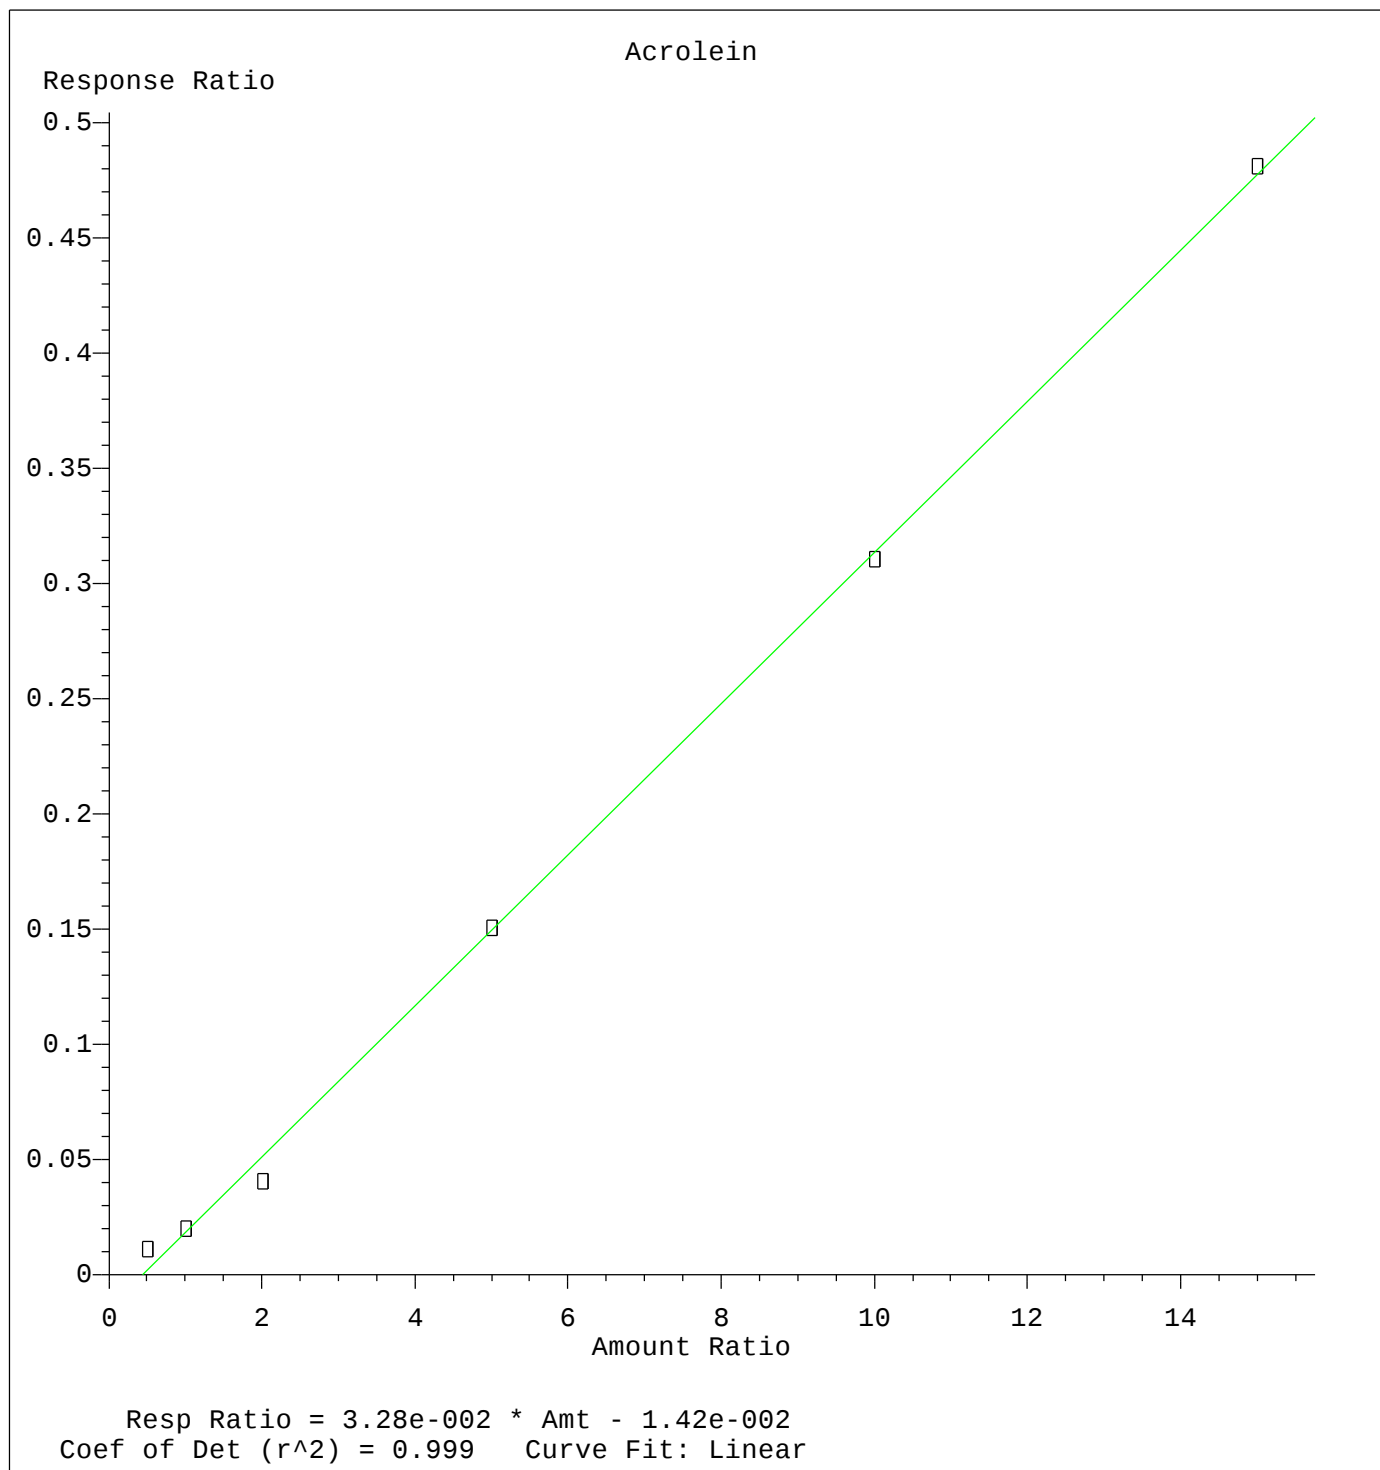

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D101320S.M
Calibration Table Last Updated: Wed Oct 14 03:30:30 2020


Methylene Chloride

Response Ratio

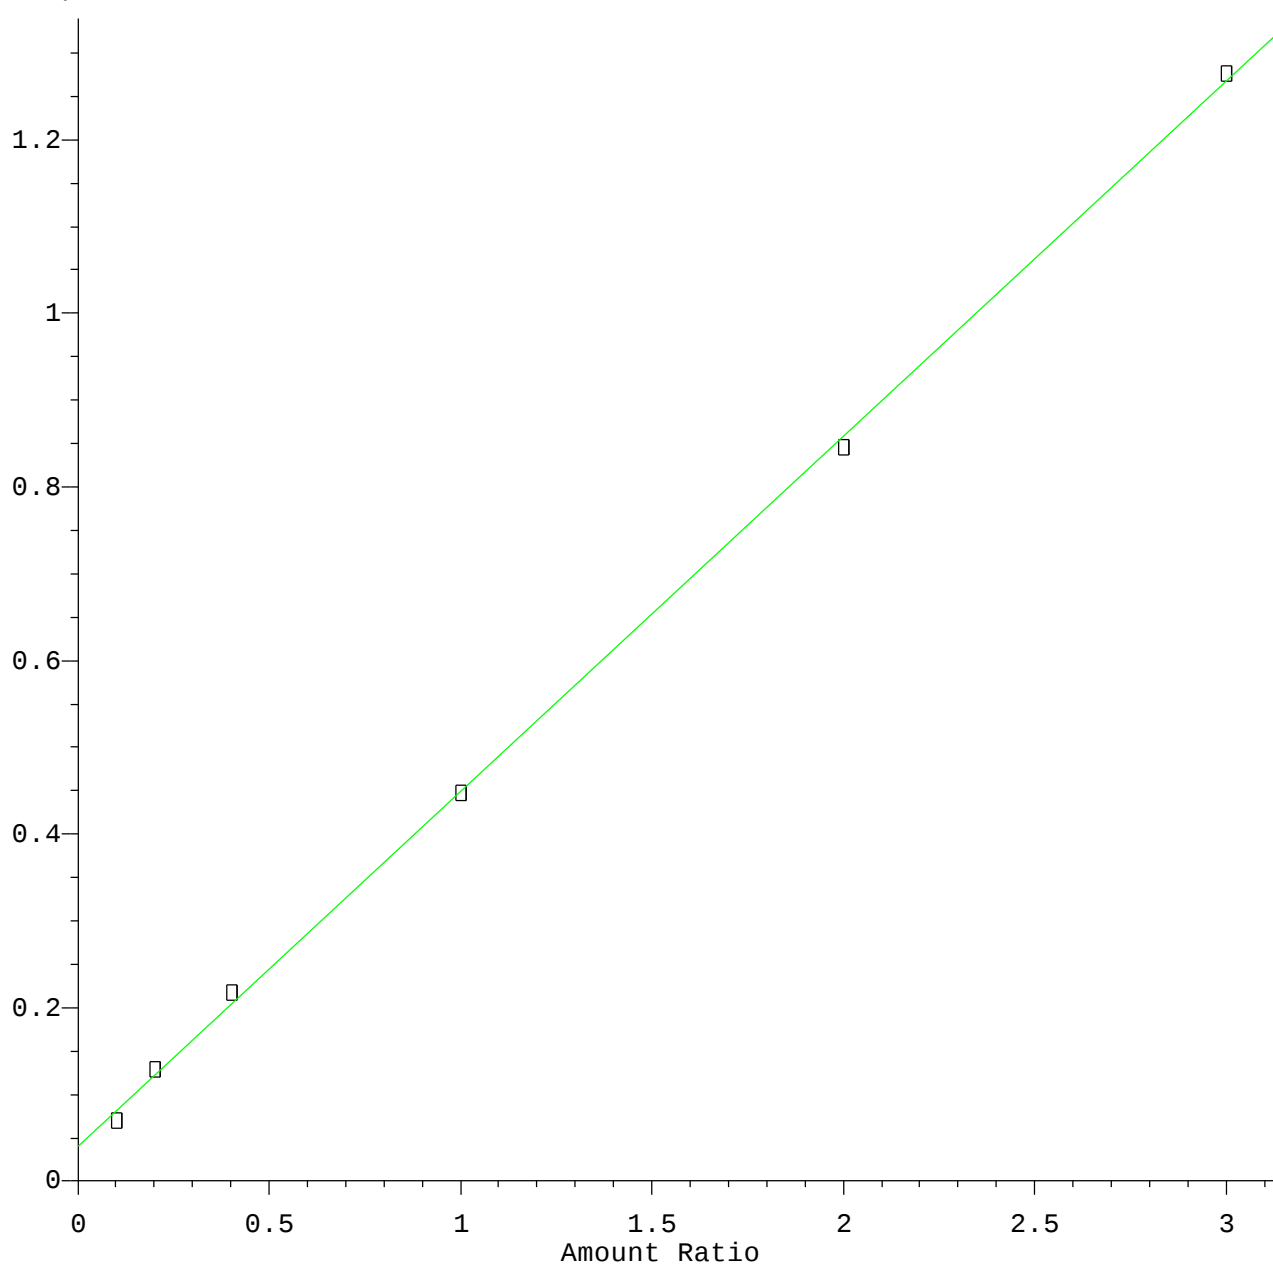

Resp Ratio = $4.09 \times 10^{-1} \times \text{Amt} + 4.03 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D101320S.M
Calibration Table Last Updated: Wed Oct 14 03:30:30 2020

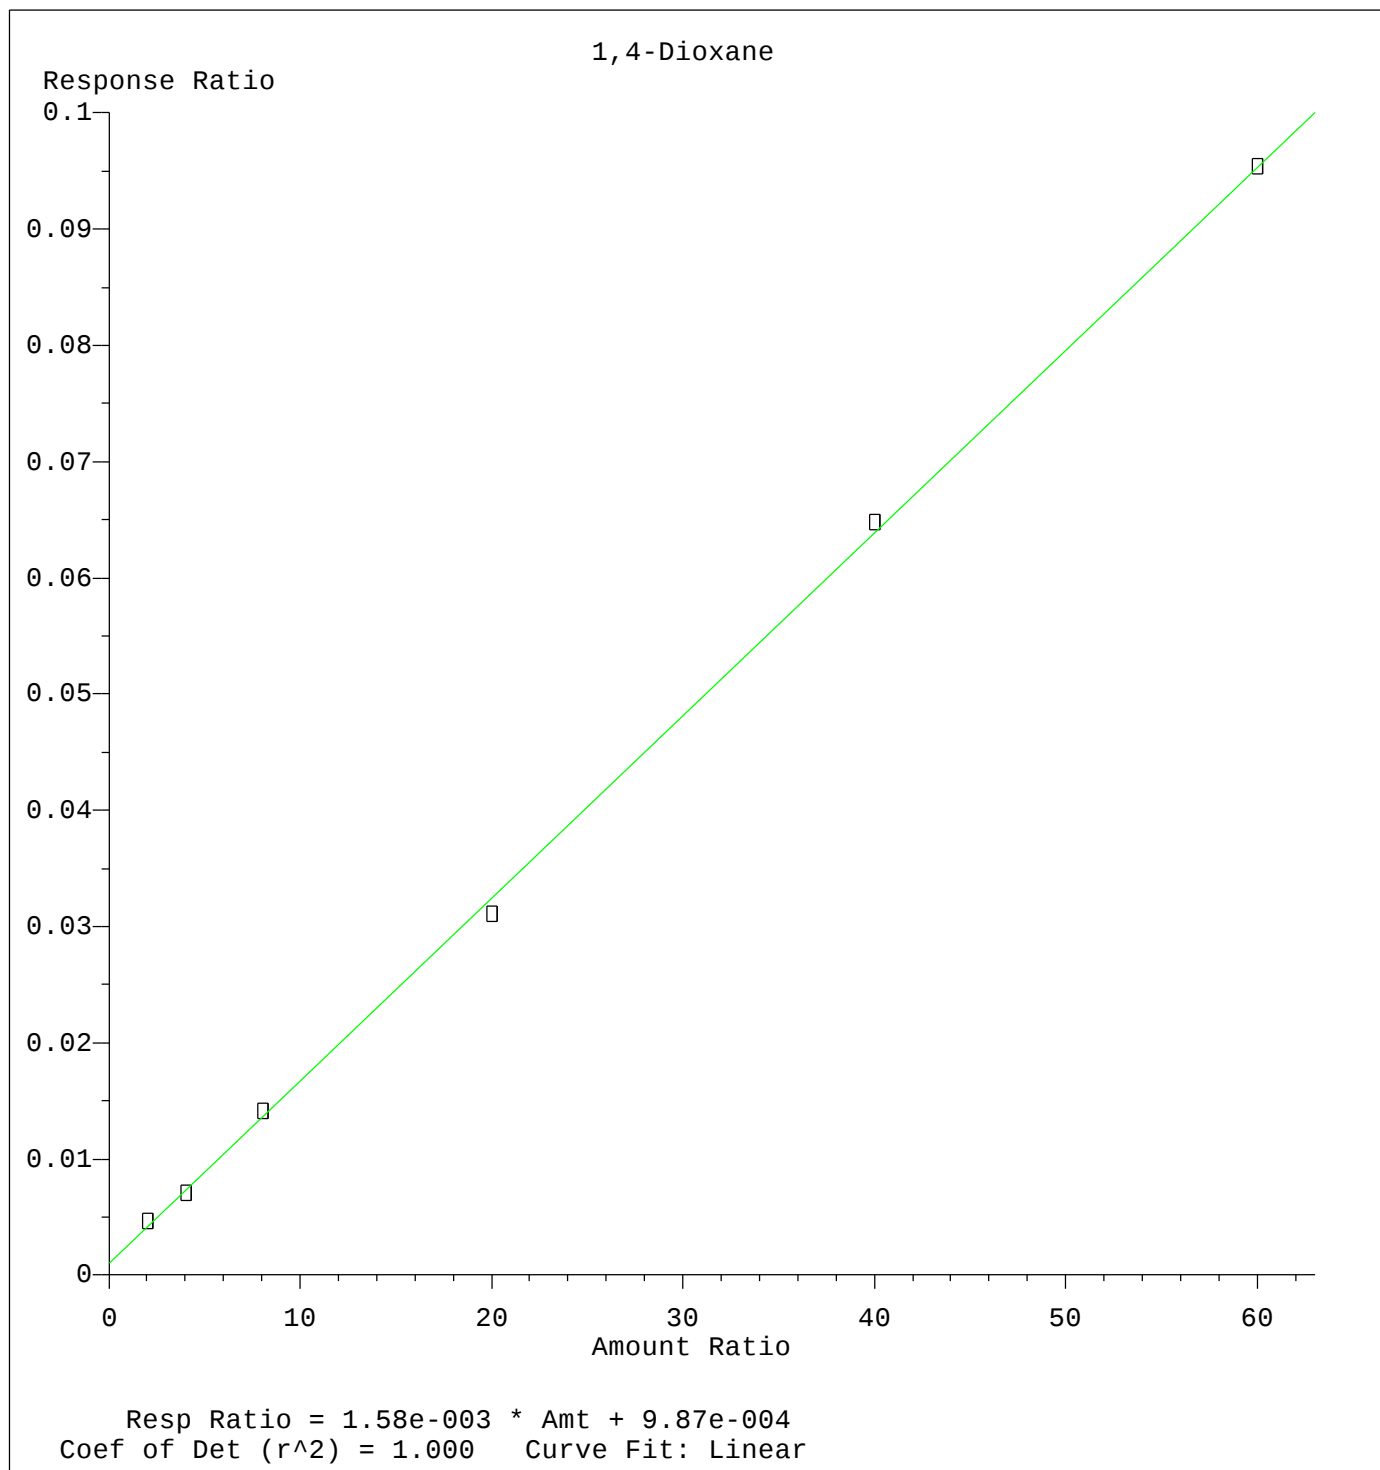

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D101320S.M
Calibration Table Last Updated: Wed Oct 14 03:30:30 2020


Dichlorodifluoromethane

Response Ratio

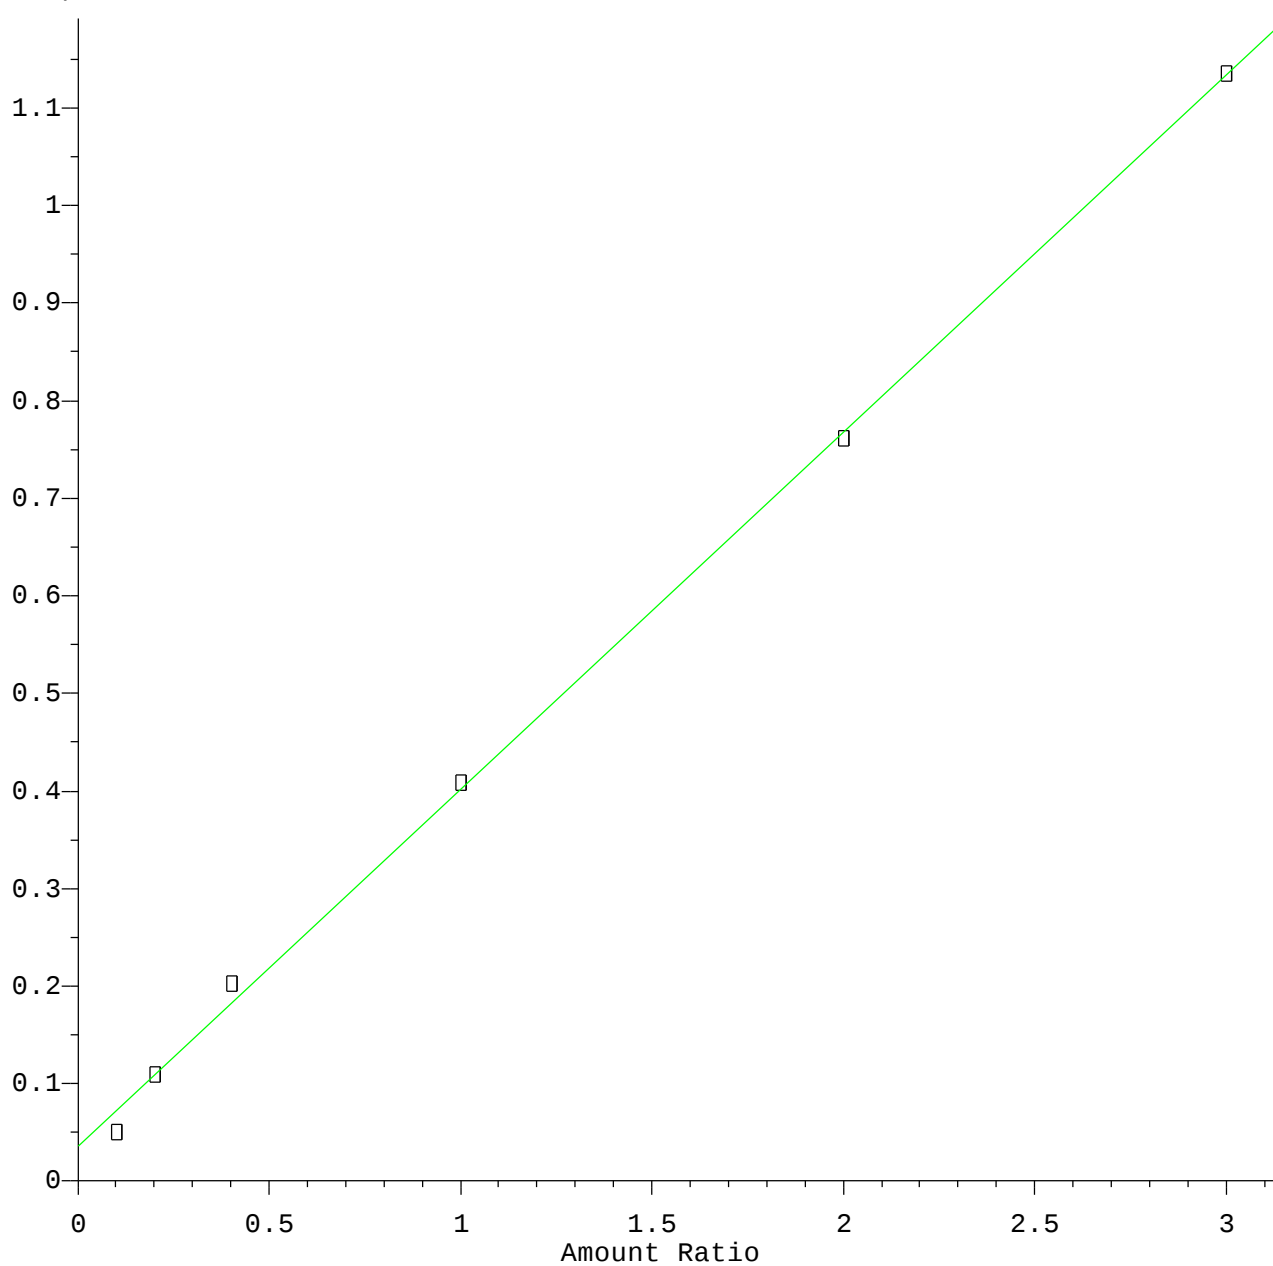


Resp Ratio = $3.66 \times 10^{-1} \times \text{Amt} + 3.51 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D101320S.M
Calibration Table Last Updated: Wed Oct 14 03:30:30 2020

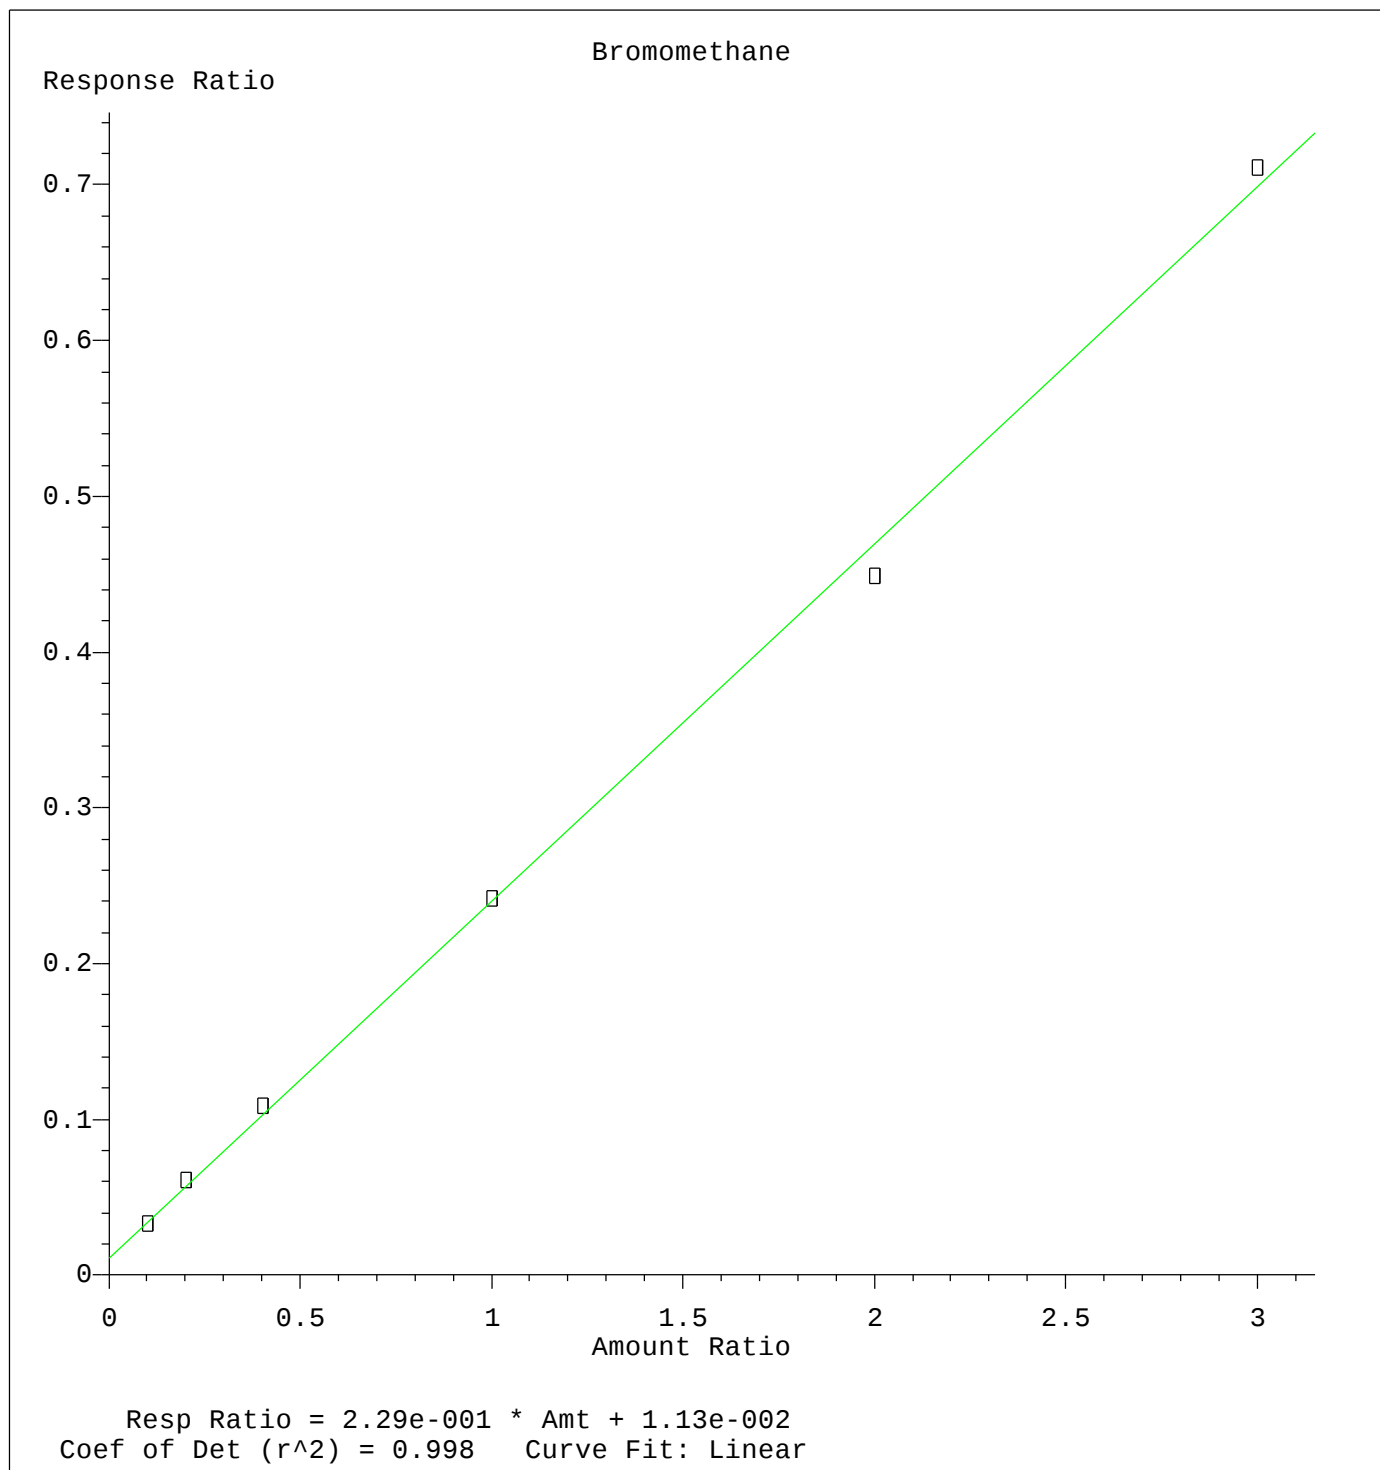

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D101320S.M
Calibration Table Last Updated: Wed Oct 14 03:30:30 2020

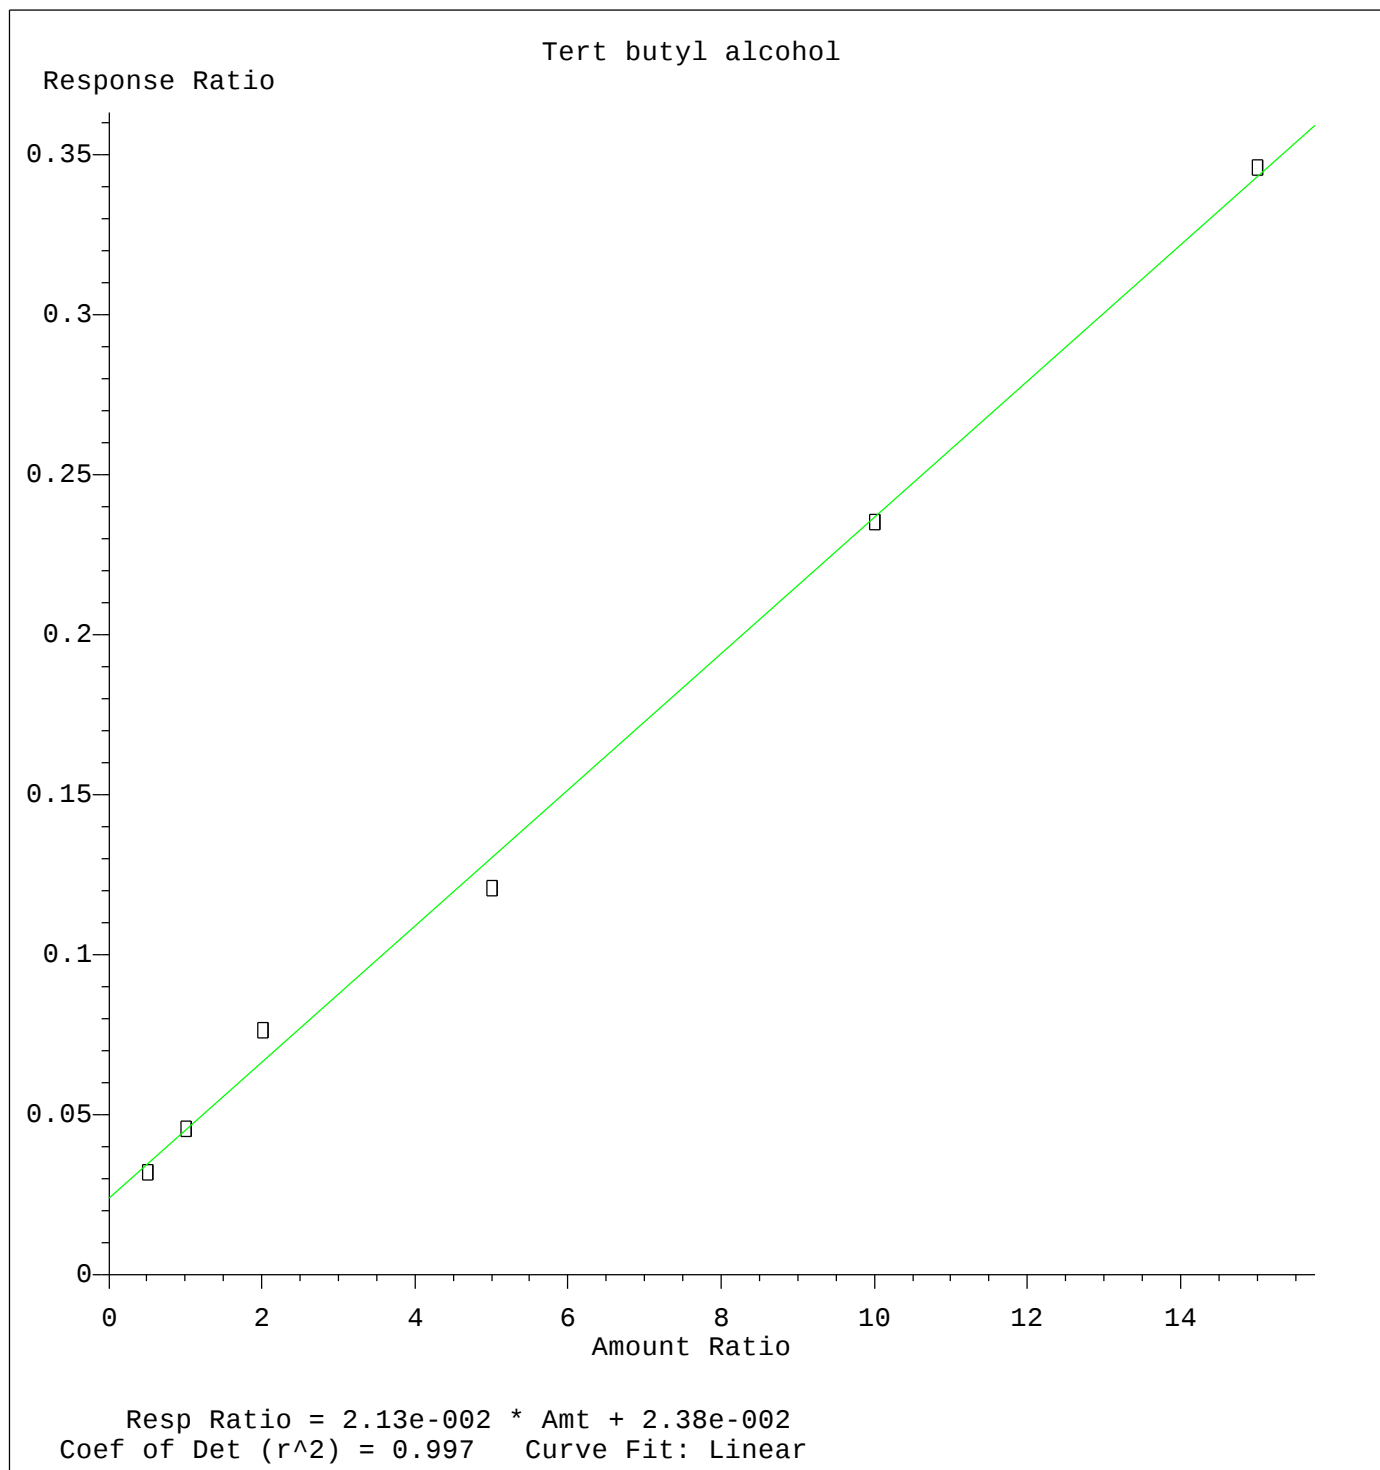

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D101320S.M
Calibration Table Last Updated: Wed Oct 14 03:30:30 2020