

Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD101320\
 Data File : VD067258.D
 Acq On : 13 Oct 2020 17:58
 Operator : VA/SY
 Sample : L4383-01
 Misc : 5.00G/5.01ml/MSVOA D/SOIL
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BB-SOIL

Quant Time: Oct 14 02:50:12 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D101320S.M
 Quant Title : SW846 8260
 QLast Update : Tue Oct 13 13:05:03 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.98	168	308125	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.87	114	505765	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.65	117	488540	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.58	152	224590	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	8.34	65	161200	52.22	ug/l	0.00
Spiked Amount						
			Recovery	=	104.44%	
35) Dibromofluoromethane	7.91	113	166172	49.37	ug/l	0.00
Spiked Amount						
			Recovery	=	98.74%	
50) Toluene-d8	10.34	98	597463	49.05	ug/l	0.00
Spiked Amount						
			Recovery	=	98.10%	
62) 4-Bromofluorobenzene	12.64	95	206605	48.78	ug/l	0.00
Spiked Amount						
			Recovery	=	97.56%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD101320\
Data File : VD067258.D
Acq On : 13 Oct 2020 17:58
Operator : VA/SY
Sample : L4383-01
Misc : 5.00G/5.01ml/MSVOA D/SOIL
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BB-SOIL

Quant Time: Oct 14 02:50:12 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D101320S.M
Quant Title : SW846 8260
QLast Update : Tue Oct 13 13:05:03 2020
Response via : Initial Calibration

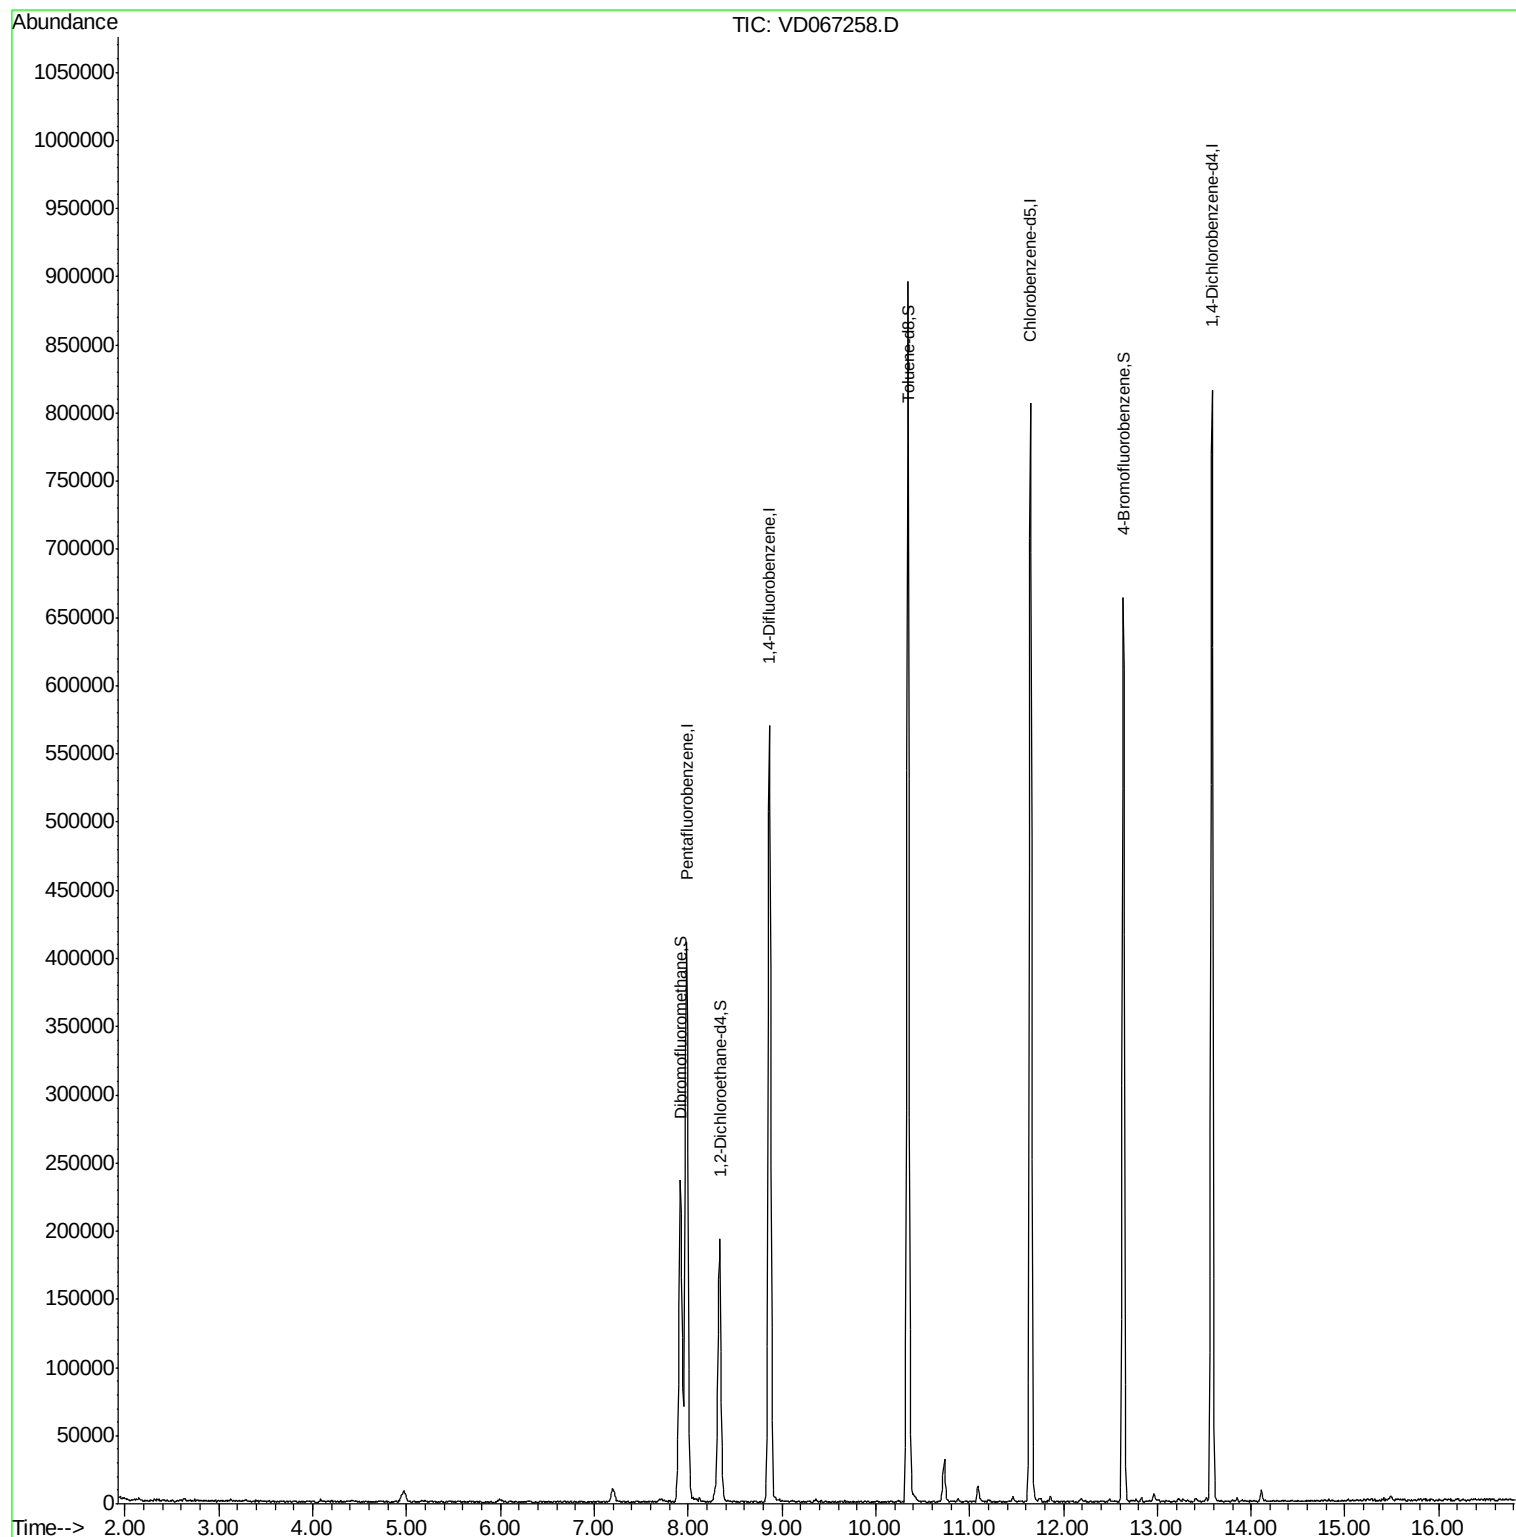

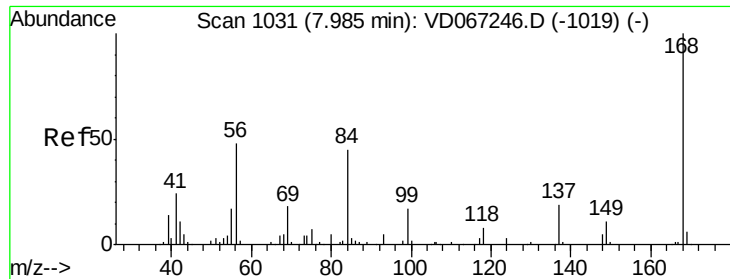

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.98 min Scan# 1031

Delta R.T. 0.00 min

Lab File: VD067258.D

Acq: 13 Oct 2020 17:58

Instrument :

MSVOA_D

ClientSampleId :


BB-SOIL

Tot Ion:168 Resp: 308125

Ion Ratio Lower Upper

168 100

99 53.5 45.9 68.9

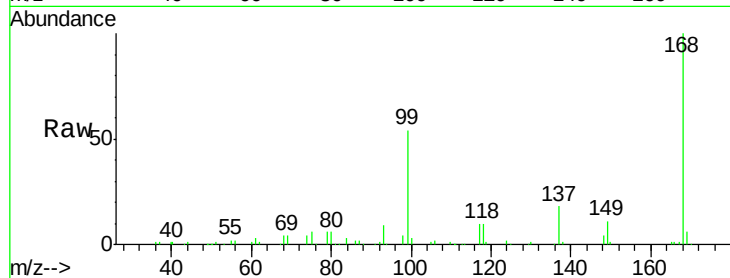

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VDC

7.98



150000

100000

50000

0

Time-->

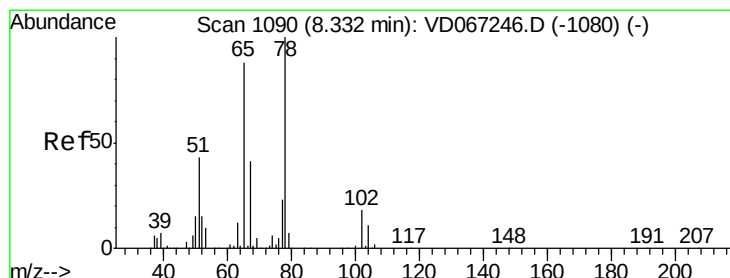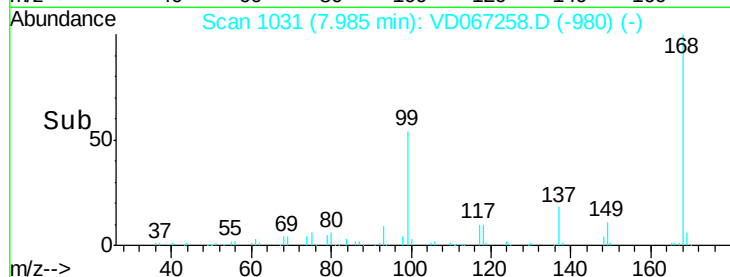

#33

1,2-Dichloroethane-d4

Concen: 52.220 ug/l

RT: 8.34 min Scan# 1091

Delta R.T. 0.01 min

Lab File: VD067258.D


Acq: 13 Oct 2020 17:58

Tgt Ion: 65 Resp: 161200

Ion Ratio Lower Upper

65 100

67 49.9 0.0 103.8

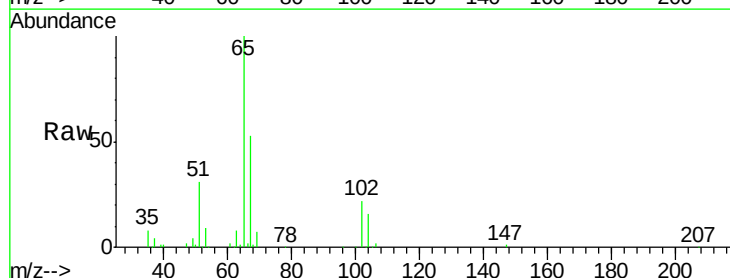

Abundance Ion 64.90 (64.60 to 65.60): VDC

Ion 66.90 (66.60 to 67.60): VDC

8.34

80000


60000


40000

20000

0

Time-->

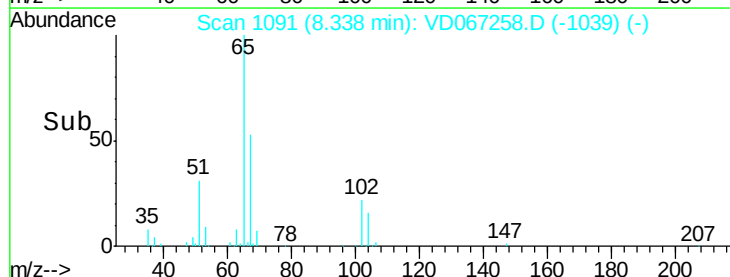

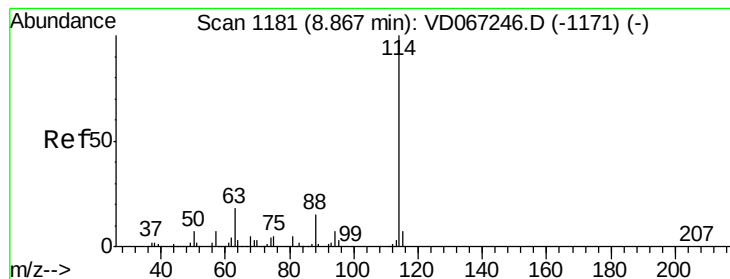

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.87 min Scan# 1181

Delta R.T. 0.00 min

Lab File: VD067258.D

Acq: 13 Oct 2020 17:58

Instrument :

MSVOA_D

ClientSampleId :

BB-SOIL


Tot Ion:114 Resp: 505765

Ion Ratio Lower Upper

114 100

63 17.4 0.0 35.0




88 15.7 0.0 30.6

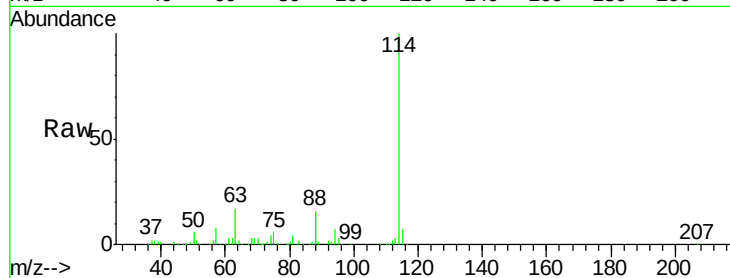

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): V

Ion 87.90 (87.60 to 88.60): V

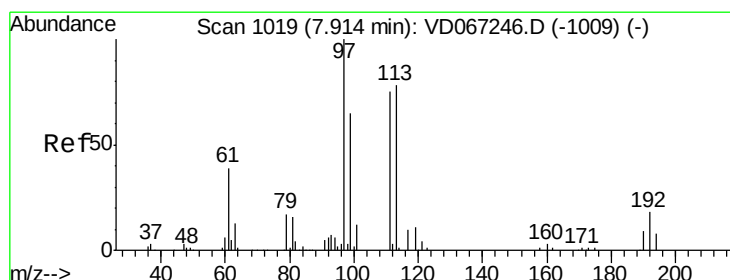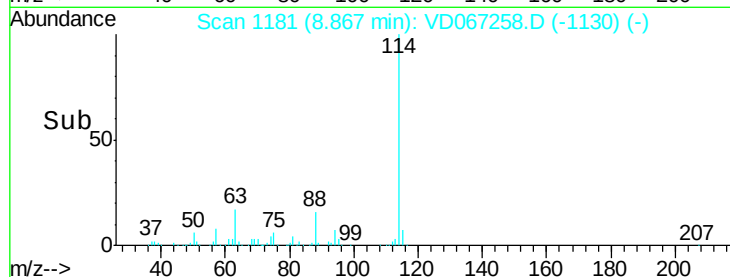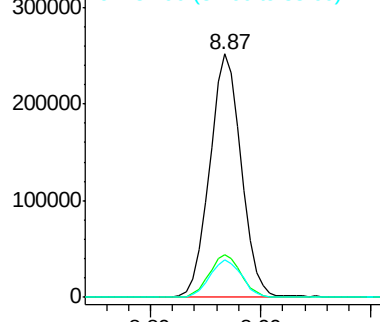

#35

Dibromofluoromethane

Concen: 49.370 ug/l

RT: 7.91 min Scan# 1019

Delta R.T. 0.00 min

Lab File: VD067258.D

Acq: 13 Oct 2020 17:58


Tgt Ion:113 Resp: 166172

Ion Ratio Lower Upper

113 100

111 104.3 81.6 122.4



192 20.6 17.0 25.4

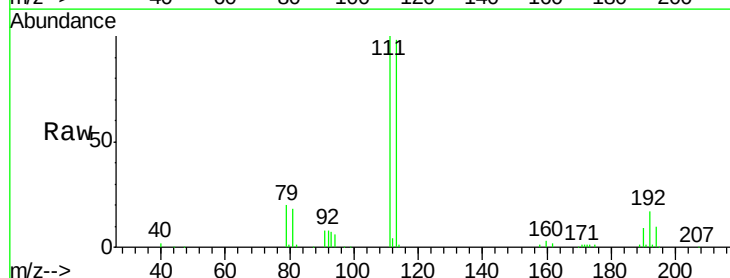


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V



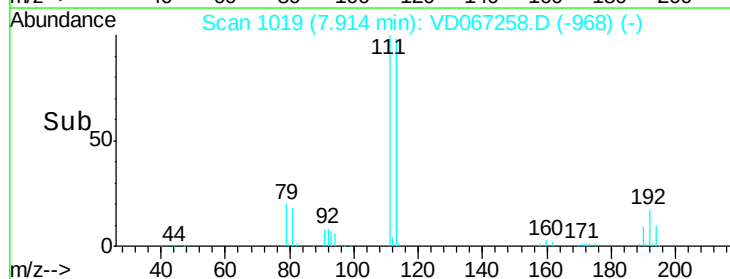
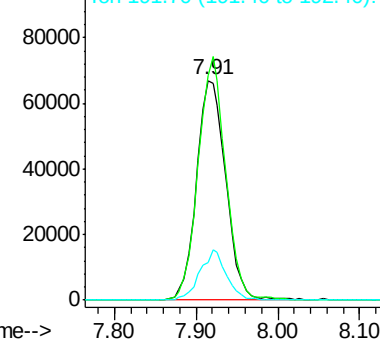


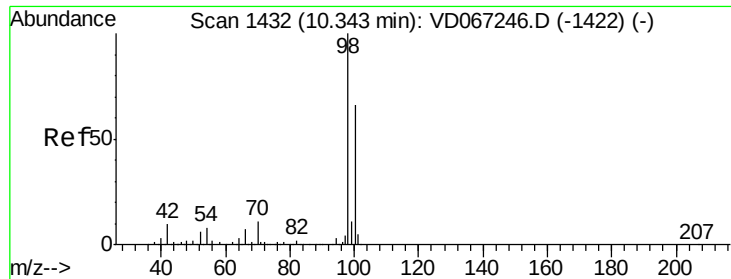

#50
Toluene-d8
Concen: 49.050 ug/l
RT: 10.34 min Scan# 1432
Delta R.T. 0.00 min
Lab File: VD067258.D
Acq: 13 Oct 2020 17:58




Instrument :
MSVOA_D
ClientSampleId :
BB-SOIL


Tot Ion: 98 Resp: 597463
Ion Ratio Lower Upper
98 100
100 67.1 53.1 79.7

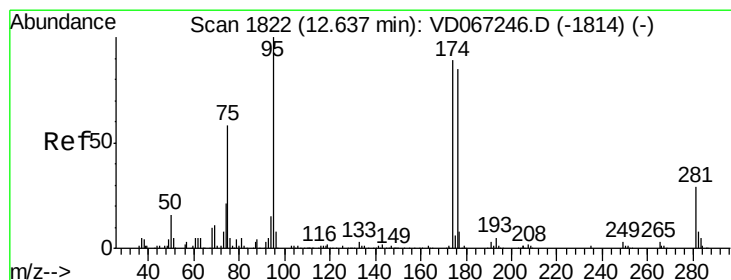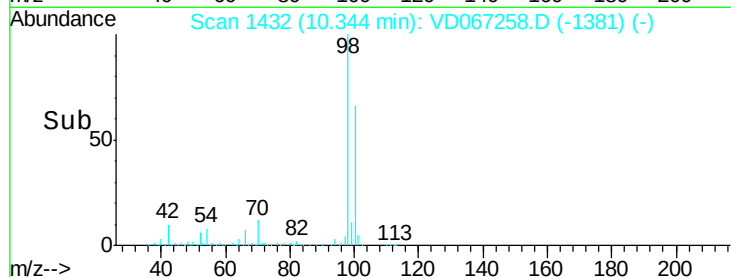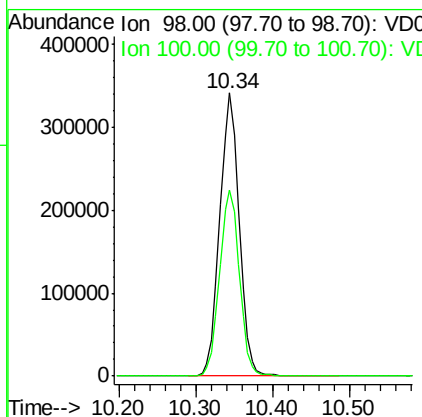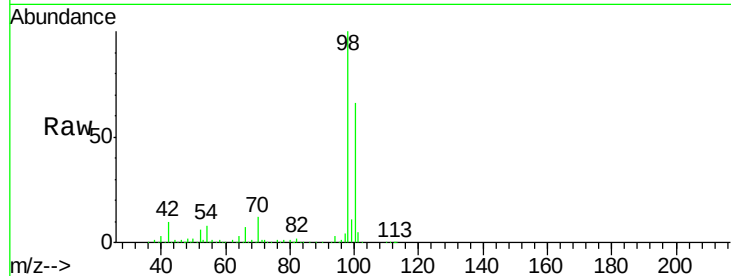

#62
4-Bromofluorobenzene
Concen: 48.779 ug/l
RT: 12.64 min Scan# 1822
Delta R.T. 0.00 min
Lab File: VD067258.D
Acq: 13 Oct 2020 17:58

Tgt Ion: 95 Resp: 206605
Ion Ratio Lower Upper
95 100
174 86.6 0.0 175.2
176 81.6 0.0 168.6

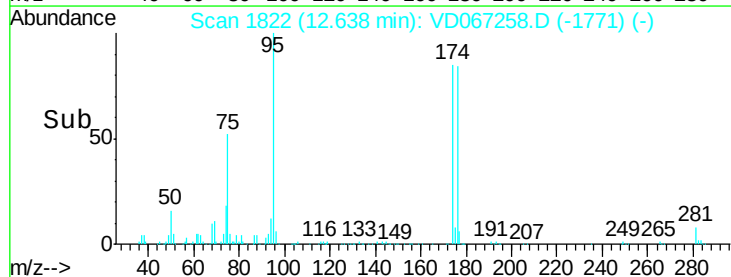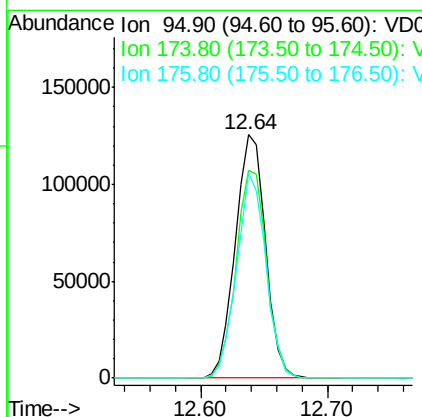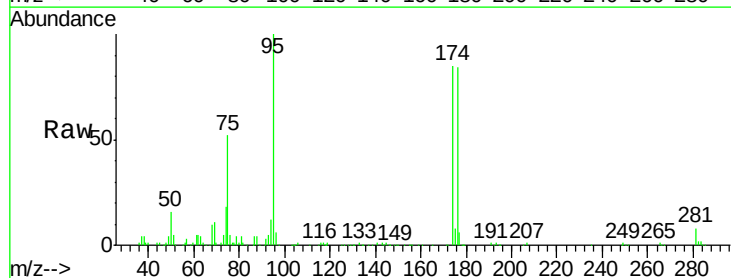


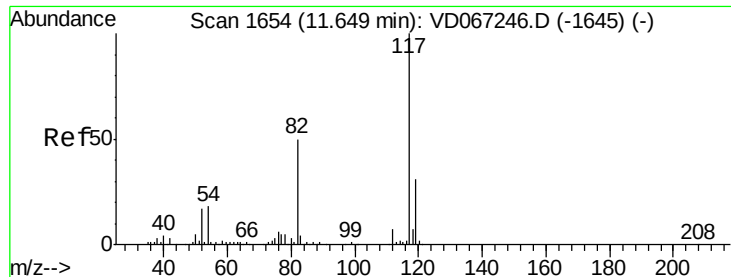




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.65 min Scan# 1654
Delta R.T. 0.00 min
Lab File: VD067258.D
Acq: 13 Oct 2020 17:58

Instrument :
MSVOA_D
ClientSampleId :
BB-SOIL

Tot Ion:117 Resp: 488540
Ion Ratio Lower Upper
117 100
82 50.7 39.9 59.9
119 32.5 24.9 37.3

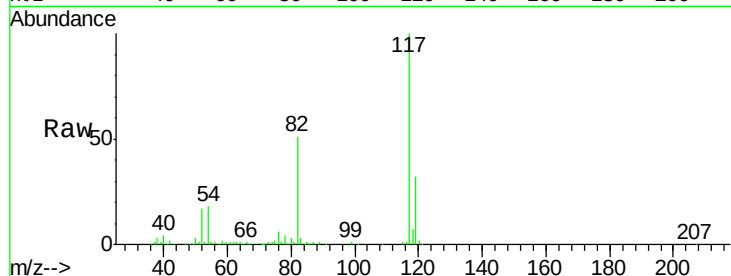


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): V
Ion 118.90 (118.60 to 119.60): V

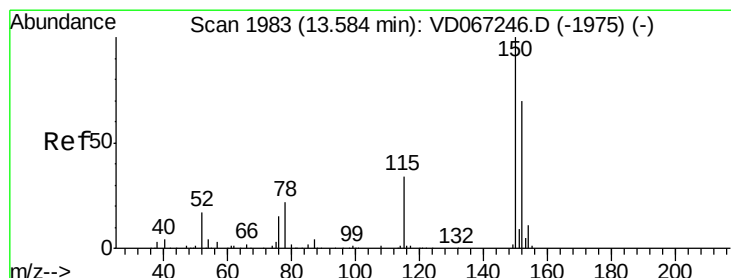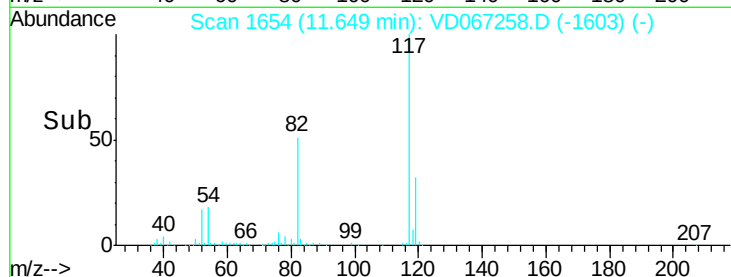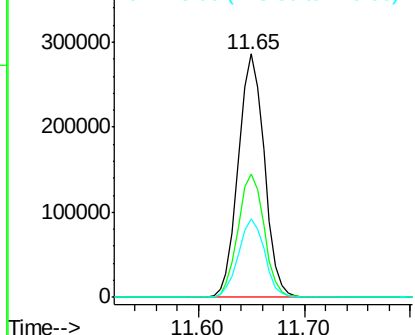

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.58 min Scan# 1983
Delta R.T. 0.00 min
Lab File: VD067258.D
Acq: 13 Oct 2020 17:58

Tgt Ion:152 Resp: 224590
Ion Ratio Lower Upper
152 100
115 59.6 29.3 87.9
150 161.7 0.0 339.0

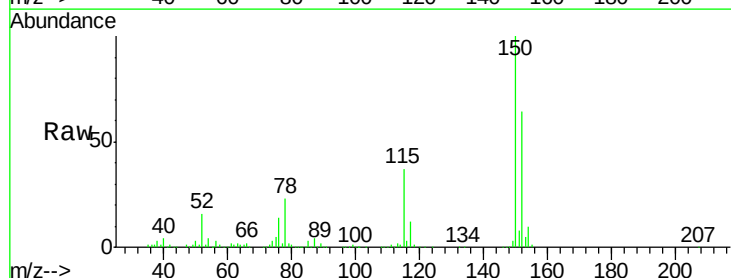

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

