


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD101321\
Data File : VD070691.D
Acq On : 13 Oct 2021 12:00
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D100521S.M
Title : SW846 8260
Last Update : Wed Oct 06 09:10:31 2021

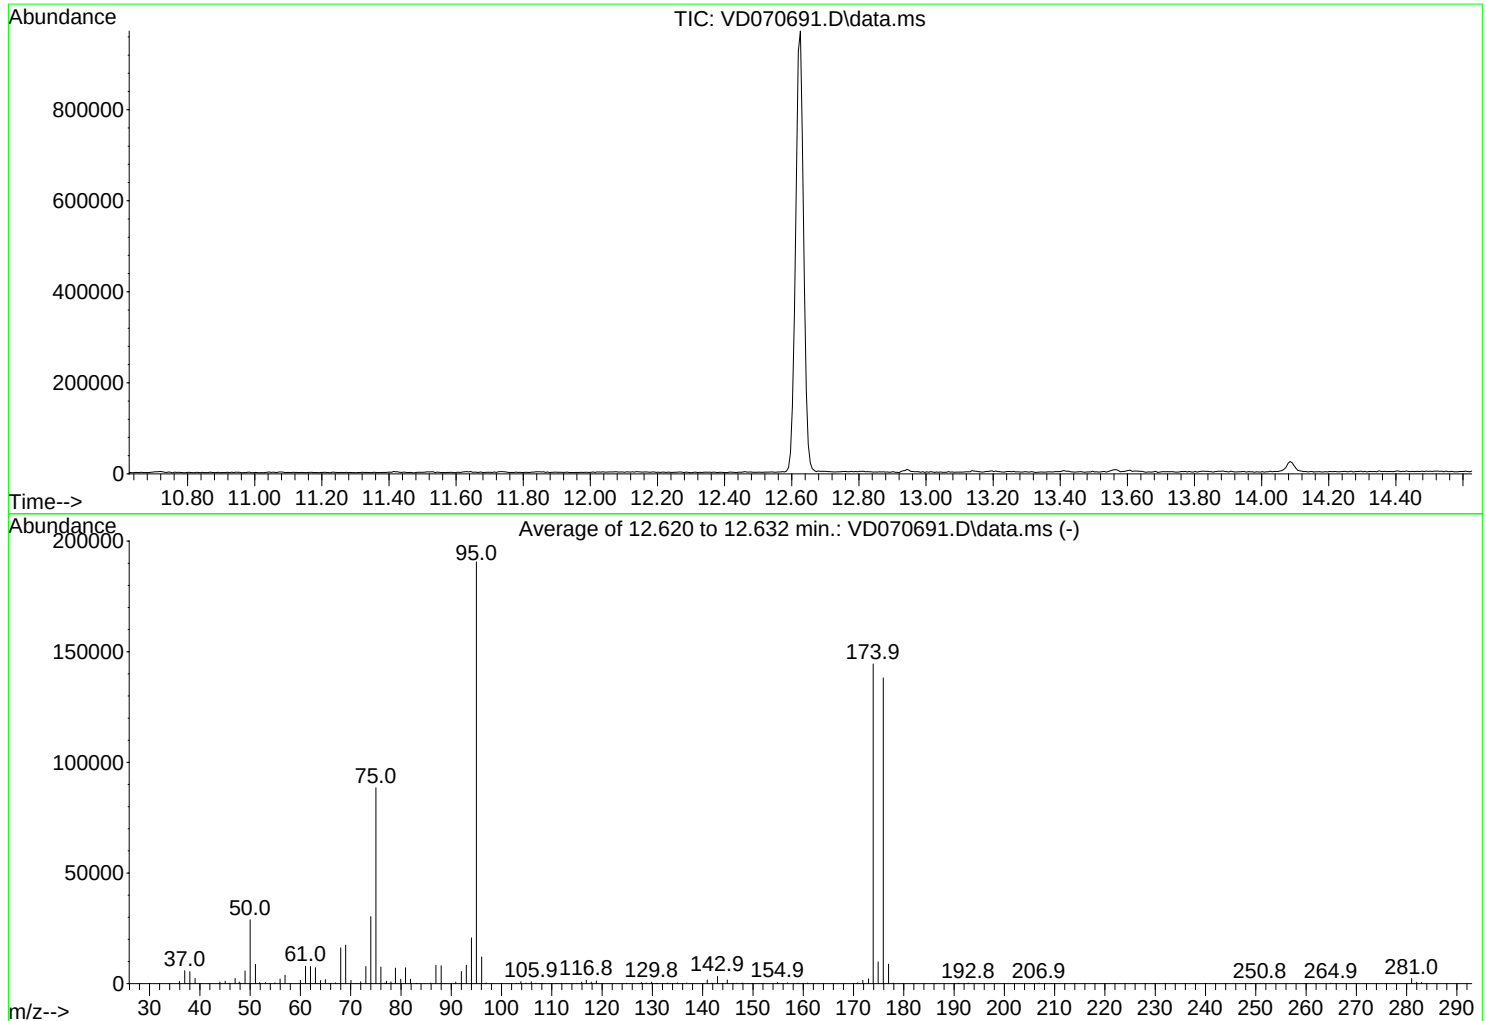

AutoFind: Scans 1819, 1820, 1821; Background Corrected with Scan 1809

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.1	28832	PASS
75	95	30	60	46.4	88485	PASS
95	95	100	100	100.0	190635	PASS
96	95	5	9	6.3	12075	PASS
173	174	0.00	2	1.5	2137	PASS
174	95	50	100	75.8	144475	PASS
175	174	5	9	6.8	9845	PASS
176	174	95	101	95.7	138205	PASS
177	176	5	9	6.4	8796	PASS