


Methyl Iodide

Response Ratio

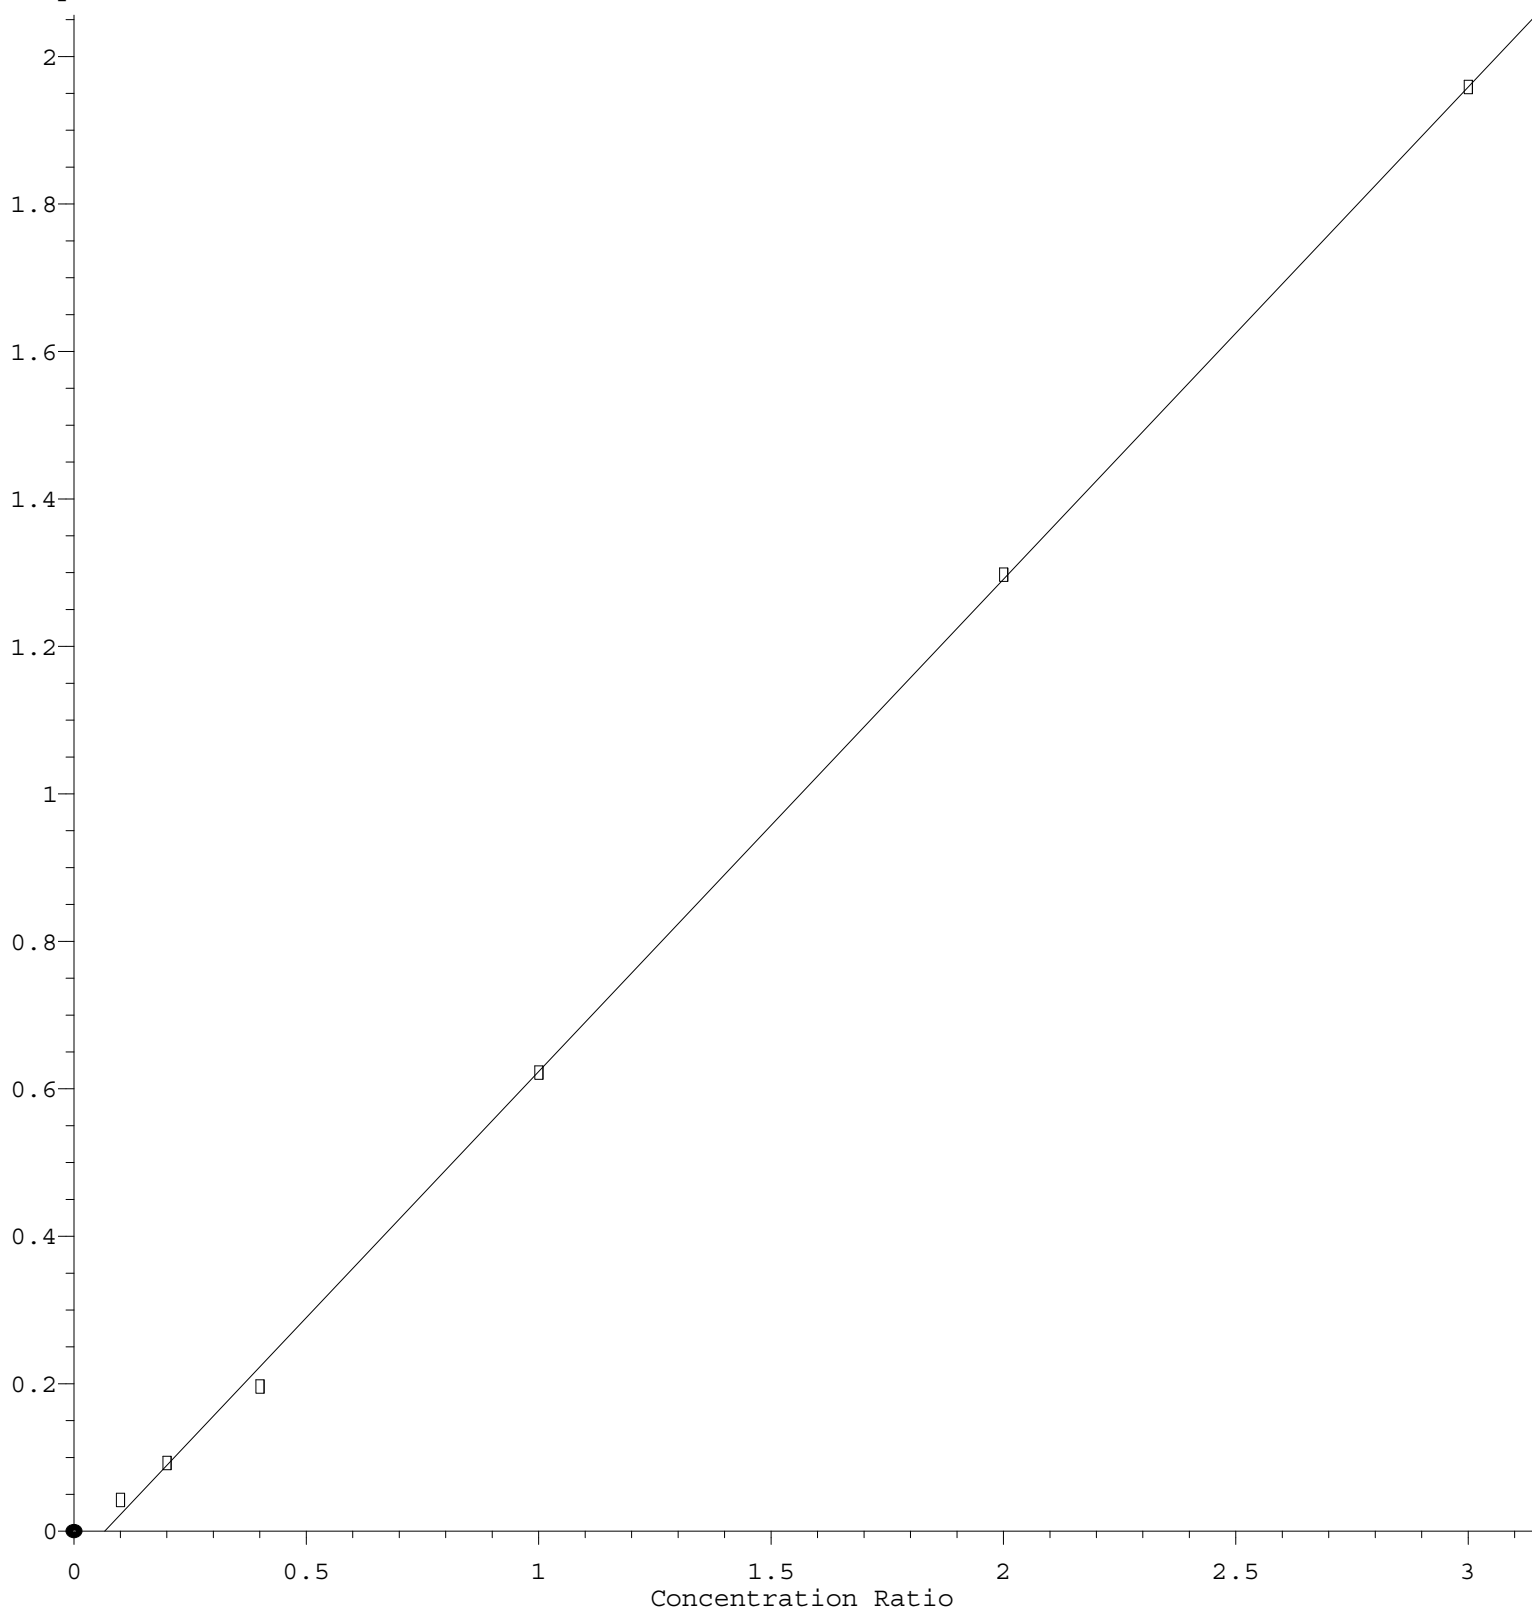

$$\text{Response} = 6.679\text{e-}001 * \text{Amt} - 4.434\text{e-}002$$


Coef of Det (r^2) = 0.999616 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D101521S.M

Calibration Table Last Updated: Mon Oct 18 08:32:03 2021

Methylene Chloride

Response Ratio

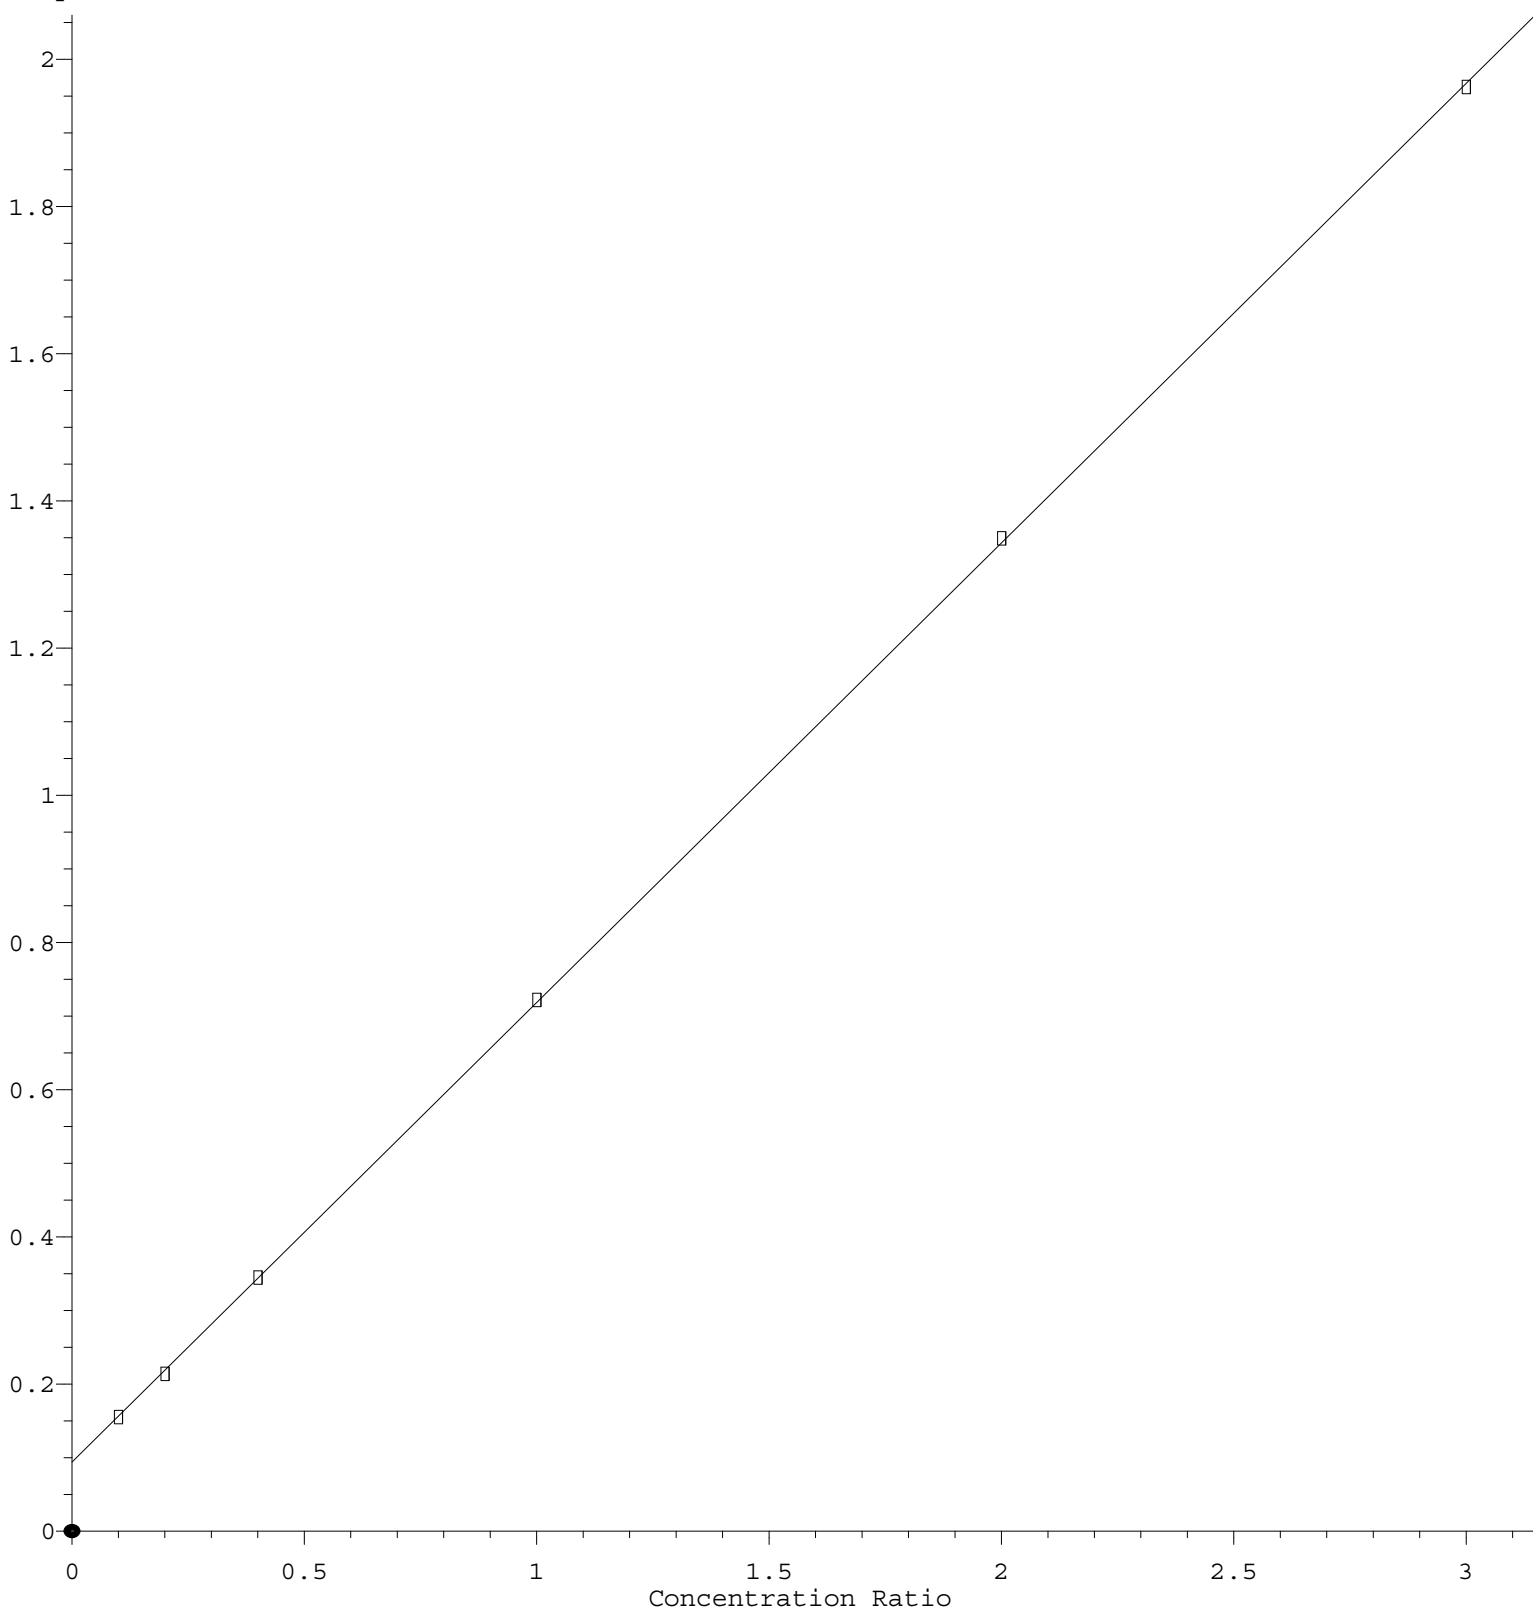

$$\text{Response} = 6.246\text{e-}001 * \text{Amt} + 9.362\text{e-}002$$


Coef of Det (r^2) = 0.999961 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D101521S.M

Calibration Table Last Updated: Mon Oct 18 08:32:03 2021

Vinyl Acetate

Response Ratio

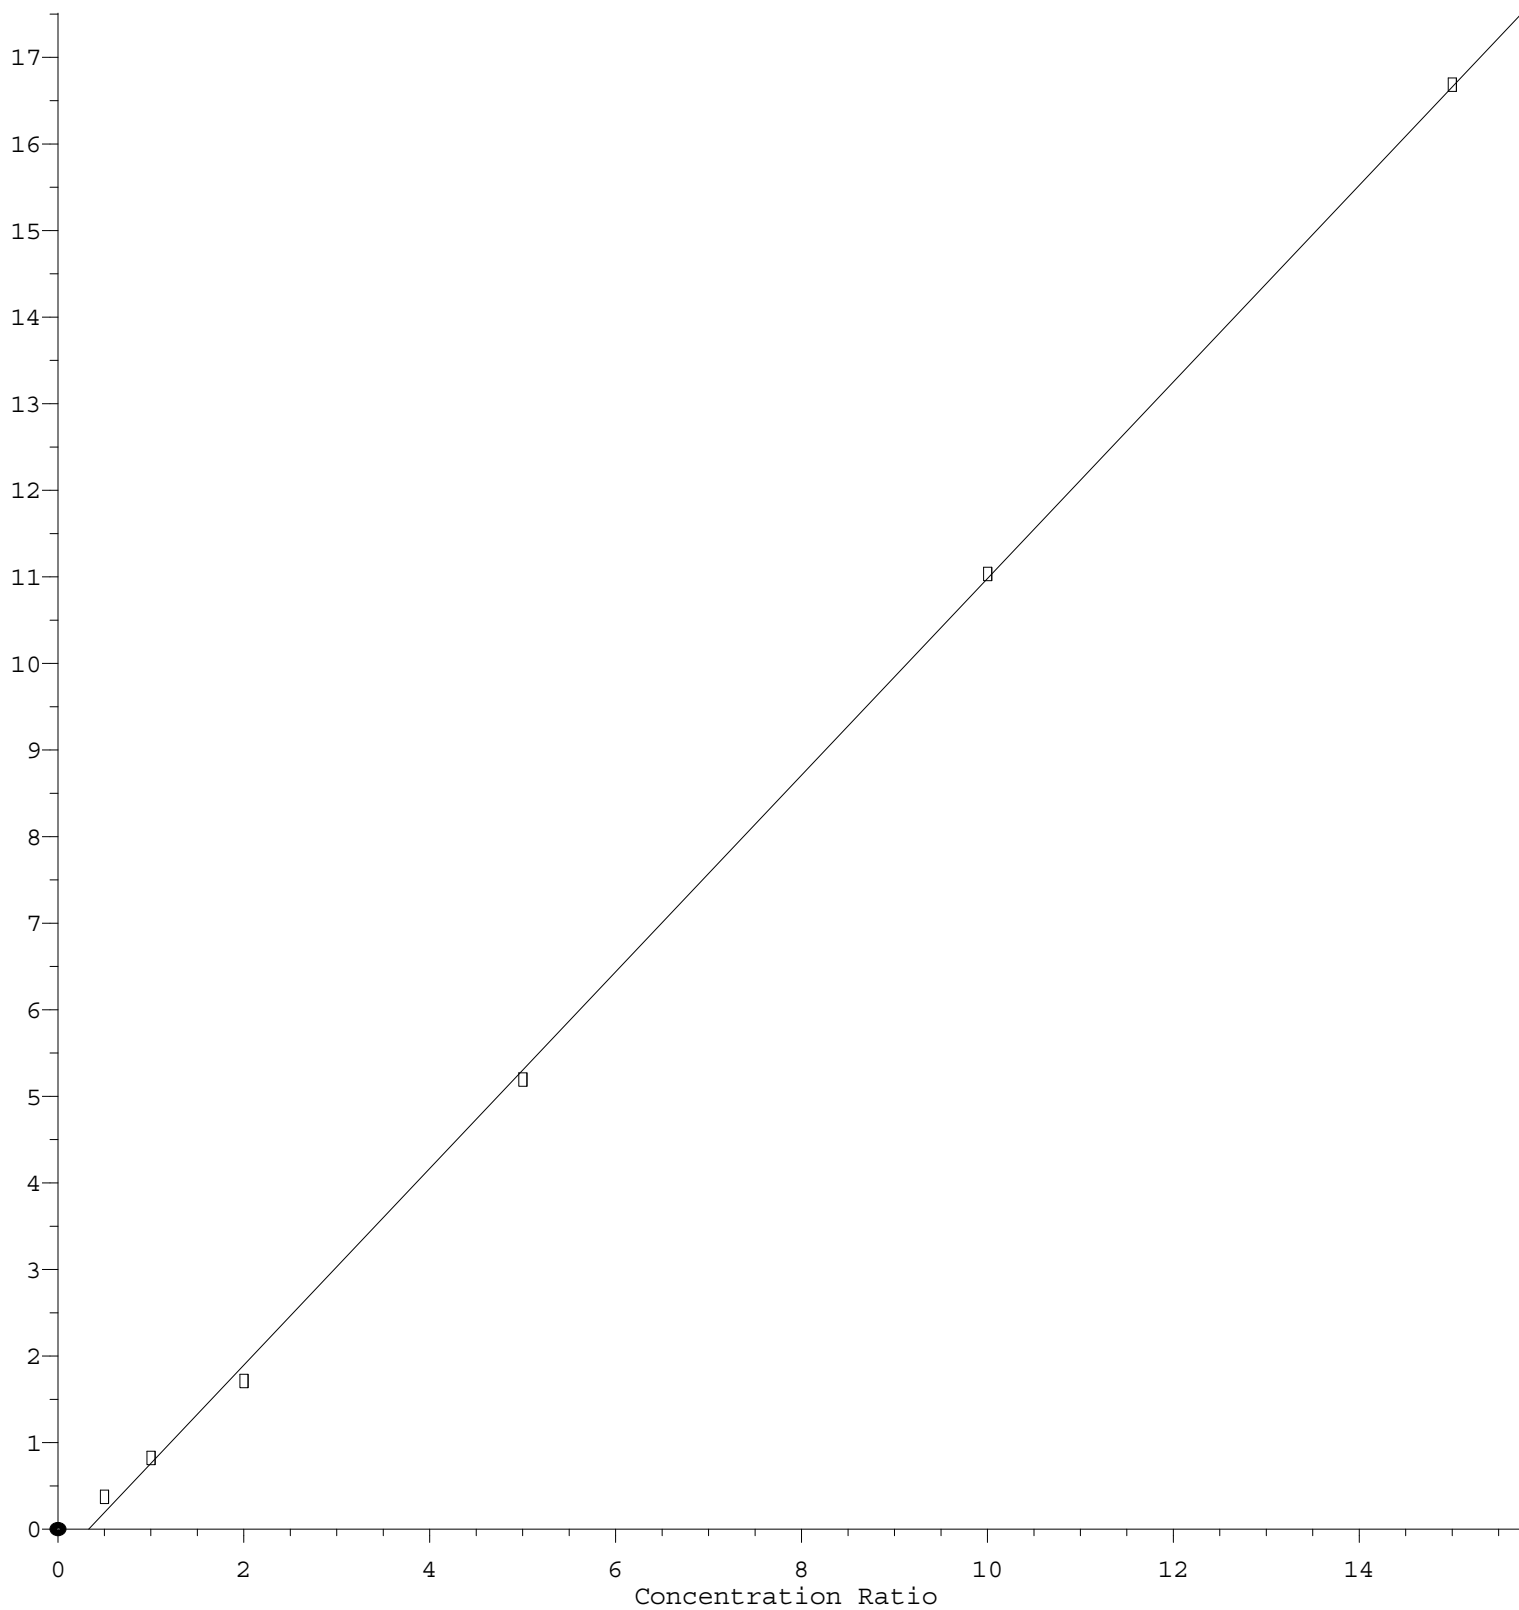


$$\text{Response} = 1.136\text{e}+000 * \text{Amt} - 3.708\text{e}-001$$

Coef of Det (r^2) = 0.999606 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D101521S.M

Calibration Table Last Updated: Mon Oct 18 08:32:03 2021


Methacrylonitrile

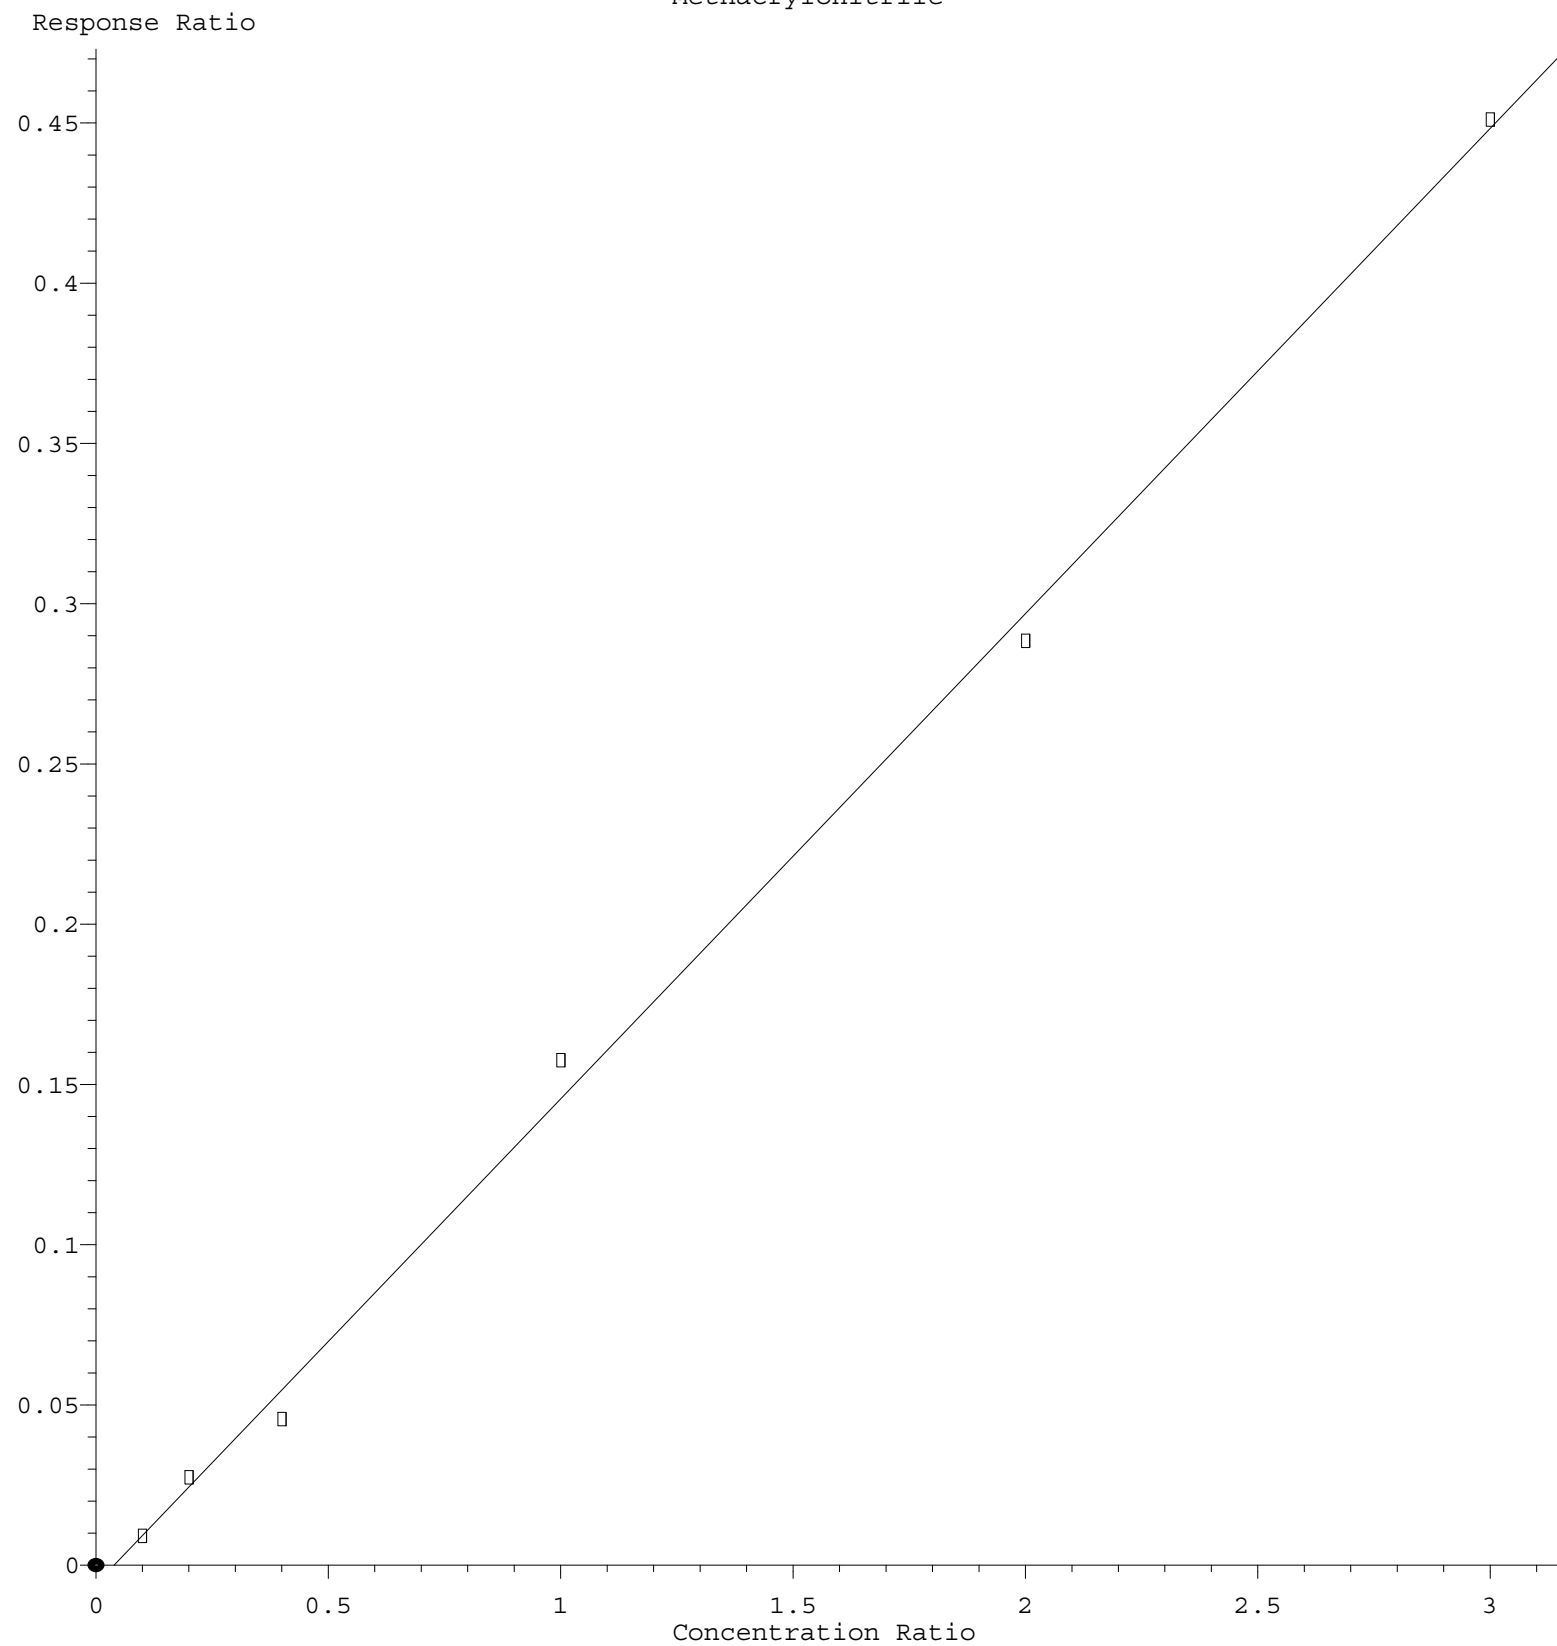

Response = 1.514e-001 * Amt - 5.885e-003
Coef of Det (r^2) = 0.997950 Curve Fit: Linear
Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D101521S.M
Calibration Table Last Updated: Mon Oct 18 08:32:03 2021

Ethyl methacrylate

Response Ratio

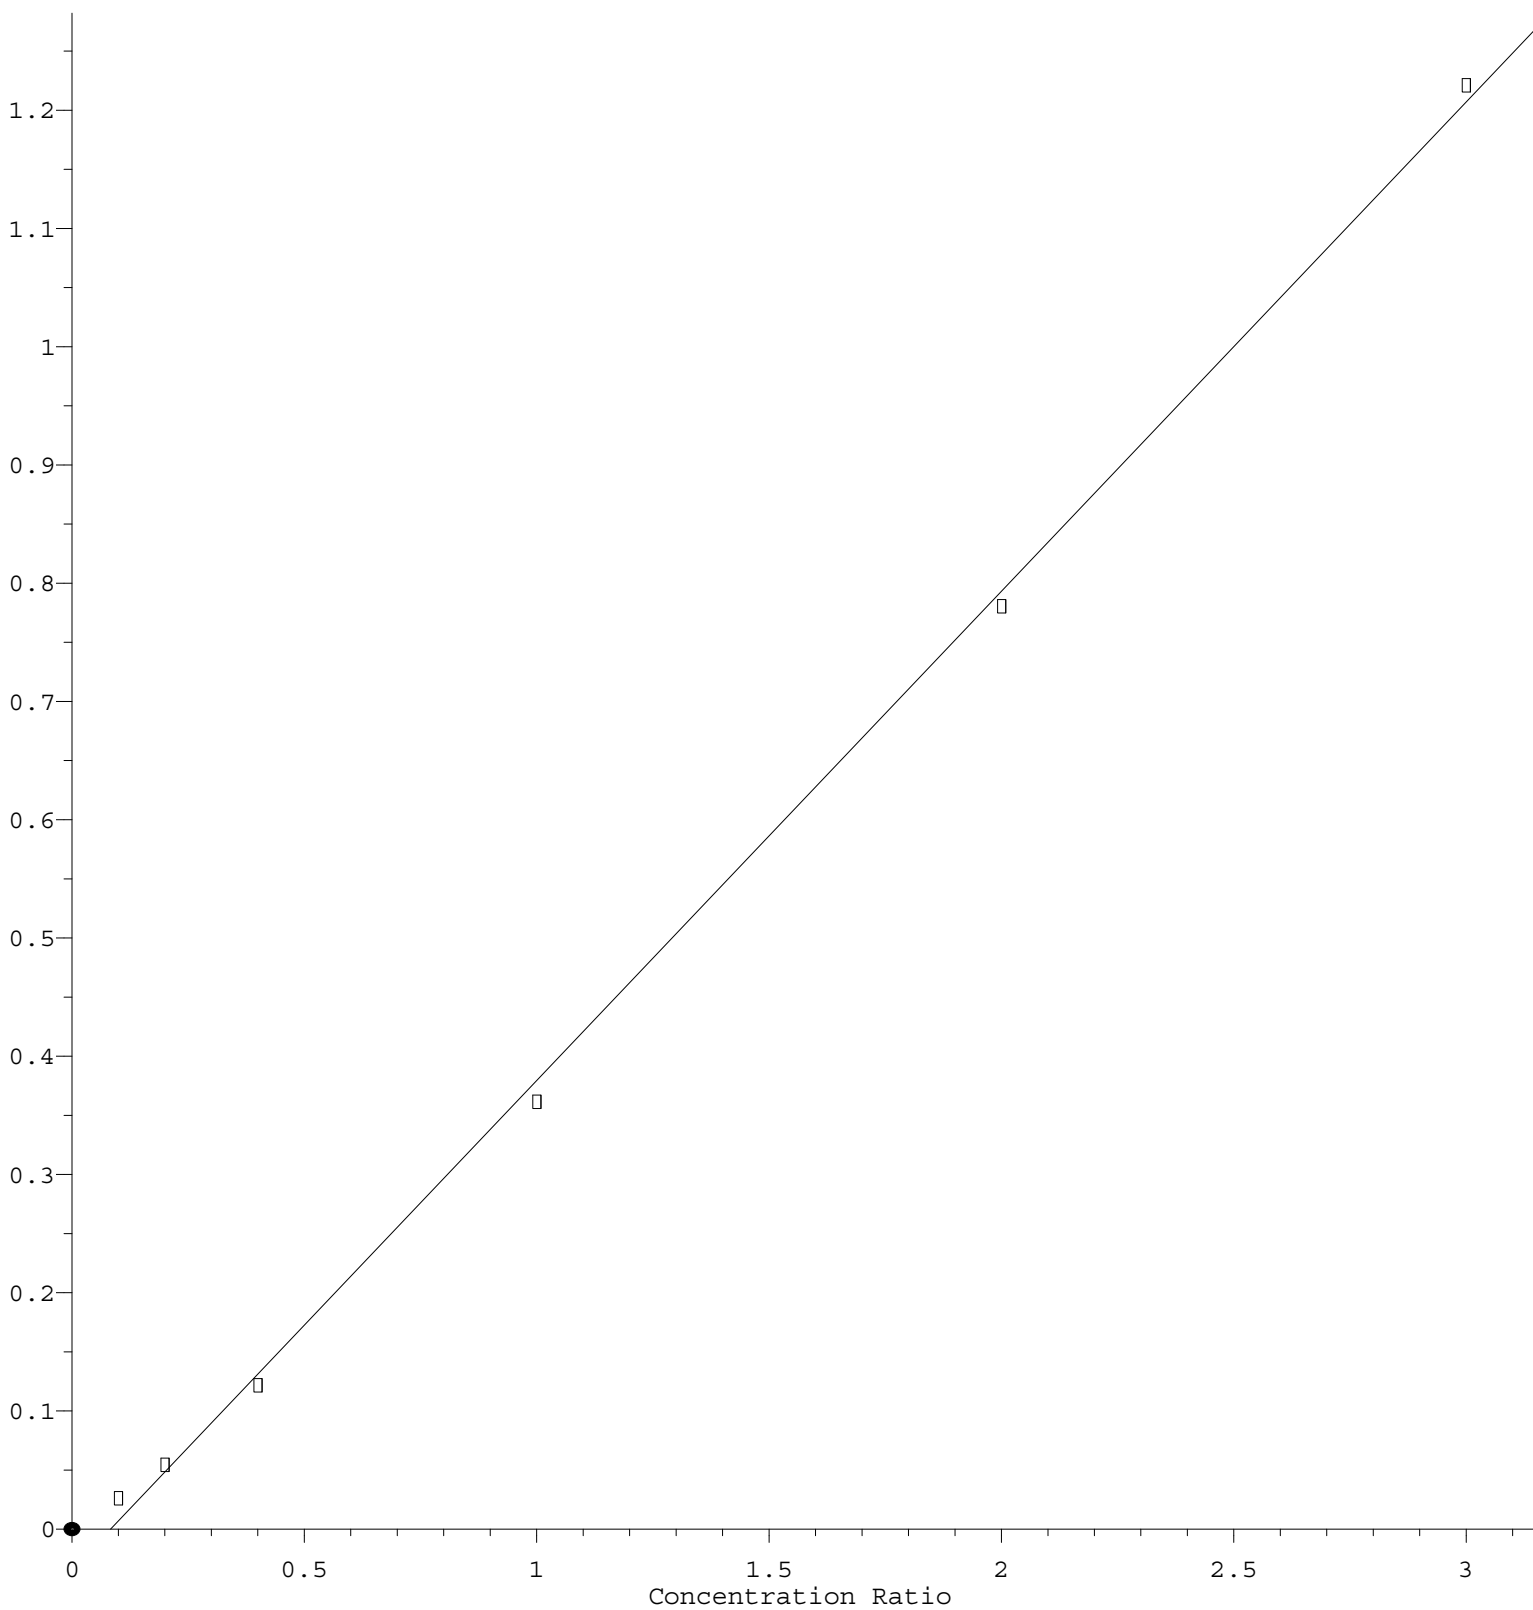

$$\text{Response} = 4.136\text{e-}001 * \text{Amt} - 3.438\text{e-}002$$


Coef of Det (r^2) = 0.998979 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D101521S.M

Calibration Table Last Updated: Mon Oct 18 08:32:03 2021

Naphthalene

Response Ratio

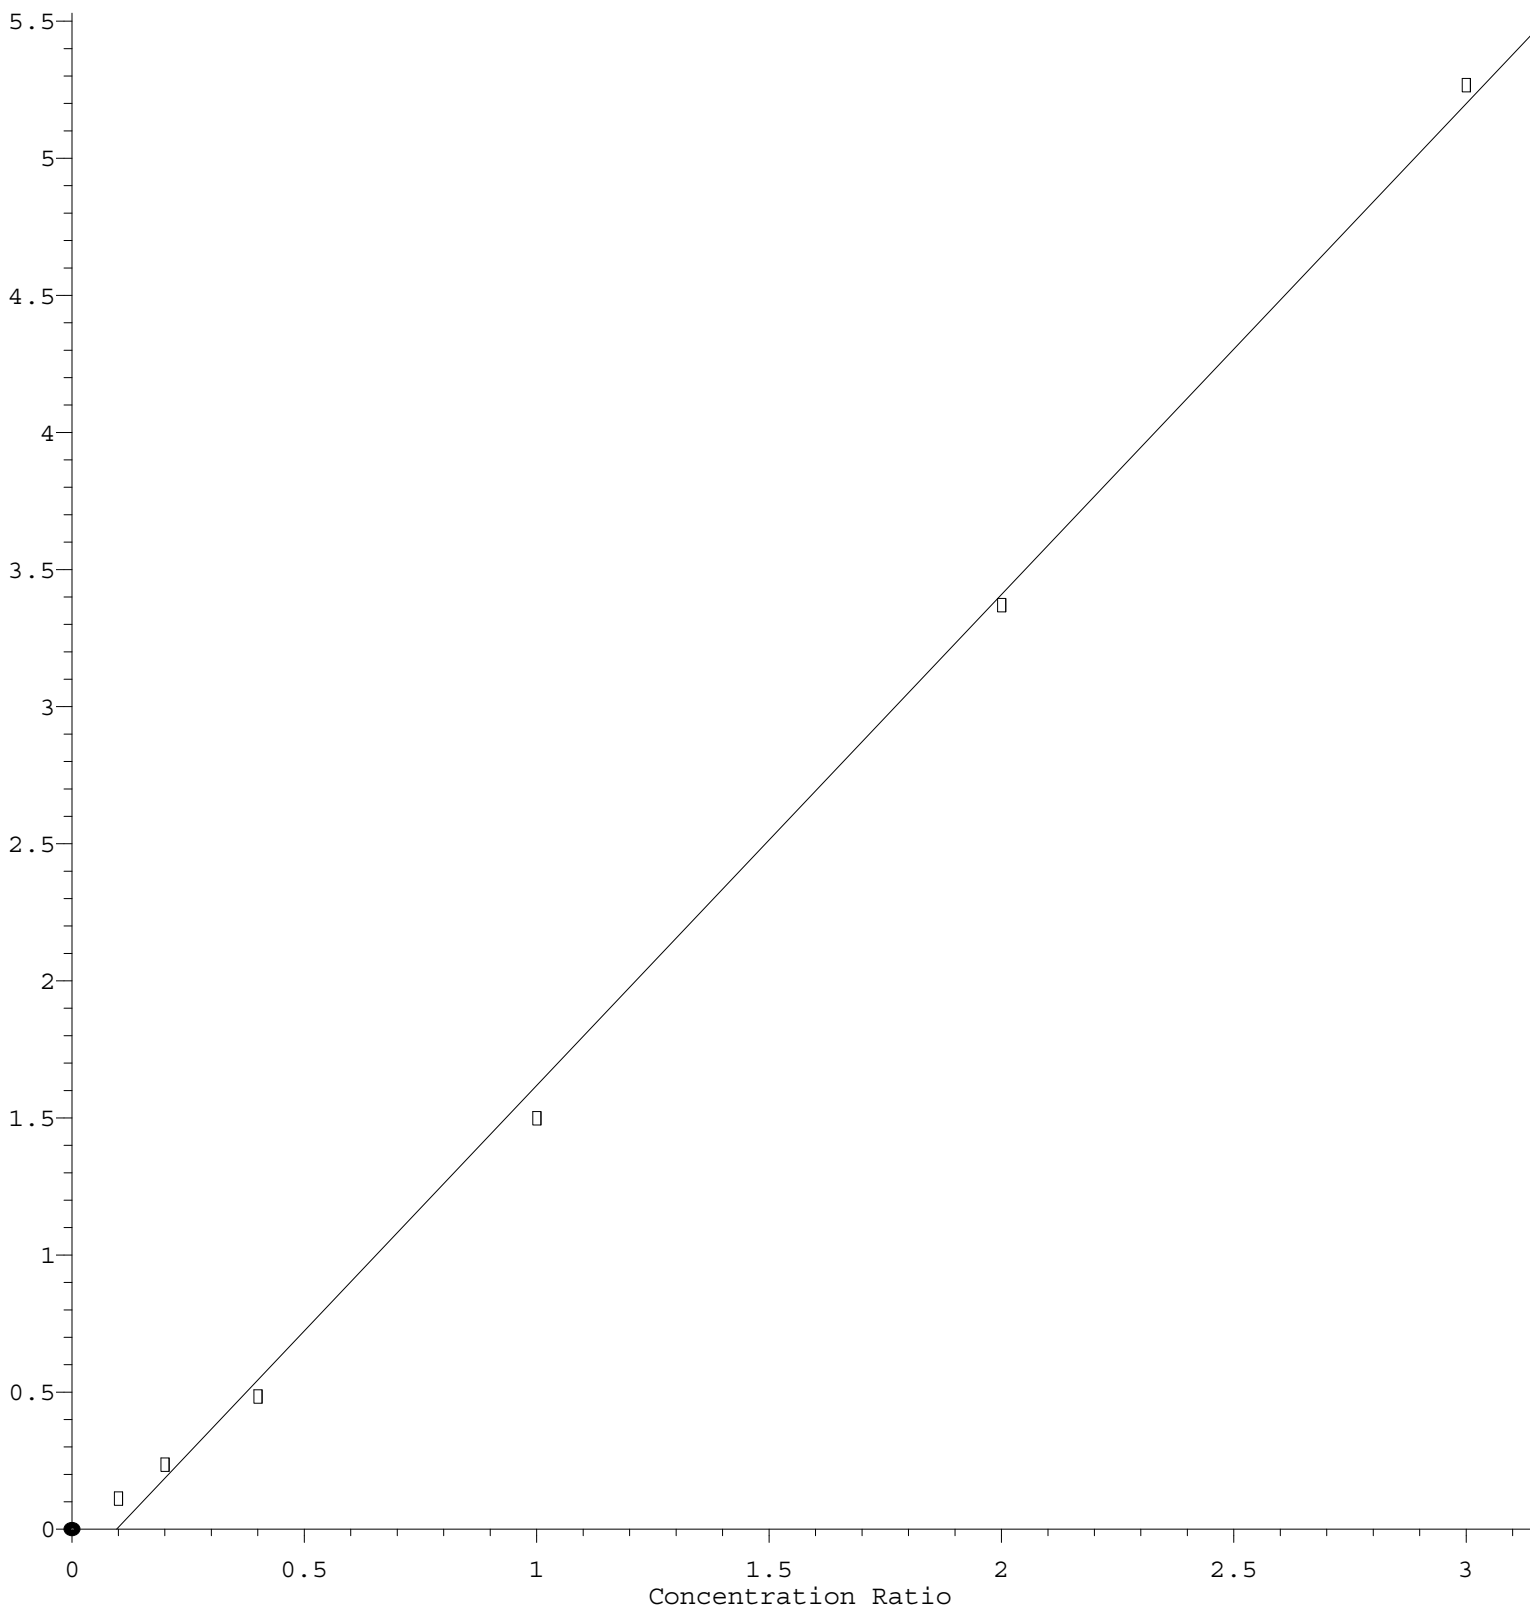

$$\text{Response} = 1.790\text{e}+000 * \text{Amt} - 1.716\text{e}-001$$

Coef of Det (r^2) = 0.998275 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D101521S.M

Calibration Table Last Updated: Mon Oct 18 08:32:03 2021