

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD101521\
 Data File : VD070717.D
 Acq On : 15 Oct 2021 15:17
 Operator : VA/SY
 Sample : VD1015SBL01
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 VD1015SBL01

Quant Time: Oct 18 08:32:59 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D101521S.M
 Quant Title : SW846 8260
 QLast Update : Mon Oct 18 08:32:03 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.973	168	506501	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.861	114	908229	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.638	117	845504	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.561	152	354111	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.326	65	318792	53.14	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	106.28%
35) Dibromofluoromethane	7.908	113	300961	51.75	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	103.50%
50) Toluene-d8	10.332	98	1165936	52.30	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	104.60%
62) 4-Bromofluorobenzene	12.620	95	371796	48.44	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	96.88%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD101521\
Data File : VD070717.D
Acq On : 15 Oct 2021 15:17
Operator : VA/SY
Sample : VD1015SBL01
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
VD1015SBL01

Quant Time: Oct 18 08:32:59 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D101521S.M
Quant Title : SW846 8260
QLast Update : Mon Oct 18 08:32:03 2021
Response via : Initial Calibration




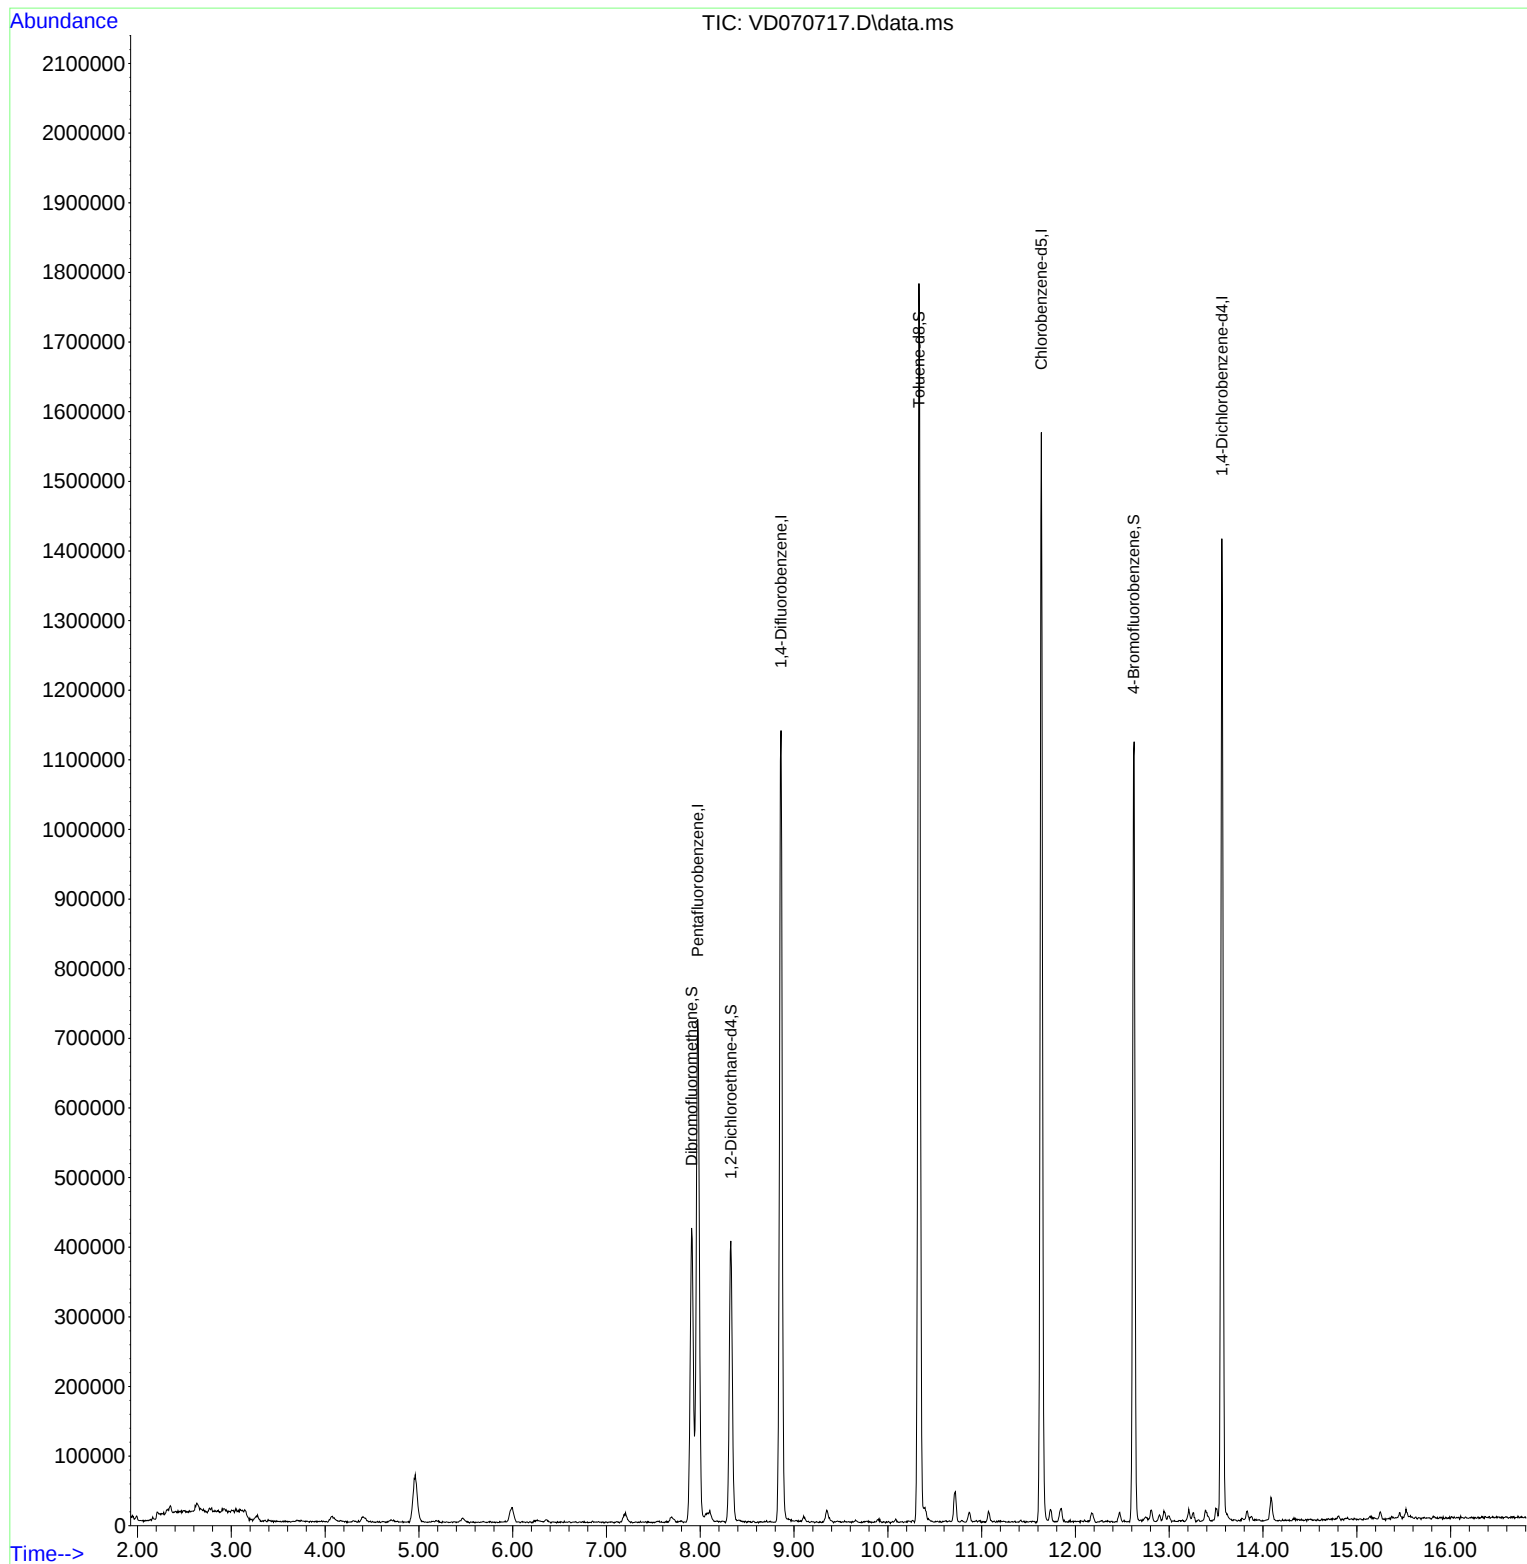


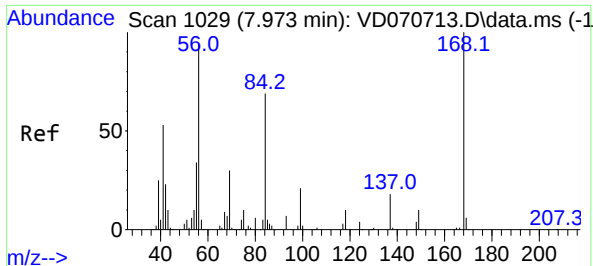

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.973 min Scan# 1029
Delta R.T. 0.000 min
Lab File: VD070717.D
Acq: 15 Oct 2021 15:17




Instrument :
MSVOA_D
ClientSampleId :
VD1015SBL01


Tgt Ion:168 Resp: 506501
Ion Ratio Lower Upper
168 100
99 63.8 51.4 77.0

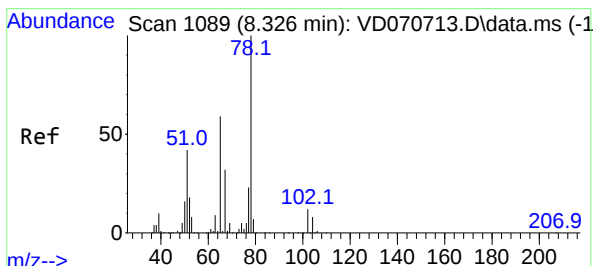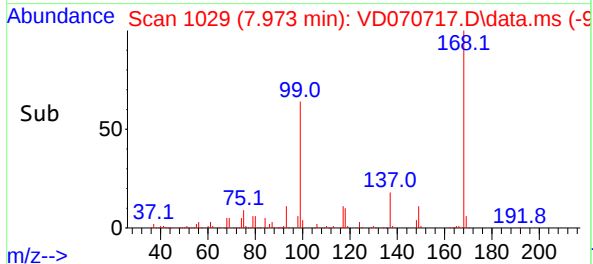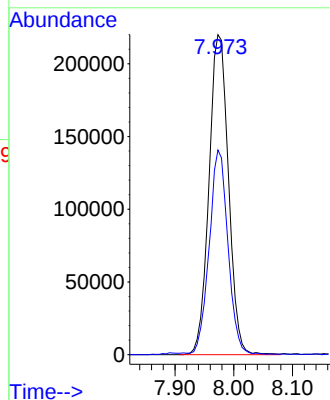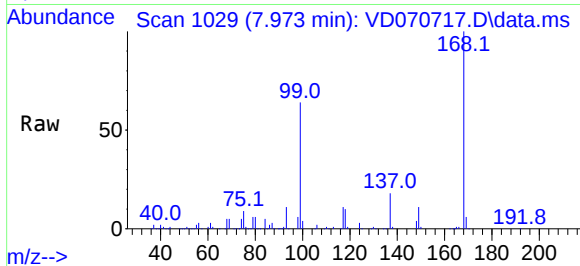

#33
1,2-Dichloroethane-d4
Concen: 53.14 ug/l
RT: 8.326 min Scan# 1089
Delta R.T. 0.000 min
Lab File: VD070717.D
Acq: 15 Oct 2021 15:17

Tgt Ion: 65 Resp: 318792
Ion Ratio Lower Upper
65 100
67 53.8 0.0 110.2

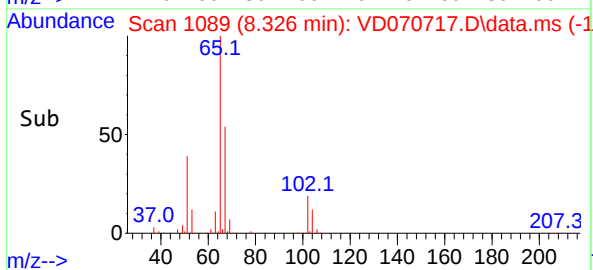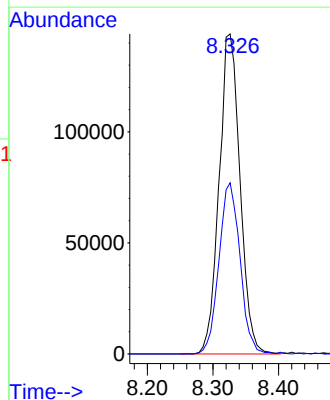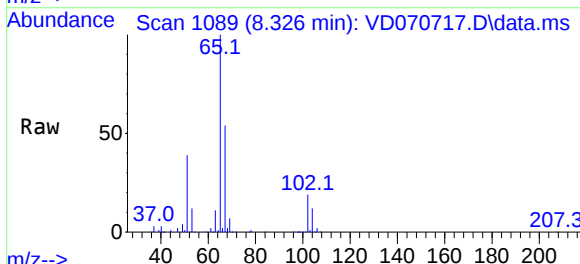




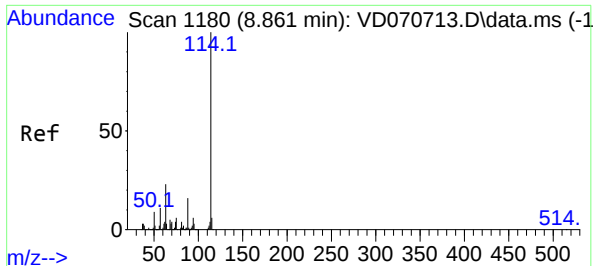


#34

1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.861 min Scan# 1180
Delta R.T. 0.000 min
Lab File: VD070717.D
Acq: 15 Oct 2021 15:17

Instrument :
MSVOA_D
ClientSampleId :
VD1015SBL01




Tgt Ion:114 Resp: 908229
Ion Ratio Lower Upper
114 100
63 24.2 0.0 41.8
88 16.9 0.0 32.6

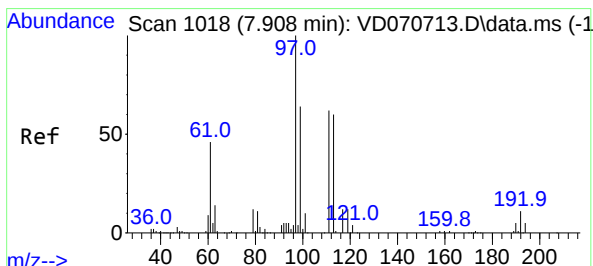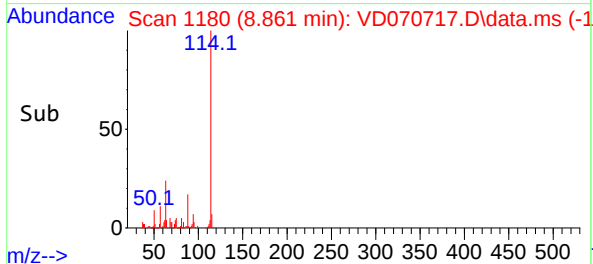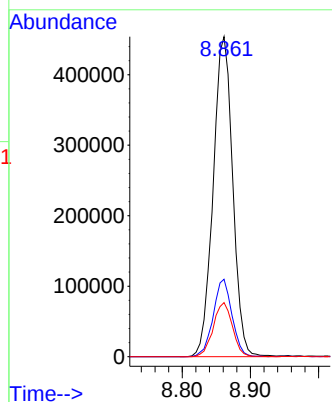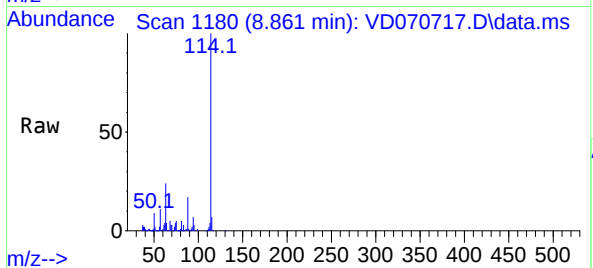


#35

Dibromofluoromethane
Concen: 51.75 ug/l
RT: 7.908 min Scan# 1018
Delta R.T. 0.000 min
Lab File: VD070717.D
Acq: 15 Oct 2021 15:17

Tgt Ion:113 Resp: 300961
Ion Ratio Lower Upper
113 100
111 101.5 83.1 124.7
192 18.7 12.7 19.1


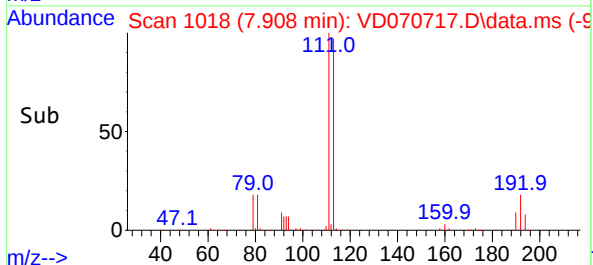
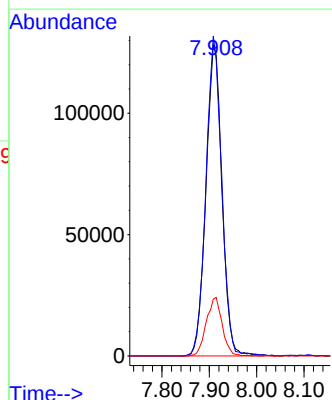
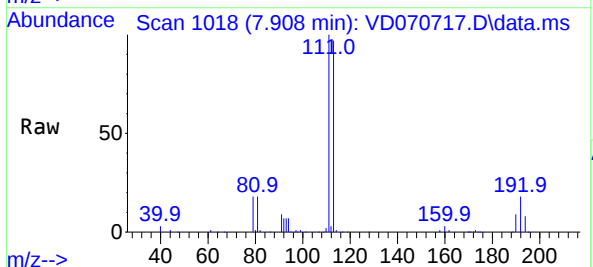


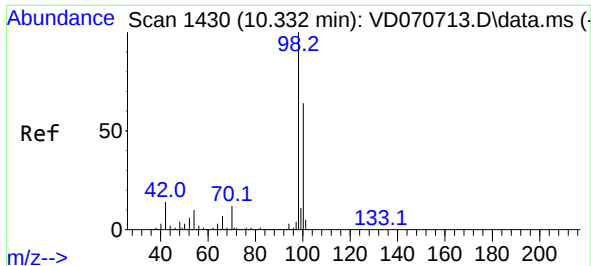

#50
Toluene-d8
Concen: 52.30 ug/l
RT: 10.332 min Scan# 1430
Delta R.T. 0.000 min
Lab File: VD070717.D
Acq: 15 Oct 2021 15:17




Instrument :
MSVOA_D
ClientSampleId :
VD1015SBL01


Tgt Ion: 98 Resp: 1165936
Ion Ratio Lower Upper
98 100
100 64.8 52.2 78.4

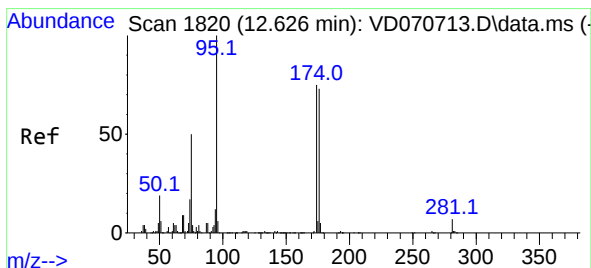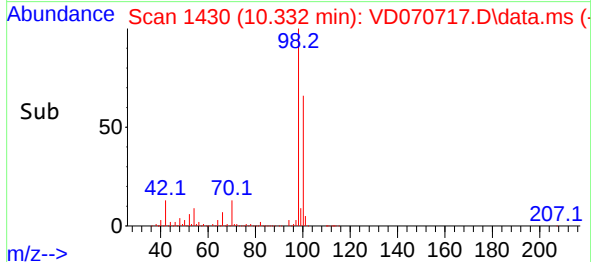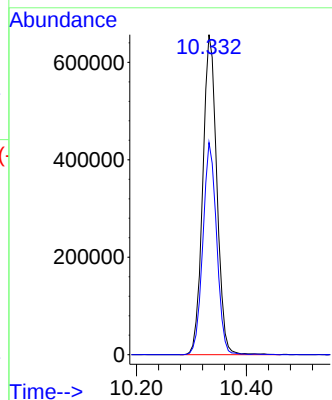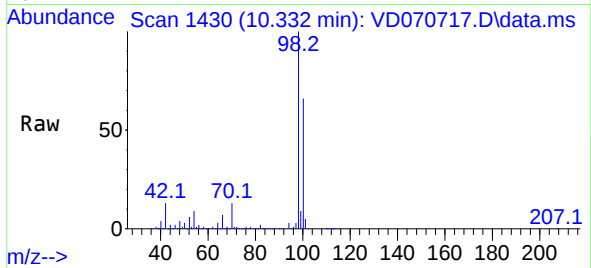

#62
4-Bromofluorobenzene
Concen: 48.44 ug/l
RT: 12.620 min Scan# 1819
Delta R.T. -0.006 min
Lab File: VD070717.D
Acq: 15 Oct 2021 15:17


Tgt Ion: 95 Resp: 371796
Ion Ratio Lower Upper
95 100
174 74.4 0.0 138.0
176 71.8 0.0 135.6

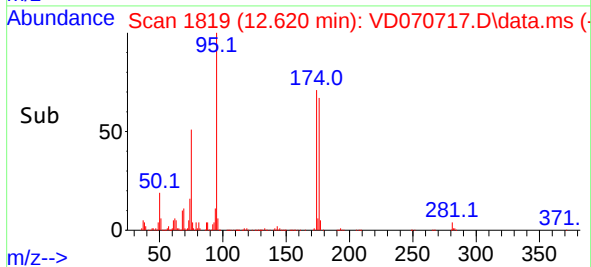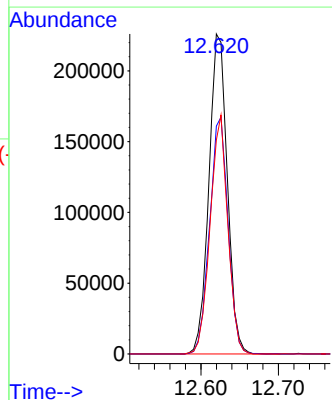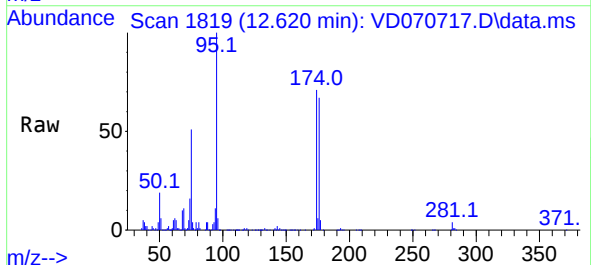



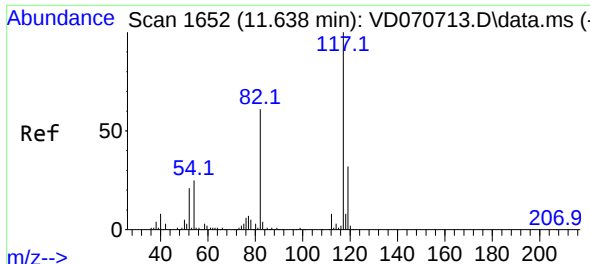


#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.638 min Scan# 1652
Delta R.T. 0.000 min
Lab File: VD070717.D
Acq: 15 Oct 2021 15:17


Instrument :
MSVOA_D
ClientSampleId :
VD1015SBL01

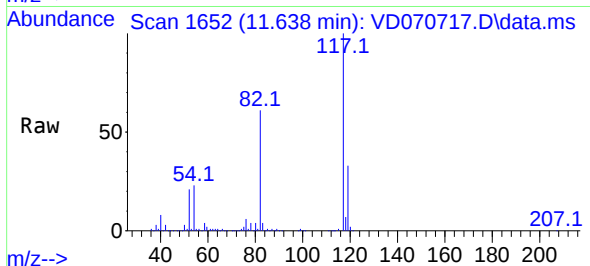

Tgt Ion:117 Resp: 845504
Ion Ratio Lower Upper
117 100
82 61.0 45.4 68.2
119 33.0 24.7 37.1

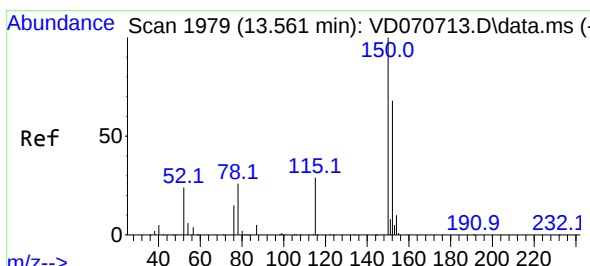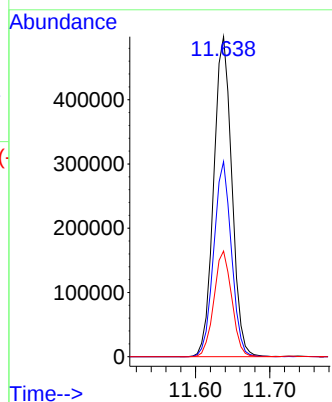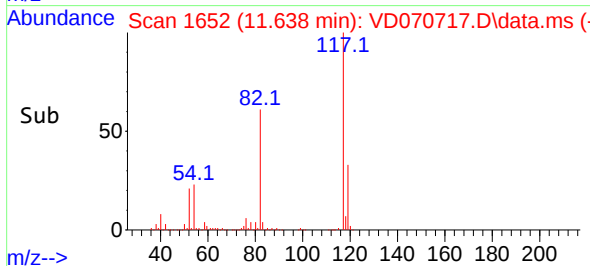

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.561 min Scan# 1979
Delta R.T. 0.000 min
Lab File: VD070717.D
Acq: 15 Oct 2021 15:17

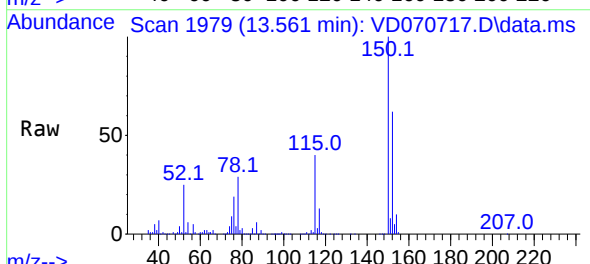

Tgt Ion:152 Resp: 354111
Ion Ratio Lower Upper
152 100
115 63.4 31.9 95.7
150 160.9 0.0 350.0

