
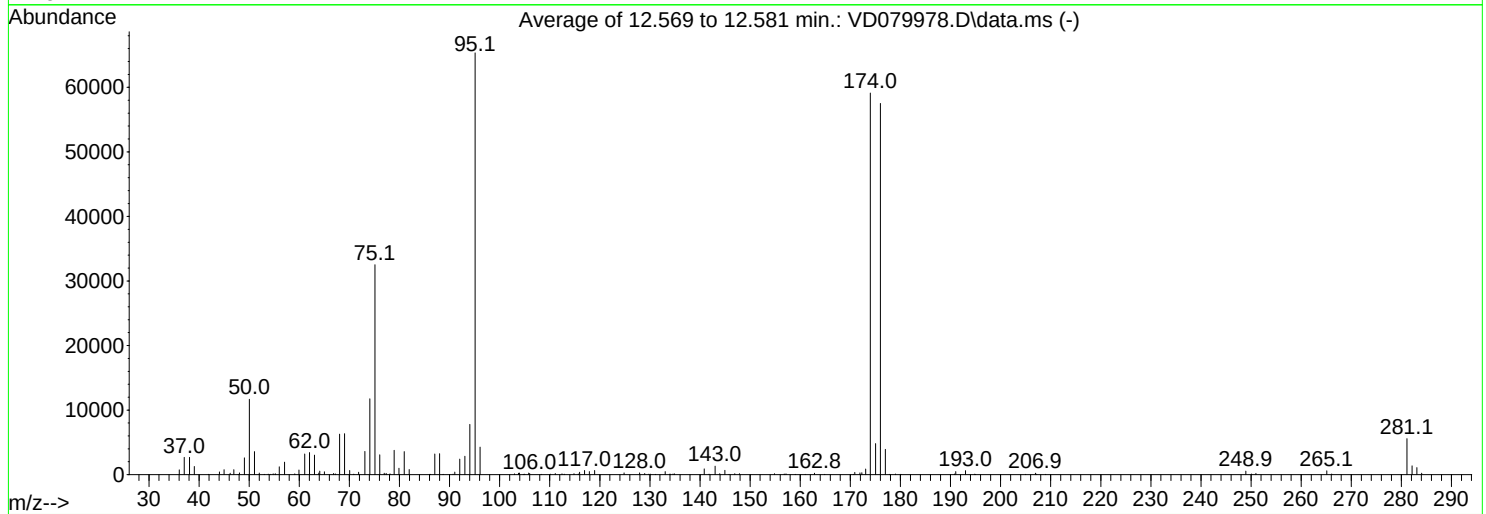


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD101524\
Data File : VD079978.D
Acq On : 15 Oct 2024 09:39
Operator : RP/MD
Sample : BFB
Misc : 5.00G/5ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D101124S.M
Title : SW846 8260
Last Update : Mon Oct 14 03:20:54 2024

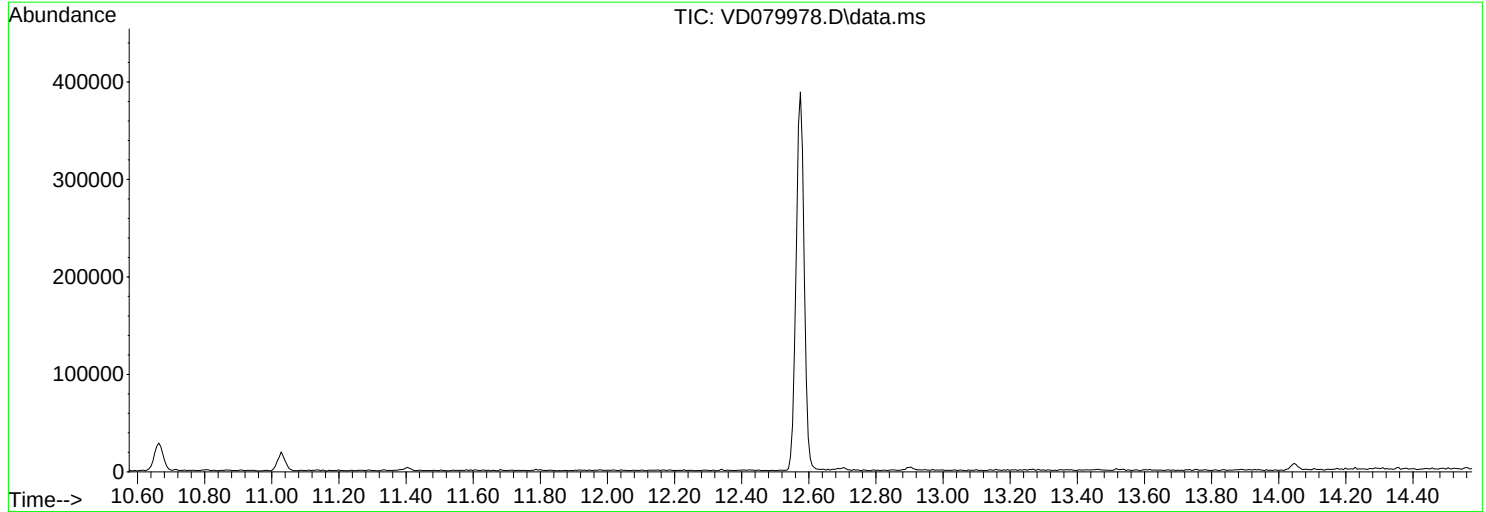

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1858

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.9	11675	PASS
75	95	30	60	49.8	32528	PASS
95	95	100	100	100.0	65344	PASS
96	95	5	9	6.5	4266	PASS
173	174	0.00	2	1.5	865	PASS
174	95	50	100	90.5	59120	PASS
175	174	5	9	8.1	4802	PASS
176	174	95	101	97.3	57517	PASS
177	176	5	9	6.8	3918	PASS