
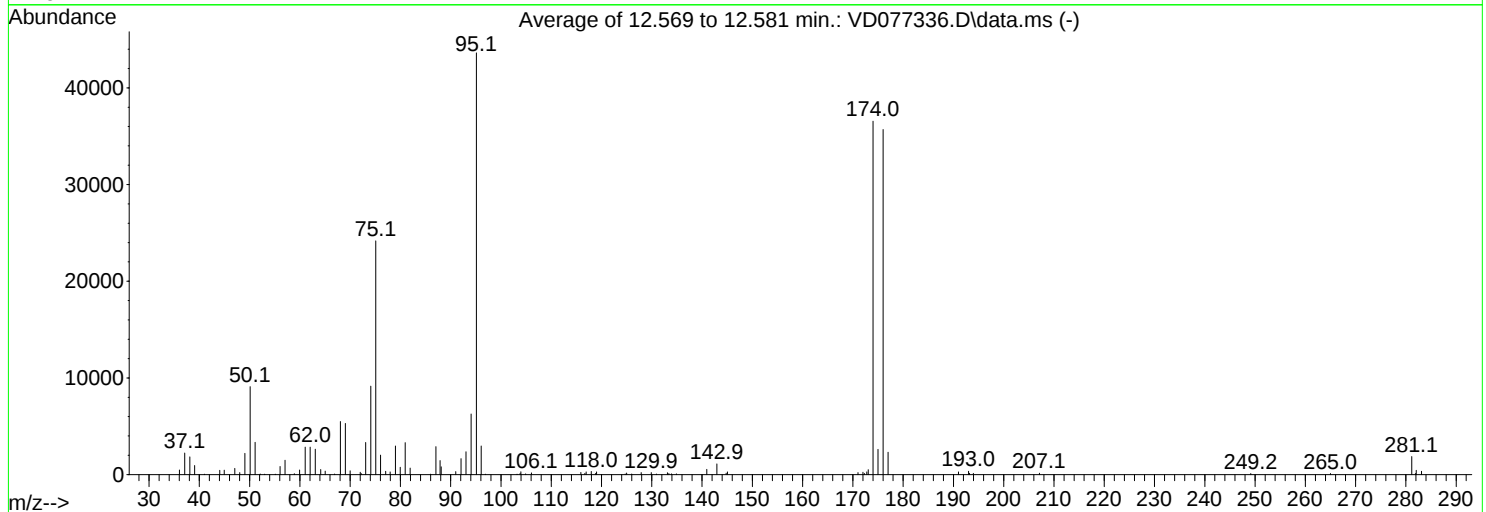


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD101723\
Data File : VD077336.D
Acq On : 17 Oct 2023 12:02
Operator : JC/SY
Sample : BFB
Misc : 5.00G/5.0ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D101723S.M
Title : SW846 8260
Last Update : Wed Oct 18 03:02:43 2023

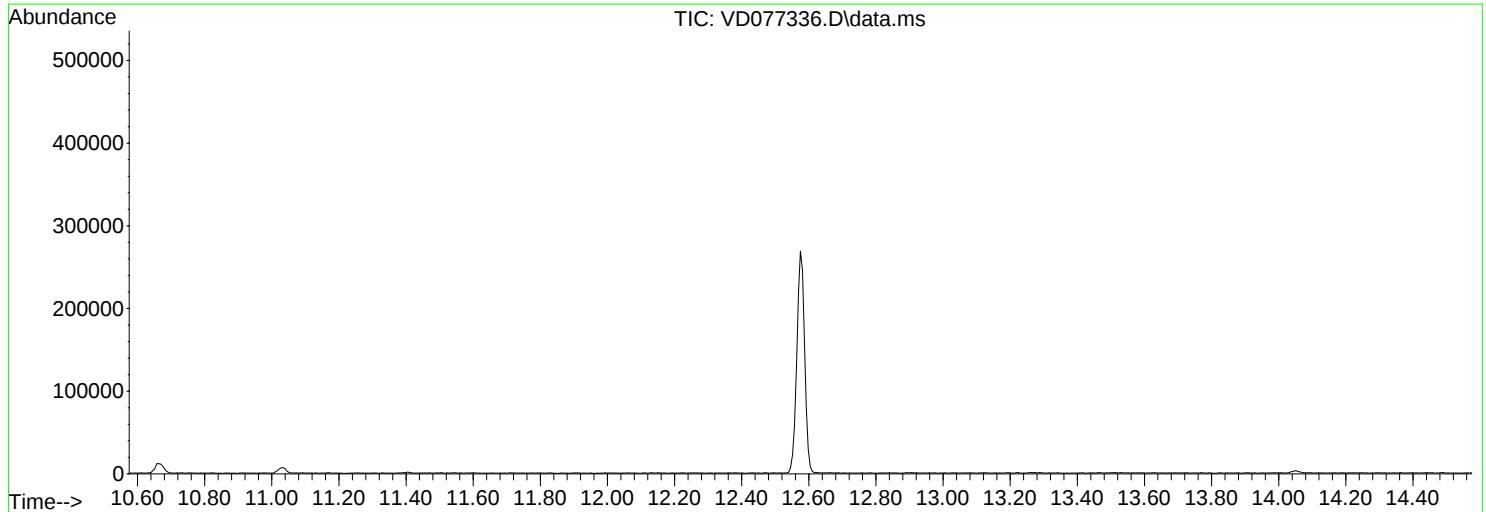

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1860

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.9	9108	PASS
75	95	30	60	55.4	24181	PASS
95	95	100	100	100.0	43621	PASS
96	95	5	9	6.8	2963	PASS
173	174	0.00	2	1.4	516	PASS
174	95	50	100	83.8	36555	PASS
175	174	5	9	7.2	2618	PASS
176	174	95	101	97.6	35693	PASS
177	176	5	9	6.5	2323	PASS