

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD101821\
 Data File : VD070743.D
 Acq On : 18 Oct 2021 21:29
 Operator : VA/SY
 Sample : M4248-01
 Misc : 5.00G/5.00ml/MSVOA_D/SoIL
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 CHVB-0513


Quant Time: Oct 19 06:43:17 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D101521S.M
 Quant Title : SW846 8260
 QLast Update : Mon Oct 18 08:32:03 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.979	168	311642	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.861	114	644420	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.638	117	512149	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.561	152	75097	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.326	65	258675	70.079	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	= 140.160%	
35) Dibromofluoromethane	7.914	113	228610	55.404	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	= 110.800%	
50) Toluene-d8	10.332	98	764044	48.304	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	= 96.600%	
62) 4-Bromofluorobenzene	12.620	95	180998	33.233	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	= 66.460%	
Target Compounds						
					Qvalue	
10) Methyl Iodide	4.303	142	324	3.398	ug/l #	62
11) Tert butyl alcohol	5.226	59	1050	5.081	ug/l #	52
16) Acetone	4.150	43	133709	150.186	ug/l #	88
17) Carbon Disulfide	4.403	76	13191	1.069	ug/l #	92
20) Methylene Chloride	4.967	84	44780	4.008	ug/l	92
23) Vinyl Acetate	6.303	43	71	16.339	ug/l #	69
25) 2-Butanone	7.214	43	19399	17.638	ug/l	93
31) Cyclohexane	7.973	56	9227	1.236	ug/l #	38
36) 1,1-Dichloropropene	7.979	75	28716	4.000	ug/l #	50
37) Ethyl Acetate	7.214	43	19399	6.522	ug/l #	65
38) Carbon Tetrachloride	7.979	117	32812	4.772	ug/l #	17
41) Methacrylonitrile	7.520	41	737	2.321	ug/l #	25
51) 4-Methyl-2-Pentanone	10.214	43	7453	2.492	ug/l #	86
52) Toluene	10.396	92	370523	30.101	ug/l	97
56) Ethyl methacrylate	10.638	69	1185	4.378	ug/l #	32
73) Isopropylbenzene	12.479	105	11021	2.060	ug/l	96
75) 1,1,2,2-Tetrachloroethane	12.720	83	68942	65.133	ug/l #	27
76) 1,2,3-Trichloropropane	12.620	75	93851	144.652	ug/l #	100
77) Bromobenzene	12.543	156	1306	1.078	ug/l #	4
80) 1,3,5-Trimethylbenzene	12.949	105	6074	1.343	ug/l	69
81) trans-1,4-Dichloro-2-b...	12.620	75	93851	316.832	ug/l #	17
83) tert-Butylbenzene	13.267	119	4710	1.260	ug/l #	16
84) 1,2,4-Trimethylbenzene	13.261	105	20154	4.481	ug/l	93
85) sec-Butylbenzene	13.390	105	23450	3.992	ug/l	95
86) p-Isopropyltoluene	13.502	119	110440	23.383	ug/l #	84
89) n-Butylbenzene	13.620	91	7814	1.639	ug/l	87
90) Hexachloroethane	14.049	117	1135	1.114	ug/l	76
92) 1,2-Dibromo-3-Chloropr...	14.514	75	630	3.732	ug/l	71
95) Naphthalene	15.379	128	10011	8.516	ug/l #	84
96) 1,2,3-Trichlorobenzene	15.602	180	19813	17.930	ug/l #	16

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Oct 19 06:43:17 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D101521S.M
Quant Title : SW846 8260
QLast Update : Mon Oct 18 08:32:03 2021
Response via : Initial Calibration




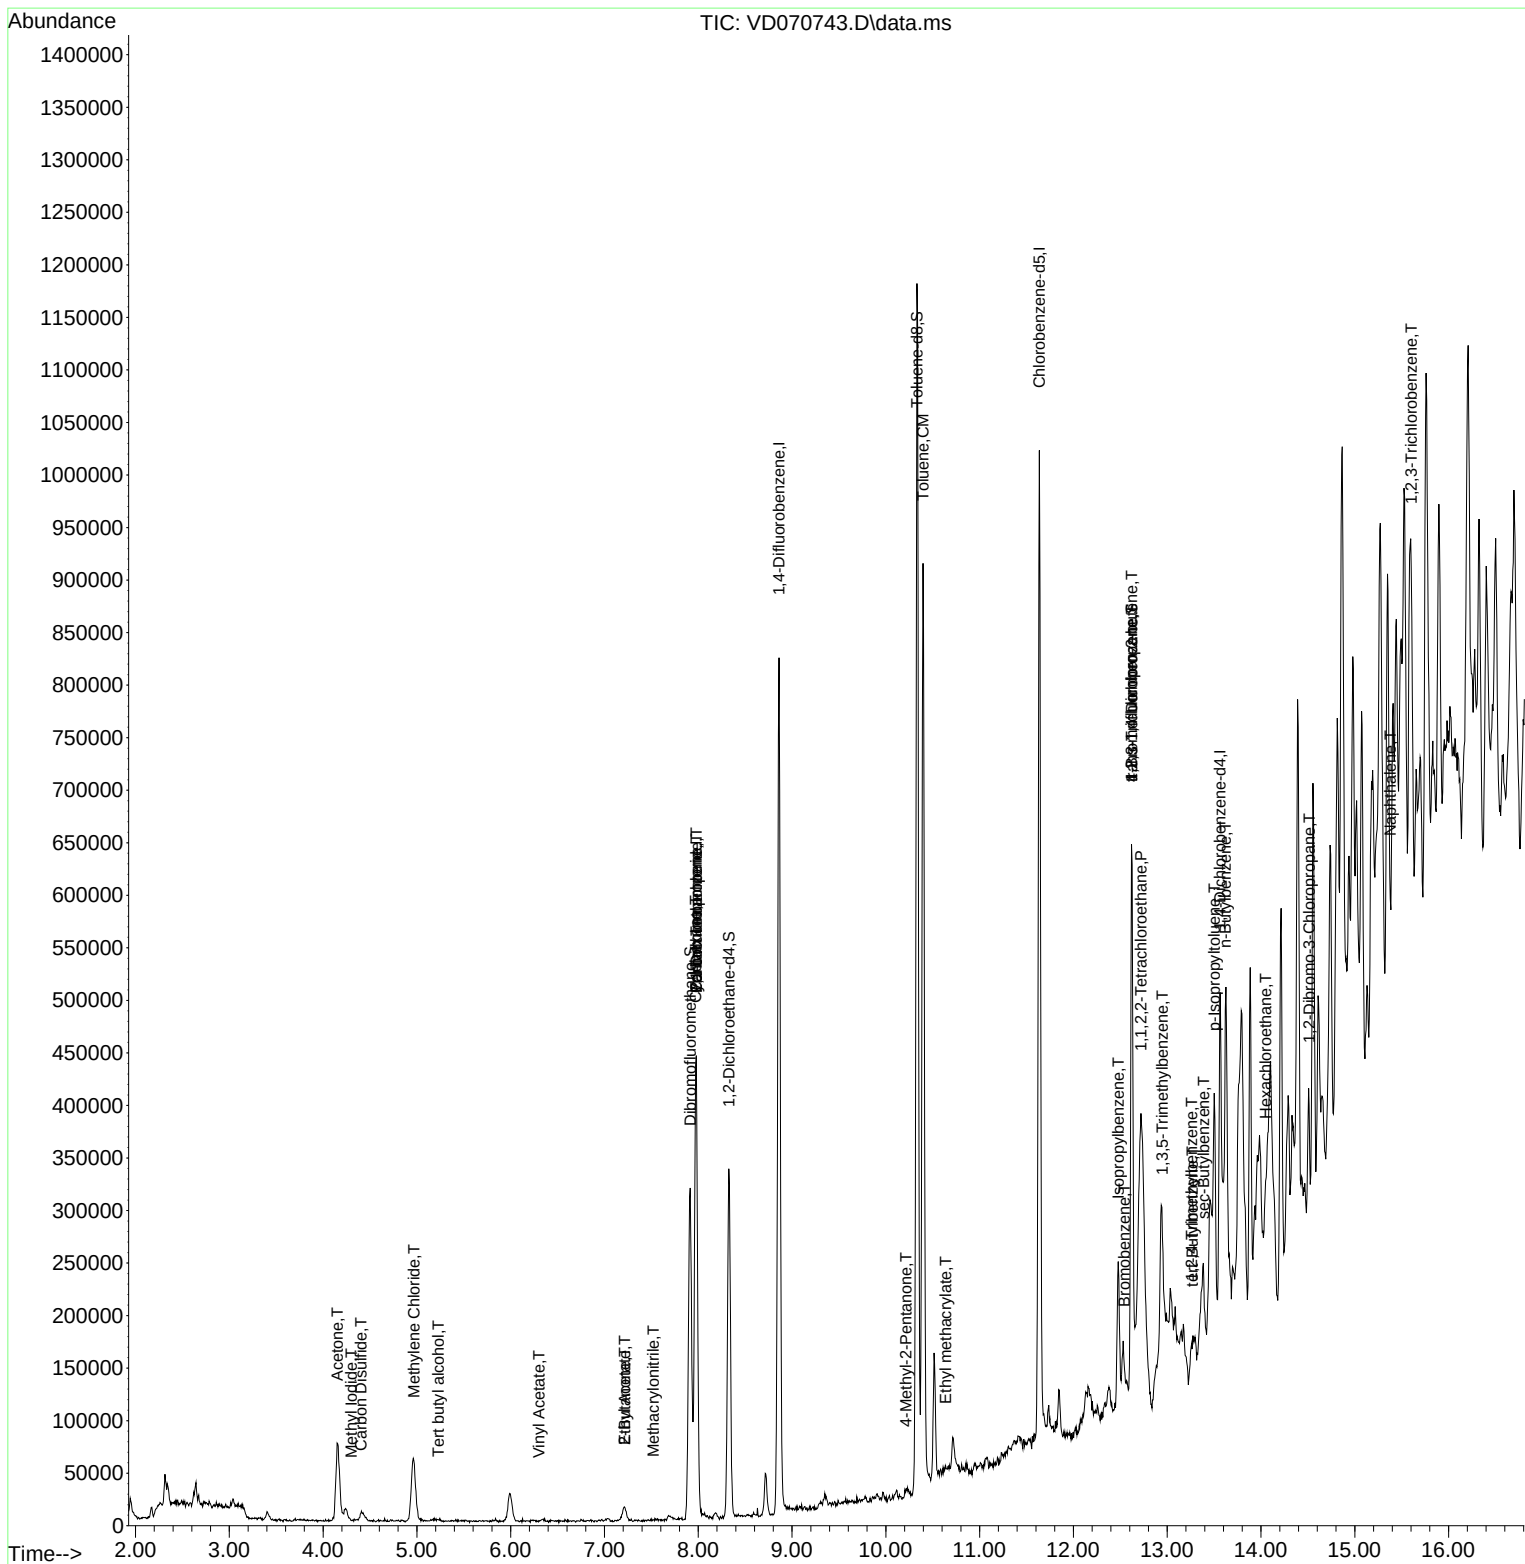


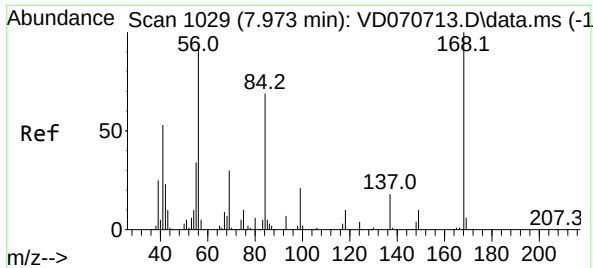

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.979 min Scan# 1030
Delta R.T. 0.006 min
Lab File: VD070743.D
Acq: 18 Oct 2021 21:29




Instrument :
MSVOA_D
ClientSampleId :
CHVB-0513


Tgt Ion:168 Resp: 311642
Ion Ratio Lower Upper
168 100
99 59.0 51.4 77.0

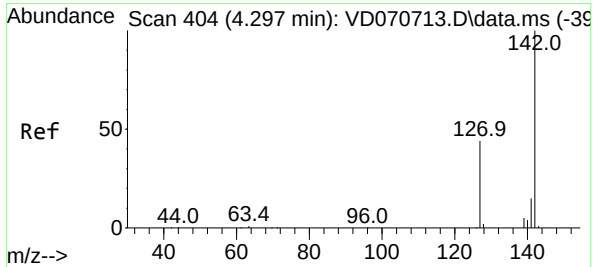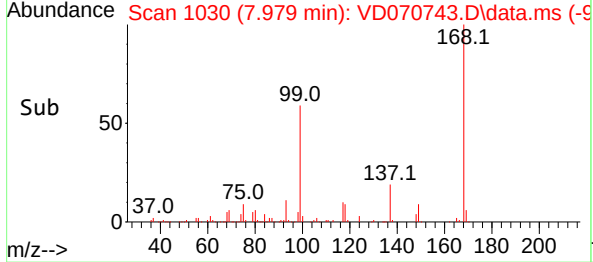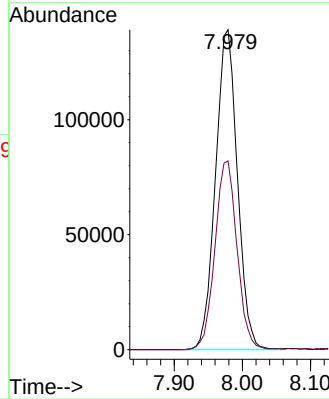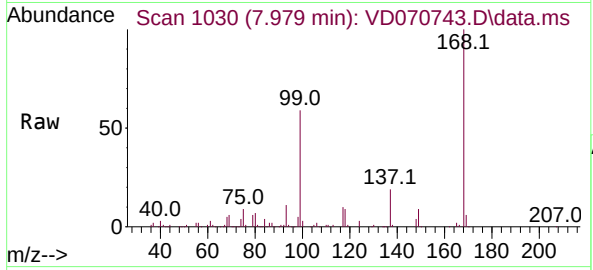

#10
Methyl Iodide
Concen: 3.398 ug/l
RT: 4.303 min Scan# 405
Delta R.T. 0.006 min
Lab File: VD070743.D
Acq: 18 Oct 2021 21:29

Tgt Ion:142 Resp: 324
Ion Ratio Lower Upper
142 100
127 21.3 37.5 56.3#
141 0.0 12.1 18.1#

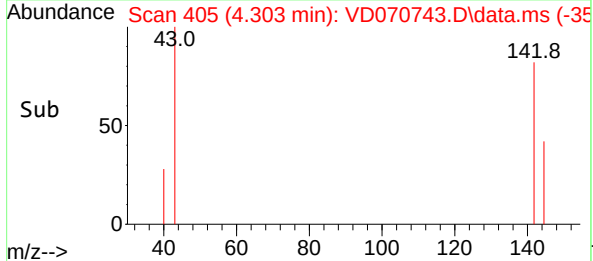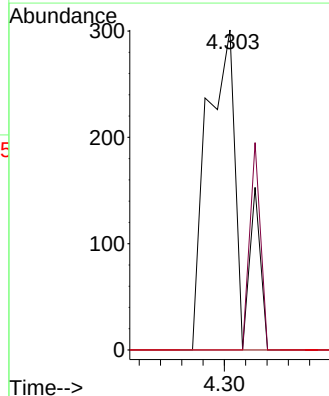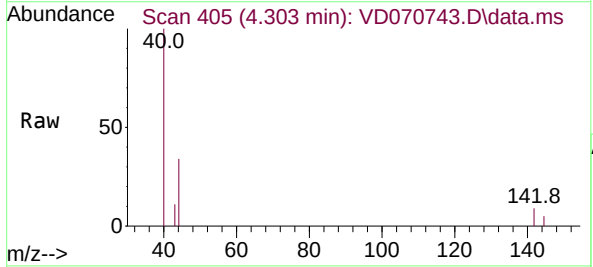







#11

Tert butyl alcohol
Concen: 5.081 ug/l
RT: 5.226 min Scan# 562
Delta R.T. 0.012 min
Lab File: VD070743.D
Acq: 18 Oct 2021 21:29

Instrument :
MSVOA_D
ClientSampleId :
CHVB-0513




Tgt Ion: 59 Resp: 1050
Ion Ratio Lower Upper
59 100
57 21.7 4.5 6.7#

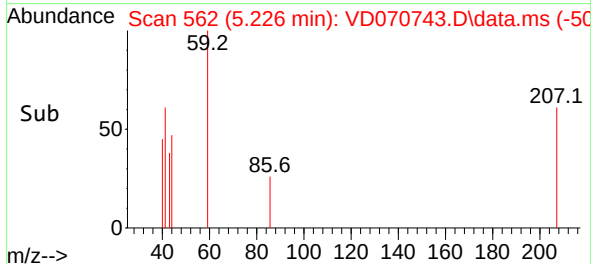


#16

Acetone
Concen: 150.186 ug/l
RT: 4.150 min Scan# 379
Delta R.T. -0.006 min
Lab File: VD070743.D
Acq: 18 Oct 2021 21:29

Tgt Ion: 43 Resp: 133709
Ion Ratio Lower Upper
43 100
58 28.0 28.2 42.2#


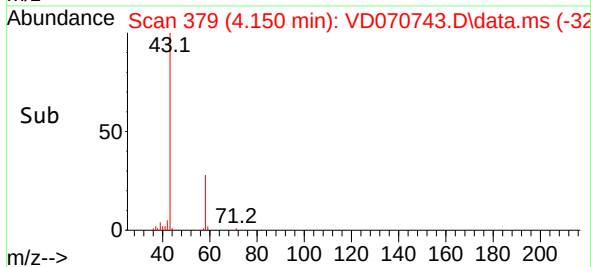

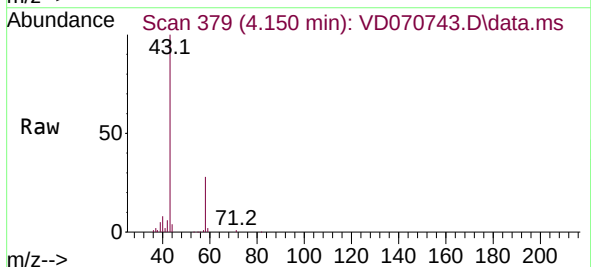




#17
Carbon Disulfide
Concen: 1.069 ug/l
RT: 4.403 min Scan# 422
Delta R.T. -0.006 min
Lab File: VD070743.D
Acq: 18 Oct 2021 21:29




Instrument :
MSVOA_D
ClientSampleId :
CHVB-0513


Tgt Ion: 76 Resp: 13191
Ion Ratio Lower Upper
76 100
78 12.1 7.4 11.2#

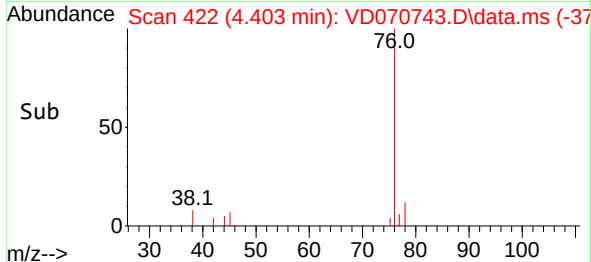

#20
Methylene Chloride
Concen: 4.008 ug/l
RT: 4.967 min Scan# 518
Delta R.T. 0.011 min
Lab File: VD070743.D
Acq: 18 Oct 2021 21:29

Tgt Ion: 84 Resp: 44780
Ion Ratio Lower Upper
84 100
49 125.6 91.4 137.2
51 37.4 26.7 40.1
86 61.4 50.8 76.2


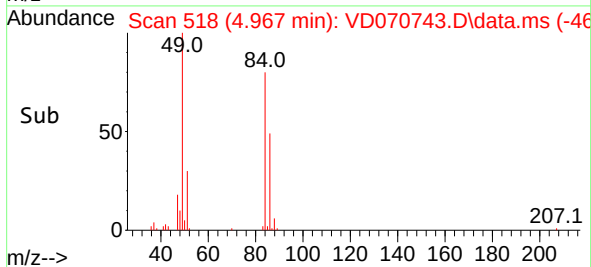

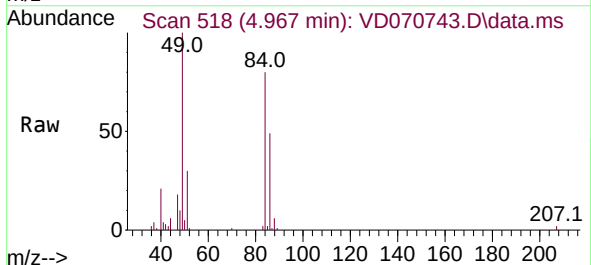




#23
 Vinyl Acetate
 Concen: 16.339 ug/l
 RT: 6.303 min Scan# 745
 Delta R.T. -0.000 min
 Lab File: VD070743.D
 Acq: 18 Oct 2021 21:29




Instrument :
 MSVOA_D
 ClientSampleId :
 CHVB-0513


Tgt Ion: 43 Resp: 71
 Ion Ratio Lower Upper
 43 100
 86 0.0 9.8 14.6#

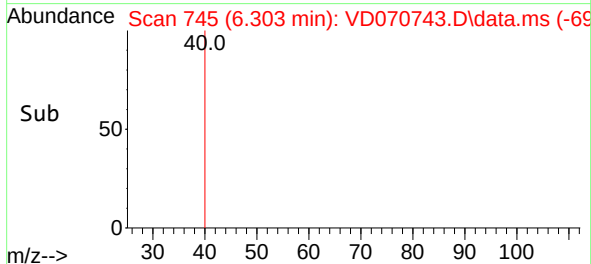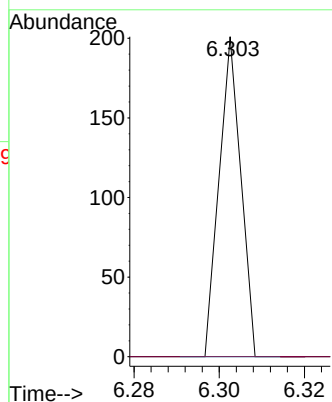

#25
 2-Butanone
 Concen: 17.638 ug/l
 RT: 7.214 min Scan# 900
 Delta R.T. 0.006 min
 Lab File: VD070743.D
 Acq: 18 Oct 2021 21:29

Tgt Ion: 43 Resp: 19399
 Ion Ratio Lower Upper
 43 100
 72 27.8 25.2 37.8




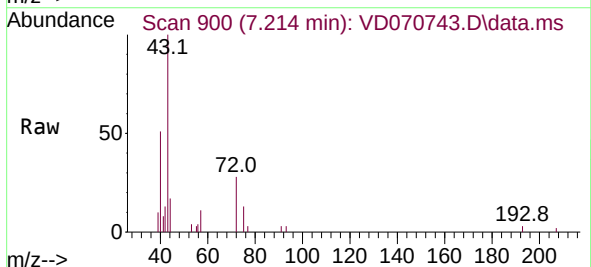


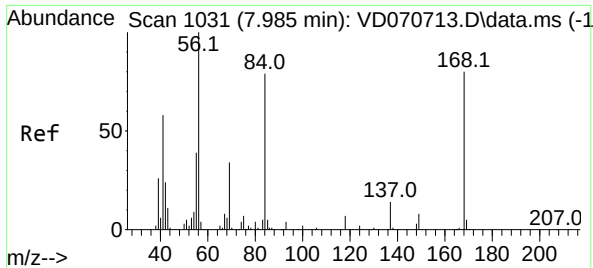

#31
Cyclohexane
Concen: 1.236 ug/l
RT: 7.973 min Scan# 1029
Delta R.T. -0.012 min
Lab File: VD070743.D
Acq: 18 Oct 2021 21:29




Instrument :
MSVOA_D
ClientSampleId :
CHVB-0513


Tgt Ion: 56 Resp: 9227
Ion Ratio Lower Upper
56 100
69 162.5 27.4 41.2#
84 89.9 73.6 110.4

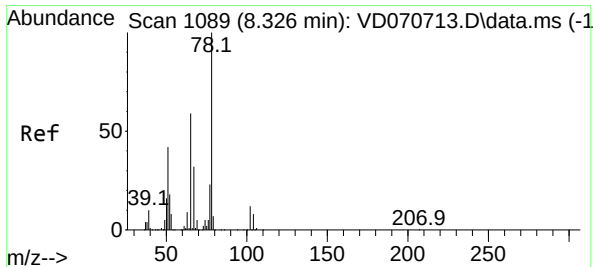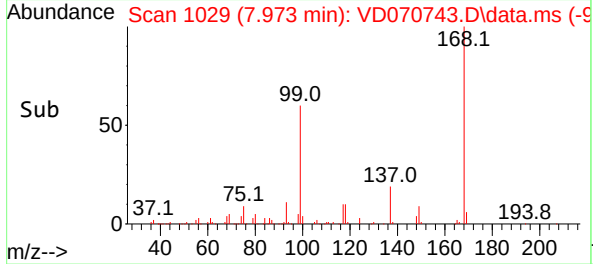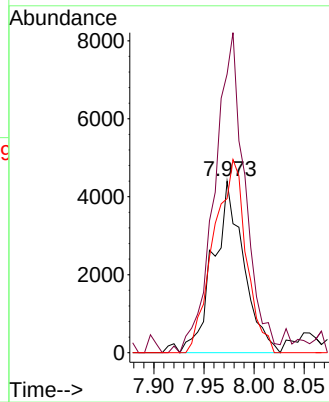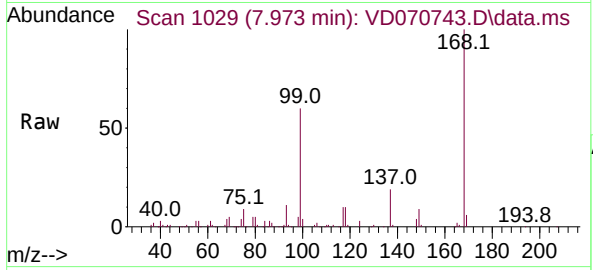

#33
1,2-Dichloroethane-d4
Concen: 70.079 ug/l
RT: 8.326 min Scan# 1089
Delta R.T. -0.000 min
Lab File: VD070743.D
Acq: 18 Oct 2021 21:29

Tgt Ion: 65 Resp: 258675
Ion Ratio Lower Upper
65 100
67 53.7 0.0 110.2

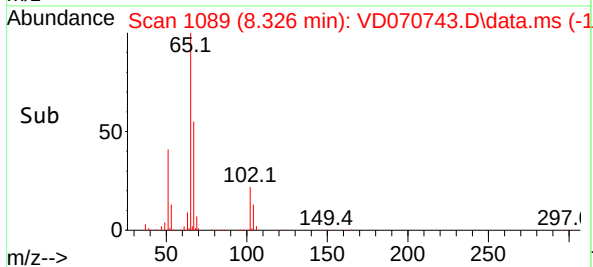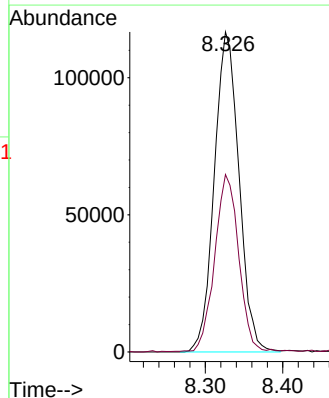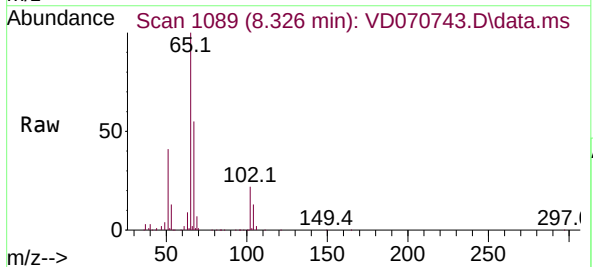




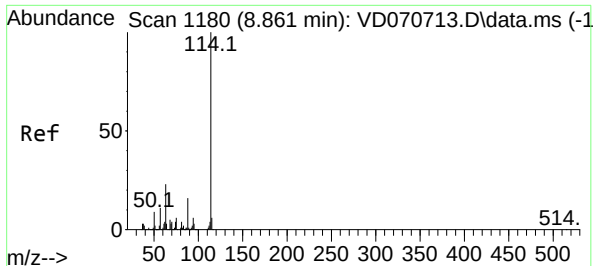


#34

1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.861 min Scan# 1180
Delta R.T. -0.000 min
Lab File: VD070743.D
Acq: 18 Oct 2021 21:29

Instrument :
MSVOA_D
ClientSampleId :
CHVB-0513




Tgt Ion:114	Resp: 644420
Ion Ratio	Lower Upper
114 100	
63 23.2	0.0 41.8
88 16.3	0.0 32.6

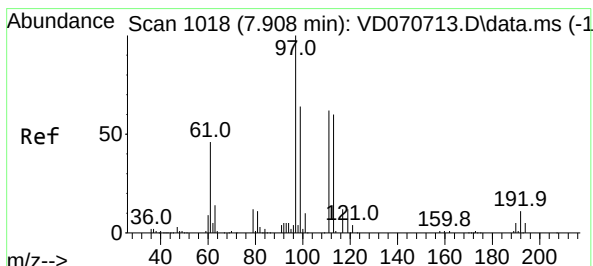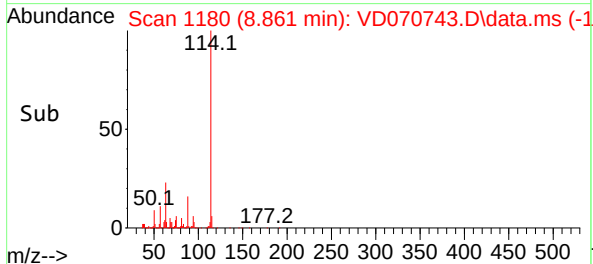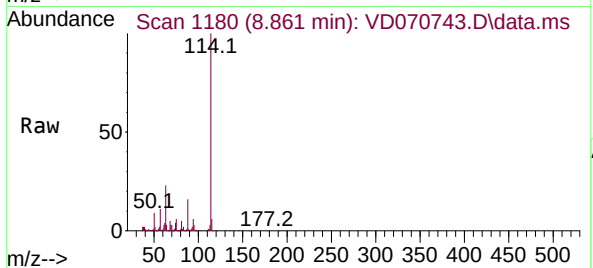


#35

Dibromofluoromethane
Concen: 55.404 ug/l
RT: 7.914 min Scan# 1019
Delta R.T. 0.006 min
Lab File: VD070743.D
Acq: 18 Oct 2021 21:29

Tgt Ion:113	Resp: 228610
Ion Ratio	Lower Upper
113 100	
111 102.8	83.1 124.7
192 18.8	12.7 19.1


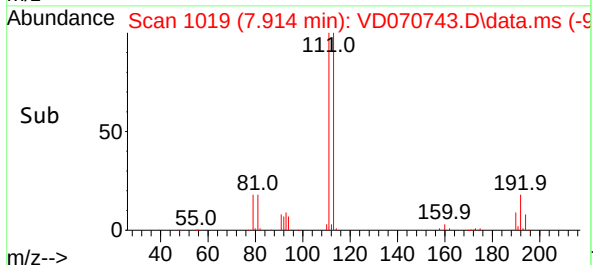
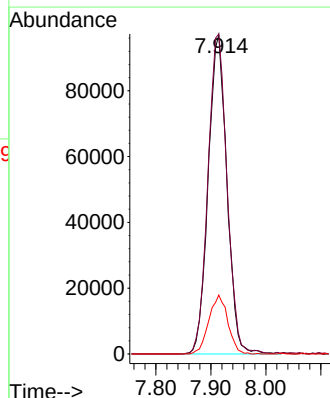
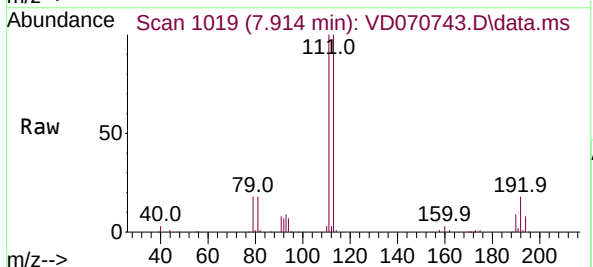


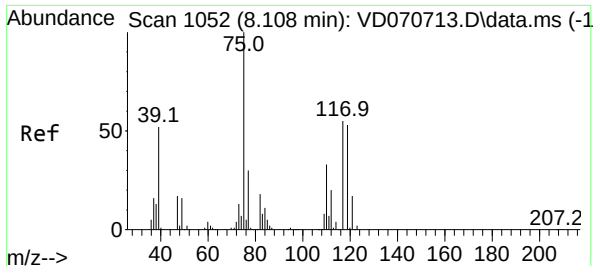

#36
1,1-Dichloropropene
Concen: 4.000 ug/l
RT: 7.979 min Scan# 1030
Delta R.T. -0.129 min
Lab File: VD070743.D
Acq: 18 Oct 2021 21:29




Instrument :
MSVOA_D
ClientSampleId :
CHVB-0513


Tgt Ion: 75 Resp: 28716
Ion Ratio Lower Upper
75 100
110 7.4 17.2 51.6#
77 1.0 24.2 36.4#

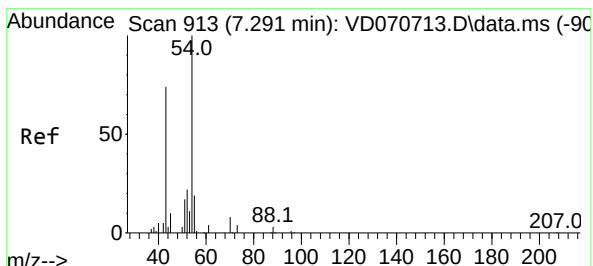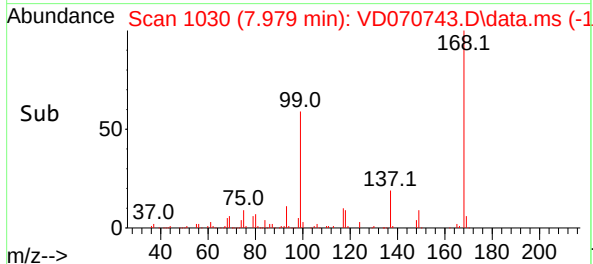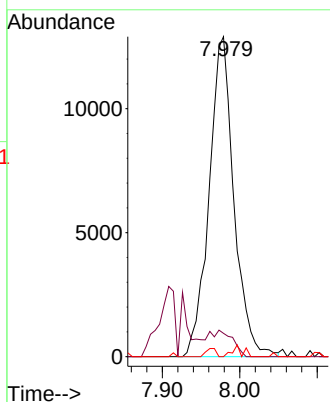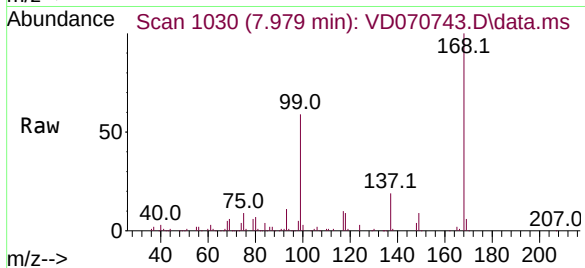

#37
Ethyl Acetate
Concen: 6.522 ug/l
RT: 7.214 min Scan# 900
Delta R.T. -0.077 min
Lab File: VD070743.D
Acq: 18 Oct 2021 21:29

Tgt Ion: 43 Resp: 19399
Ion Ratio Lower Upper
43 100
61 0.4 12.9 19.3#
70 0.0 9.9 14.9#

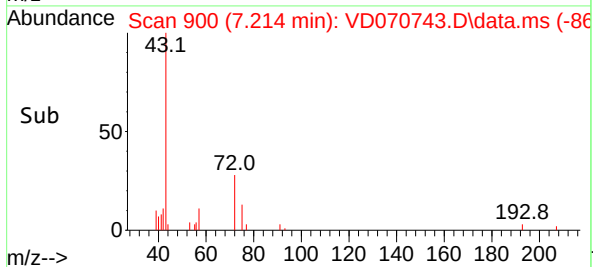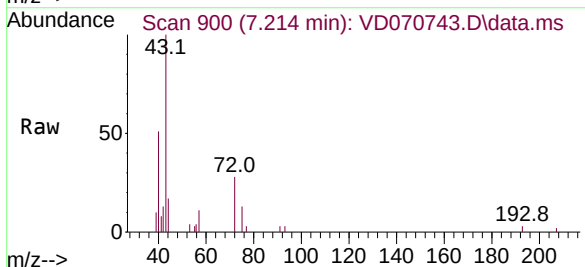







#38

Carbon Tetrachloride
Concen: 4.772 ug/l
RT: 7.979 min Scan# 1030
Delta R.T. -0.112 min
Lab File: VD070743.D
Acq: 18 Oct 2021 21:29

Instrument :
MSVOA_D
ClientSampleId :
CHVB-0513




Tgt Ion:117 Resp: 32812
Ion Ratio Lower Upper
117 100
119 6.6 77.4 116.0#
121 0.0 25.4 38.0#

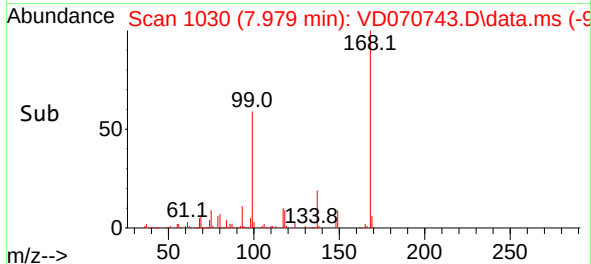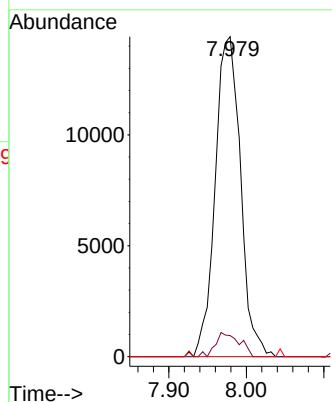


#41

Methacrylonitrile
Concen: 2.321 ug/l
RT: 7.520 min Scan# 952
Delta R.T. 0.006 min
Lab File: VD070743.D
Acq: 18 Oct 2021 21:29

Tgt Ion: 41 Resp: 737
Ion Ratio Lower Upper
41 100
39 7.5 45.2 67.8#
67 12.3 75.8 113.6#
52 0.0 27.8 41.8#


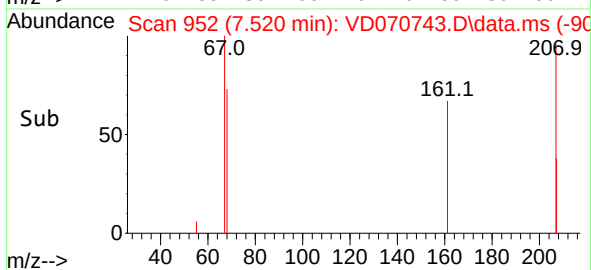

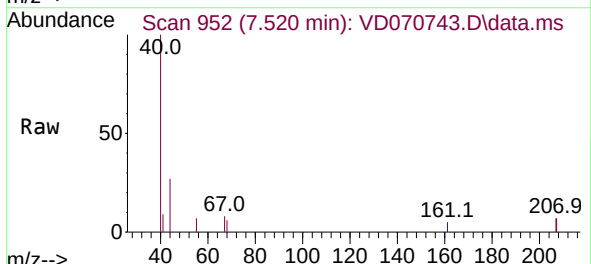




#50
Toluene-d8
Concen: 48.304 ug/l
RT: 10.332 min Scan# 1430
Delta R.T. -0.000 min
Lab File: VD070743.D
Acq: 18 Oct 2021 21:29




Instrument :
MSVOA_D
ClientSampleId :
CHVB-0513


Tgt Ion: 98 Resp: 764044
Ion Ratio Lower Upper
98 100
100 65.3 52.2 78.4

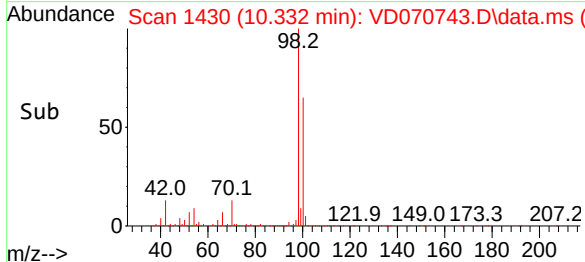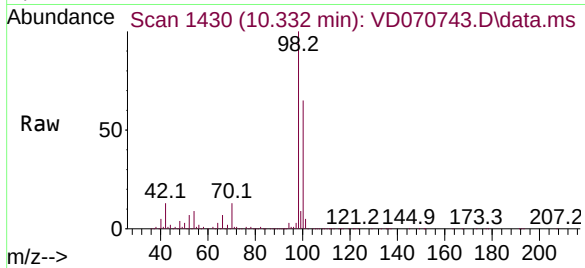

#51
4-Methyl-2-Pentanone
Concen: 2.492 ug/l
RT: 10.214 min Scan# 1410
Delta R.T. -0.006 min
Lab File: VD070743.D
Acq: 18 Oct 2021 21:29

Tgt Ion: 43 Resp: 7453
Ion Ratio Lower Upper
43 100
58 34.8 35.0 52.6#


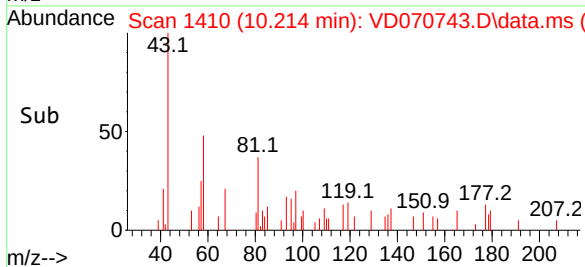

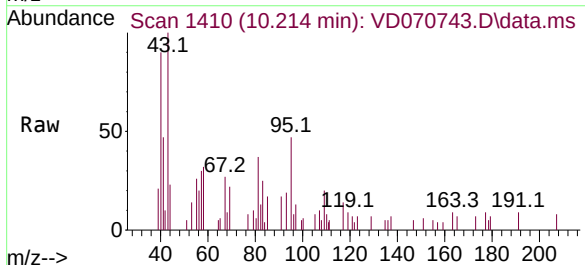




#52
Toluene
Concen: 30.101 ug/l
RT: 10.396 min Scan# 1441
Delta R.T. -0.000 min
Lab File: VD070743.D
Acq: 18 Oct 2021 21:29




Instrument :
MSVOA_D
ClientSampleId :
CHVB-0513


Tgt Ion: 92 Resp: 370523
Ion Ratio Lower Upper
92 100
91 174.1 136.3 204.5

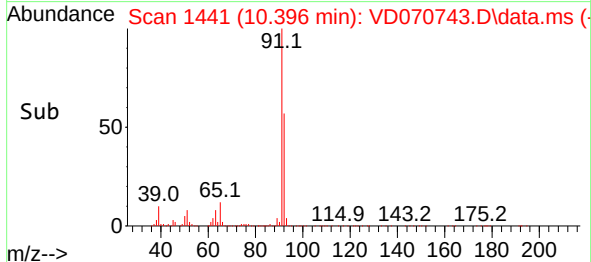

#56
Ethyl methacrylate
Concen: 4.378 ug/l
RT: 10.638 min Scan# 1482
Delta R.T. -0.017 min
Lab File: VD070743.D
Acq: 18 Oct 2021 21:29

Tgt Ion: 69 Resp: 1185
Ion Ratio Lower Upper
69 100
41 0.0 44.7 67.1#
39 0.0 19.5 29.3#


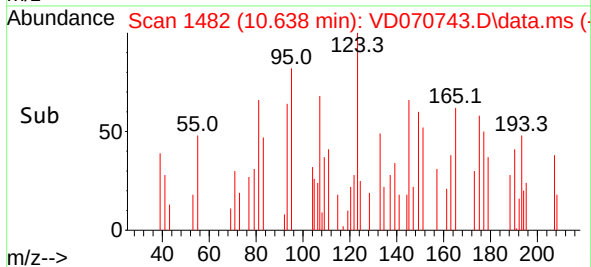

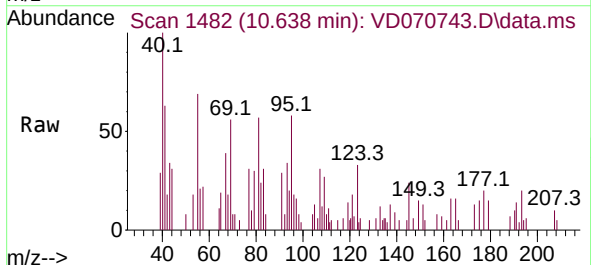


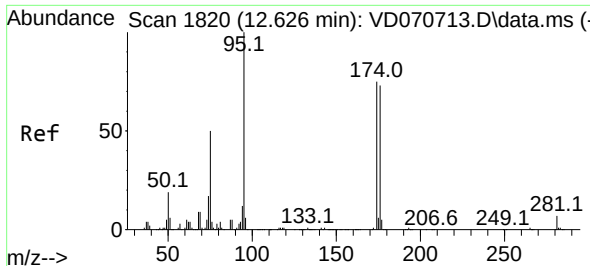

#62
4-Bromofluorobenzene
Concen: 33.233 ug/l
RT: 12.620 min Scan# 1819
Delta R.T. -0.006 min
Lab File: VD070743.D
Acq: 18 Oct 2021 21:29




Instrument :
MSVOA_D
ClientSampleId :
CHVB-0513


Tgt Ion: 95 Resp: 180998
Ion Ratio Lower Upper
95 100
174 71.8 0.0 138.0
176 68.5 0.0 135.6

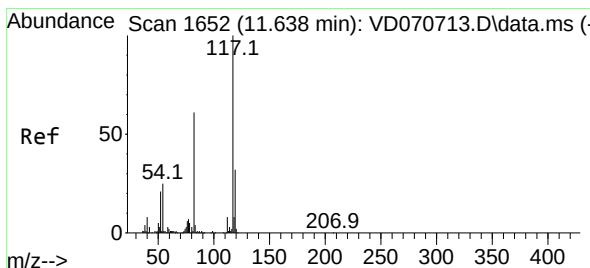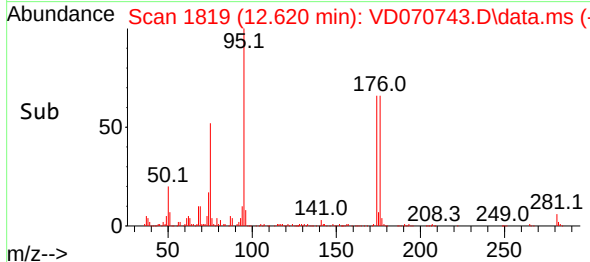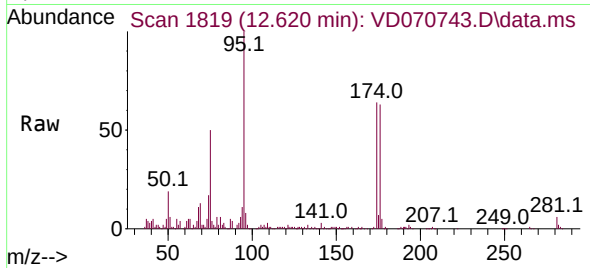

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.638 min Scan# 1652
Delta R.T. -0.000 min
Lab File: VD070743.D
Acq: 18 Oct 2021 21:29

Tgt Ion: 117 Resp: 512149
Ion Ratio Lower Upper
117 100
82 62.1 45.4 68.2
119 32.6 24.7 37.1


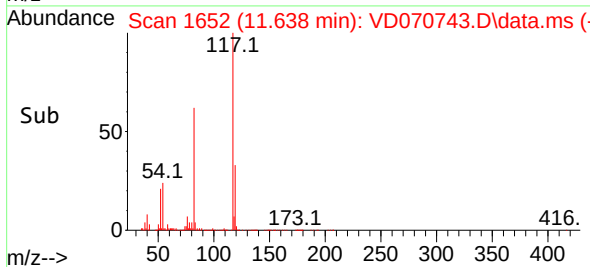

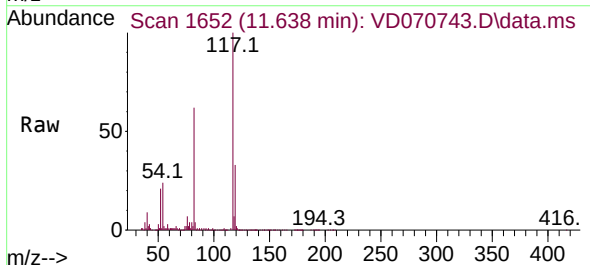




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.561 min Scan# 1799
Delta R.T. -0.000 min
Lab File: VD070743.D
Acq: 18 Oct 2021 21:29




Instrument :
MSVOA_D
ClientSampleId :
CHVB-0513


Tgt Ion:152 Resp: 75097
Ion Ratio Lower Upper
152 100
115 61.0 31.9 95.7
150 148.8 0.0 350.0

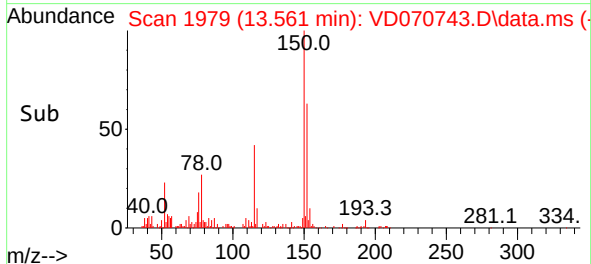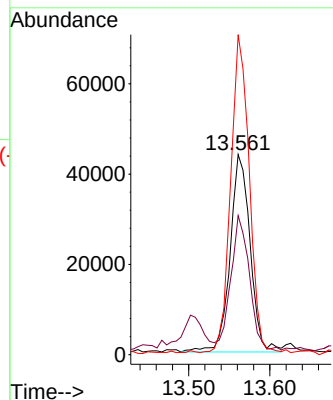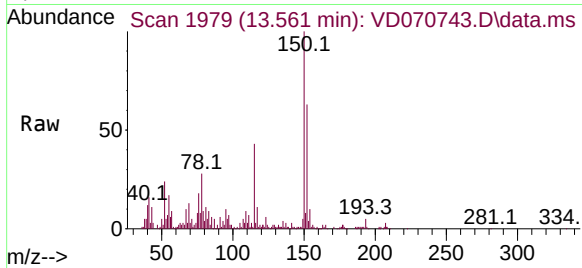

#73
Isopropylbenzene
Concen: 2.060 ug/l
RT: 12.479 min Scan# 1795
Delta R.T. 0.006 min
Lab File: VD070743.D
Acq: 18 Oct 2021 21:29

Tgt Ion:105 Resp: 11021
Ion Ratio Lower Upper
105 100
120 27.3 12.8 38.3


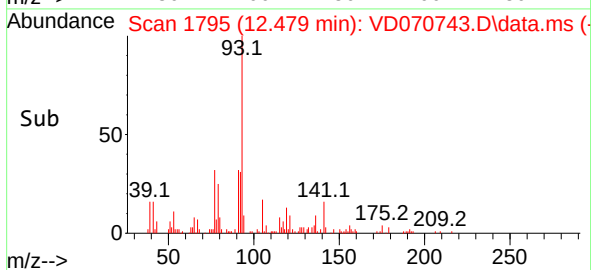
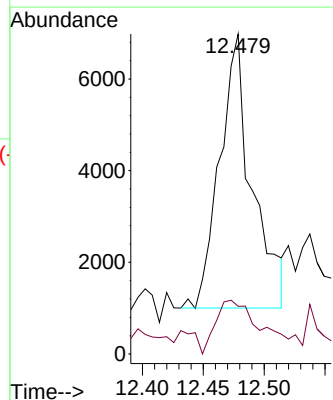
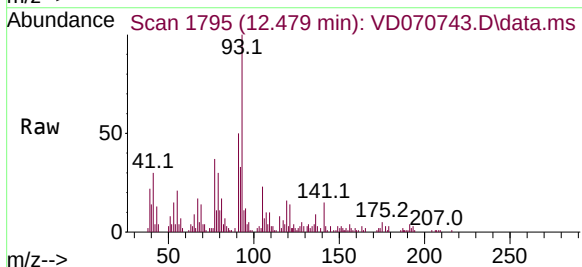


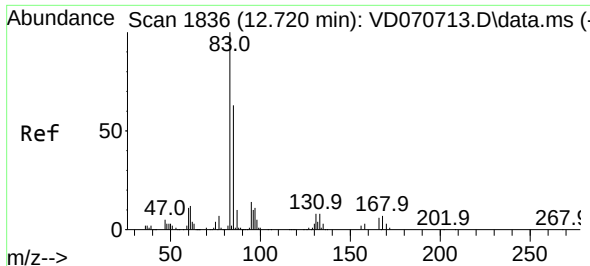

#75
 1,1,2,2-Tetrachloroethane
 Concen: 65.133 ug/l
 RT: 12.720 min Scan# 1836
 Delta R.T. -0.000 min
 Lab File: VD070743.D
 Acq: 18 Oct 2021 21:29




Instrument :
 MSVOA_D
 ClientSampleId :
 CHVB-0513


Tgt Ion: 83 Resp: 68942
 Ion Ratio Lower Upper
 83 100
 131 2.7 4.9 14.7#
 85 0.0 31.9 95.7#

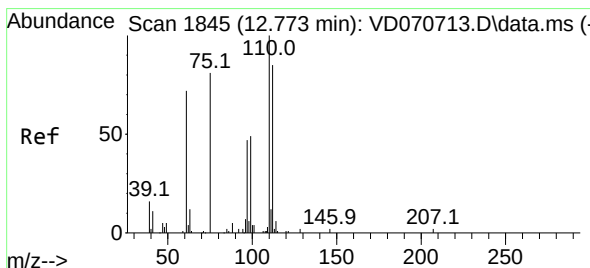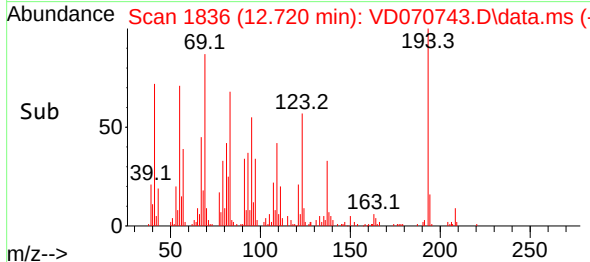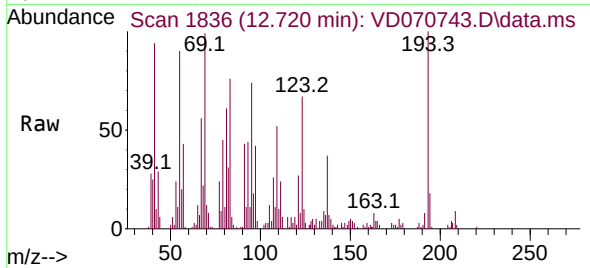

#76
 1,2,3-Trichloropropane
 Concen: 144.652 ug/l
 RT: 12.620 min Scan# 1819
 Delta R.T. -0.153 min
 Lab File: VD070743.D
 Acq: 18 Oct 2021 21:29

Tgt Ion: 75 Resp: 93851
 Ion Ratio Lower Upper
 75 100
 77 2.1 0.0 0.0#


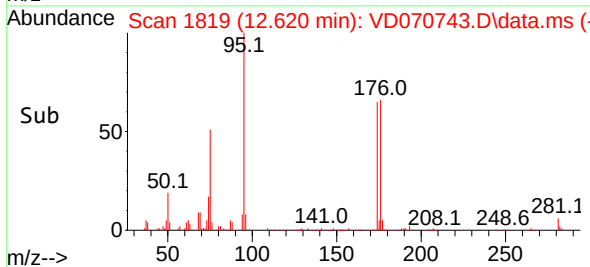

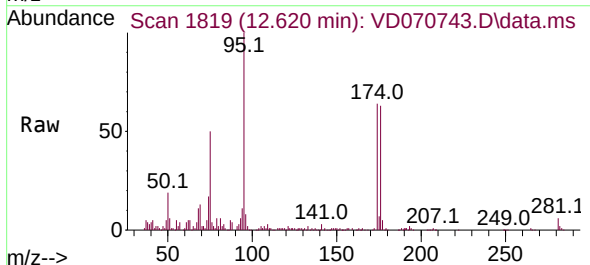




#77
Bromobenzene
Concen: 1.078 ug/l
RT: 12.543 min Scan# 1806
Delta R.T. -0.206 min
Lab File: VD070743.D
Acq: 18 Oct 2021 21:29




Instrument :
MSVOA_D
ClientSampleId :
CHVB-0513


Tgt Ion:156 Resp: 1306
Ion Ratio Lower Upper
156 100
77 62.6 105.7 317.1#
158 0.0 48.9 146.6#

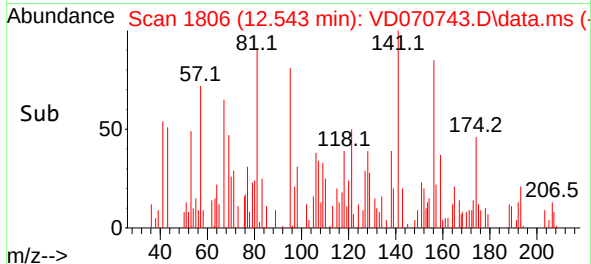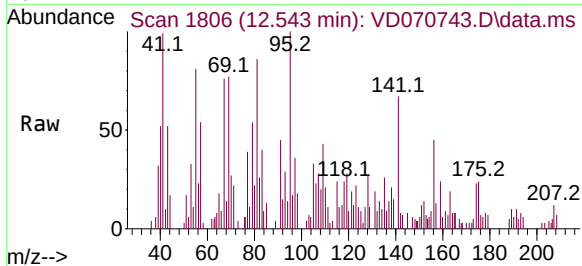

#80
1,3,5-Trimethylbenzene
Concen: 1.343 ug/l
RT: 12.949 min Scan# 1875
Delta R.T. -0.000 min
Lab File: VD070743.D
Acq: 18 Oct 2021 21:29

Tgt Ion:105 Resp: 6074
Ion Ratio Lower Upper
105 100
120 69.9 24.4 73.2


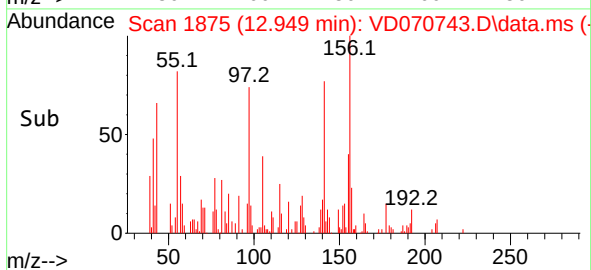

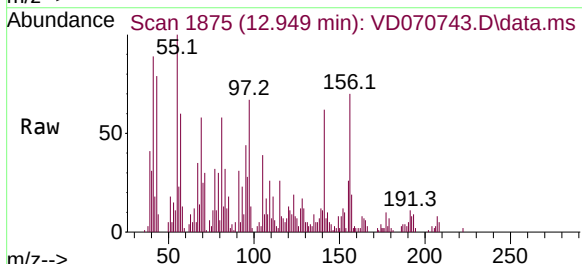




#81
trans-1,4-Dichloro-2-butene
Concen: 316.832 ug/l
RT: 12.620 min Scan# 1819
Delta R.T. 0.100 min
Lab File: VD070743.D
Acq: 18 Oct 2021 21:29




Instrument :
MSVOA_D
ClientSampleId :
CHVB-0513


Tgt Ion: 75 Resp: 93851
Ion Ratio Lower Upper
75 100
53 0.0 64.5 96.7#
89 0.3 35.3 52.9#

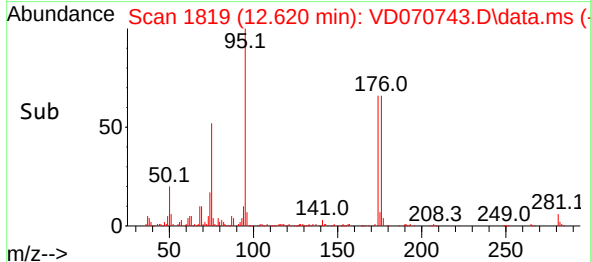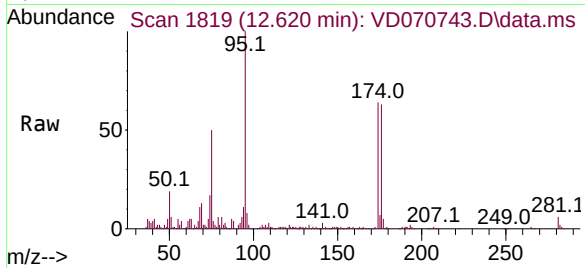

#83
tert-Butylbenzene
Concen: 1.260 ug/l
RT: 13.267 min Scan# 1929
Delta R.T. 0.053 min
Lab File: VD070743.D
Acq: 18 Oct 2021 21:29

Tgt Ion: 119 Resp: 4710
Ion Ratio Lower Upper
119 100
91 153.7 33.1 99.3#
134 17.0 13.2 39.5


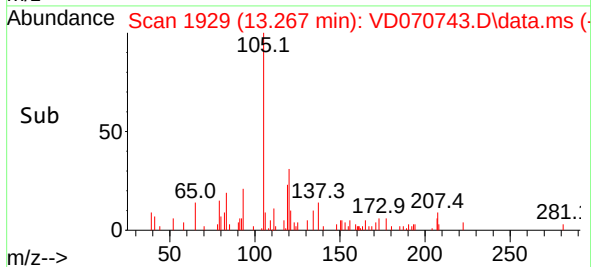

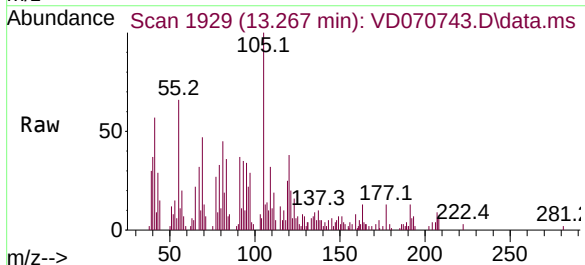




#84
1,2,4-Trimethylbenzene
Concen: 4.481 ug/l
RT: 13.261 min Scan# 1928
Delta R.T. 0.006 min
Lab File: VD070743.D
Acq: 18 Oct 2021 21:29




Instrument :
MSVOA_D
ClientSampleId :
CHVB-0513


Tgt Ion:105 Resp: 20154
Ion Ratio Lower Upper
105 100
120 48.4 21.9 65.8

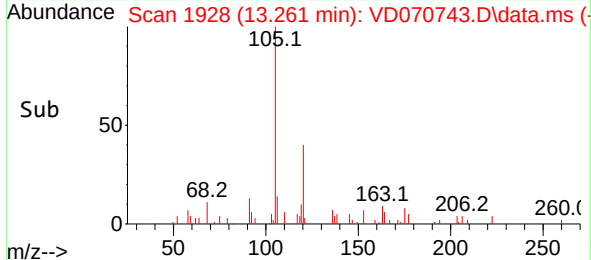

#85
sec-Butylbenzene
Concen: 3.992 ug/l
RT: 13.390 min Scan# 1950
Delta R.T. -0.000 min
Lab File: VD070743.D
Acq: 18 Oct 2021 21:29

Tgt Ion:105 Resp: 23450
Ion Ratio Lower Upper
105 100
134 21.0 9.3 28.0


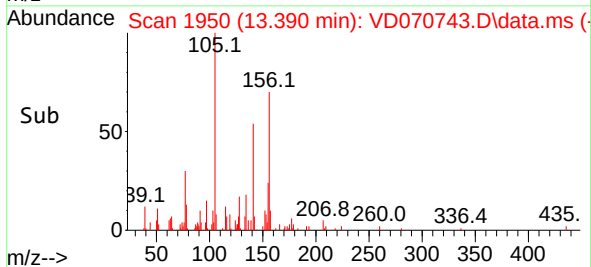

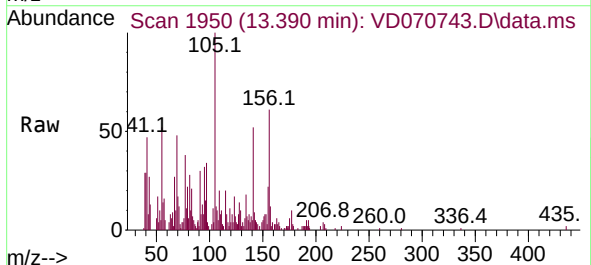


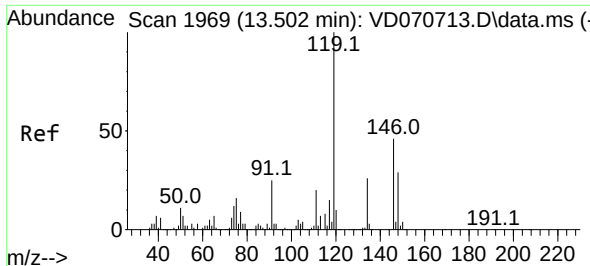

#86
p-Isopropyltoluene
Concen: 23.383 ug/l
RT: 13.502 min Scan# 1969
Delta R.T. -0.000 min
Lab File: VD070743.D
Acq: 18 Oct 2021 21:29




Instrument :
MSVOA_D
ClientSampleId :
CHVB-0513


Tgt Ion:119 Resp: 110440
Ion Ratio Lower Upper
119 100
134 25.5 12.5 37.5
91 39.4 11.9 35.5#

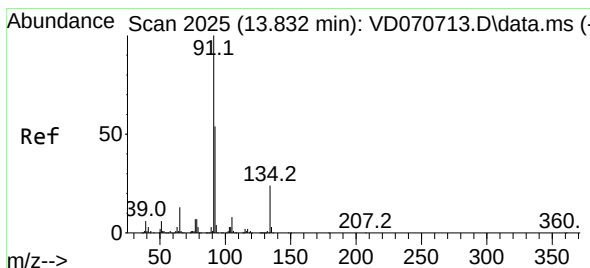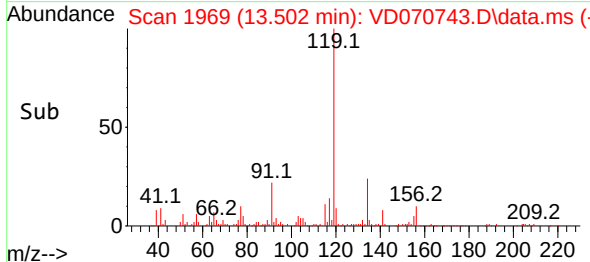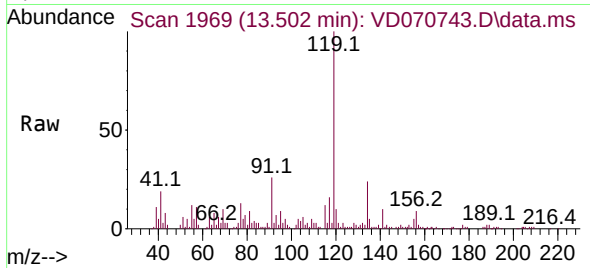

#89
n-Butylbenzene
Concen: 1.639 ug/l
RT: 13.620 min Scan# 1989
Delta R.T. -0.212 min
Lab File: VD070743.D
Acq: 18 Oct 2021 21:29

Tgt Ion: 91 Resp: 7814
Ion Ratio Lower Upper
91 100
92 59.8 26.8 80.4
134 13.8 12.2 36.4


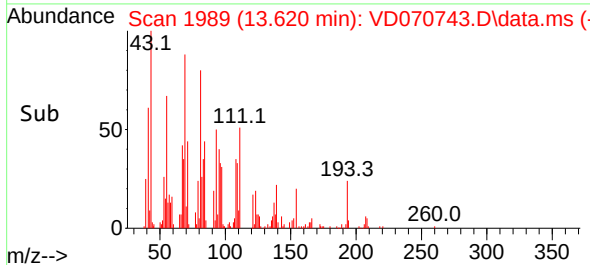

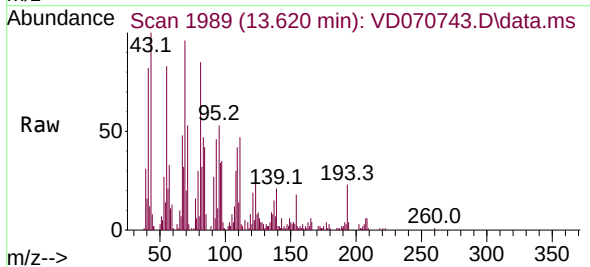


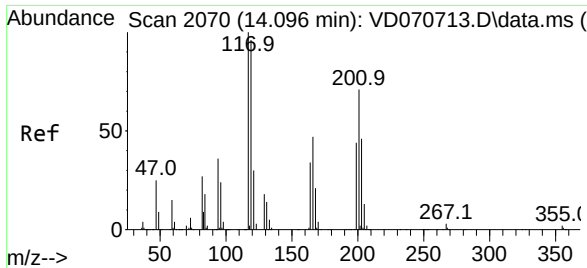

#90
Hexachloroethane
Concen: 1.114 ug/l
RT: 14.049 min Scan# 2062
Delta R.T. -0.047 min
Lab File: VD070743.D
Acq: 18 Oct 2021 21:29




Instrument :
MSVOA_D
ClientSampleId :
CHVB-0513


Tgt Ion:117 Resp: 1135
Ion Ratio Lower Upper
117 100
201 45.0 31.9 95.9

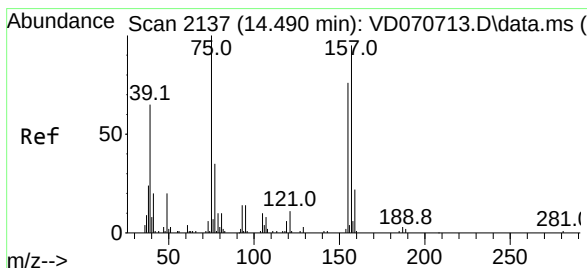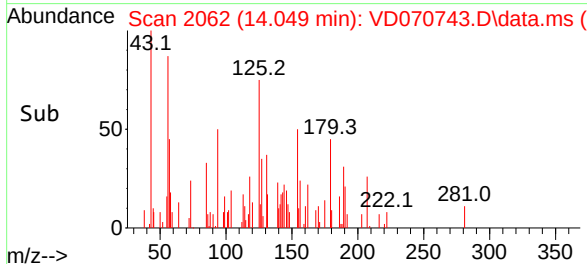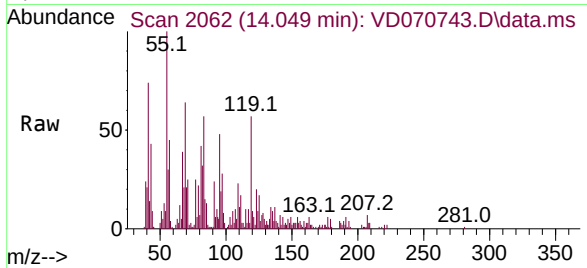

#92
1,2-Dibromo-3-Chloropropane
Concen: 3.732 ug/l
RT: 14.514 min Scan# 2141
Delta R.T. 0.024 min
Lab File: VD070743.D
Acq: 18 Oct 2021 21:29

Tgt Ion: 75 Resp: 630
Ion Ratio Lower Upper
75 100
155 92.5 38.1 114.5
157 130.8 47.6 142.9


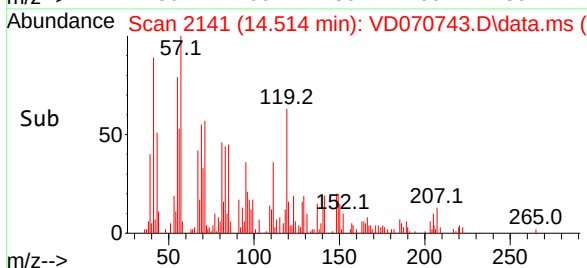

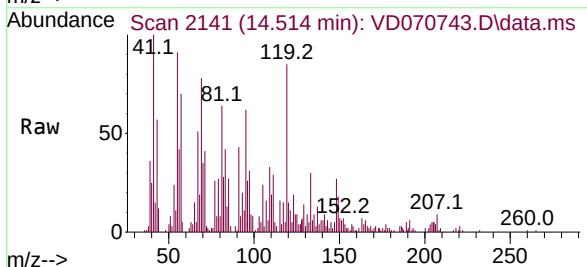




#95
Naphthalene
Concen: 8.516 ug/l
RT: 15.379 min Scan# 2288
Delta R.T. -0.005 min
Lab File: VD070743.D
Acq: 18 Oct 2021 21:29

Instrument :
MSVOA_D
ClientSampleId :
CHVB-0513

Tgt Ion:128 Resp: 10011
Ion Ratio Lower Upper
128 100
127 15.8 10.9 16.3
129 0.0 8.6 12.8#

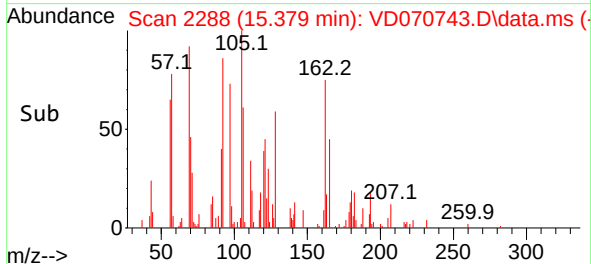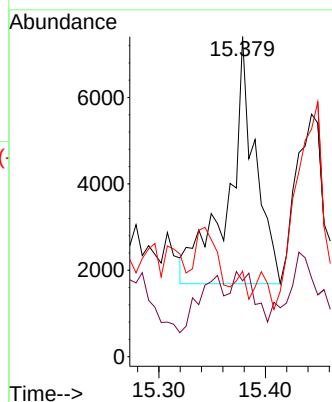

#96
1,2,3-Trichlorobenzene
Concen: 17.930 ug/l
RT: 15.602 min Scan# 2326
Delta R.T. 0.024 min
Lab File: VD070743.D
Acq: 18 Oct 2021 21:29

Tgt Ion:180 Resp: 19813
Ion Ratio Lower Upper
180 100
182 3.9 46.2 138.5#
145 0.0 17.1 51.3#

