

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD101921\
 Data File : VD070756.D
 Acq On : 19 Oct 2021 14:05
 Operator : VA/SY
 Sample : M4252-07RE
 Misc : 6.13G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 MH-CA-(1)RE

Quant Time: Oct 20 04:40:35 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D101521S.M
 Quant Title : SW846 8260
 QLast Update : Mon Oct 18 08:32:03 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.979	168	419958	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.861	114	810875	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.638	117	787174	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.561	152	326214	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.326	65	317087	63.75	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	127.50%
35) Dibromofluoromethane	7.908	113	286156	55.11	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	110.22%
50) Toluene-d8	10.338	98	1075274	54.03	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	108.06%
62) 4-Bromofluorobenzene	12.620	95	336816	49.15	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	98.30%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD101921\
Data File : VD070756.D
Acq On : 19 Oct 2021 14:05
Operator : VA/SY
Sample : M4252-07RE
Misc : 6.13G/5.00ml/MSVOA_D/SOIL
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
MH-CA-(1)RE

Quant Time: Oct 20 04:40:35 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D101521S.M
Quant Title : SW846 8260
QLast Update : Mon Oct 18 08:32:03 2021
Response via : Initial Calibration




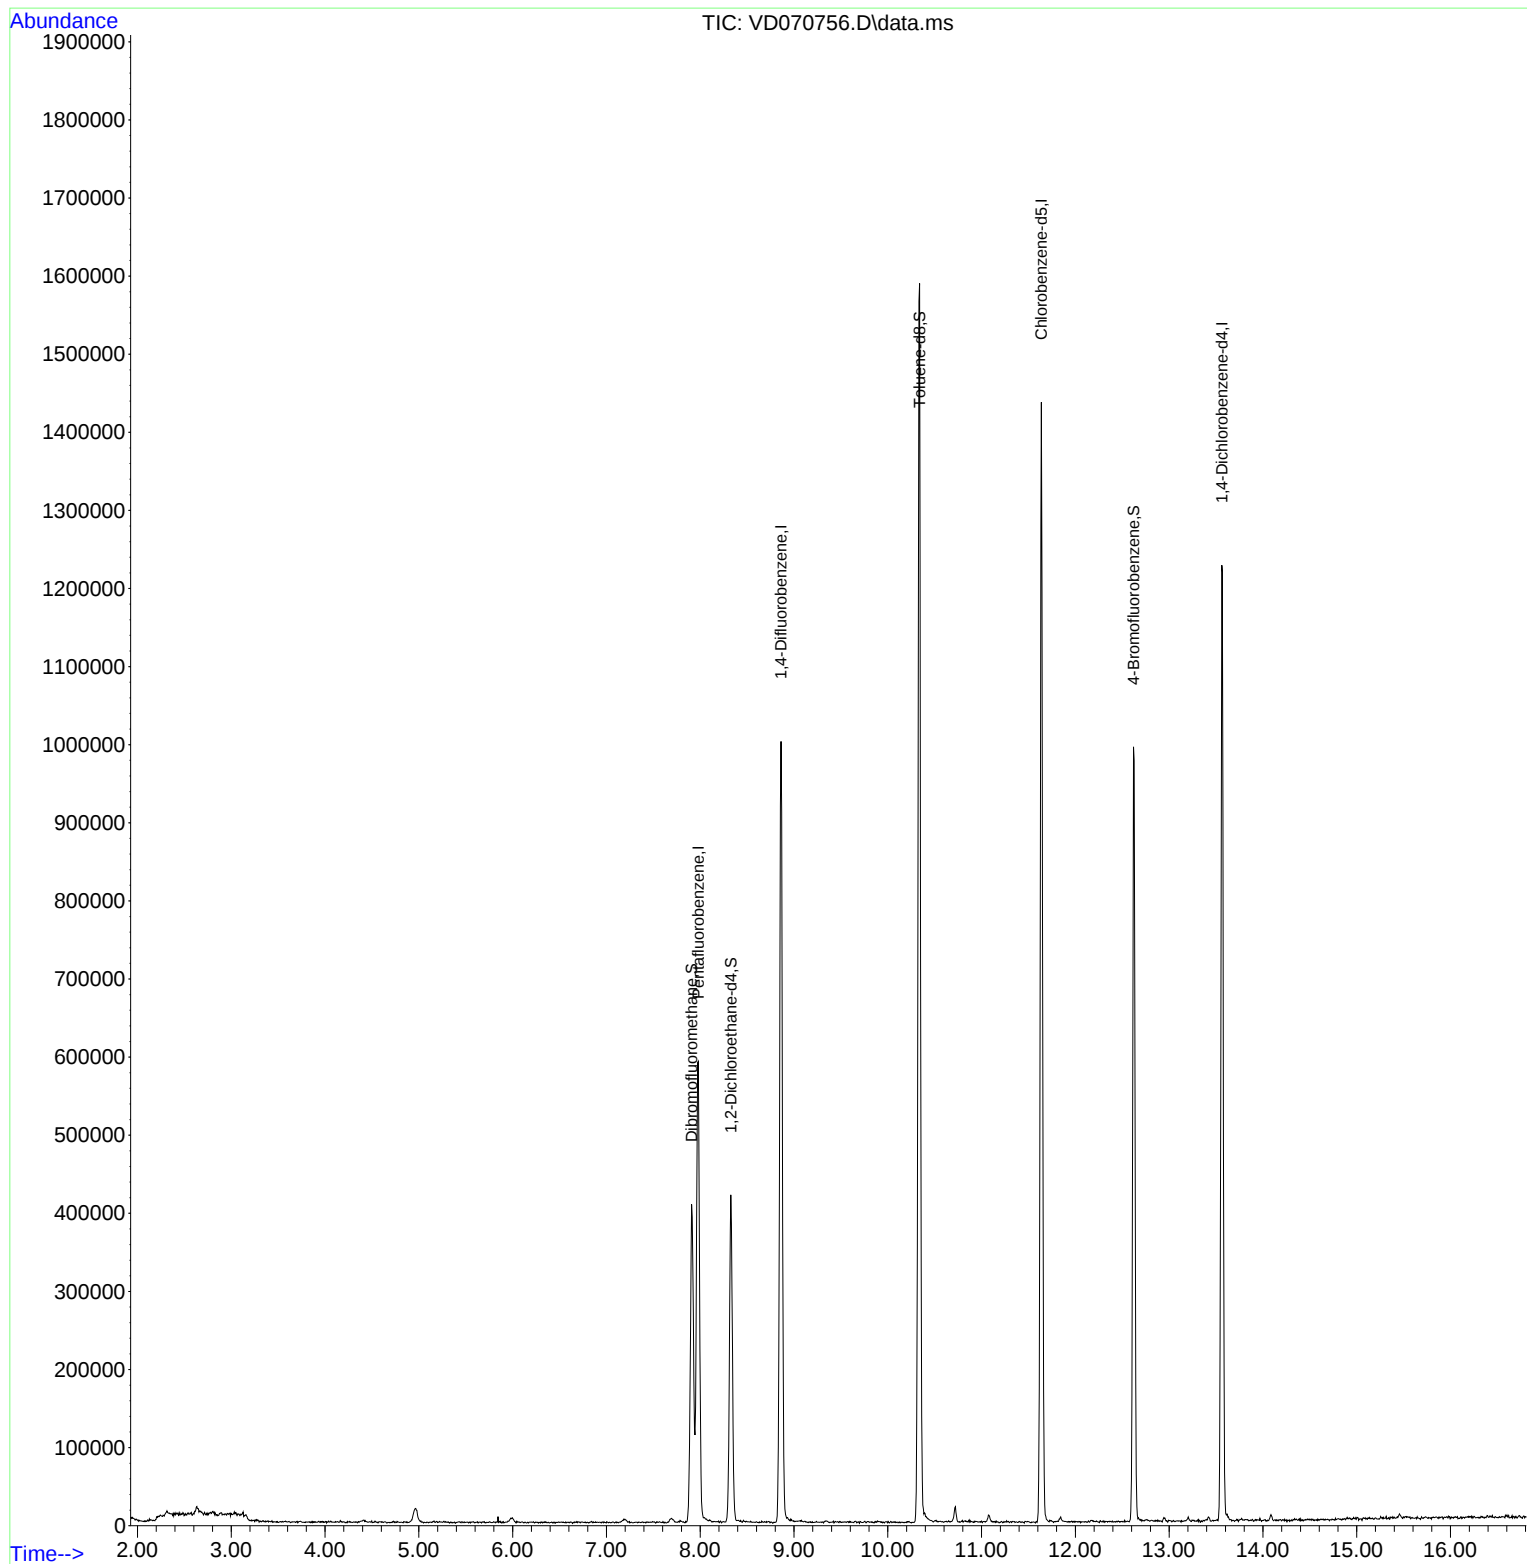


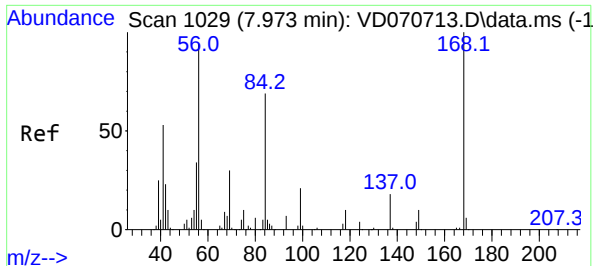

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.979 min Scan# 1030
Delta R.T. 0.006 min
Lab File: VD070756.D
Acq: 19 Oct 2021 14:05




Instrument :
MSVOA_D
ClientSampleId :
MH-CA-(1)RE


Tgt Ion:168 Resp: 419958
Ion Ratio Lower Upper
168 100
99 61.2 51.4 77.0

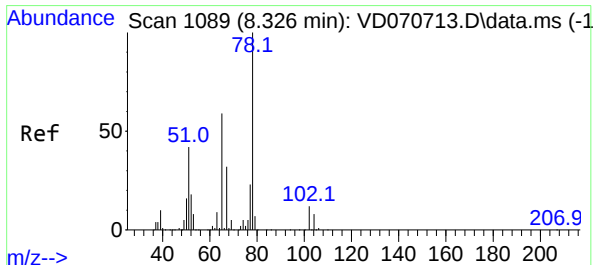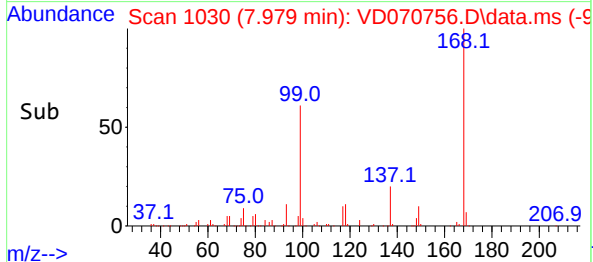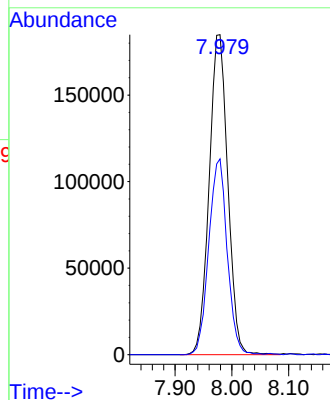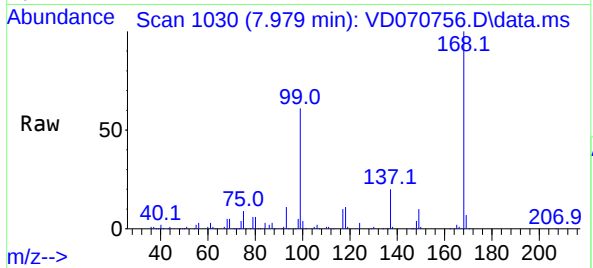

#33
1,2-Dichloroethane-d4
Concen: 63.75 ug/l
RT: 8.326 min Scan# 1089
Delta R.T. 0.000 min
Lab File: VD070756.D
Acq: 19 Oct 2021 14:05

Tgt Ion: 65 Resp: 317087
Ion Ratio Lower Upper
65 100
67 53.0 0.0 110.2


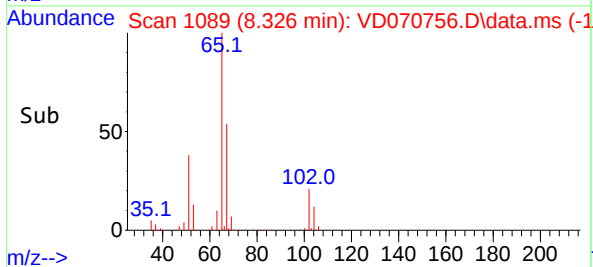
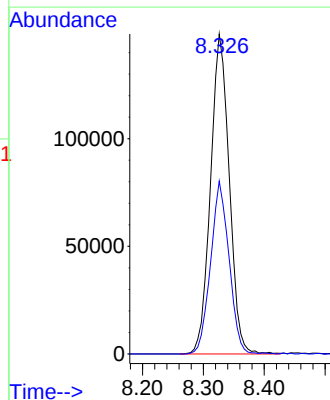
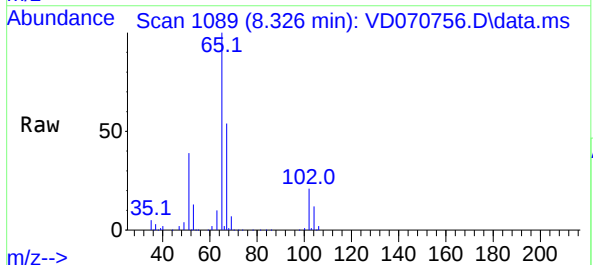


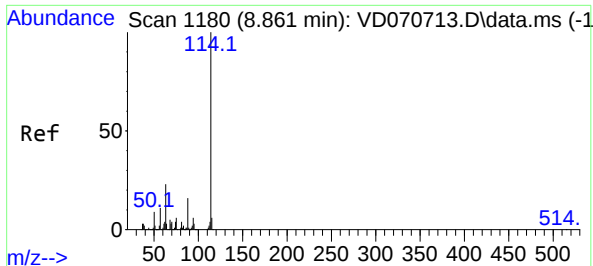

#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.861 min Scan# 1180
Delta R.T. 0.000 min
Lab File: VD070756.D
Acq: 19 Oct 2021 14:05




Instrument :
MSVOA_D
ClientSampleId :
MH-CA-(1)RE


Tgt Ion:114 Resp: 810875
Ion Ratio Lower Upper
114 100
63 23.4 0.0 41.8
88 16.3 0.0 32.6

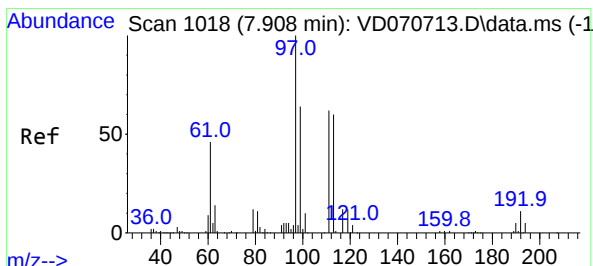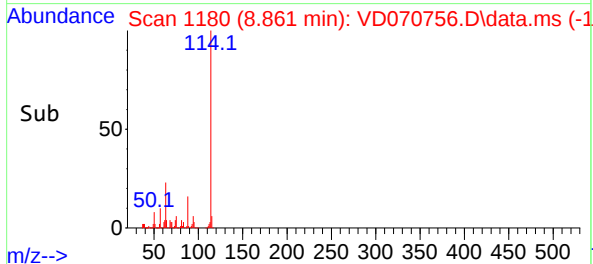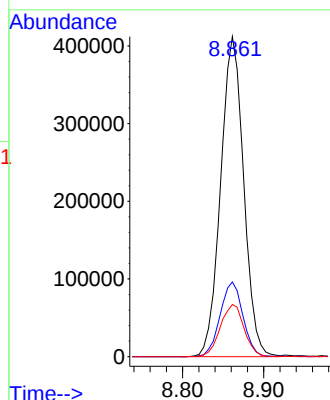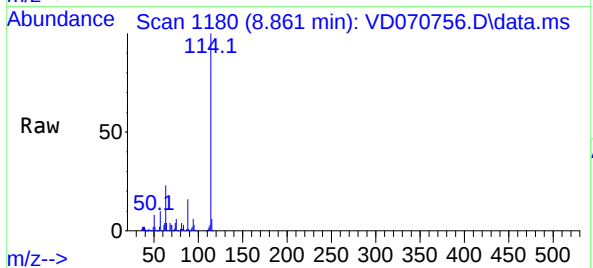

#35
Dibromofluoromethane
Concen: 55.11 ug/l
RT: 7.908 min Scan# 1018
Delta R.T. 0.000 min
Lab File: VD070756.D
Acq: 19 Oct 2021 14:05

Tgt Ion:113 Resp: 286156
Ion Ratio Lower Upper
113 100
111 105.3 83.1 124.7
192 18.9 12.7 19.1


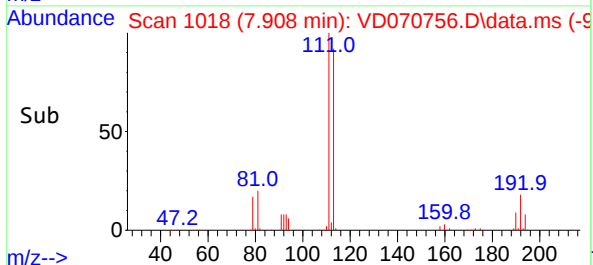
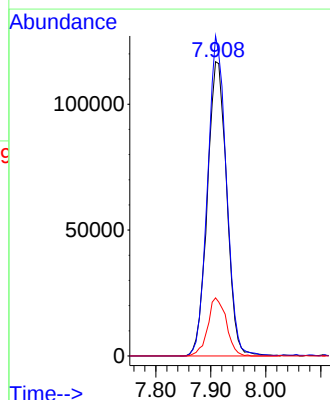
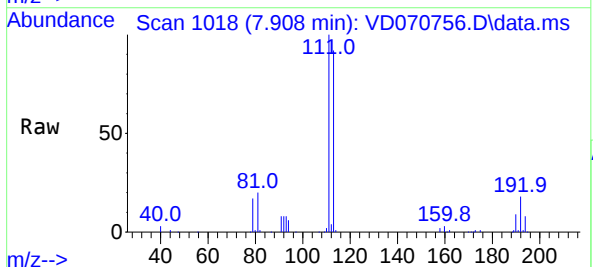


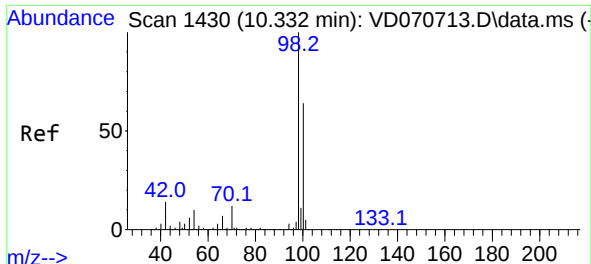

#50
Toluene-d8
Concen: 54.03 ug/l
RT: 10.338 min Scan# 1431
Delta R.T. 0.006 min
Lab File: VD070756.D
Acq: 19 Oct 2021 14:05




Instrument :
MSVOA_D
ClientSampleId :
MH-CA-(1)RE


Tgt Ion: 98 Resp: 1075274
Ion Ratio Lower Upper
98 100
100 64.0 52.2 78.4

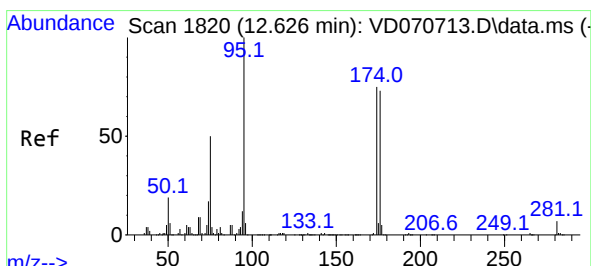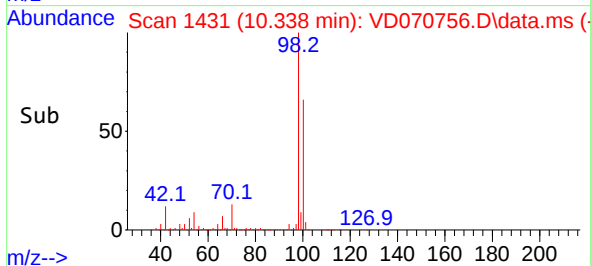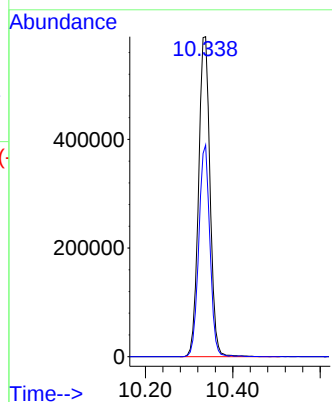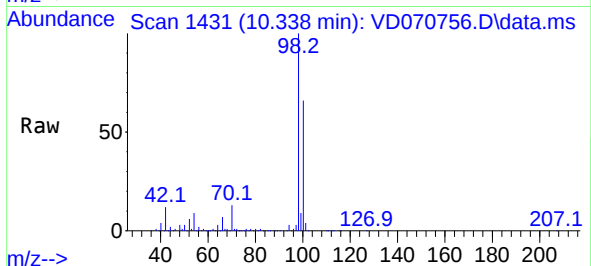

#62
4-Bromofluorobenzene
Concen: 49.15 ug/l
RT: 12.620 min Scan# 1819
Delta R.T. -0.006 min
Lab File: VD070756.D
Acq: 19 Oct 2021 14:05

Tgt Ion: 95 Resp: 336816
Ion Ratio Lower Upper
95 100
174 75.1 0.0 138.0
176 72.6 0.0 135.6


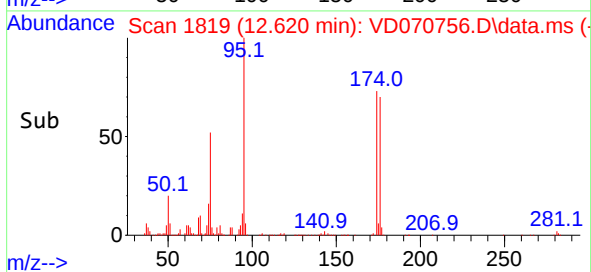
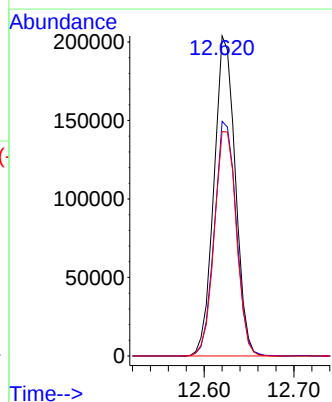
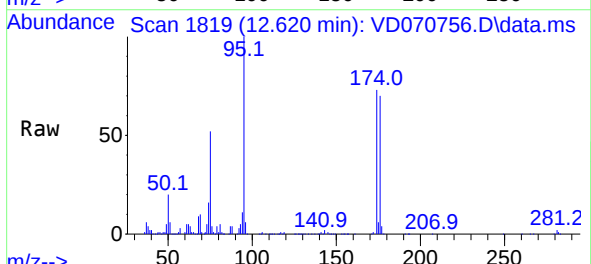


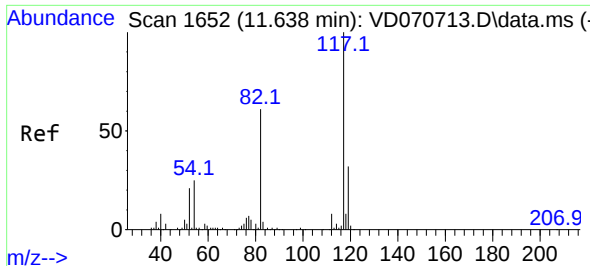

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.638 min Scan# 1652
Delta R.T. 0.000 min
Lab File: VD070756.D
Acq: 19 Oct 2021 14:05

Instrument :
MSVOA_D
ClientSampleId :
MH-CA-(1)RE

Tgt Ion:117 Resp: 787174
Ion Ratio Lower Upper
117 100
82 59.4 45.4 68.2
119 31.9 24.7 37.1

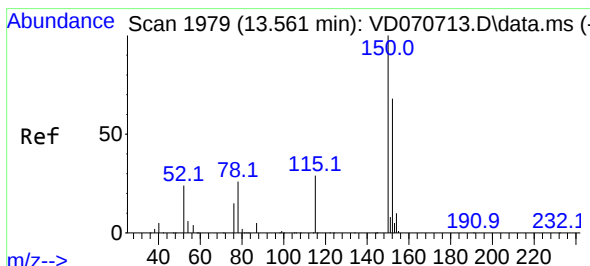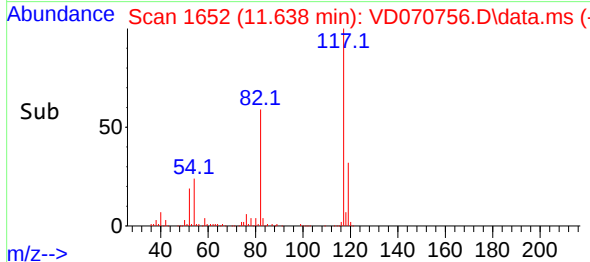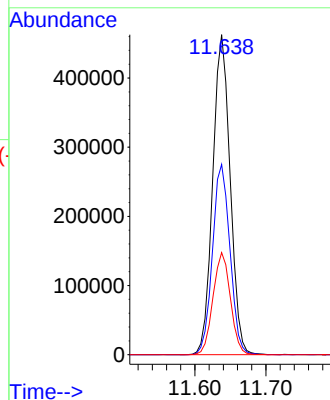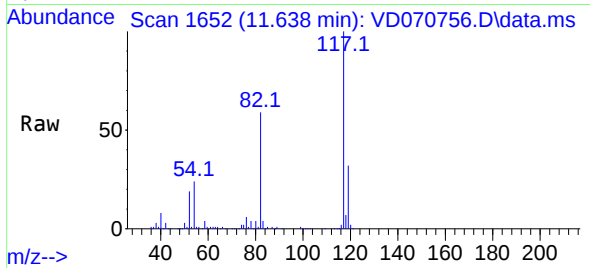

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.561 min Scan# 1979
Delta R.T. 0.000 min
Lab File: VD070756.D
Acq: 19 Oct 2021 14:05

Tgt Ion:152 Resp: 326214
Ion Ratio Lower Upper
152 100
115 63.0 31.9 95.7
150 157.4 0.0 350.0

