
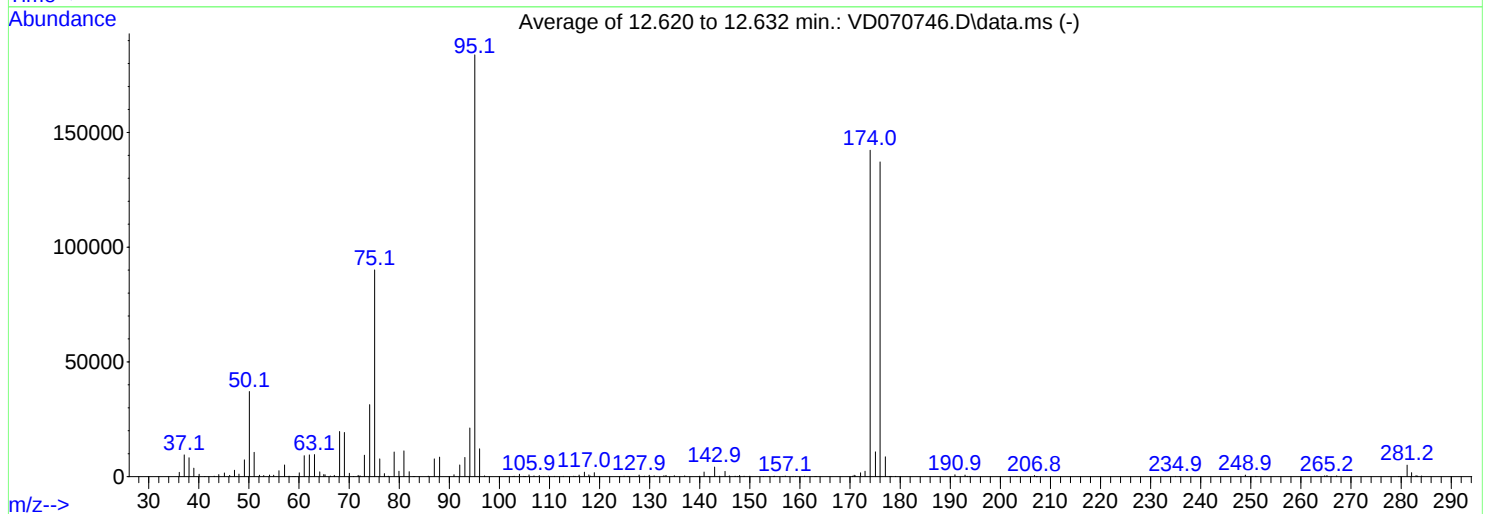


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD101921\
Data File : VD070746.D
Acq On : 19 Oct 2021 09:05
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D101521S.M
Title : SW846 8260
Last Update : Mon Oct 18 08:32:03 2021

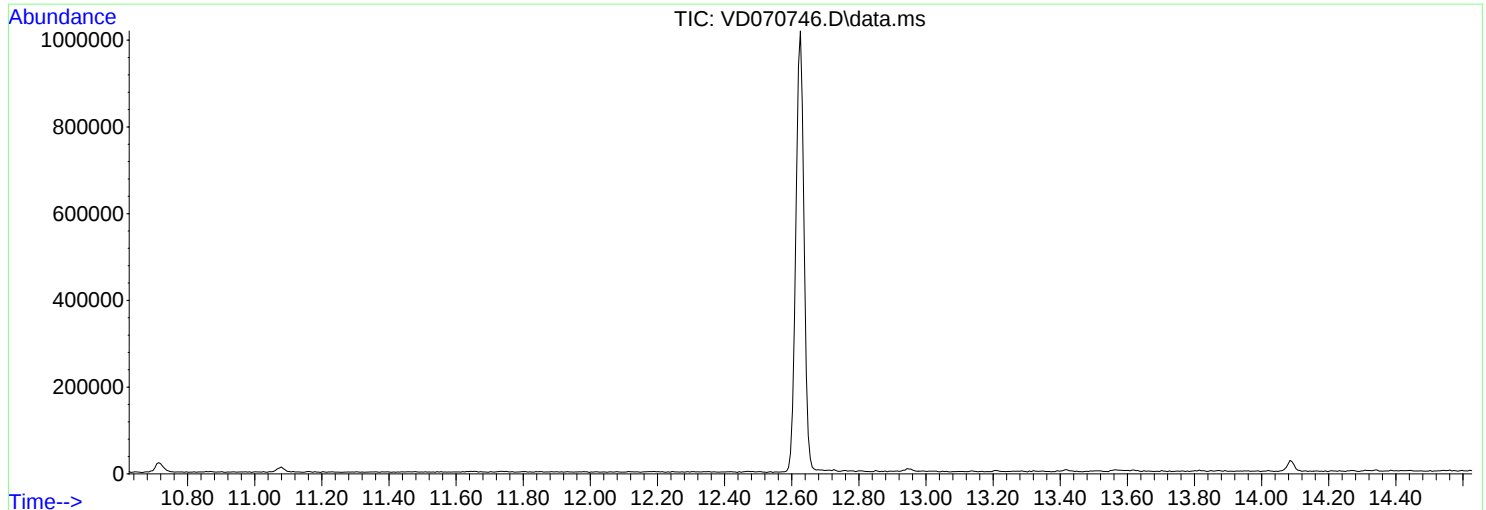

AutoFind: Scans 1819, 1820, 1821; Background Corrected with Scan 1810

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.2	37064	PASS
75	95	30	60	49.0	90069	PASS
95	95	100	100	100.0	183808	PASS
96	95	5	9	6.6	12158	PASS
173	174	0.00	2	1.7	2358	PASS
174	95	50	100	77.4	142229	PASS
175	174	5	9	7.6	10828	PASS
176	174	95	101	96.4	137173	PASS
177	176	5	9	6.3	8669	PASS