
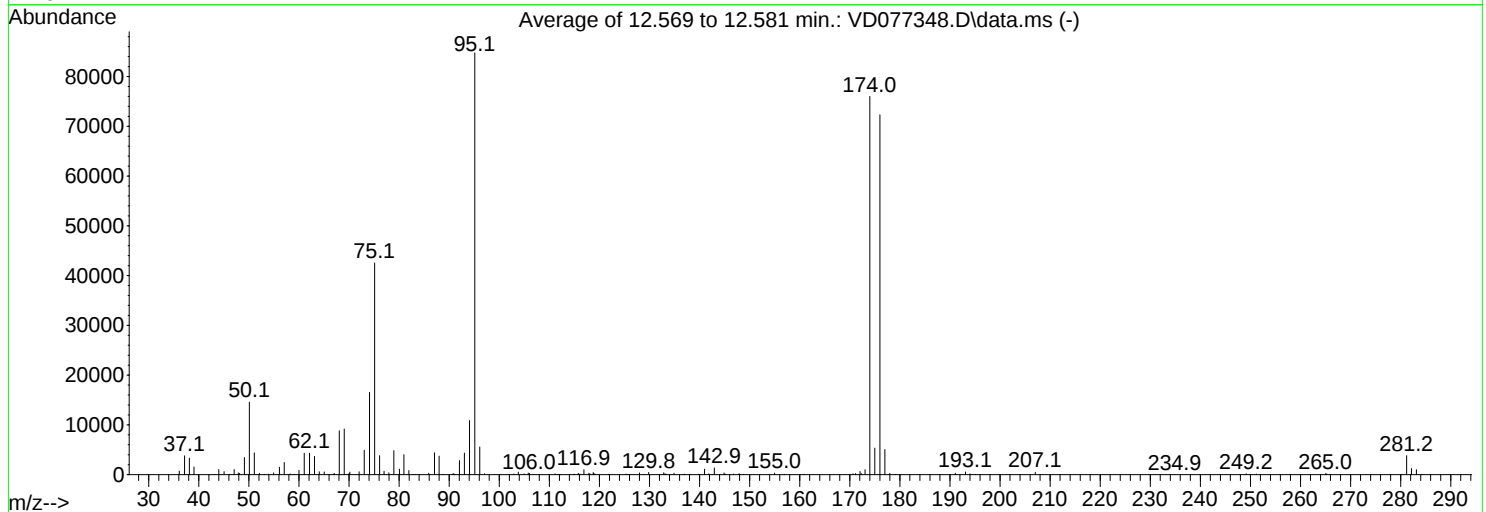


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD101923\
Data File : VD077348.D
Acq On : 19 Oct 2023 08:45
Operator : JC/SY
Sample : BFB
Misc : 5.00G/5.0ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D101723S.M
Title : SW846 8260
Last Update : Wed Oct 18 03:02:43 2023

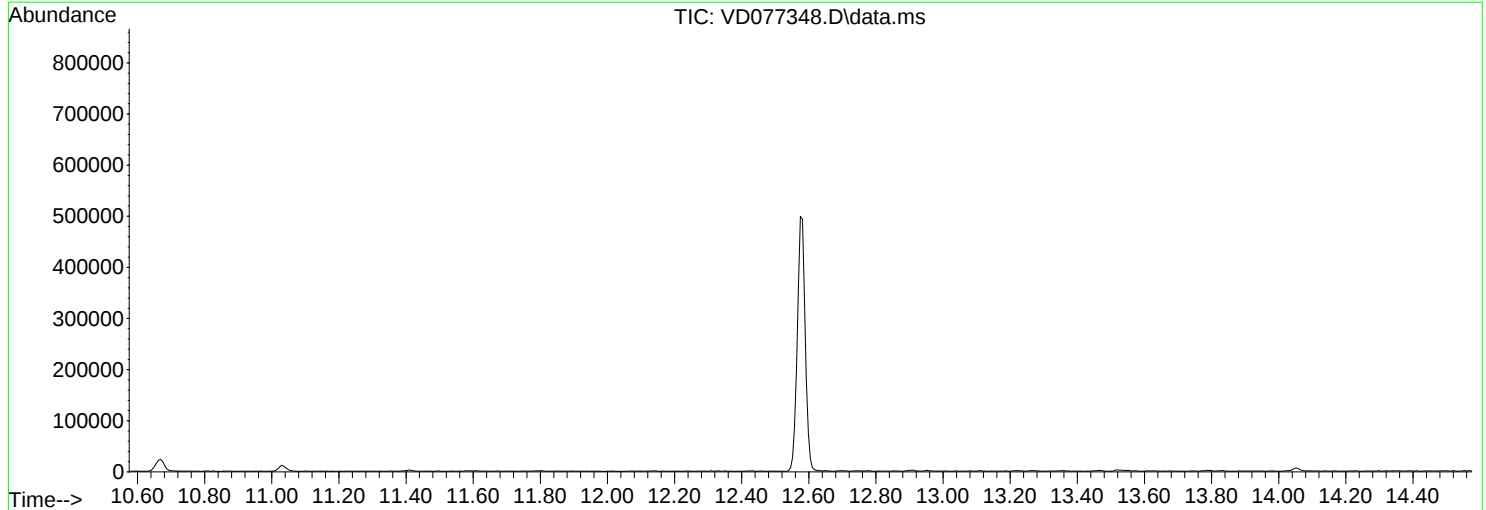

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1859

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	14569	PASS
75	95	30	60	50.2	42549	PASS
95	95	100	100	100.0	84757	PASS
96	95	5	9	6.5	5548	PASS
173	174	0.00	2	1.3	1000	PASS
174	95	50	100	89.7	75997	PASS
175	174	5	9	7.0	5329	PASS
176	174	95	101	95.1	72293	PASS
177	176	5	9	7.0	5055	PASS