

Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD102020\
 Data File : VD067331.D
 Acq On : 20 Oct 2020 18:30
 Operator : VA/SY
 Sample : L4436-11
 Misc : 11.78G/5.00ml/MSVOA D/SOIL
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 37B

Quant Time: Oct 21 02:51:10 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D101320S.M
 Quant Title : SW846 8260
 QLast Update : Mon Oct 19 19:13:29 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.98	168	283323	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.87	114	486351	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.65	117	454045	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.58	152	176048	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.33	65	157084	55.34	ug/l	0.00
Spiked Amount	50.000		Recovery	=	110.68%	
35) Dibromofluoromethane	7.92	113	161174	49.80	ug/l	0.00
Spiked Amount	50.000		Recovery	=	99.60%	
50) Toluene-d8	10.34	98	573454	48.96	ug/l	0.00
Spiked Amount	50.000		Recovery	=	97.92%	
62) 4-Bromofluorobenzene	12.64	95	175200	43.02	ug/l	0.00
Spiked Amount	50.000		Recovery	=	86.04%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD102020\
Data File : VD067331.D
Acq On : 20 Oct 2020 18:30
Operator : VA/SY
Sample : L4436-11
Misc : 11.78G/5.00ml/MSVOA D/SOIL
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
37B

Quant Time: Oct 21 02:51:10 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D101320S.M
Quant Title : SW846 8260
QLast Update : Mon Oct 19 19:13:29 2020
Response via : Initial Calibration

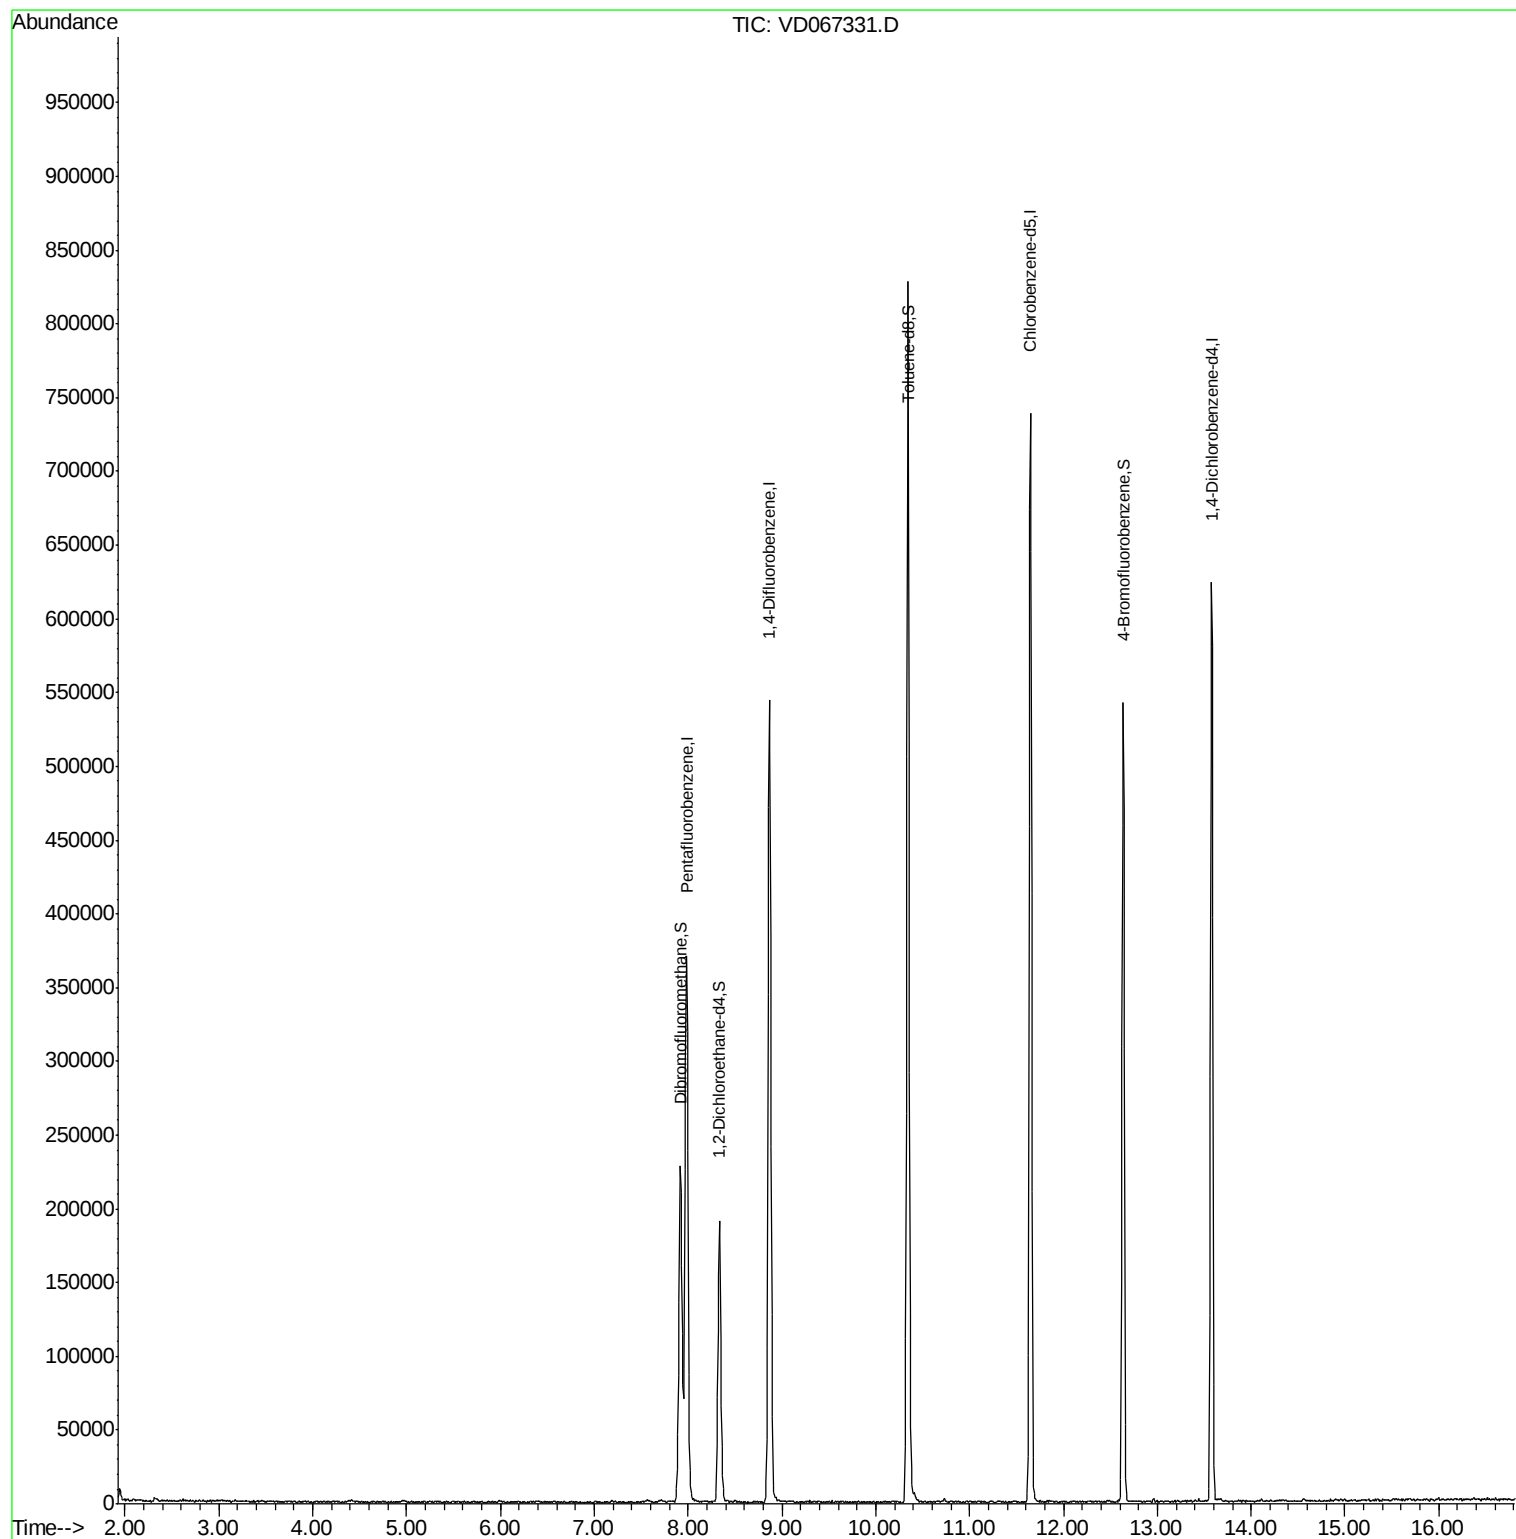

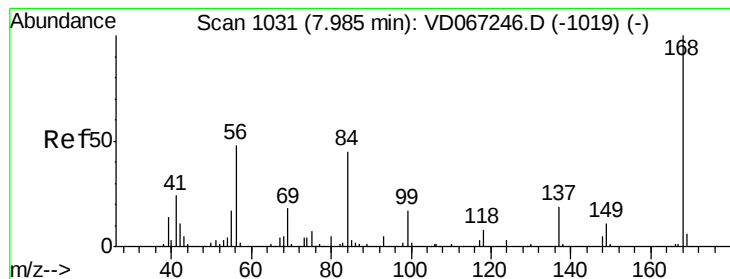

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.98 min Scan# 1031

Delta R.T. 0.00 min

Lab File: VD067331.D

Acq: 20 Oct 2020 18:30

Instrument :

MSVOA_D

ClientSampleId :


37B

Tot Ion:168 Resp: 283323

Ion Ratio Lower Upper




168 100

99 58.0 45.9 68.9

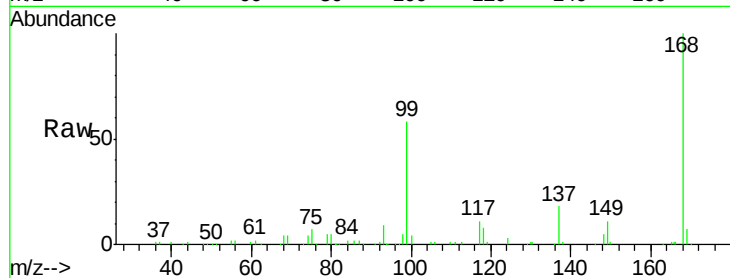

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VDC

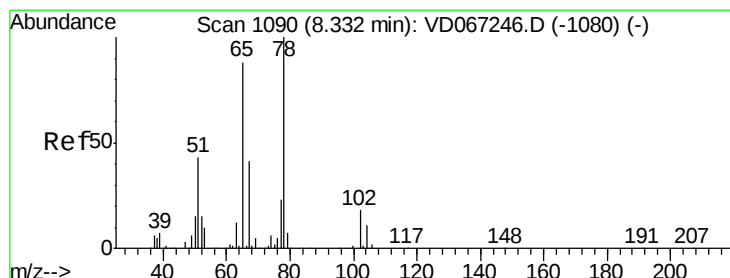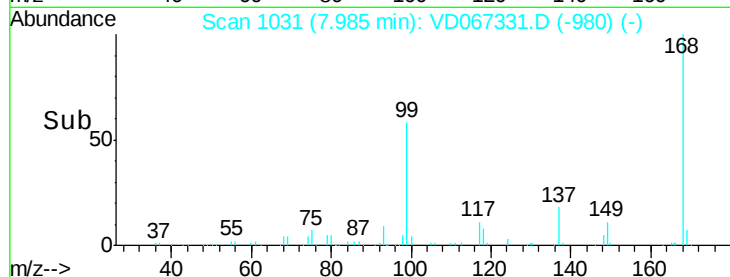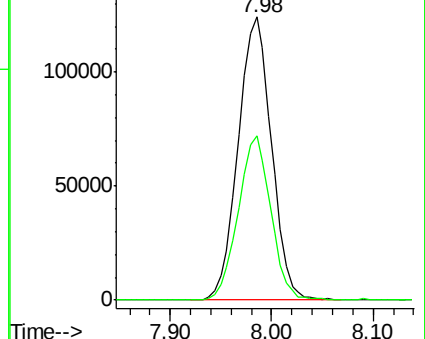

#33

1,2-Dichloroethane-d4

Concen: 55.341 ug/l

RT: 8.33 min Scan# 1090

Delta R.T. 0.00 min

Lab File: VD067331.D


Acq: 20 Oct 2020 18:30

Tgt Ion: 65 Resp: 157084

Ion Ratio Lower Upper



65 100


67 49.7 0.0 103.8

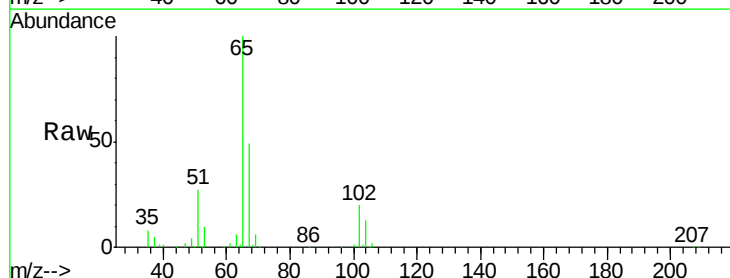

Abundance Ion 64.90 (64.60 to 65.60): VDC

Ion 66.90 (66.60 to 67.60): VDC

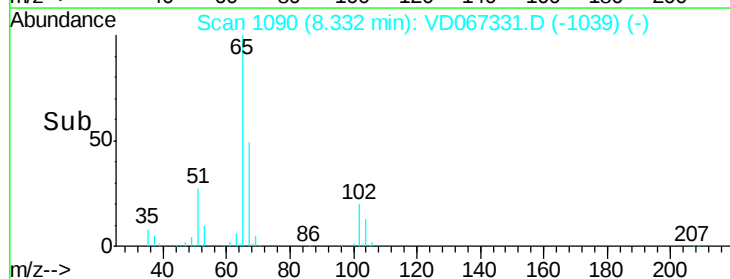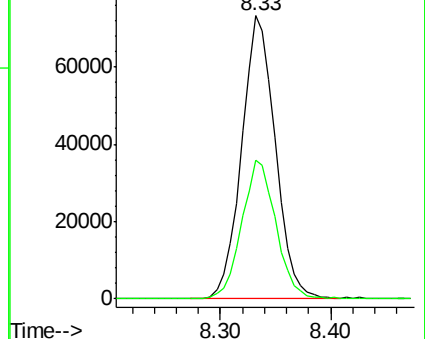

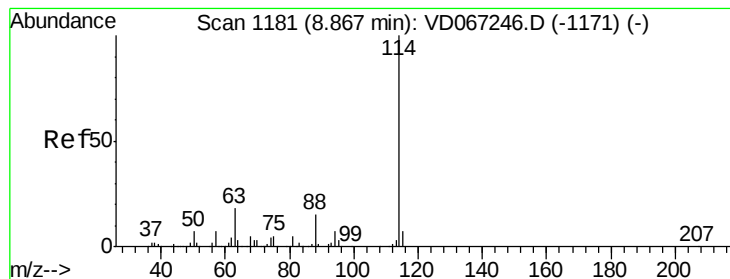

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.87 min Scan# 1181

Delta R.T. 0.00 min

Lab File: VD067331.D

Acq: 20 Oct 2020 18:30

Instrument :

MSVOA_D

ClientSampleId :

37B


Tot Ion:114 Resp: 486351

Ion Ratio Lower Upper

114 100

63 18.0 0.0 35.0

88 15.6 0.0 30.6

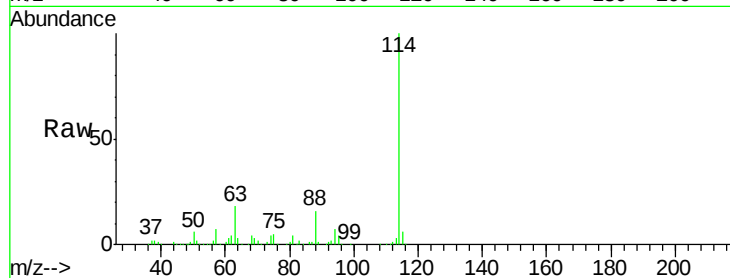

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): V

Ion 87.90 (87.60 to 88.60): V

300000

250000

200000

150000

100000

50000

0



8.87

8.80

8.90

9.00

Time-->

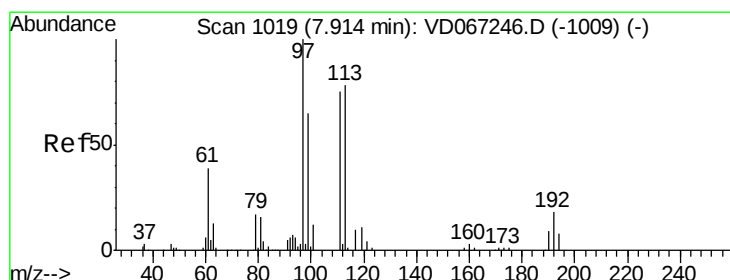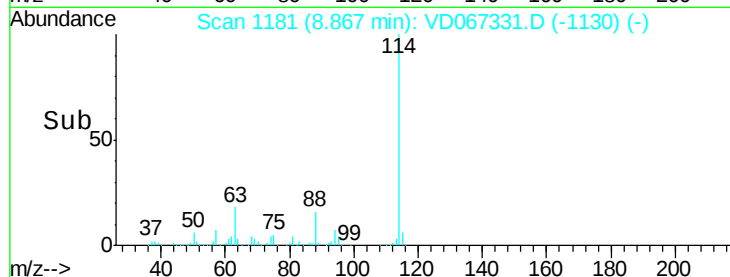

#35

Dibromofluoromethane

Concen: 49.796 ug/l

RT: 7.92 min Scan# 1020

Delta R.T. 0.01 min

Lab File: VD067331.D

Acq: 20 Oct 2020 18:30


Tgt Ion:113 Resp: 161174

Ion Ratio Lower Upper

113 100

111 103.3 81.6 122.4

192 20.2 17.0 25.4

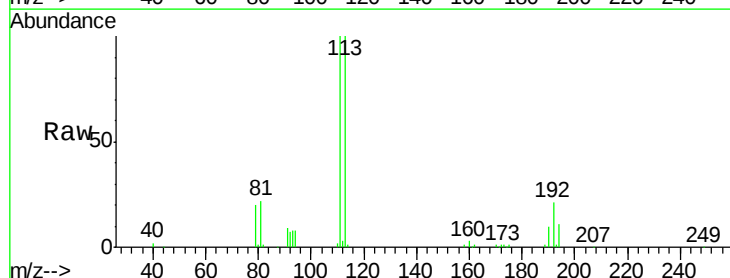

Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

80000

60000

40000

20000

0


7.92


7.80

7.90

8.00

Time-->

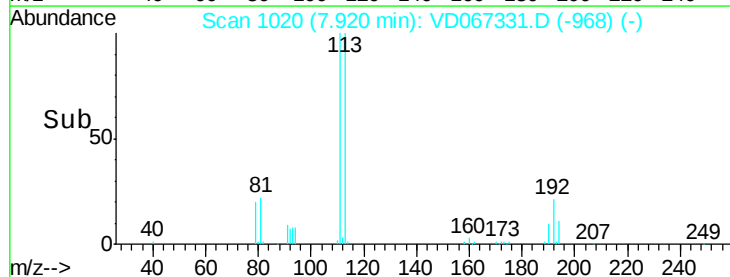

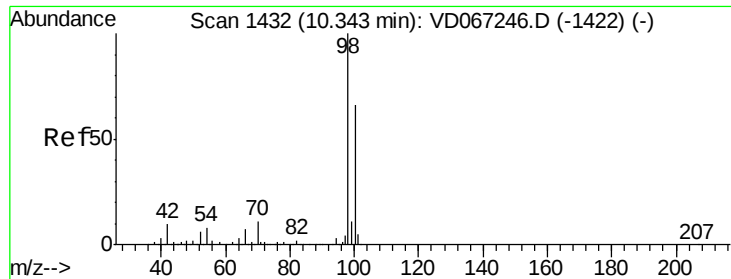

#50

Toluene-d8

Concen: 48.958 ug/l

RT: 10.34 min Scan# 1432

Delta R.T. 0.00 min

Lab File: VD067331.D

Acq: 20 Oct 2020 18:30

Instrument :

MSVOA_D

ClientSampleId :


37B

Tot Ion: 98 Resp: 573454

Ion Ratio Lower Upper




98 100

100 67.0 53.1 79.7

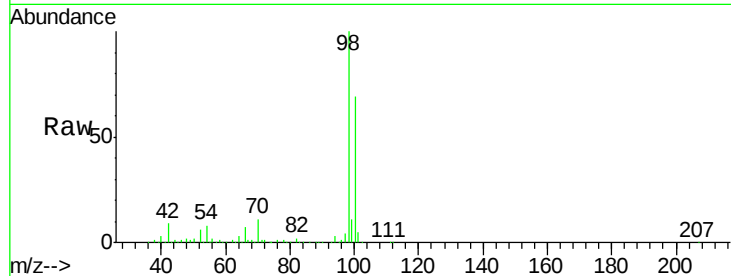

Abundance Ion 98.00 (97.70 to 98.70): VDC

Ion 100.00 (99.70 to 100.70): VDC

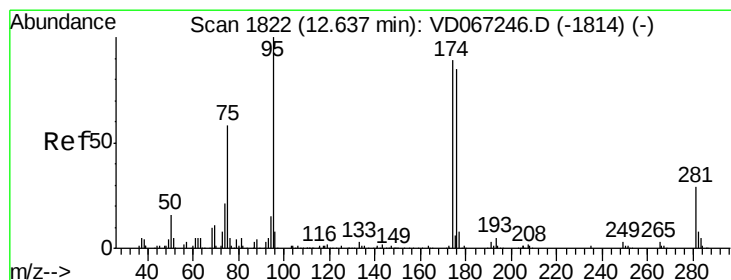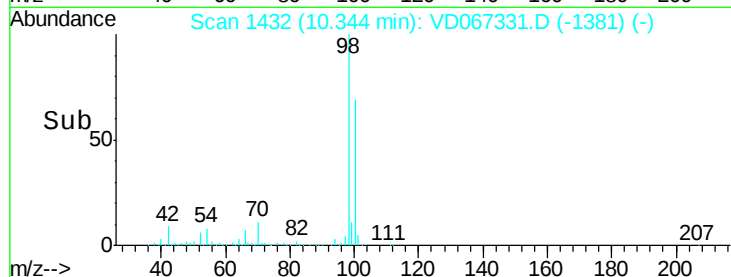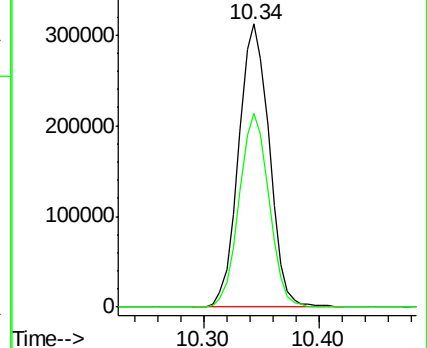

#62

4-Bromofluorobenzene

Concen: 43.016 ug/l

RT: 12.64 min Scan# 1822

Delta R.T. 0.00 min

Lab File: VD067331.D

Acq: 20 Oct 2020 18:30


Tgt Ion: 95 Resp: 175200

Ion Ratio Lower Upper

95 100

174 87.5 0.0 175.2



176 85.3 0.0 168.6

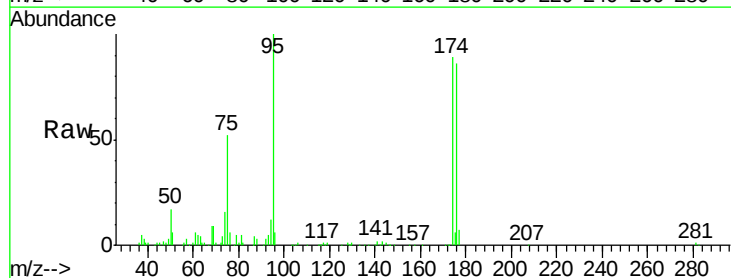

Abundance Ion 94.90 (94.60 to 95.60): VDC

Ion 173.80 (173.50 to 174.50): VDC

Ion 175.80 (175.50 to 176.50): VDC



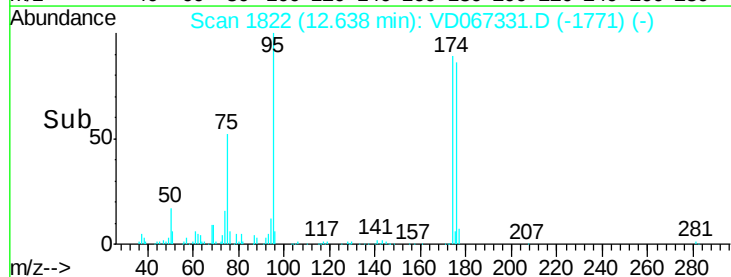
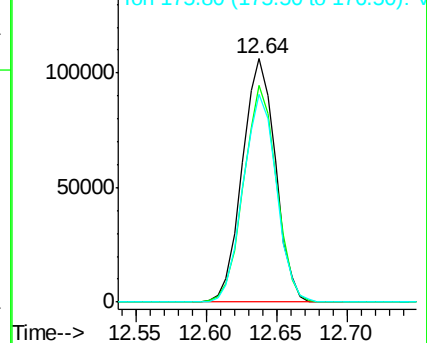




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.65 min Scan# 1654
Delta R.T. 0.00 min
Lab File: VD067331.D
Acq: 20 Oct 2020 18:30

Instrument :
MSVOA_D
ClientSampleId :
37B

Tot Ion	Ratio	Lower	Upper
117	100		
82	49.8	39.9	59.9
119	32.2	24.9	37.3

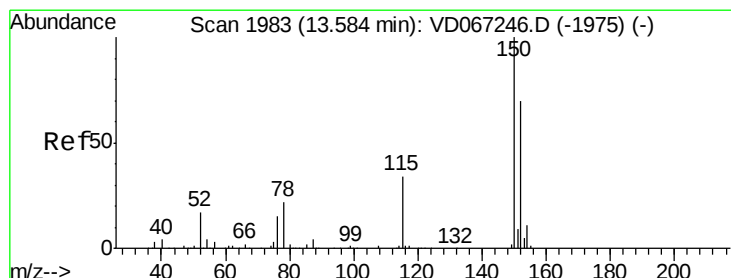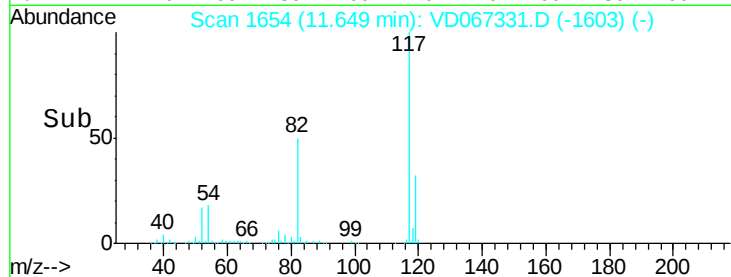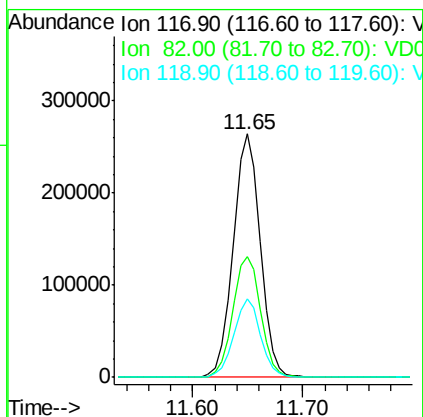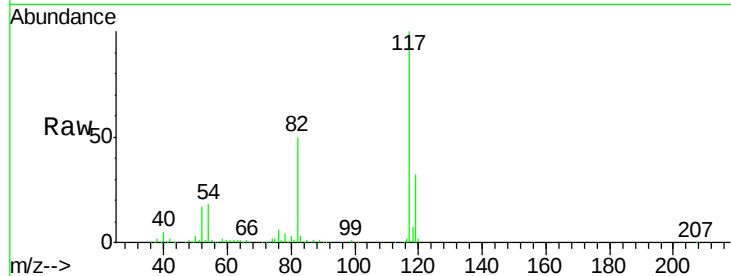

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.58 min Scan# 1982
Delta R.T. -0.01 min
Lab File: VD067331.D
Acq: 20 Oct 2020 18:30

Tgt Ion	Ratio	Lower	Upper
152	100		
115	56.6	29.3	87.9
150	156.5	0.0	339.0

