
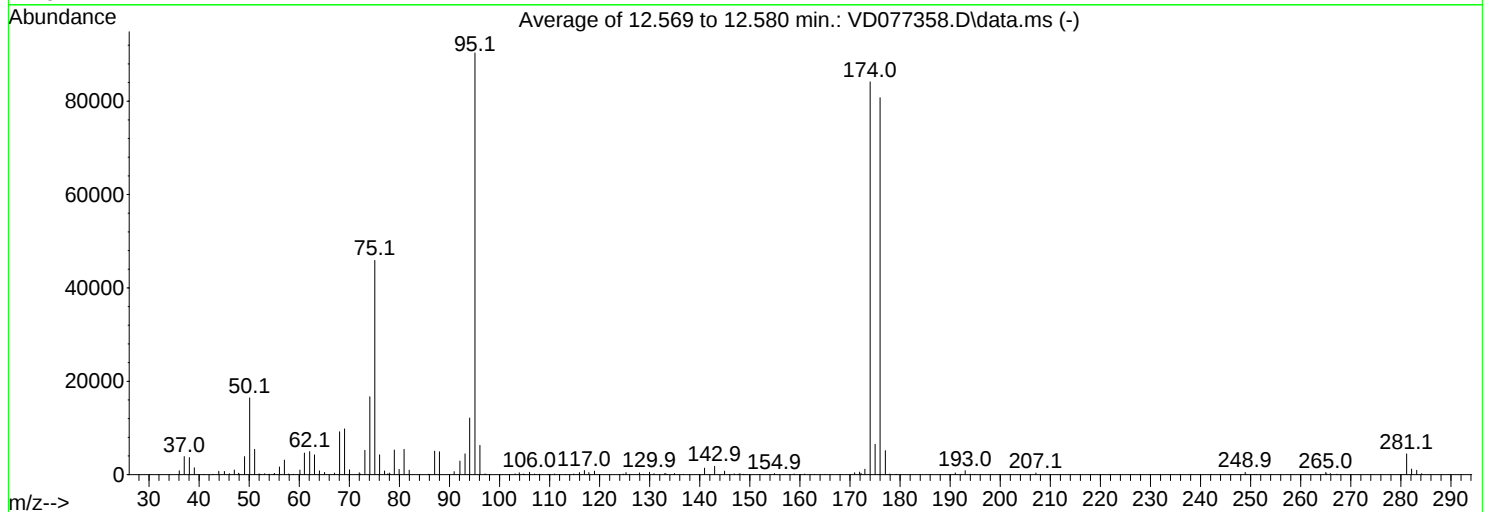


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD102023\
 Data File : VD077358.D
 Acq On : 20 Oct 2023 10:09
 Operator : JC/SY
 Sample : BFB
 Misc : 5.00G/5.0ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D101723S.M
 Title : SW846 8260
 Last Update : Wed Oct 18 03:02:43 2023

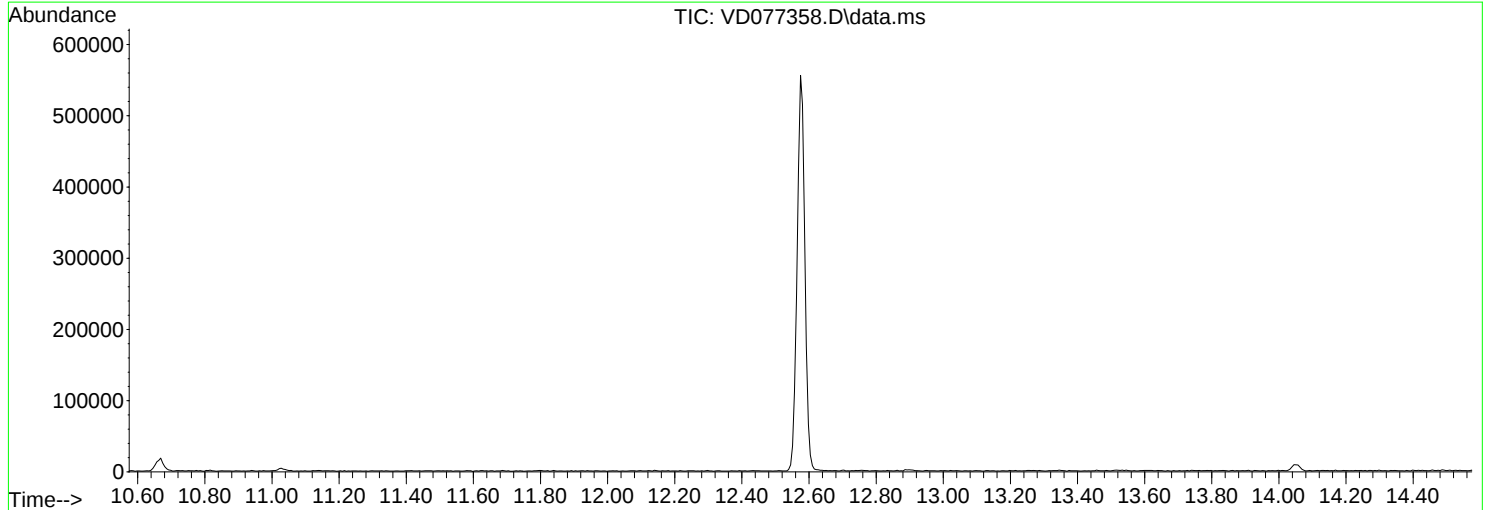

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1859

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	16438	PASS
75	95	30	60	50.8	45896	PASS
95	95	100	100	100.0	90357	PASS
96	95	5	9	6.9	6262	PASS
173	174	0.00	2	1.4	1183	PASS
174	95	50	100	93.1	84131	PASS
175	174	5	9	7.7	6518	PASS
176	174	95	101	96.0	80765	PASS
177	176	5	9	6.4	5155	PASS