

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD102221\
 Data File : VD070815.D
 Acq On : 22 Oct 2021 10:30
 Operator : VA/SY
 Sample : VD1022SBL01
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 VD1022SBL01

Quant Time: Oct 23 04:08:56 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D101521S.M
 Quant Title : SW846 8260
 QLast Update : Mon Oct 18 08:32:03 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.973	168	459537	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.861	114	846425	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.638	117	809701	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.561	152	347408	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.326	65	312972	57.501	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	115.000%
35) Dibromofluoromethane	7.914	113	278026	51.299	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	102.600%
50) Toluene-d8	10.338	98	1101439	53.016	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	106.040%
62) 4-Bromofluorobenzene	12.620	95	355292	49.666	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	99.340%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD102221\
Data File : VD070815.D
Acq On : 22 Oct 2021 10:30
Operator : VA/SY
Sample : VD1022SBL01
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
VD1022SBL01

Quant Time: Oct 23 04:08:56 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D101521S.M
Quant Title : SW846 8260
QLast Update : Mon Oct 18 08:32:03 2021
Response via : Initial Calibration




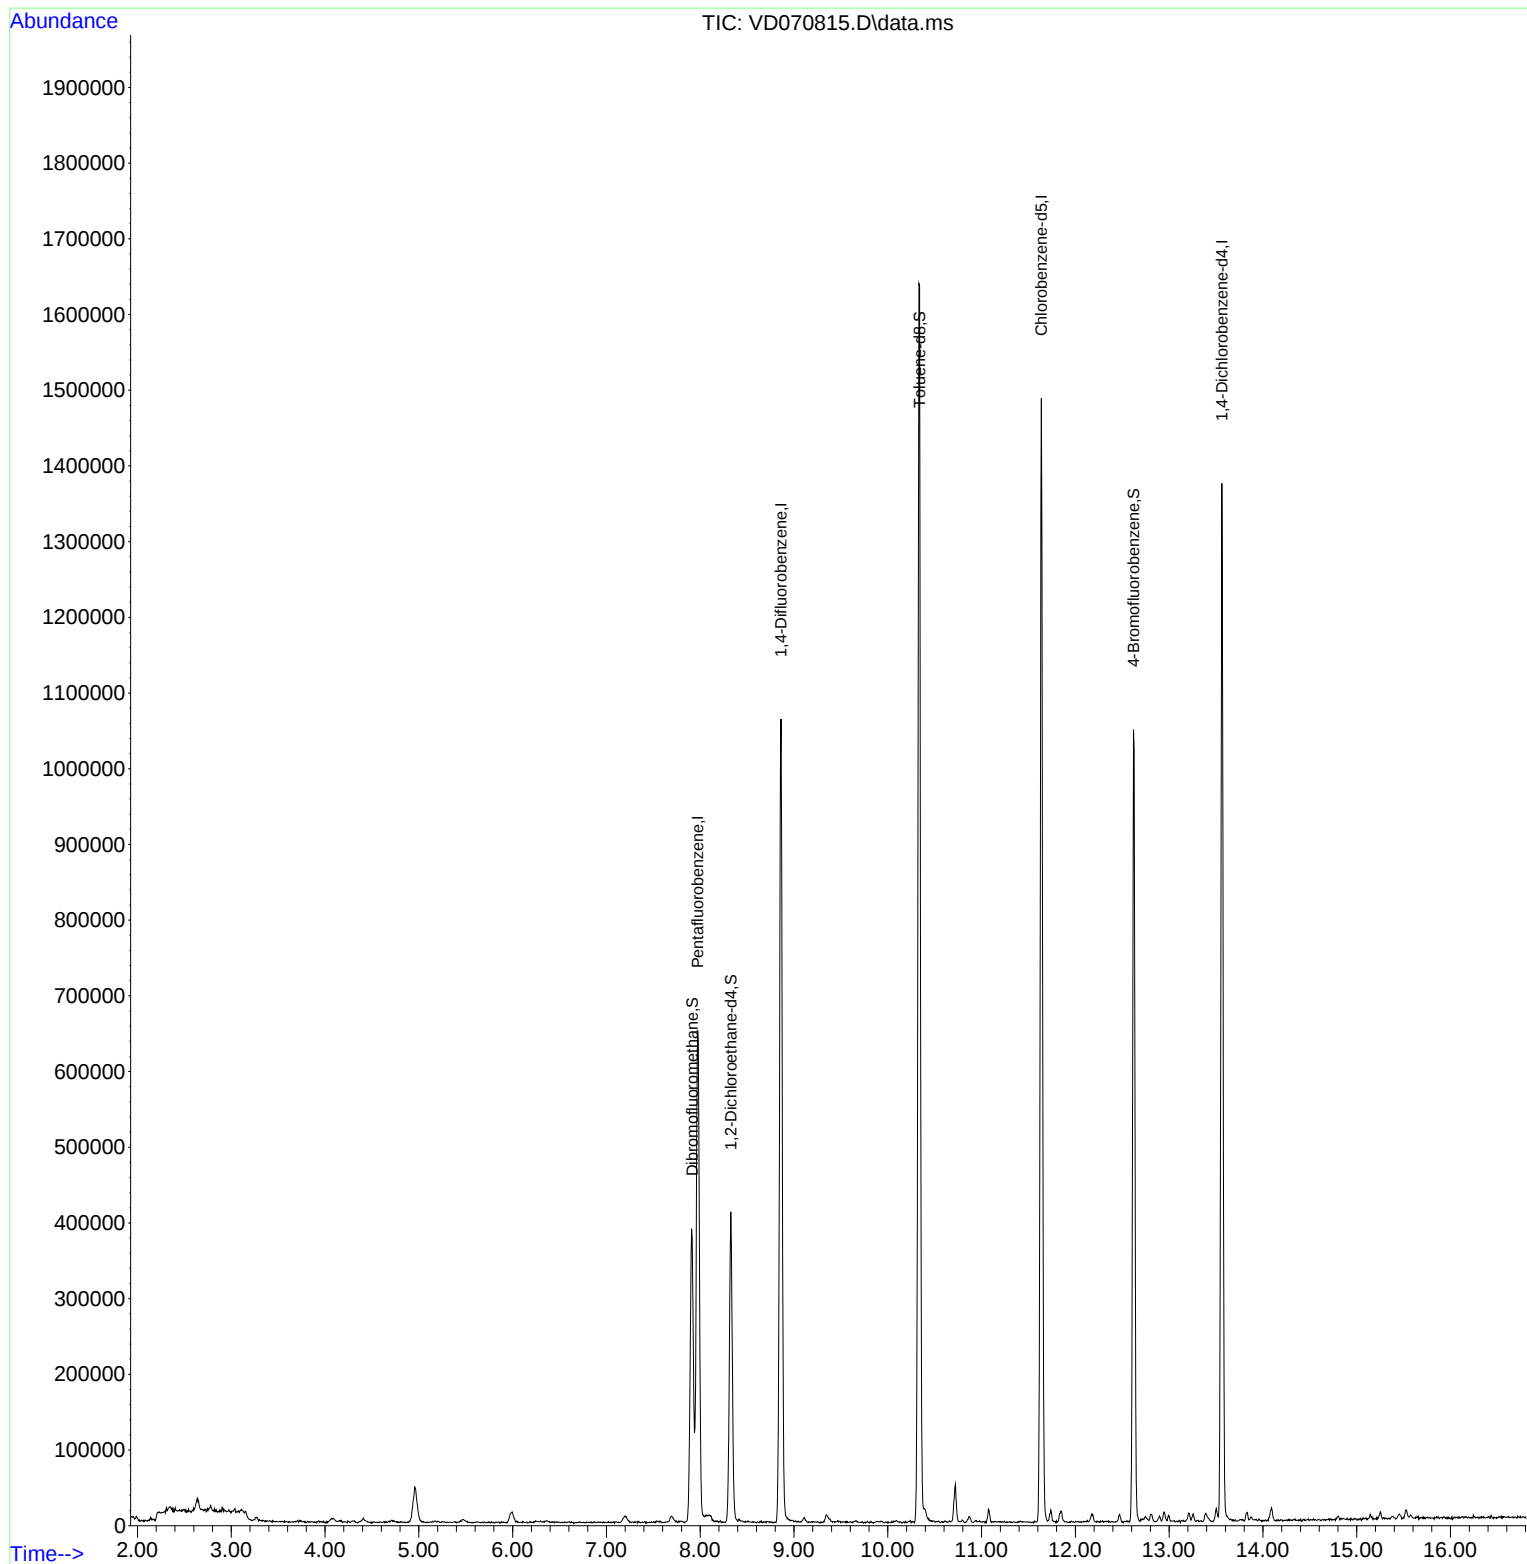


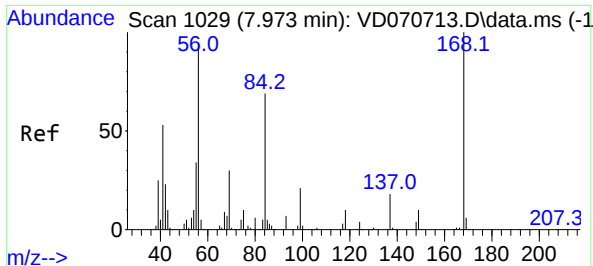

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.973 min Scan# 1029
Delta R.T. 0.000 min
Lab File: VD070815.D
Acq: 22 Oct 2021 10:30




Instrument :
MSVOA_D
ClientSampleId :
VD1022SBL01

Tgt Ion:168 Resp: 459537
Ion Ratio Lower Upper
168 100
99 60.8 51.4 77.0

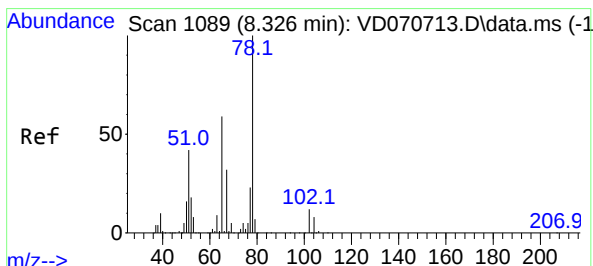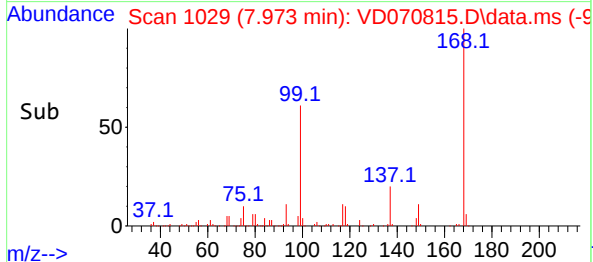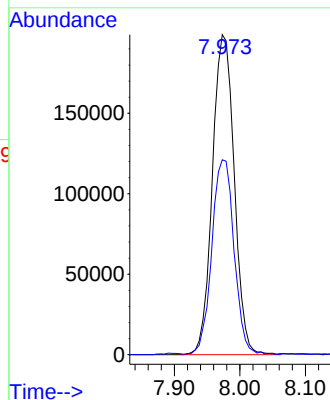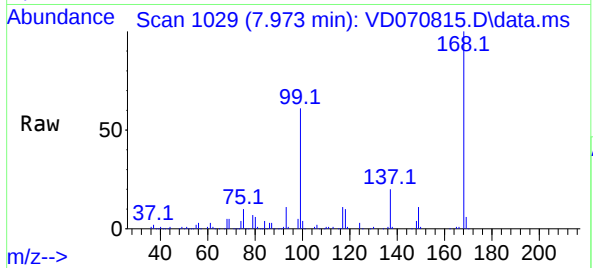

#33
1,2-Dichloroethane-d4
Concen: 57.501 ug/l
RT: 8.326 min Scan# 1089
Delta R.T. 0.000 min
Lab File: VD070815.D
Acq: 22 Oct 2021 10:30

Tgt Ion: 65 Resp: 312972
Ion Ratio Lower Upper
65 100
67 52.1 0.0 110.2

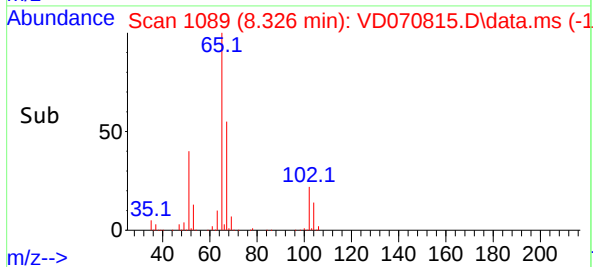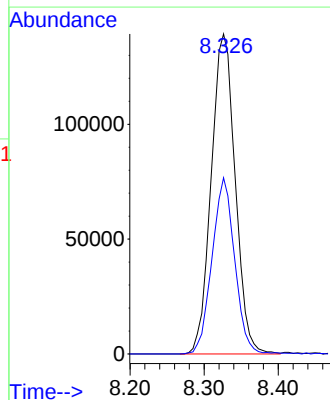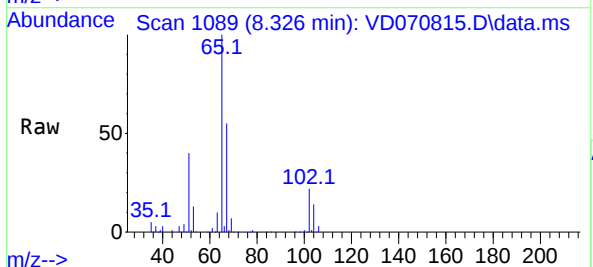







#34

1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.861 min Scan# 1180
Delta R.T. 0.000 min
Lab File: VD070815.D
Acq: 22 Oct 2021 10:30

Instrument :
MSVOA_D
ClientSampleId :
VD1022SBL01




Tgt Ion:114 Resp: 846425
Ion Ratio Lower Upper
114 100
63 24.0 0.0 41.8
88 16.0 0.0 32.6

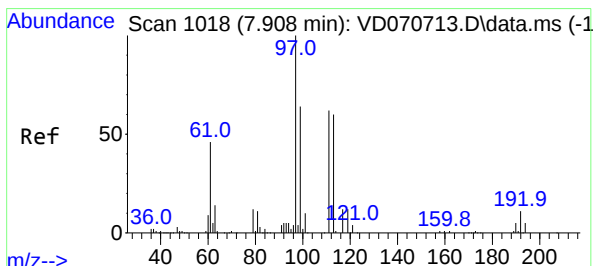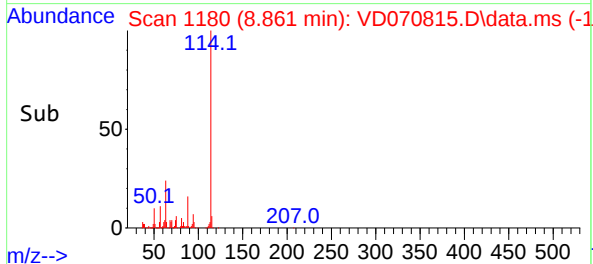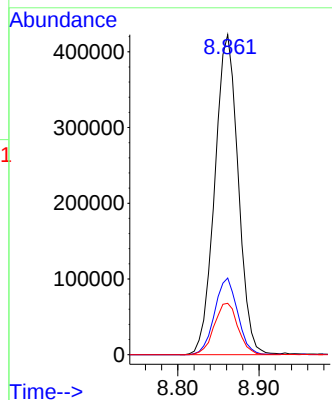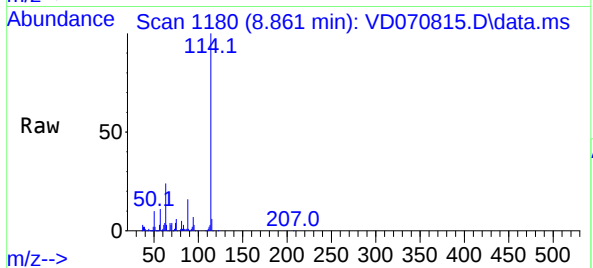


#35

Dibromofluoromethane
Concen: 51.299 ug/l
RT: 7.914 min Scan# 1019
Delta R.T. 0.006 min
Lab File: VD070815.D
Acq: 22 Oct 2021 10:30

Tgt Ion:113 Resp: 278026
Ion Ratio Lower Upper
113 100
111 104.9 83.1 124.7
192 18.0 12.7 19.1


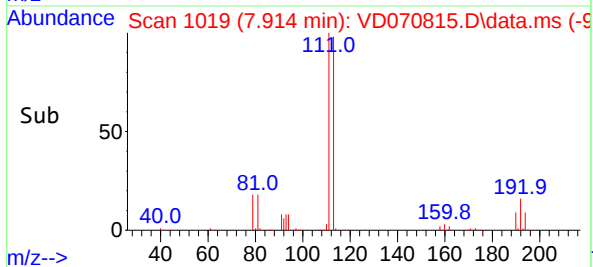
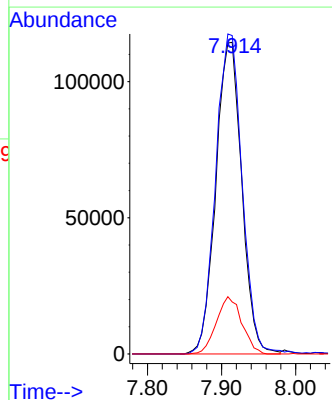
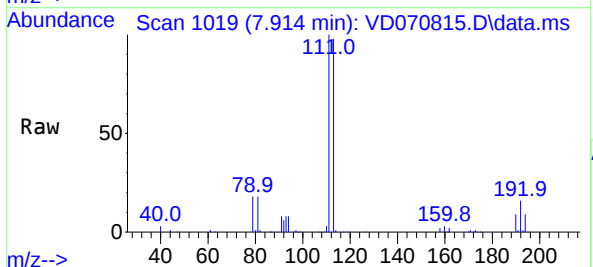


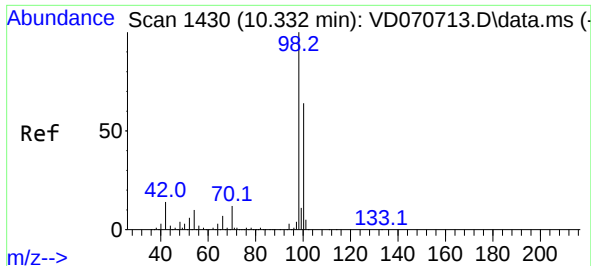

#50
Toluene-d8
Concen: 53.016 ug/l
RT: 10.338 min Scan# 1431
Delta R.T. 0.006 min
Lab File: VD070815.D
Acq: 22 Oct 2021 10:30




Instrument :
MSVOA_D
ClientSampleId :
VD1022SBL01


Tgt Ion: 98 Resp: 1101439
Ion Ratio Lower Upper
98 100
100 63.8 52.2 78.4

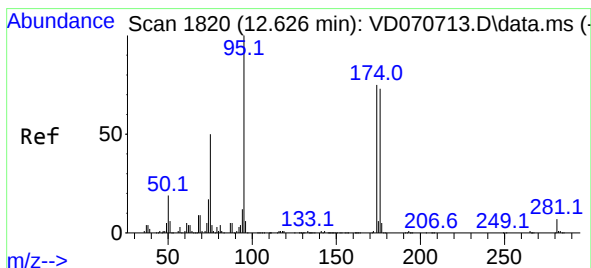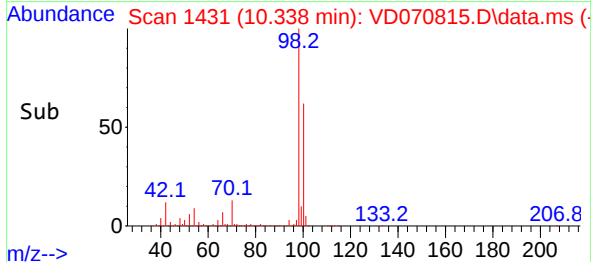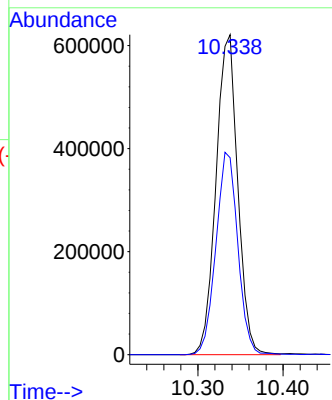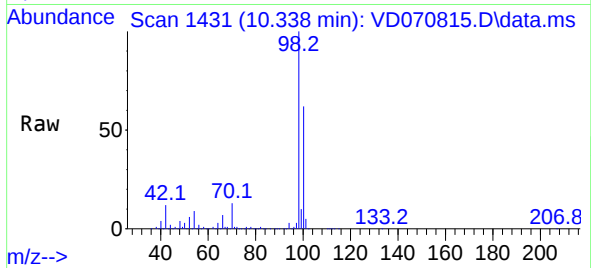

#62
4-Bromofluorobenzene
Concen: 49.666 ug/l
RT: 12.620 min Scan# 1819
Delta R.T. -0.006 min
Lab File: VD070815.D
Acq: 22 Oct 2021 10:30

Tgt Ion: 95 Resp: 355292
Ion Ratio Lower Upper
95 100
174 73.4 0.0 138.0
176 70.5 0.0 135.6


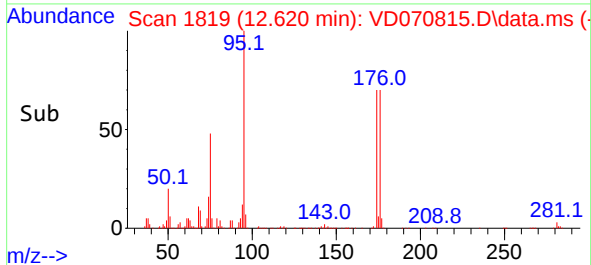
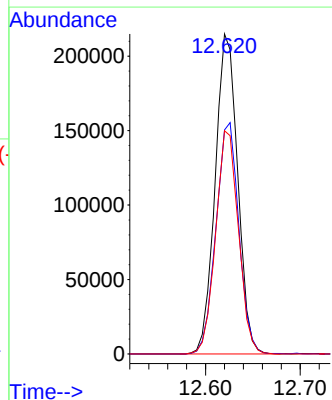
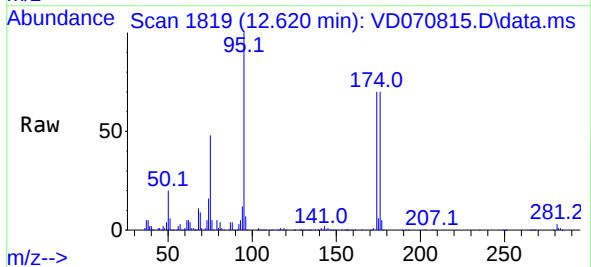


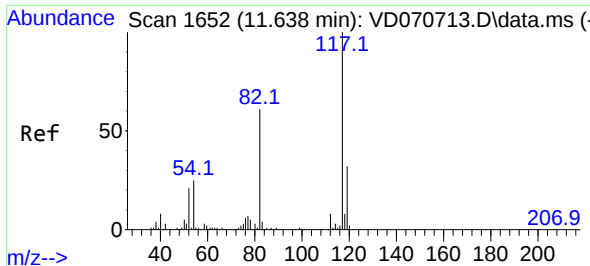

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.638 min Scan# 1652
Delta R.T. 0.000 min
Lab File: VD070815.D
Acq: 22 Oct 2021 10:30

Instrument :
MSVOA_D
ClientSampleId :
VD1022SBL01

Tgt Ion:117 Resp: 809701
Ion Ratio Lower Upper
117 100
82 59.0 45.4 68.2
119 32.8 24.7 37.1

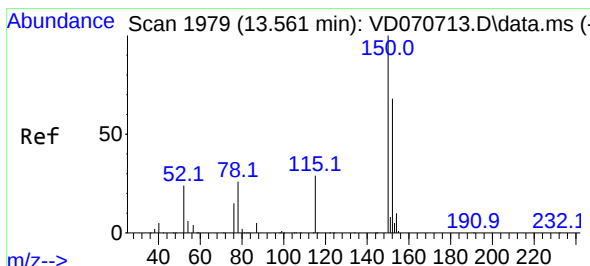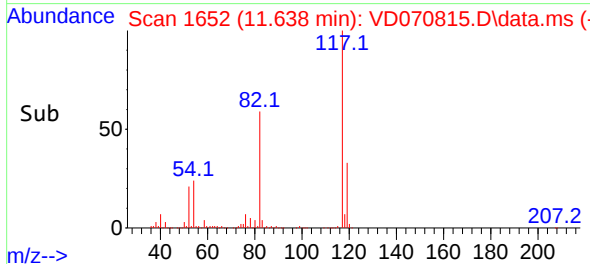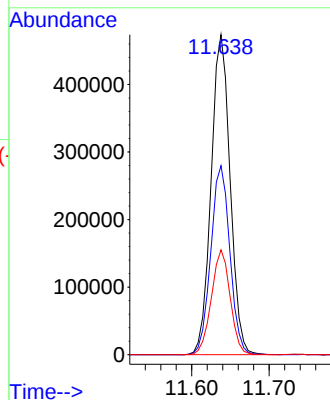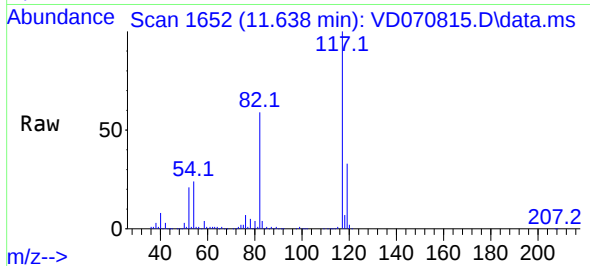

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.561 min Scan# 1979
Delta R.T. 0.000 min
Lab File: VD070815.D
Acq: 22 Oct 2021 10:30

Tgt Ion:152 Resp: 347408
Ion Ratio Lower Upper
152 100
115 62.4 31.9 95.7
150 156.8 0.0 350.0

