
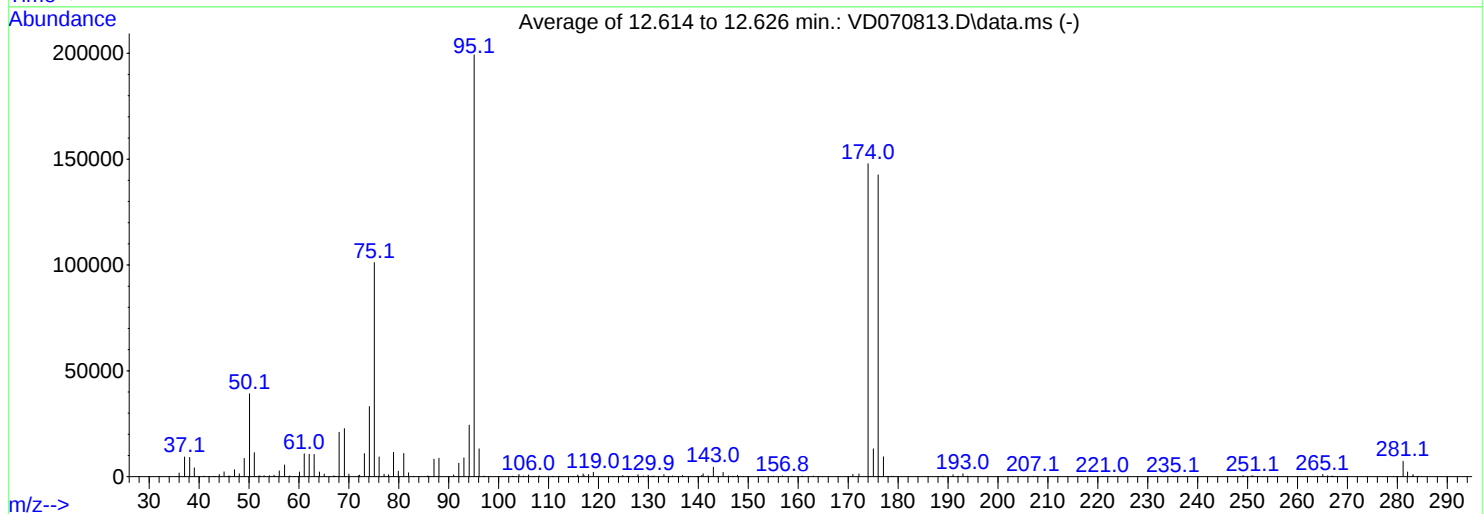


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD102221\
Data File : VD070813.D
Acq On : 22 Oct 2021 09:12
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D101521S.M
Title : SW846 8260
Last Update : Mon Oct 18 08:32:03 2021

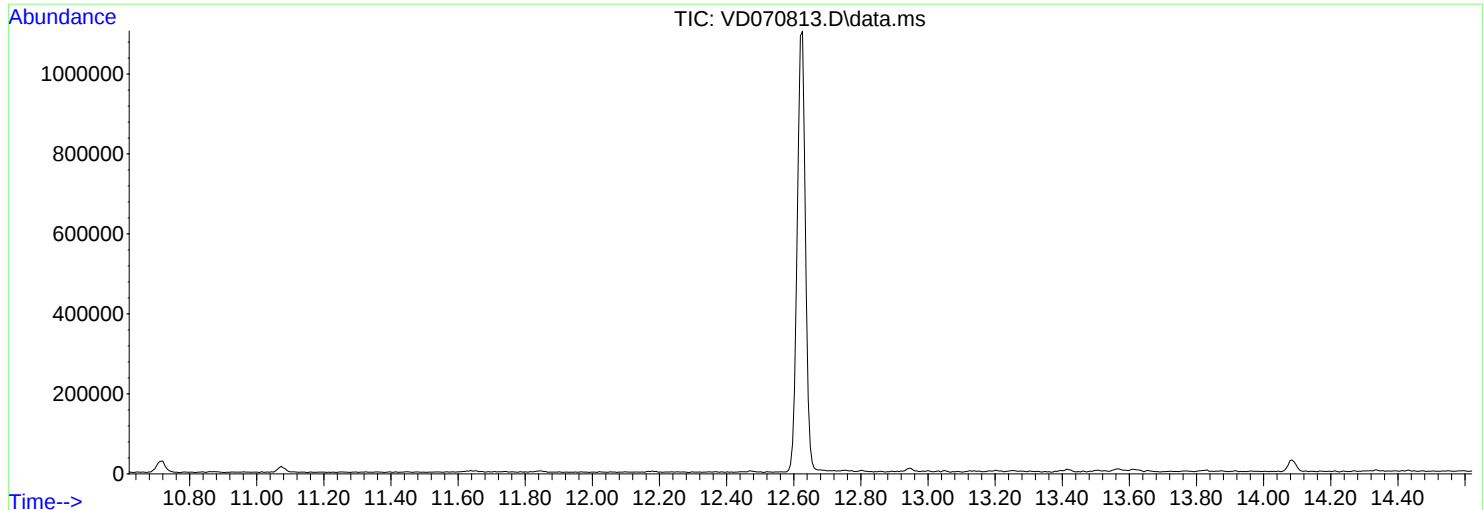

AutoFind: Scans 1818, 1819, 1820; Background Corrected with Scan 1809

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.6	39147	PASS
75	95	30	60	50.8	101144	PASS
95	95	100	100	100.0	199296	PASS
96	95	5	9	6.6	13123	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	74.2	147880	PASS
175	174	5	9	8.9	13179	PASS
176	174	95	101	96.4	142571	PASS
177	176	5	9	6.6	9361	PASS