


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD102418\
 Data File : VD060174.D
 Acq On : 24 Oct 2018 10:16
 Operator : JC/SY
 Sample : BFB
 Misc : 5.00g/5ml/MSVOA D/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D100118S.M
 Title : SW846 8260
 Last Update : Tue Oct 02 06:56:35 2018

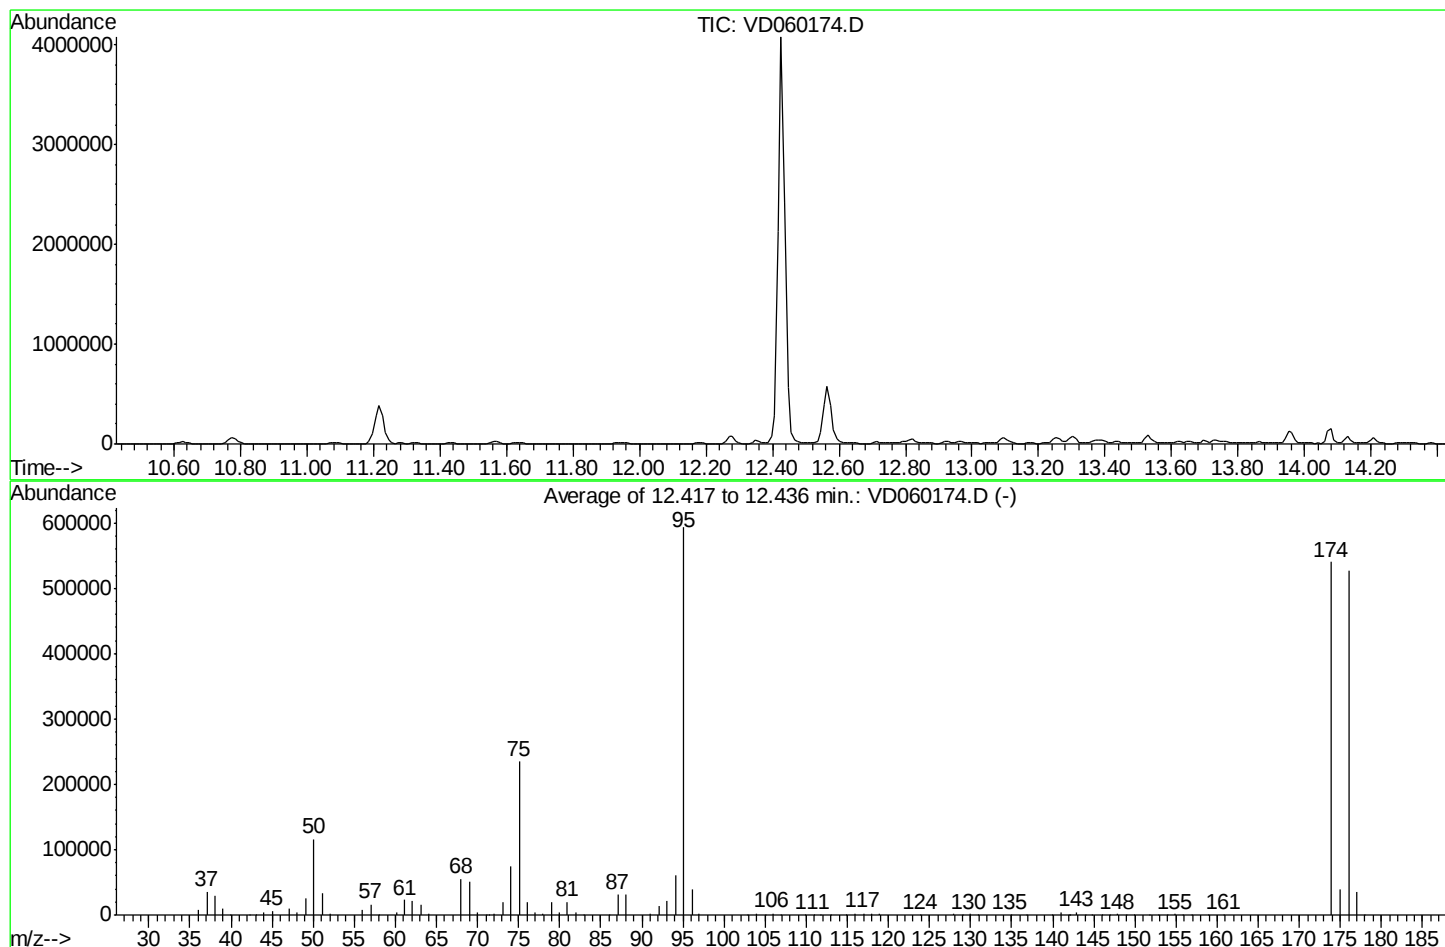

AutoFind: Scans 1107, 1108, 1109; Background Corrected with Scan 1102

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.5	115730	PASS
75	95	30	60	39.5	234453	PASS
95	95	100	100	100.0	593258	PASS
96	95	5	9	6.7	39914	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	91.1	540373	PASS
175	174	5	9	7.1	38626	PASS
176	174	95	101	97.4	526229	PASS
177	176	5	9	6.6	34970	PASS