


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD102519\
Data File : VD064060.D
Acq On : 25 Oct 2019 11:09
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D100219S.M
Title : SW846 8260
Last Update : Sat Oct 05 03:51:17 2019

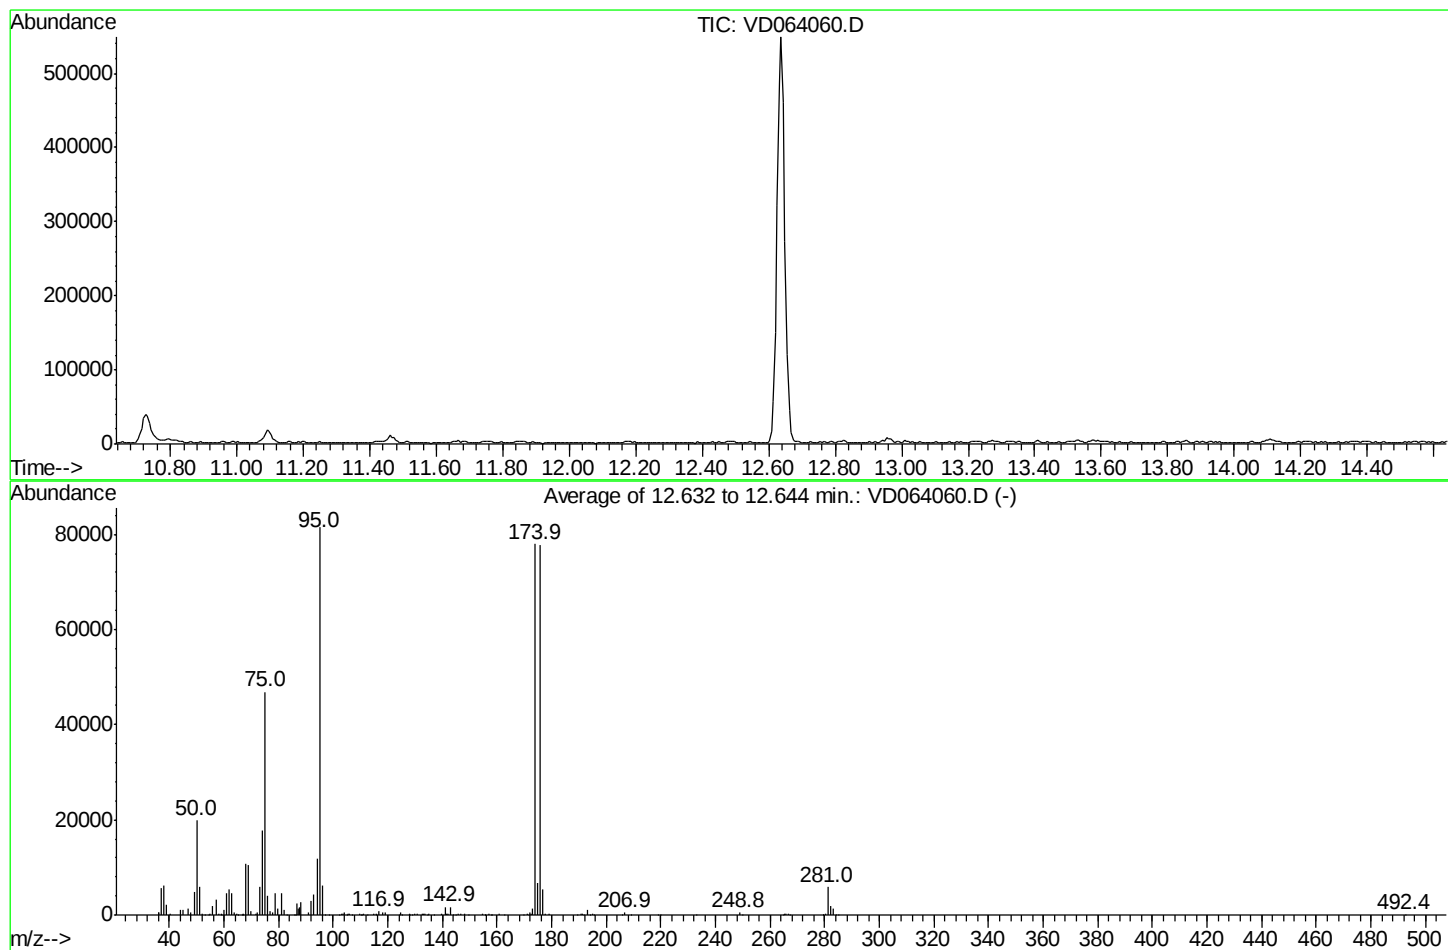

AutoFind: Scans 1821, 1822, 1823; Background Corrected with Scan 1813

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.4	19882	PASS
75	95	30	60	57.5	46882	PASS
95	95	100	100	100.0	81472	PASS
96	95	5	9	7.7	6237	PASS
173	174	0.00	2	1.6	1235	PASS
174	95	50	100	95.7	77933	PASS
175	174	5	9	8.7	6818	PASS
176	174	95	101	99.8	77773	PASS
177	176	5	9	6.8	5298	PASS