
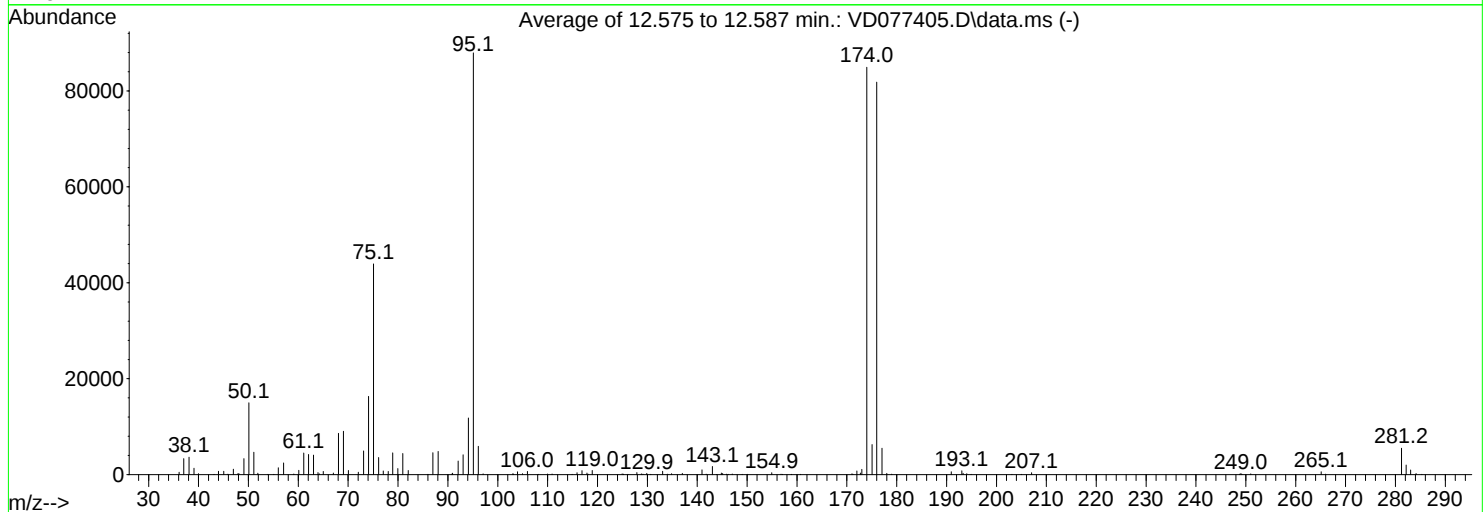


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD102523\
Data File : VD077405.D
Acq On : 25 Oct 2023 08:50
Operator : JC/SY
Sample : BFB
Misc : 5.00G/5.0ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D101723S.M
Title : SW846 8260
Last Update : Wed Oct 18 03:02:43 2023

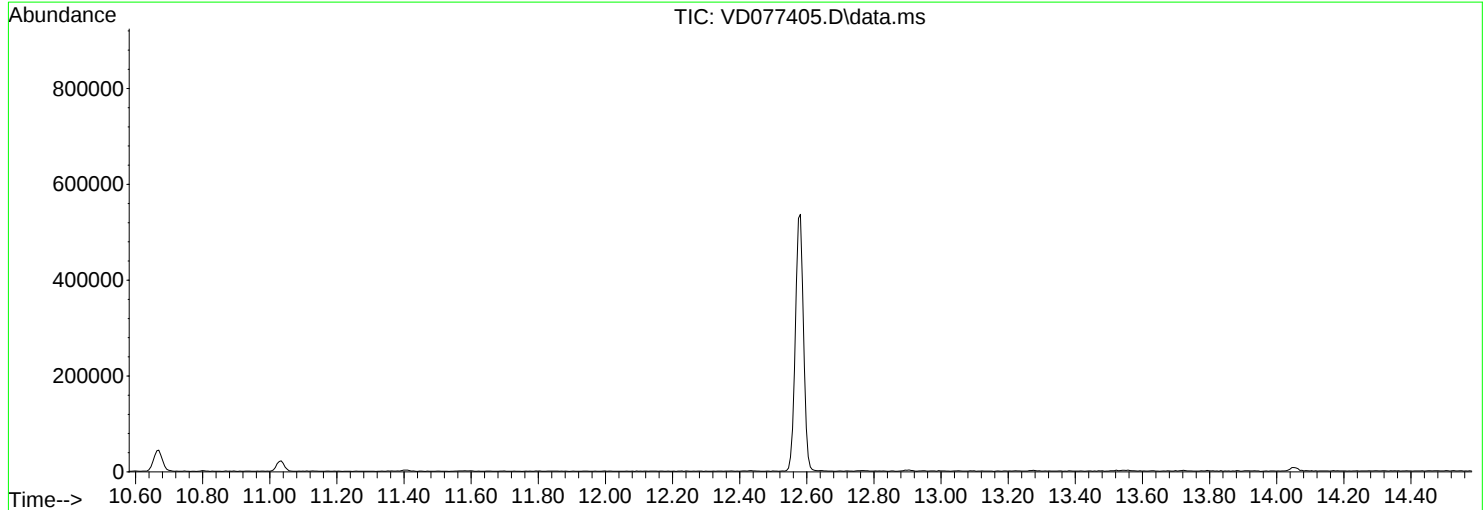

AutoFind: Scans 1868, 1869, 1870; Background Corrected with Scan 1859

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.0	14991	PASS
75	95	30	60	50.0	43944	PASS
95	95	100	100	100.0	87941	PASS
96	95	5	9	6.7	5916	PASS
173	174	0.00	2	1.3	1119	PASS
174	95	50	100	96.6	84941	PASS
175	174	5	9	7.4	6291	PASS
176	174	95	101	96.3	81821	PASS
177	176	5	9	6.7	5517	PASS