

Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD102618\
 Data File : VD060218.D
 Acq On : 26 Oct 2018 16:08
 Operator : JC/SY
 Sample : J5658-07
 Misc : 5.02g/5ml/MSVOA D/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 JC-TS-005

Quant Time: Oct 27 00:15:00 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D100118S.M
 Quant Title : SW846 8260
 QLast Update : Tue Oct 02 06:56:35 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	6.41	168	1519672	50.00	ug/l	0.02
34) 1,4-Difluorobenzene	7.44	114	2121612	50.00	ug/l	0.02
63) Chlorobenzene-d5	11.28	117	1576437	50.00	ug/l	0.01
72) 1,4-Dichlorobenzene-d4	13.37	152	626353	50.00	ug/l	0.01

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.78	65	670313	58.19	ug/l	0.02
Spiked Amount	50.000		Recovery	=	116.38%	
35) Dibromofluoromethane	6.32	113	831870	51.63	ug/l	0.02
Spiked Amount	50.000		Recovery	=	103.26%	
50) Toluene-d8	9.46	98	2178639	47.42	ug/l	0.02
Spiked Amount	50.000		Recovery	=	94.84%	
62) 4-Bromofluorobenzene	12.42	95	669447	38.92	ug/l	0.00
Spiked Amount	50.000		Recovery	=	77.84%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD102618\
Data File : VD060218.D
Acq On : 26 Oct 2018 16:08
Operator : JC/SY
Sample : J5658-07
Misc : 5.02g/5ml/MSVOA D/SOIL
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
JC-TS-005

Quant Time: Oct 27 00:15:00 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D100118S.M
Quant Title : SW846 8260
QLast Update : Tue Oct 02 06:56:35 2018
Response via : Initial Calibration

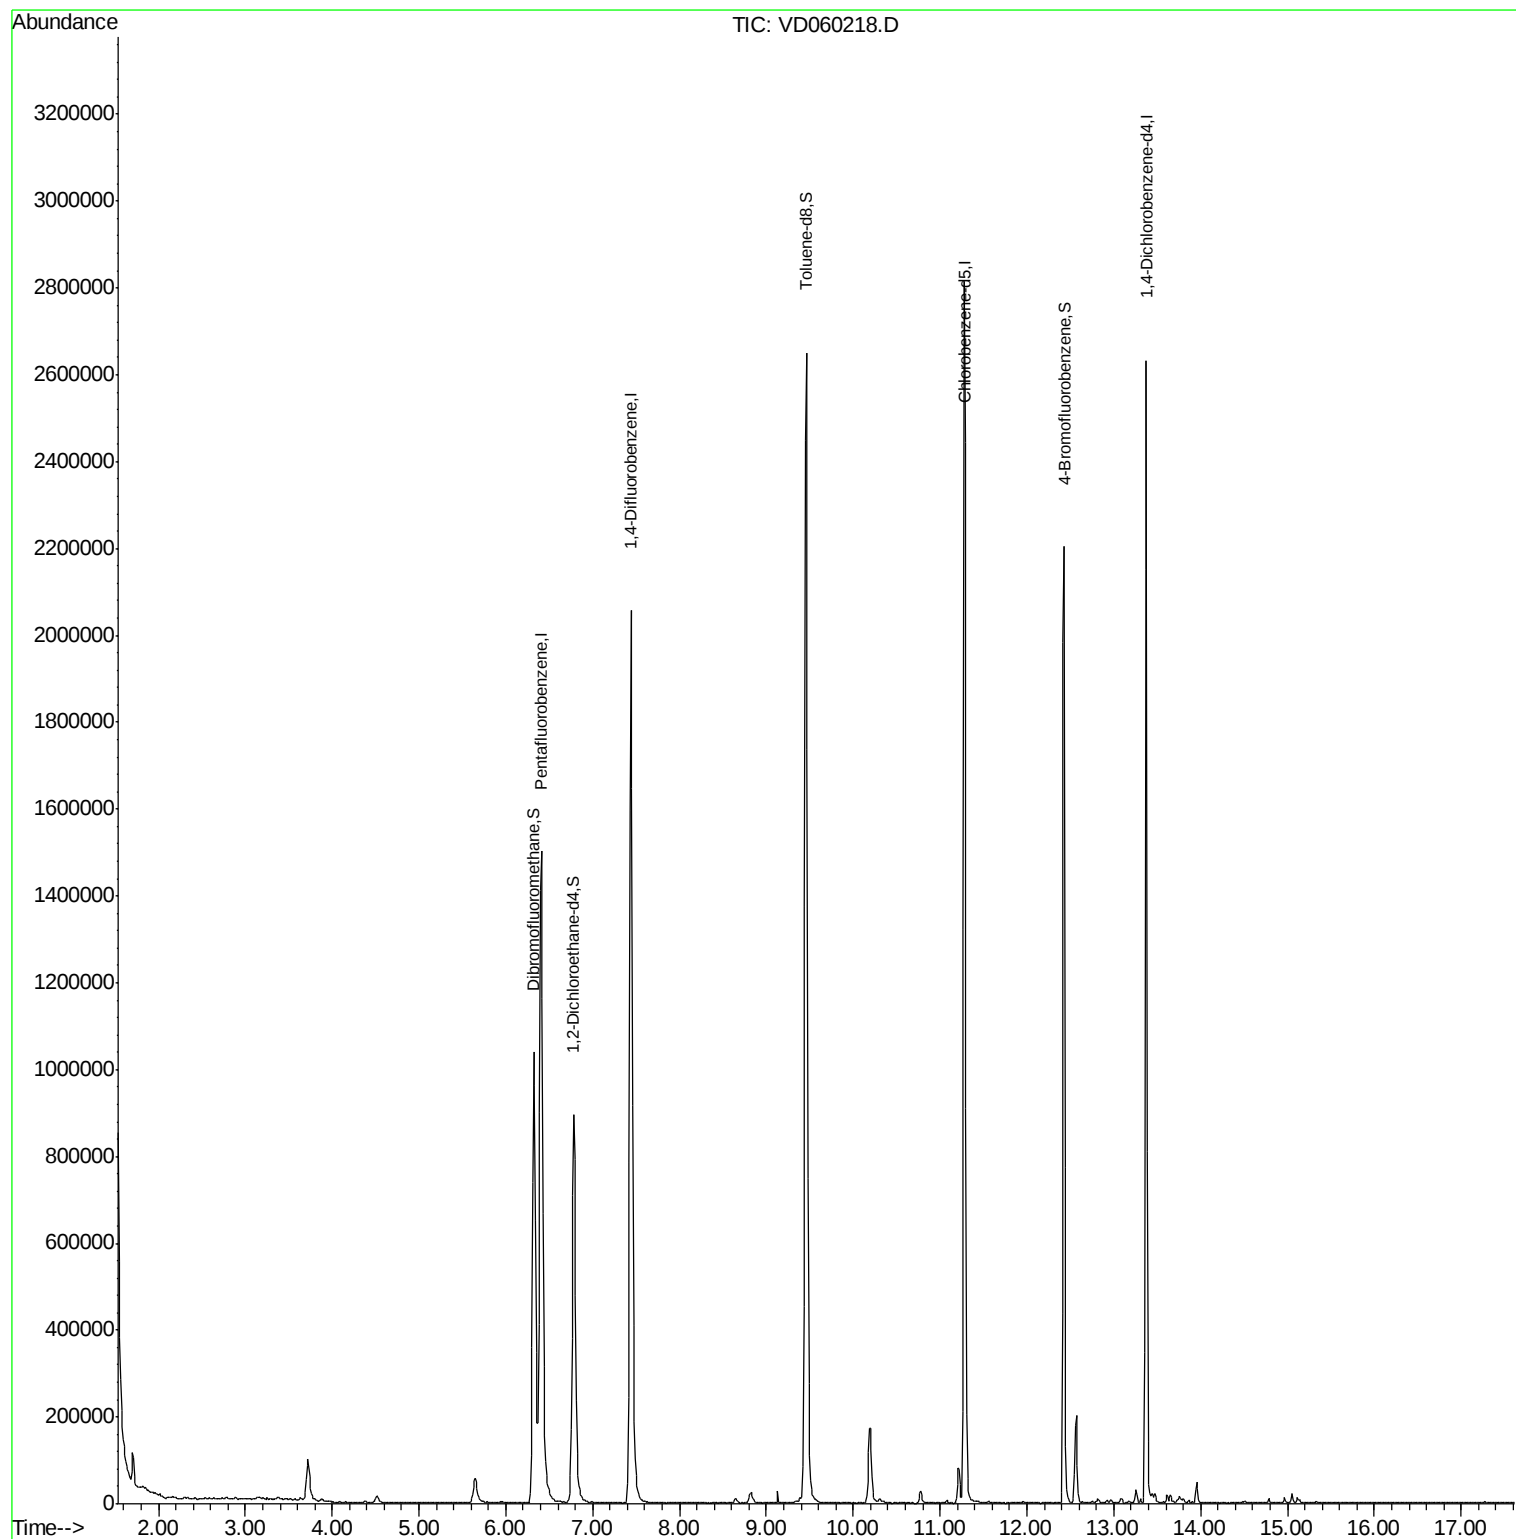

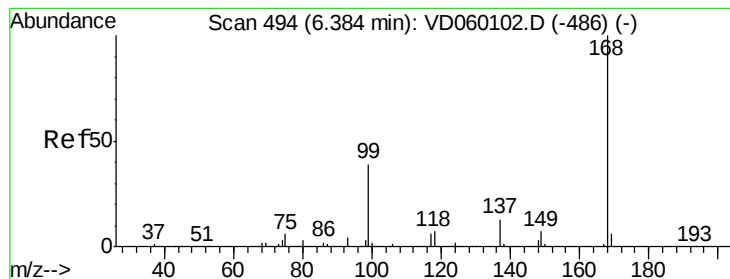

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 6.41 min Scan# 496

Delta R.T. 0.02 min

Lab File: VD060218.D

Acq: 26 Oct 2018 16:08

Instrument :

MSVOA_D

ClientSampleId :


JC-TS-005

Tot Ion:168 Resp: 1519672

Ion Ratio Lower Upper

168 100

99 47.3 35.4 53.0

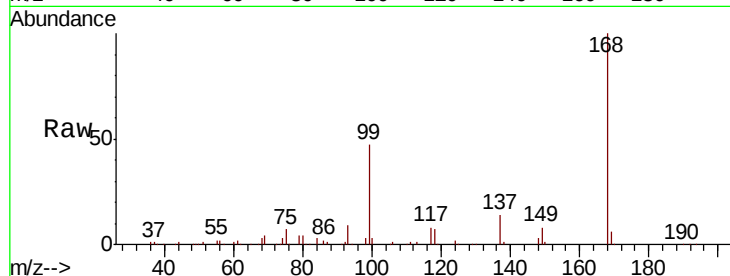

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.95 (98.65 to 99.65): VDC

6.41



600000

400000

200000

0

Time-->

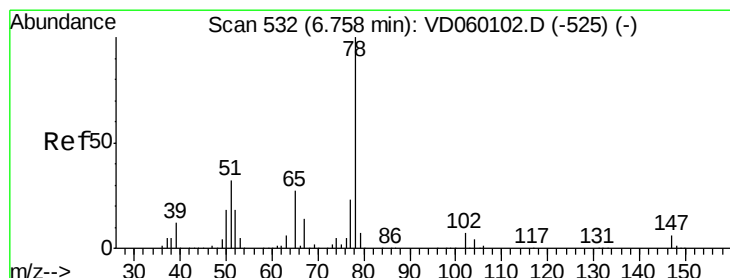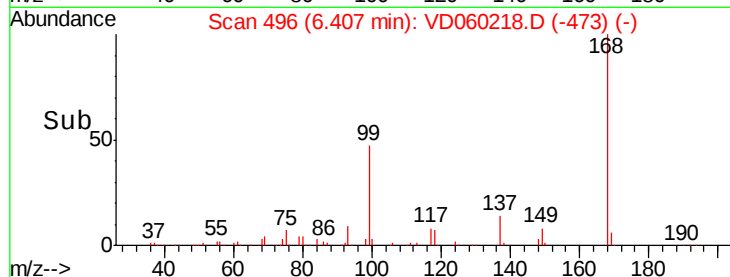

#33

1,2-Dichloroethane-d4

Concen: N.D. ug/l

RT: 6.78 min Scan# 534

Delta R.T. 0.02 min

Lab File: VD060218.D


Acq: 26 Oct 2018 16:08

Tgt Ion: 65 Resp: 670313

Ion Ratio Lower Upper

65 100

67 50.8 0.0 106.2

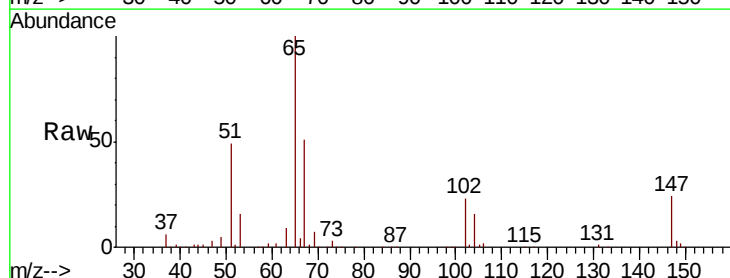

Abundance Ion 64.95 (64.65 to 65.65): VDC

Ion 66.90 (66.60 to 67.60): VDC

6.78

300000

250000

200000


150000


100000

50000

0

Time-->

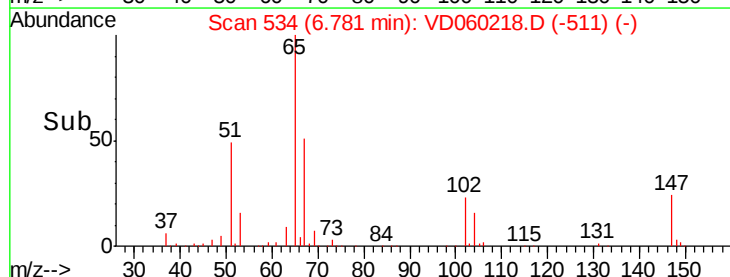


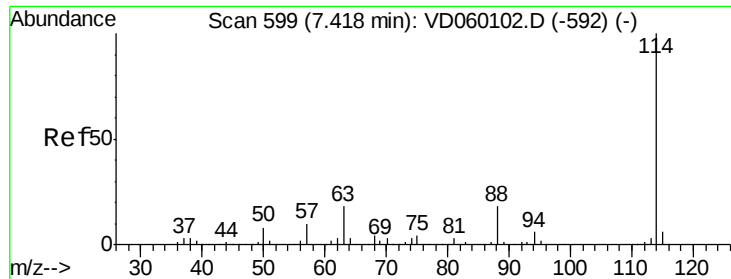




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 7.44 min Scan# 601
 Delta R.T. 0.02 min
 Lab File: VD060218.D
 Acq: 26 Oct 2018 16:08

Instrument :
 MSVOA_D
 ClientSampleId :
 JC-TS-005

Tot Ion:114 Resp: 2121612
 Ion Ratio Lower Upper
 114 100
 63 18.6 0.0 36.0
 88 19.0 0.0 36.2

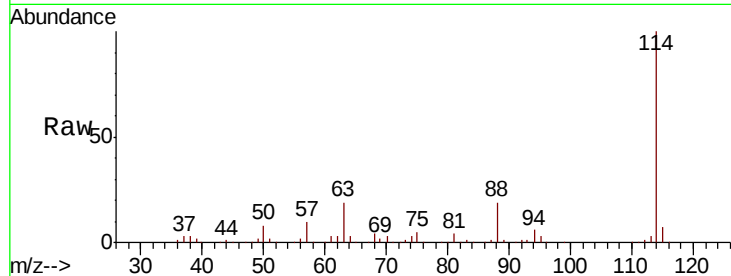


Abundance Ion 114.00 (113.70 to 114.70): V
 Ion 62.95 (62.65 to 63.65): V
 Ion 87.90 (87.60 to 88.60): V

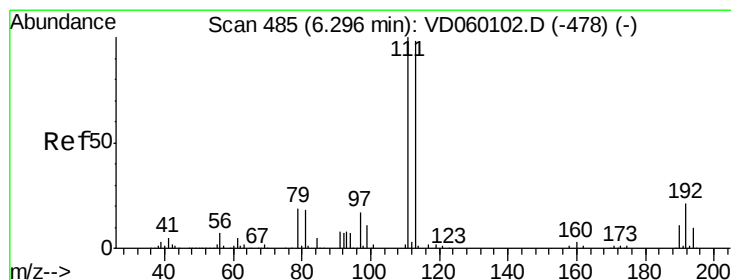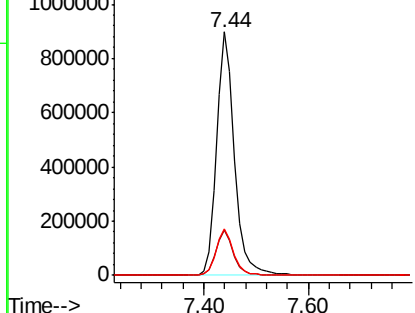
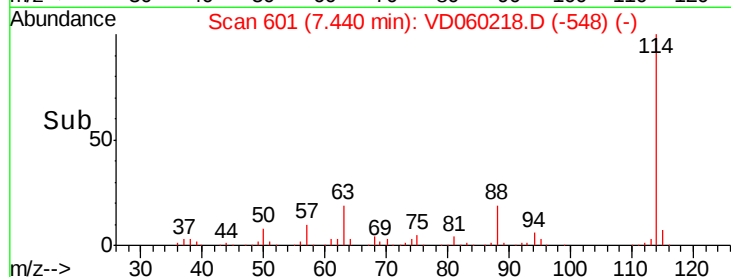



#35
 Dibromofluoromethane
 Concen: 50.000 ug/l
 RT: 6.32 min Scan# 487
 Delta R.T. 0.02 min
 Lab File: VD060218.D
 Acq: 26 Oct 2018 16:08

Tgt Ion:113 Resp: 831870
 Ion Ratio Lower Upper
 113 100
 111 104.8 81.5 122.3
 192 20.0 17.4 26.0

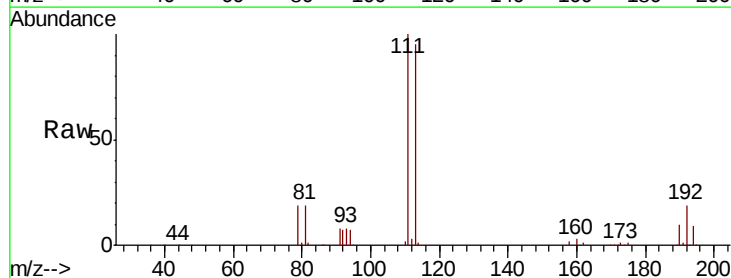

Abundance Ion 112.90 (112.60 to 113.60): V
 Ion 110.90 (110.60 to 111.60): V
 Ion 191.80 (191.50 to 192.50): V

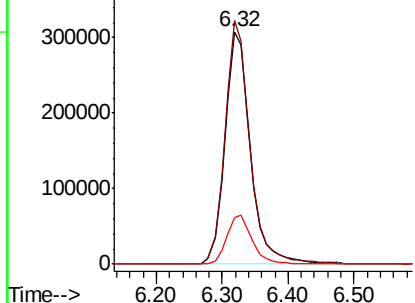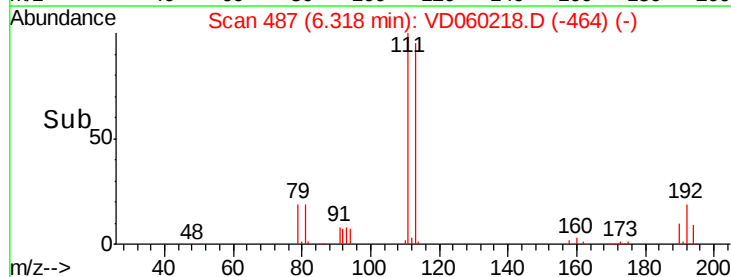


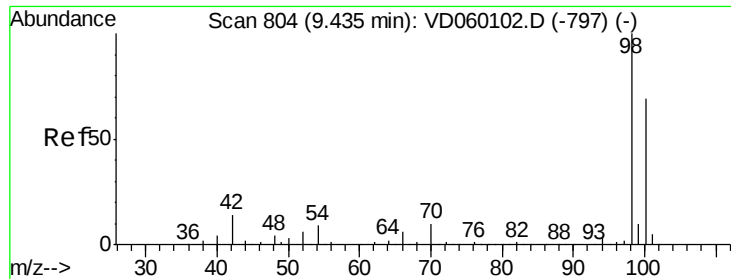




#50
Toluene-d8
Concen: N.D. ug/l
RT: 9.46 min Scan# 806
Delta R.T. 0.02 min
Lab File: VD060218.D
Acq: 26 Oct 2018 16:08

Instrument :
MSVOA_D
ClientSampleId :
JC-TS-005

Tot Ion: 98 Resp: 2178639
Ion Ratio Lower Upper
98 100
100 69.5 55.4 83.0

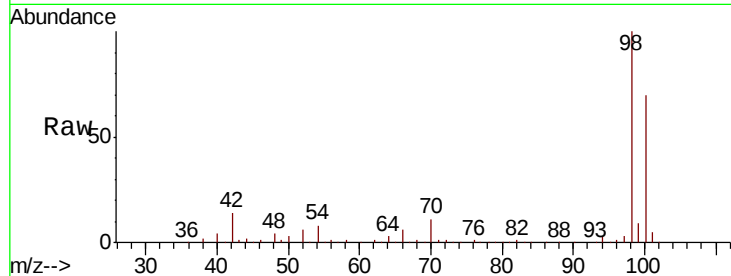


Abundance Ion 98.05 (97.75 to 98.75): VD060102.D (-797) (-)
Ion 100.05 (99.75 to 100.75): VD060102.D (-797) (-)

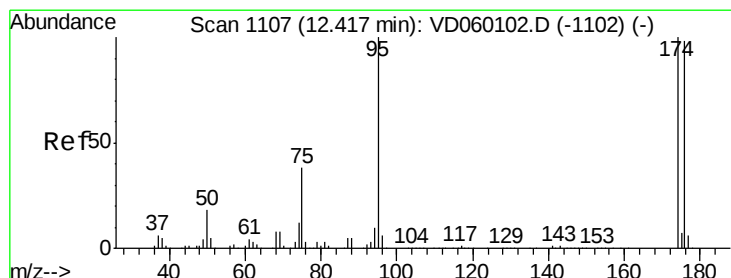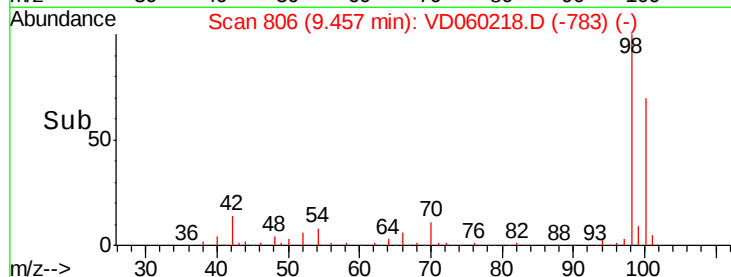
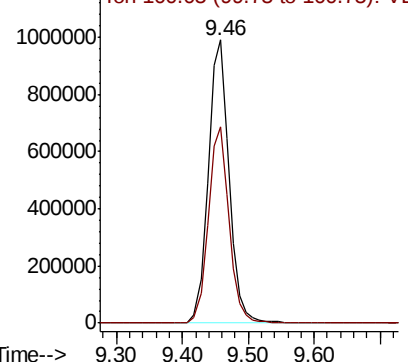



#62
4-Bromofluorobenzene
Concen: Below ug/l
RT: 12.42 min Scan# 1107
Delta R.T. 0.00 min
Lab File: VD060218.D
Acq: 26 Oct 2018 16:08

Tgt Ion: 95 Resp: 669447
Ion Ratio Lower Upper
95 100
174 73.1 0.0 200.2
176 69.7 0.0 195.6

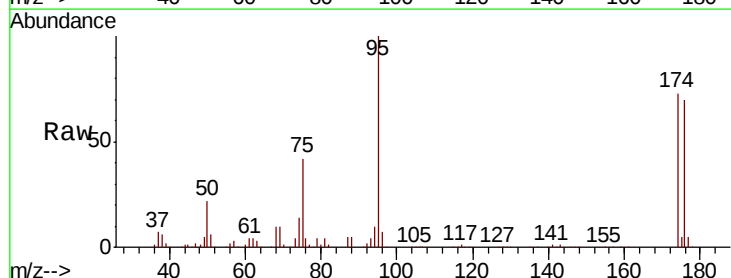

Abundance Ion 95.00 (94.70 to 95.70): VD060102.D (-1102) (-)
Ion 173.90 (173.60 to 174.60): VD060102.D (-1102) (-)
Ion 175.90 (175.60 to 176.60): VD060102.D (-1102) (-)

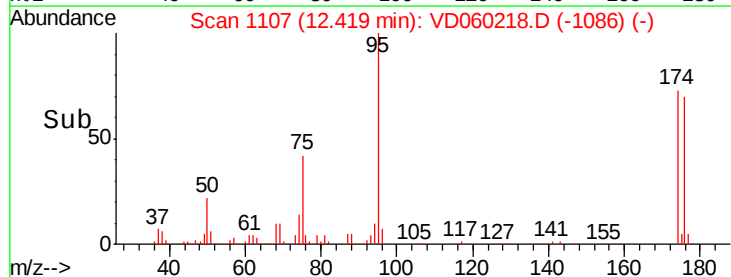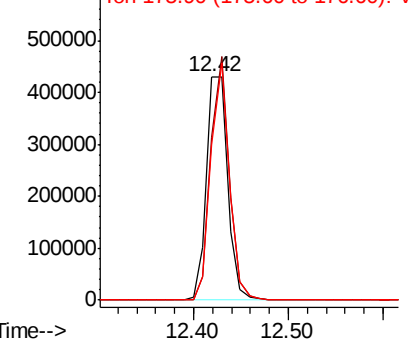


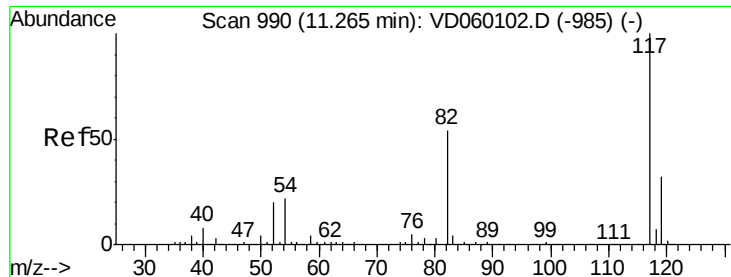




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.28 min Scan# 991
Delta R.T. 0.01 min
Lab File: VD060218.D
Acq: 26 Oct 2018 16:08

Instrument :
MSVOA_D
ClientSampleId :
JC-TS-005

Tot Ion:117 Resp: 1576437
Ion Ratio Lower Upper
117 100
82 57.9 43.4 65.2
119 32.6 26.0 39.0

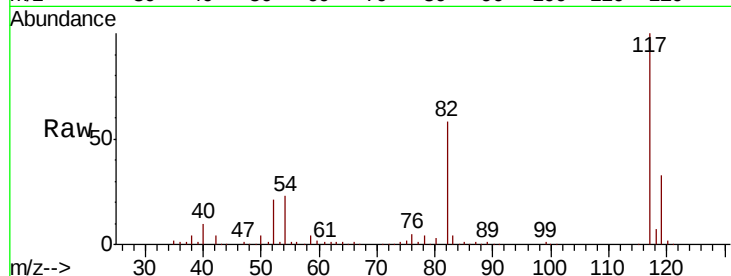


Abundance Ion 116.95 (116.65 to 117.65): V
Ion 82.05 (81.75 to 82.75): V
Ion 118.95 (118.65 to 119.65): V

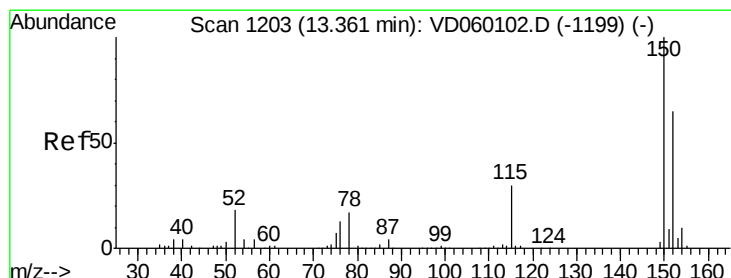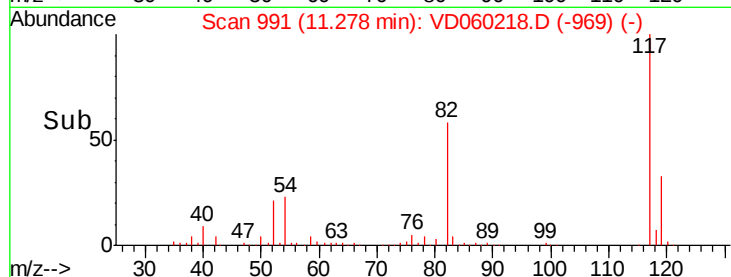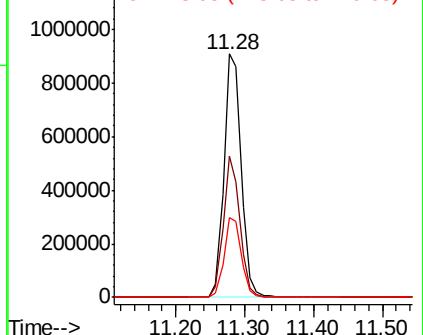

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.37 min Scan# 1204
Delta R.T. 0.01 min
Lab File: VD060218.D
Acq: 26 Oct 2018 16:08

Tgt Ion:152 Resp: 626353
Ion Ratio Lower Upper
152 100
115 48.4 27.1 81.2
150 155.0 0.0 311.8

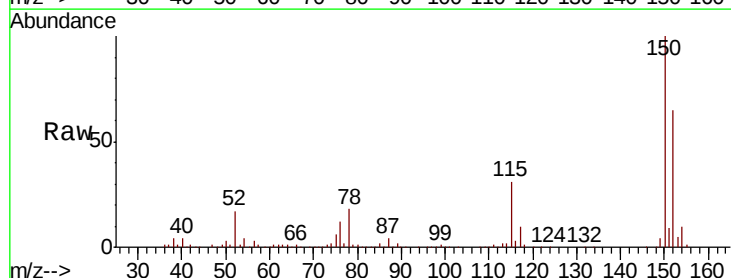

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 115.00 (114.70 to 115.70): V
Ion 149.90 (149.60 to 150.60): V

