


Bromomethane

Response Ratio

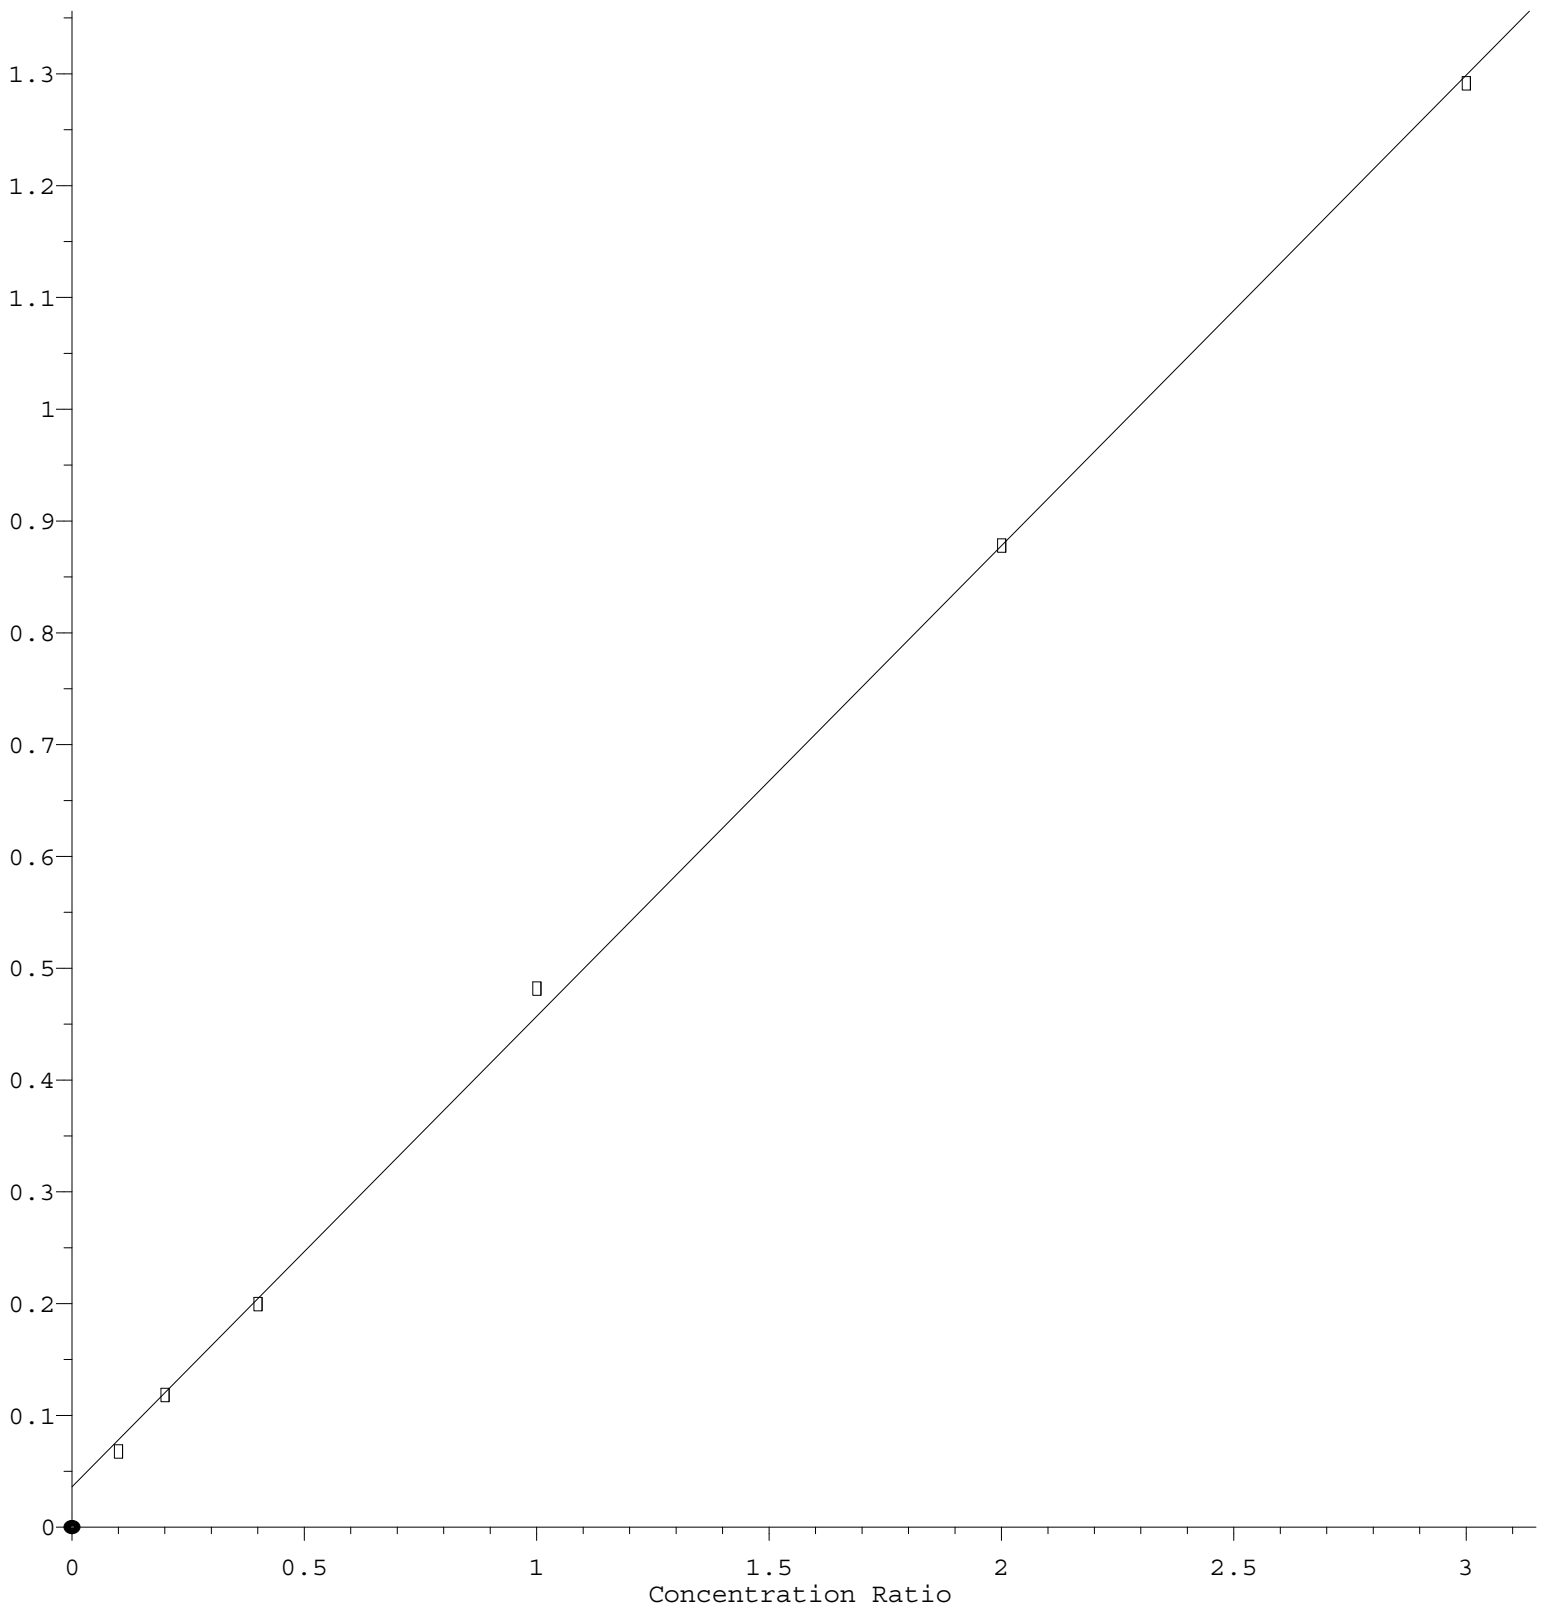

Response = 4.208e-001 \* Amt + 3.619e-002


Coef of Det (r^2) = 0.999328 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D102621S.M

Calibration Table Last Updated: Wed Oct 27 05:34:47 2021

# Naphthalene

Response Ratio

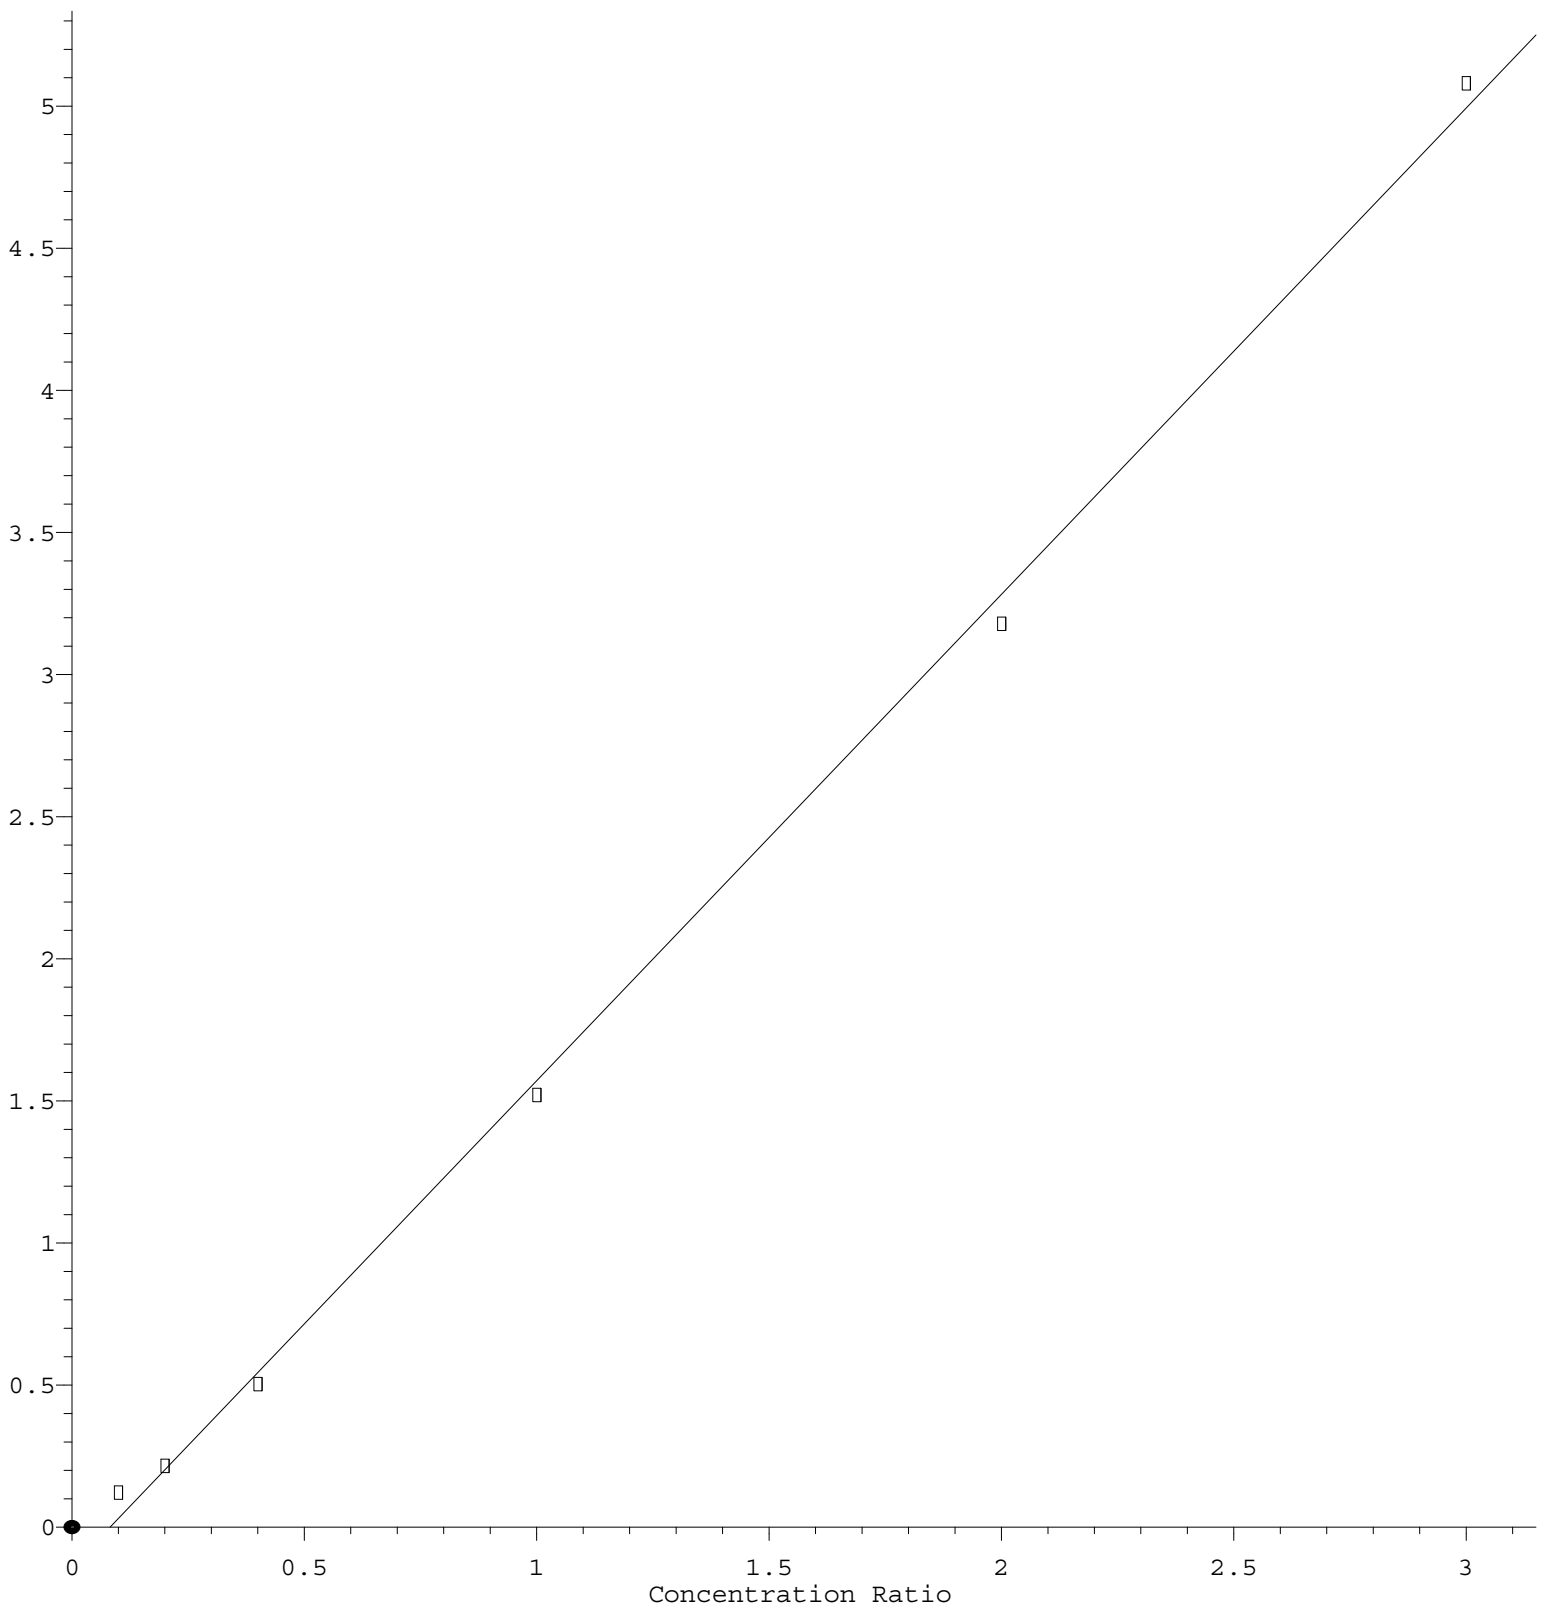

$$\text{Response} = 1.712e+000 * \text{Amt} - 1.412e-001$$


Coef of Det ( $r^2$ ) = 0.998433 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D102621S.M

Calibration Table Last Updated: Wed Oct 27 05:34:47 2021

Methyl Iodide

Response Ratio

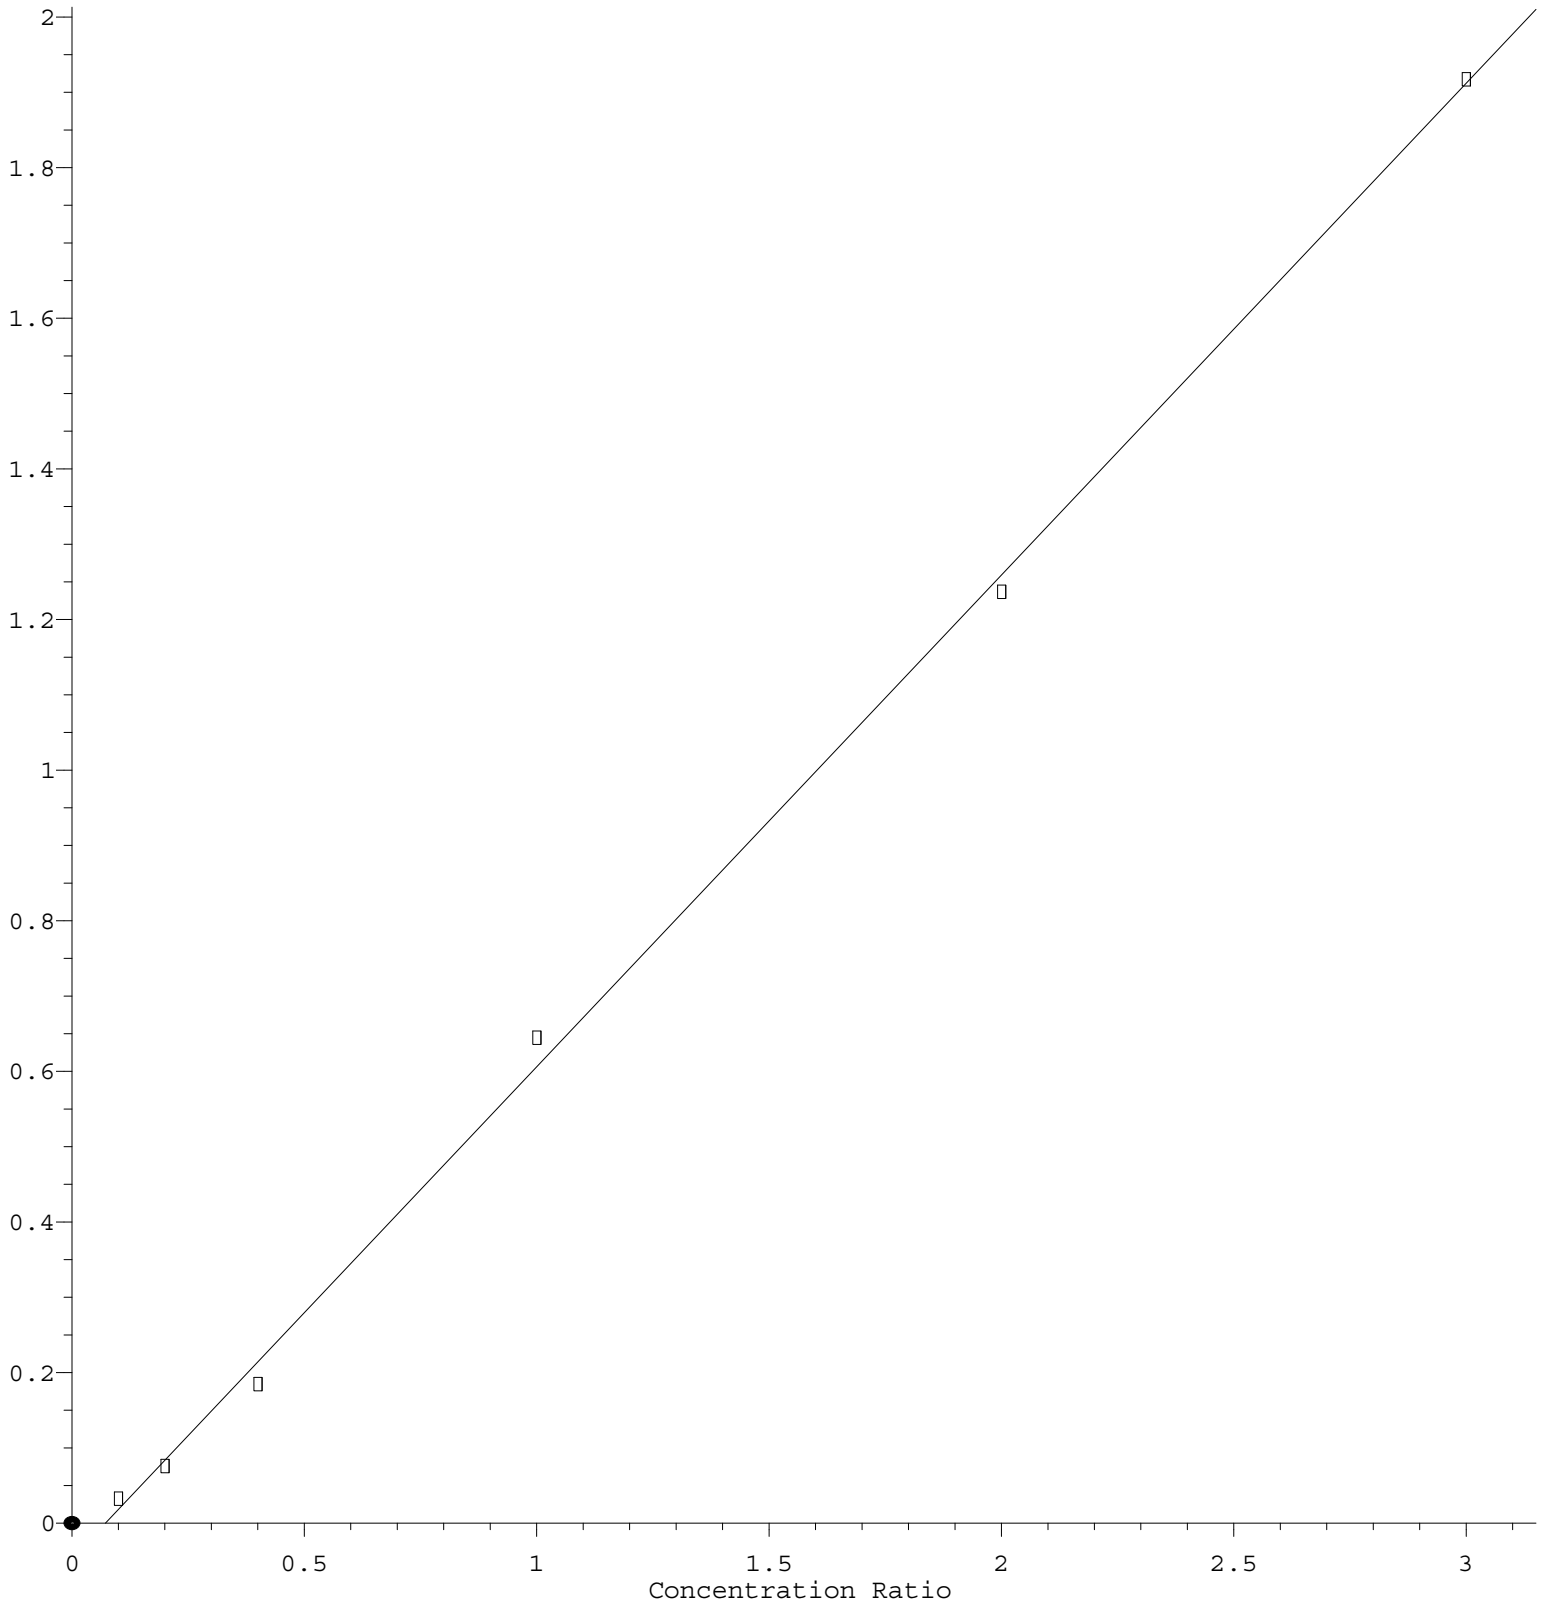

Response = 6.529e-001 \* Amt - 4.714e-002


Coef of Det (r^2) = 0.998900 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D102621S.M

Calibration Table Last Updated: Wed Oct 27 05:34:47 2021

Methylene Chloride

Response Ratio

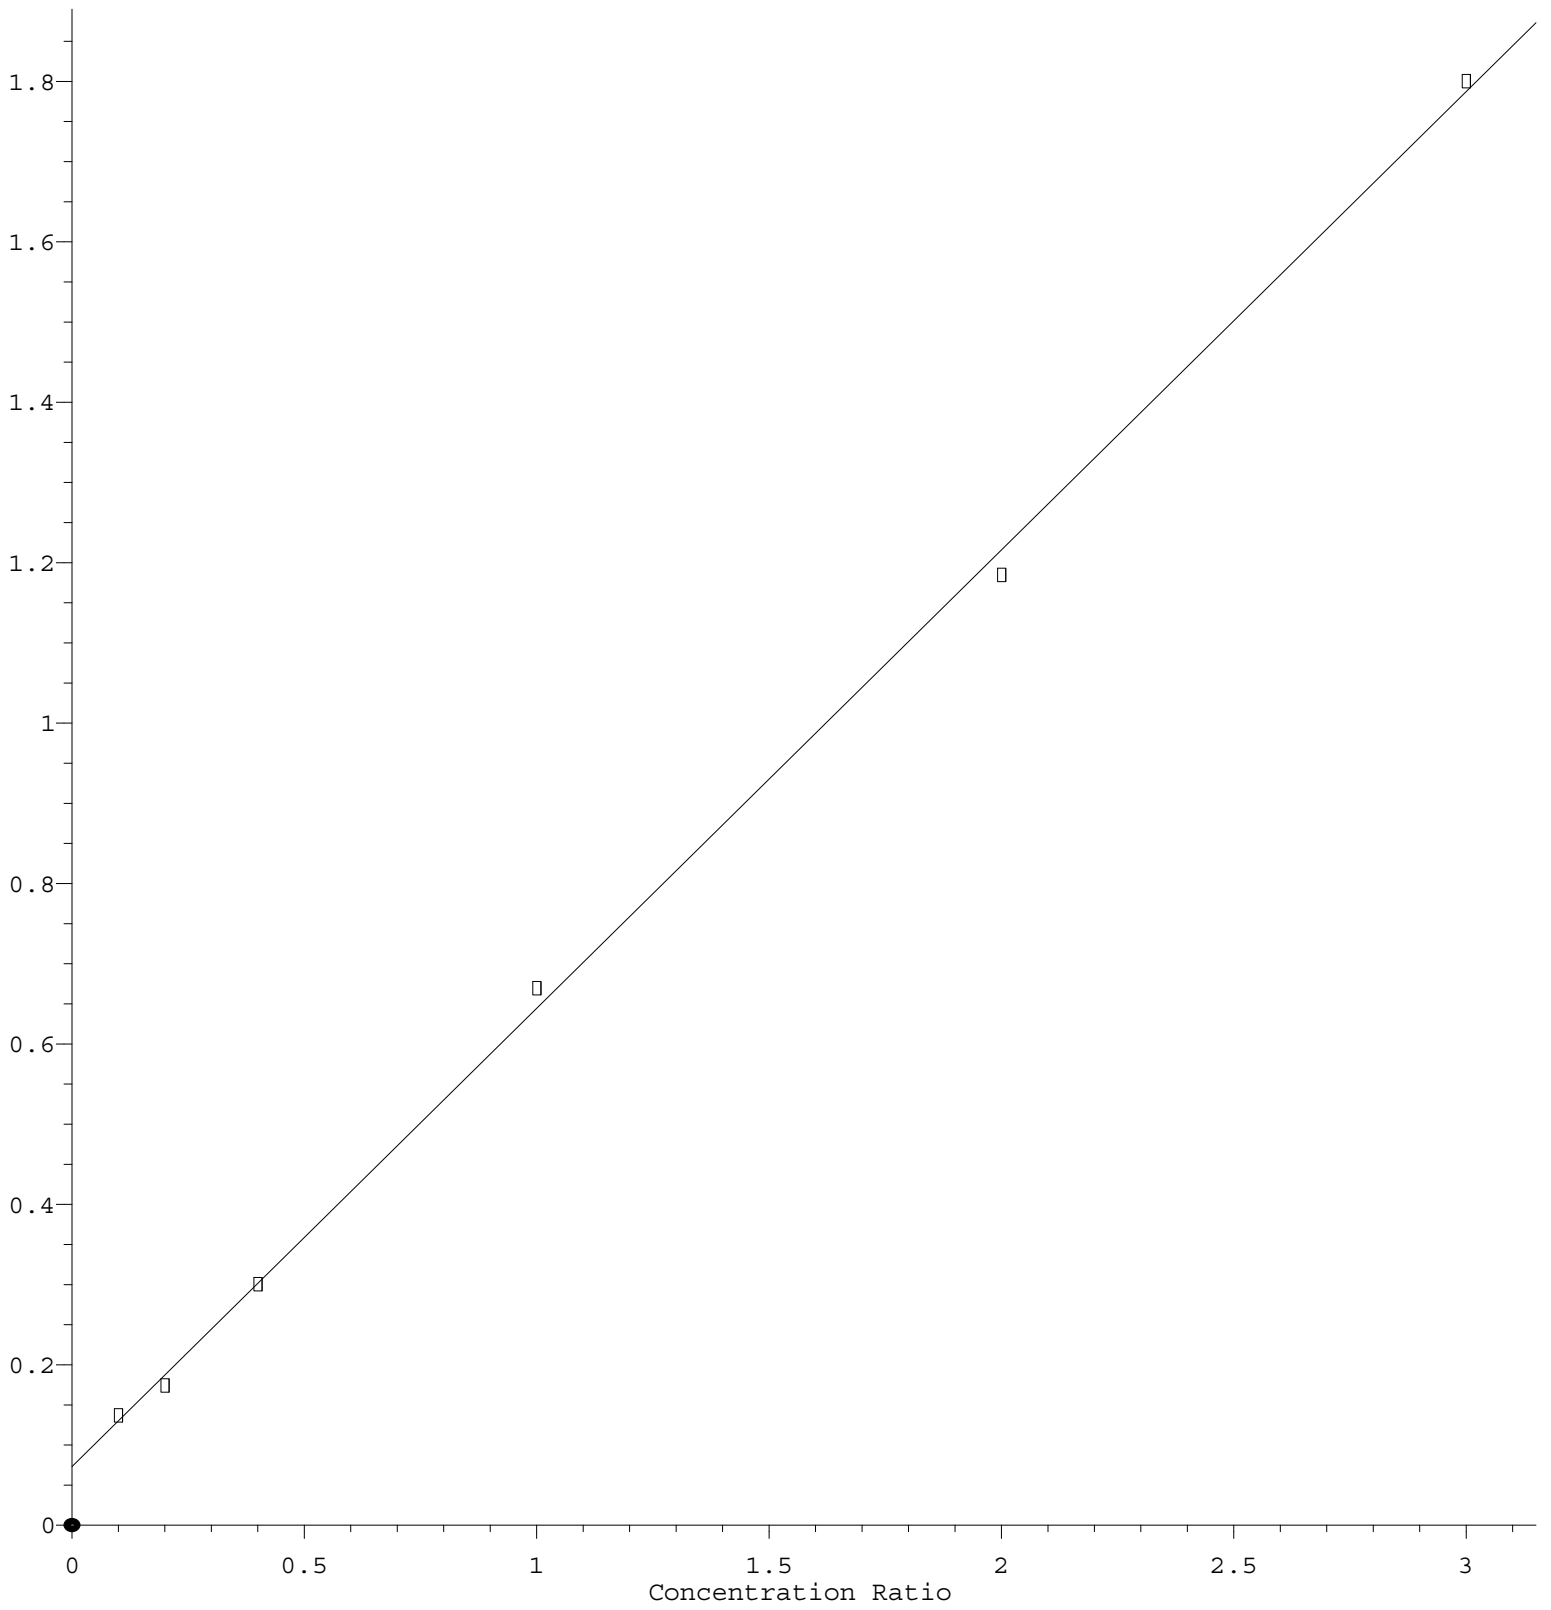

Response = 5.714e-001 \* Amt + 7.287e-002


Coef of Det (r^2) = 0.999099 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D102621S.M

Calibration Table Last Updated: Wed Oct 27 05:34:47 2021

Vinyl Acetate

Response Ratio

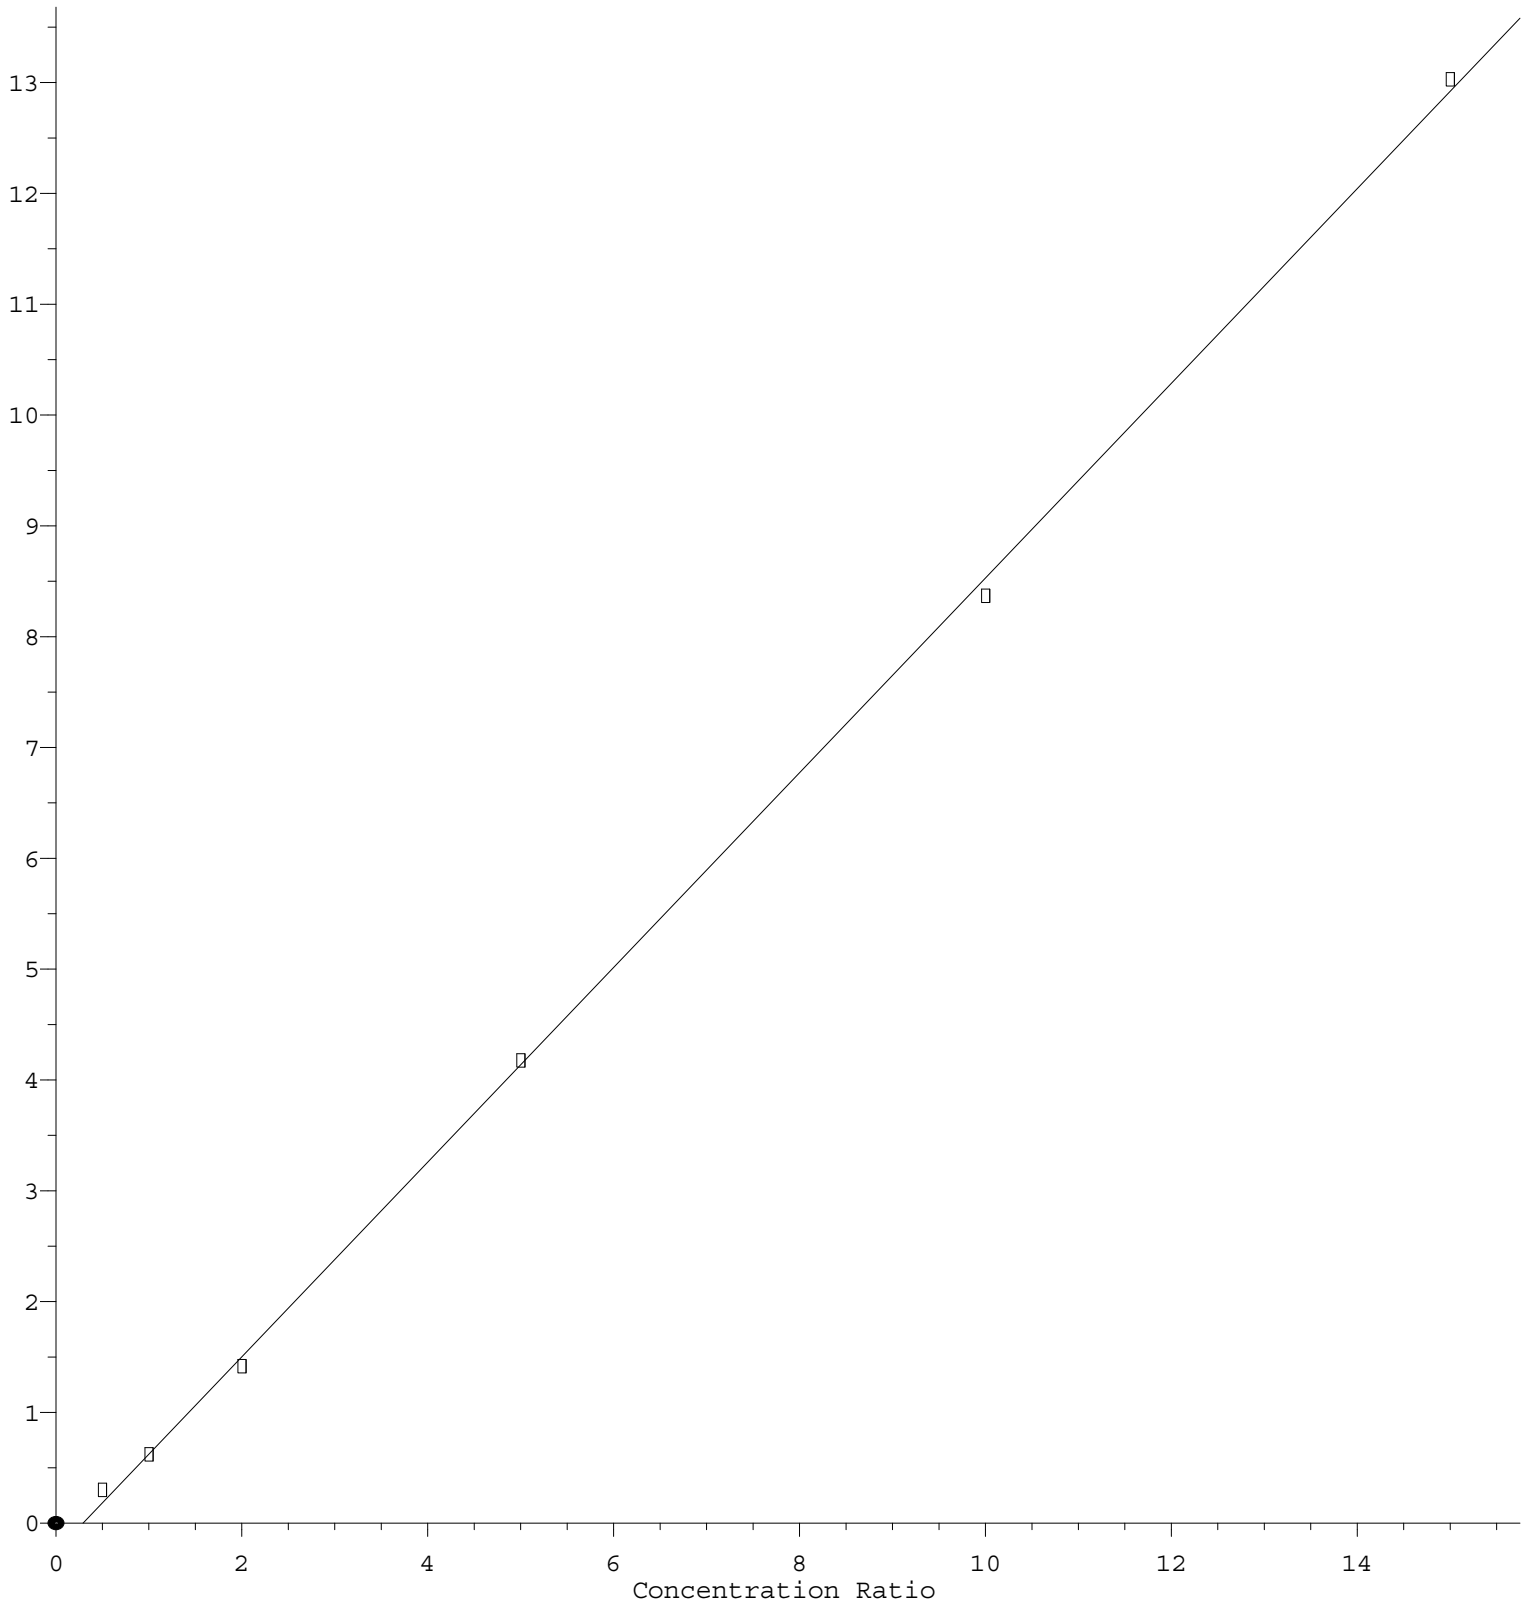

Response = 8.785e-001 \* Amt - 2.533e-001


Coef of Det (r^2) = 0.999540 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D102621S.M

Calibration Table Last Updated: Wed Oct 27 05:34:47 2021

Ethyl methacrylate

Response Ratio

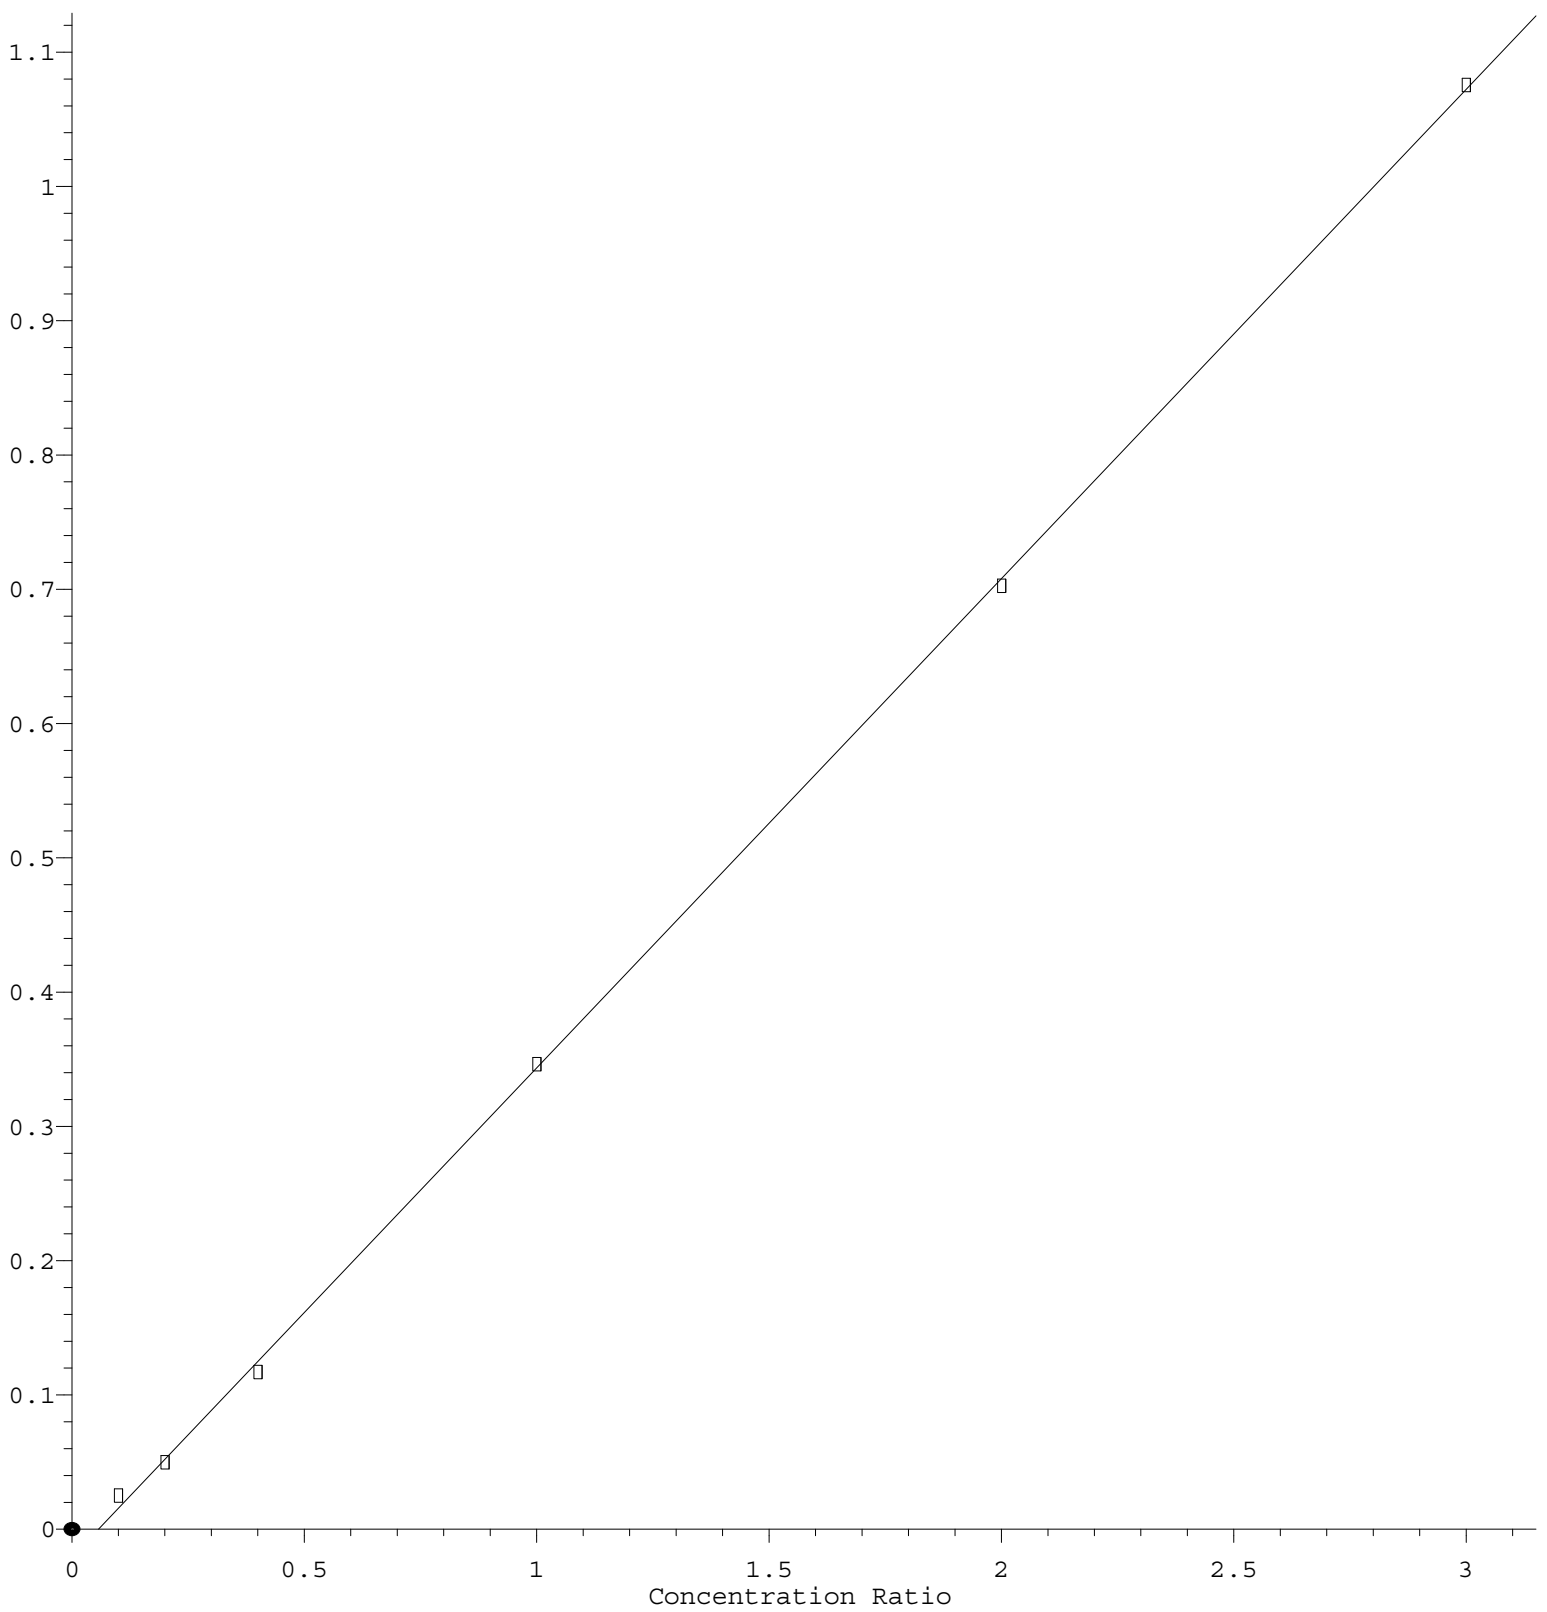

Response = 3.642e-001 \* Amt - 2.070e-002

Coef of Det (r^2) = 0.999773 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D102621S.M

Calibration Table Last Updated: Wed Oct 27 05:34:47 2021