

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD102623\
 Data File : VD077430.D
 Acq On : 26 Oct 2023 16:41
 Operator : JC/SY
 Sample : 05010-01RE
 Misc : 5.04G/5.0ml/MSVOA_D/SOIL
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 343RE

Quant Time: Oct 27 07:48:08 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D101723S.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 18 03:02:43 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.875	168	165951	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.775	114	354285	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.581	117	255383	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.516	152	85844	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.228	65	93622	63.179	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	126.360%
35) Dibromofluoromethane	7.805	113	105526	42.397	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	84.800%
50) Toluene-d8	10.269	98	317209	35.586	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	71.180%
62) 4-Bromofluorobenzene	12.575	95	72901	28.411	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	56.820%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD102623\
Data File : VD077430.D
Acq On : 26 Oct 2023 16:41
Operator : JC/SY
Sample : 05010-01RE
Misc : 5.04G/5.0ml/MSVOA_D/SOIL
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
343RE

Quant Time: Oct 27 07:48:08 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D101723S.M
Quant Title : SW846 8260
QLast Update : Wed Oct 18 03:02:43 2023
Response via : Initial Calibration




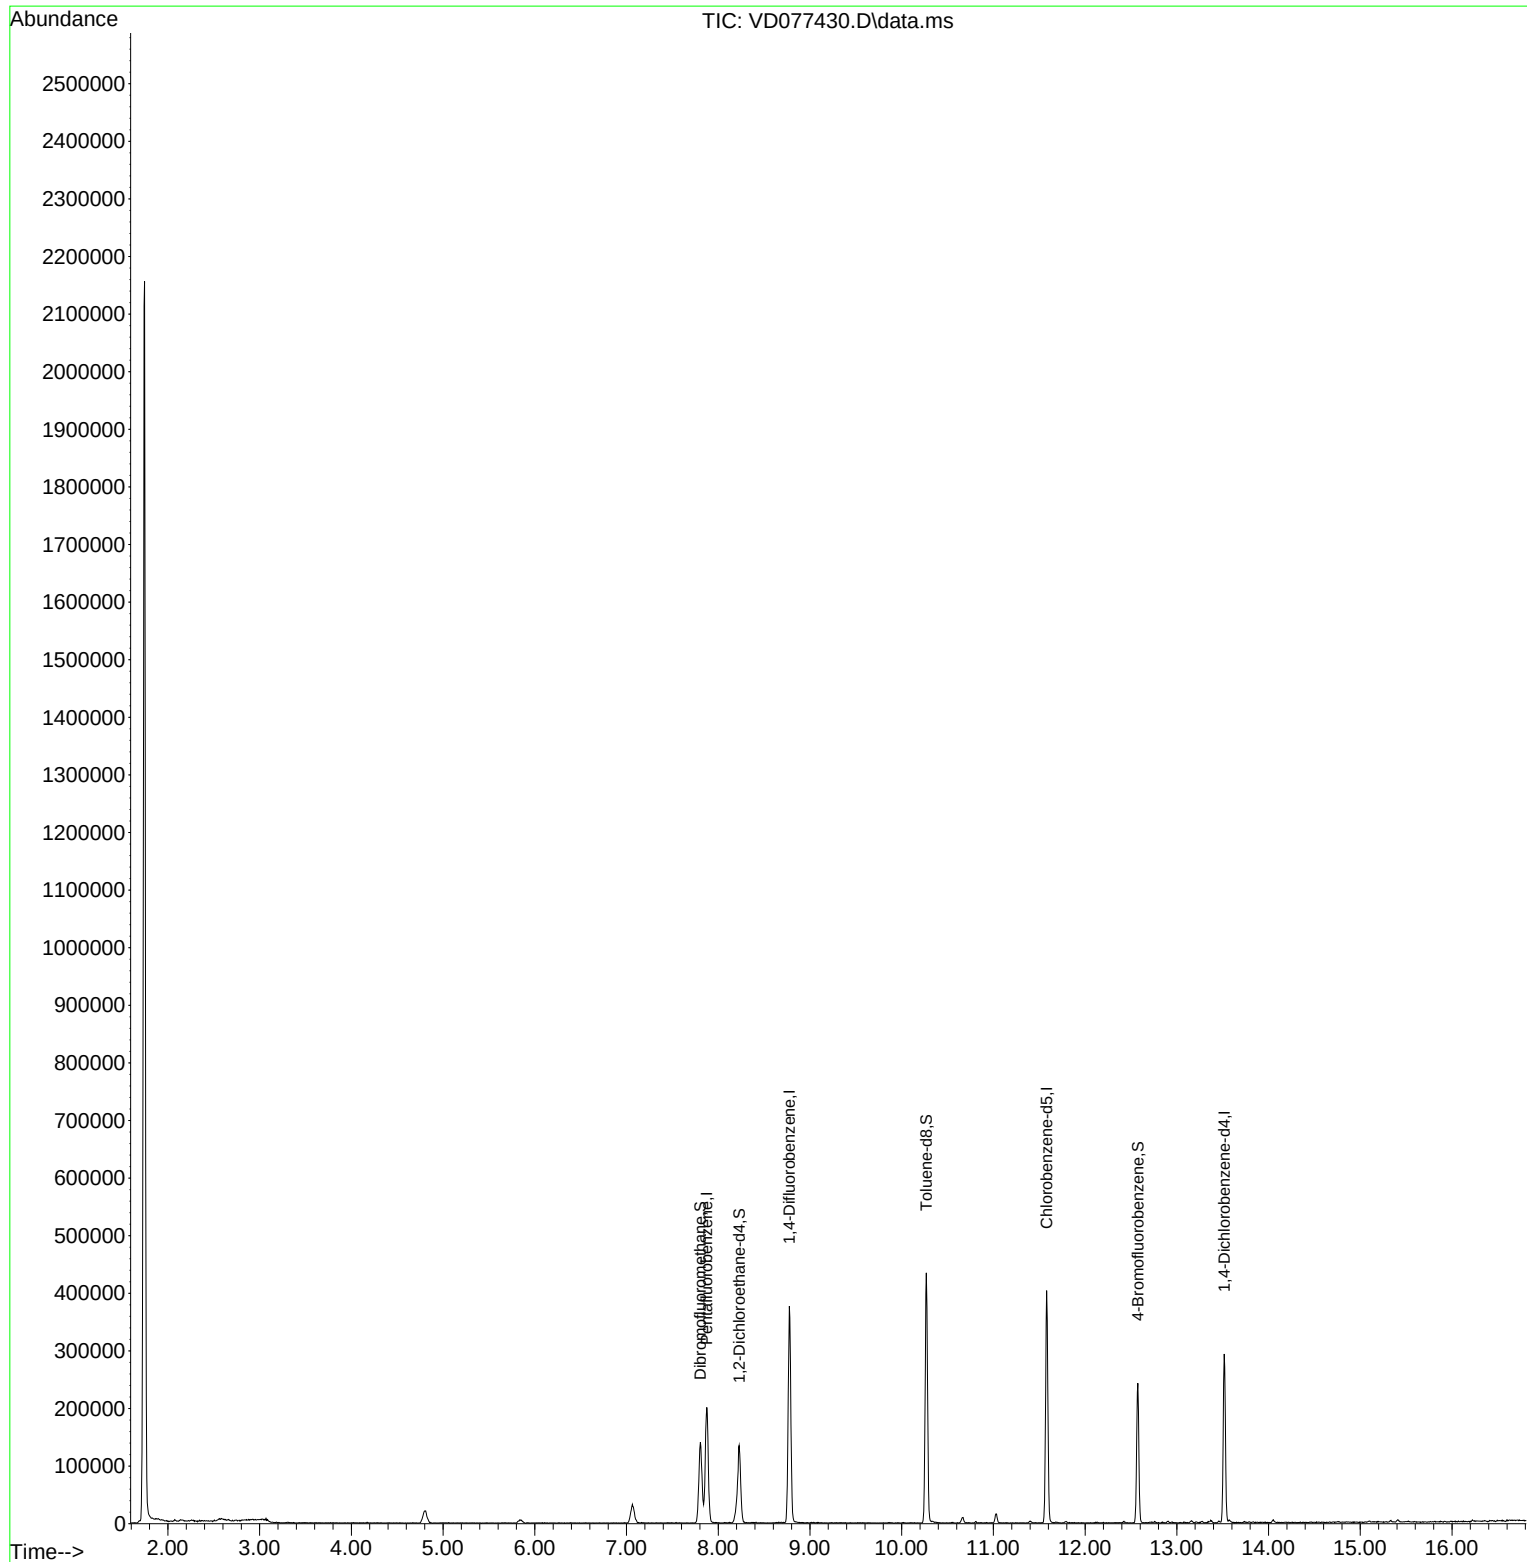


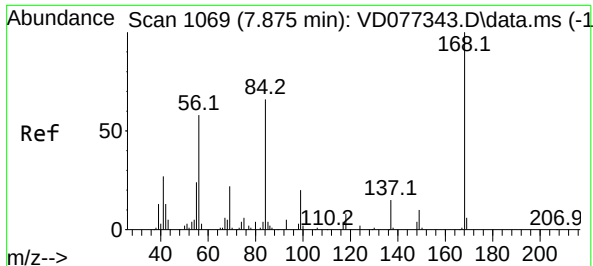

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.875 min Scan# 1069
Delta R.T. 0.000 min
Lab File: VD077430.D
Acq: 26 Oct 2023 16:41




Instrument :
MSVOA_D
ClientSampleId :
343RE


Tgt Ion:168 Resp: 165951
Ion Ratio Lower Upper
168 100
99 47.9 36.7 55.1

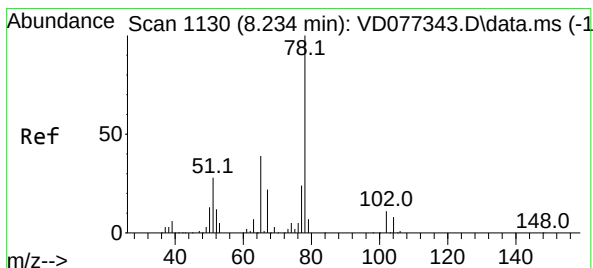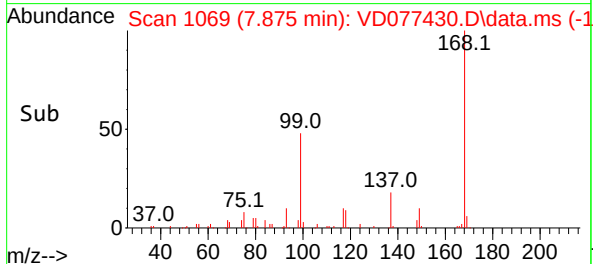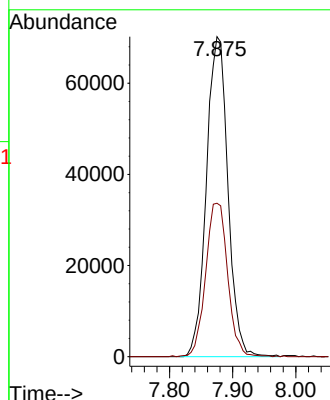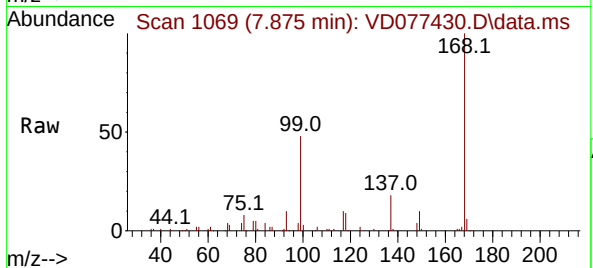

#33
1,2-Dichloroethane-d4
Concen: 63.179 ug/l
RT: 8.228 min Scan# 1129
Delta R.T. -0.006 min
Lab File: VD077430.D
Acq: 26 Oct 2023 16:41

Tgt Ion: 65 Resp: 93622
Ion Ratio Lower Upper
65 100
67 56.8 0.0 115.0


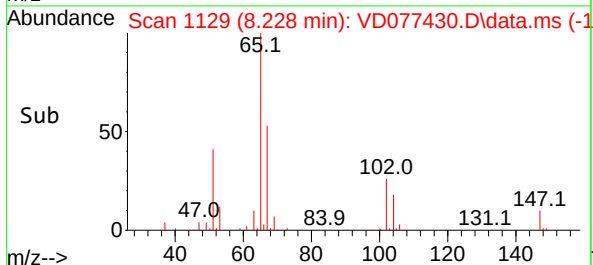
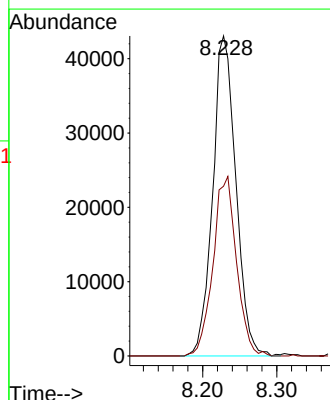
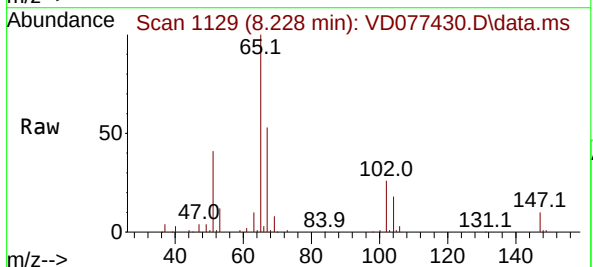


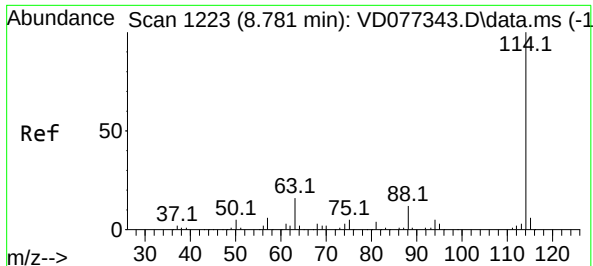

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.775 min Scan# 11
Delta R.T. -0.006 min
Lab File: VD077430.D
Acq: 26 Oct 2023 16:41




Instrument :
MSVOA_D
ClientSampleId :
343RE


Tgt Ion:114 Resp: 354285
Ion Ratio Lower Upper
114 100
63 16.0 0.0 33.4
88 13.0 0.0 26.2

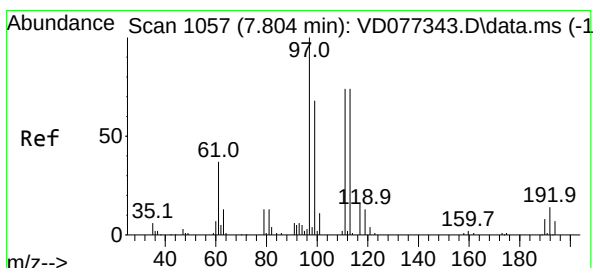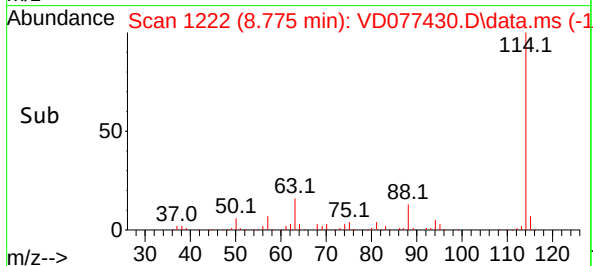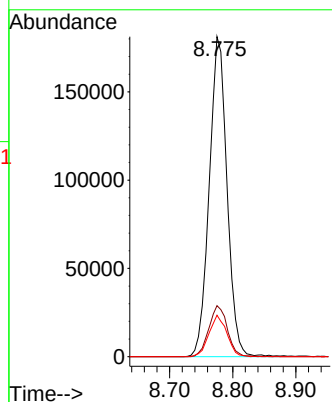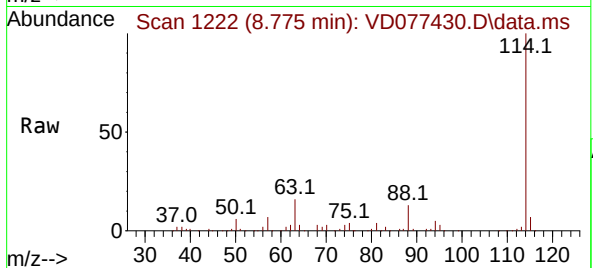

#35
Dibromofluoromethane
Concen: 42.397 ug/l
RT: 7.805 min Scan# 1057
Delta R.T. 0.001 min
Lab File: VD077430.D
Acq: 26 Oct 2023 16:41

Tgt Ion:113 Resp: 105526
Ion Ratio Lower Upper
113 100
111 100.4 84.7 127.1
192 20.0 16.8 25.2


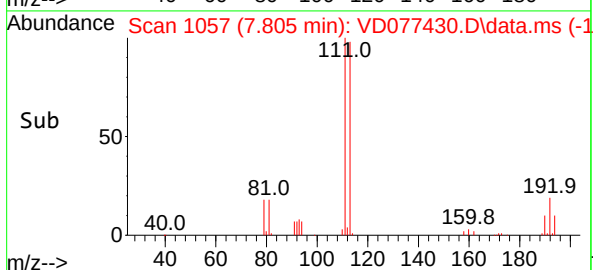
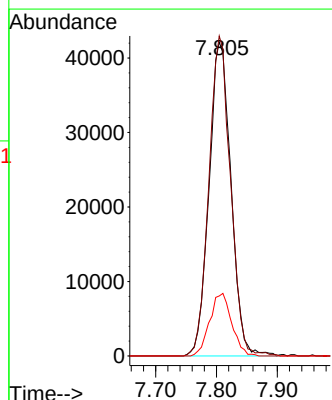
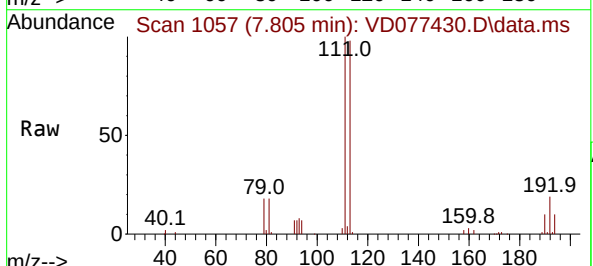


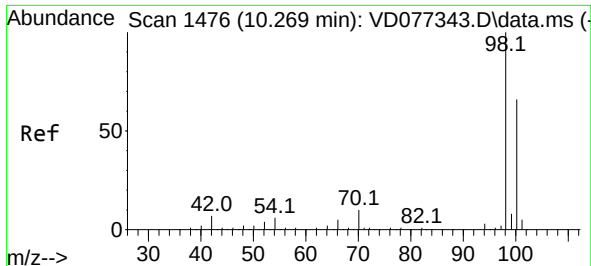

#50
Toluene-d8
Concen: 35.586 ug/l
RT: 10.269 min Scan# 1476
Delta R.T. 0.000 min
Lab File: VD077430.D
Acq: 26 Oct 2023 16:41




Instrument :
MSVOA_D
ClientSampleId :
343RE


Tgt Ion: 98 Resp: 317209
Ion Ratio Lower Upper
98 100
100 63.8 50.3 75.5

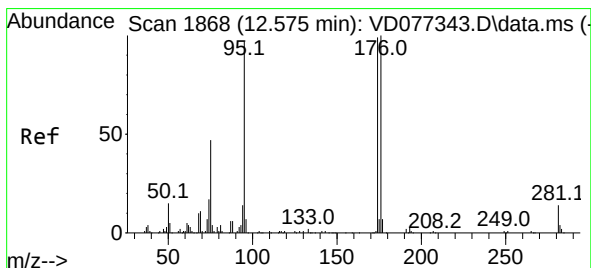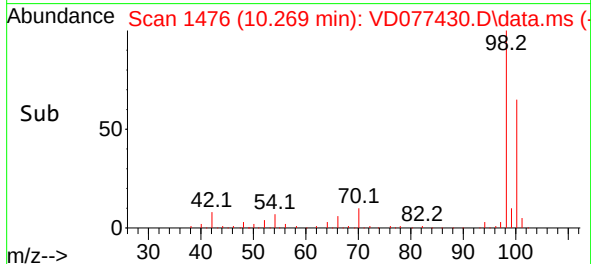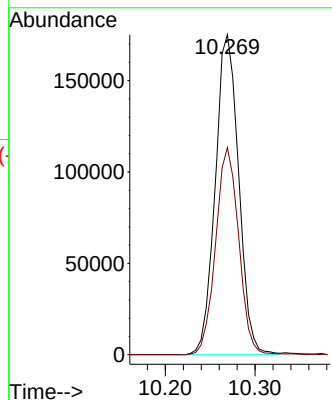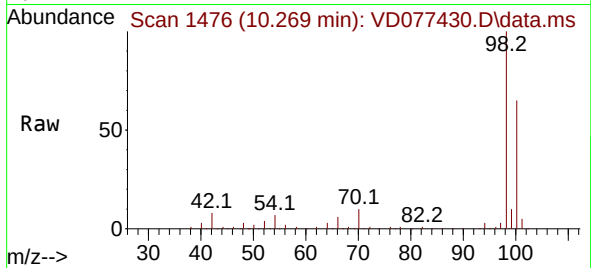

#62
4-Bromofluorobenzene
Concen: 28.411 ug/l
RT: 12.575 min Scan# 1868
Delta R.T. -0.000 min
Lab File: VD077430.D
Acq: 26 Oct 2023 16:41

Tgt Ion: 95 Resp: 72901
Ion Ratio Lower Upper
95 100
174 96.0 0.0 201.8
176 92.6 0.0 191.8


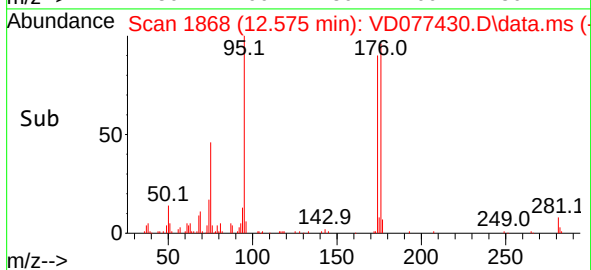
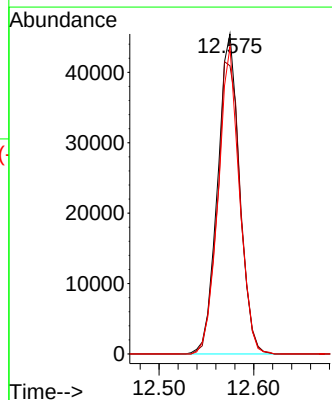
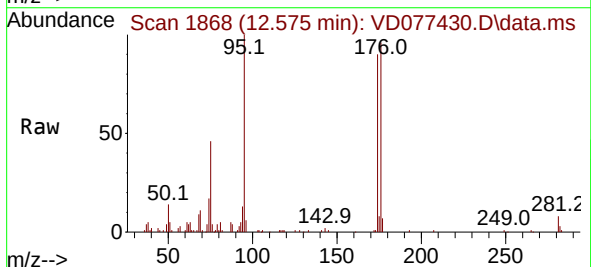


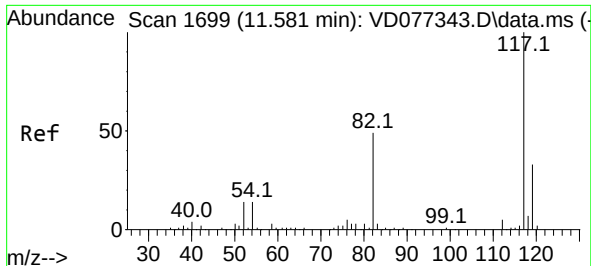

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.581 min Scan# 117
Delta R.T. -0.000 min
Lab File: VD077430.D
Acq: 26 Oct 2023 16:41

Instrument :
MSVOA_D
ClientSampleId :
343RE

Tgt Ion:117 Resp: 255383
Ion Ratio Lower Upper
117 100
82 46.3 38.3 57.5
119 28.7 25.0 37.4

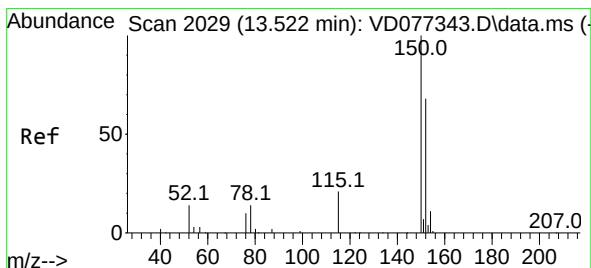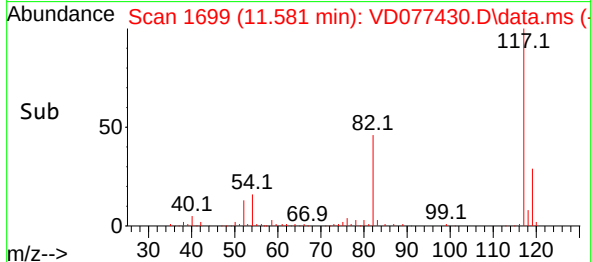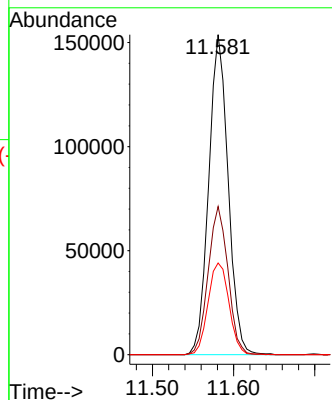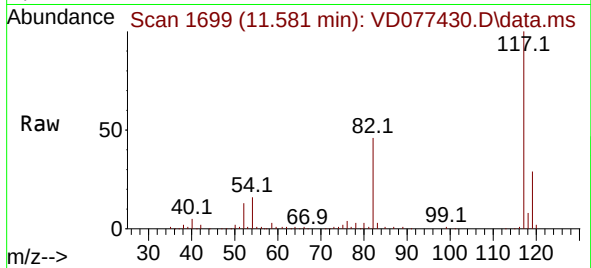

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.516 min Scan# 2028
Delta R.T. -0.006 min
Lab File: VD077430.D
Acq: 26 Oct 2023 16:41

Tgt Ion:152 Resp: 85844
Ion Ratio Lower Upper
152 100
115 52.5 27.1 81.3
150 157.3 0.0 353.6

