

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD102821\
 Data File : VD070894.D
 Acq On : 28 Oct 2021 15:55
 Operator : VA/SY
 Sample : M4372-07
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 SB-4

Quant Time: Oct 29 06:35:27 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D102621S.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 27 05:34:47 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.979	168	608834	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.861	114	1043053	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.638	117	1044895	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.561	152	494349	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.326	65	245933	40.163	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	80.320%
35) Dibromofluoromethane	7.914	113	300785	43.736	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	87.480%
50) Toluene-d8	10.332	98	1380824	53.368	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	106.740%
62) 4-Bromofluorobenzene	12.620	95	496443	58.152	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	116.300%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD102821\
Data File : VD070894.D
Acq On : 28 Oct 2021 15:55
Operator : VA/SY
Sample : M4372-07
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampled :
SB-4

Quant Time: Oct 29 06:35:27 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D102621S.M
Quant Title : SW846 8260
QLast Update : Wed Oct 27 05:34:47 2021
Response via : Initial Calibration




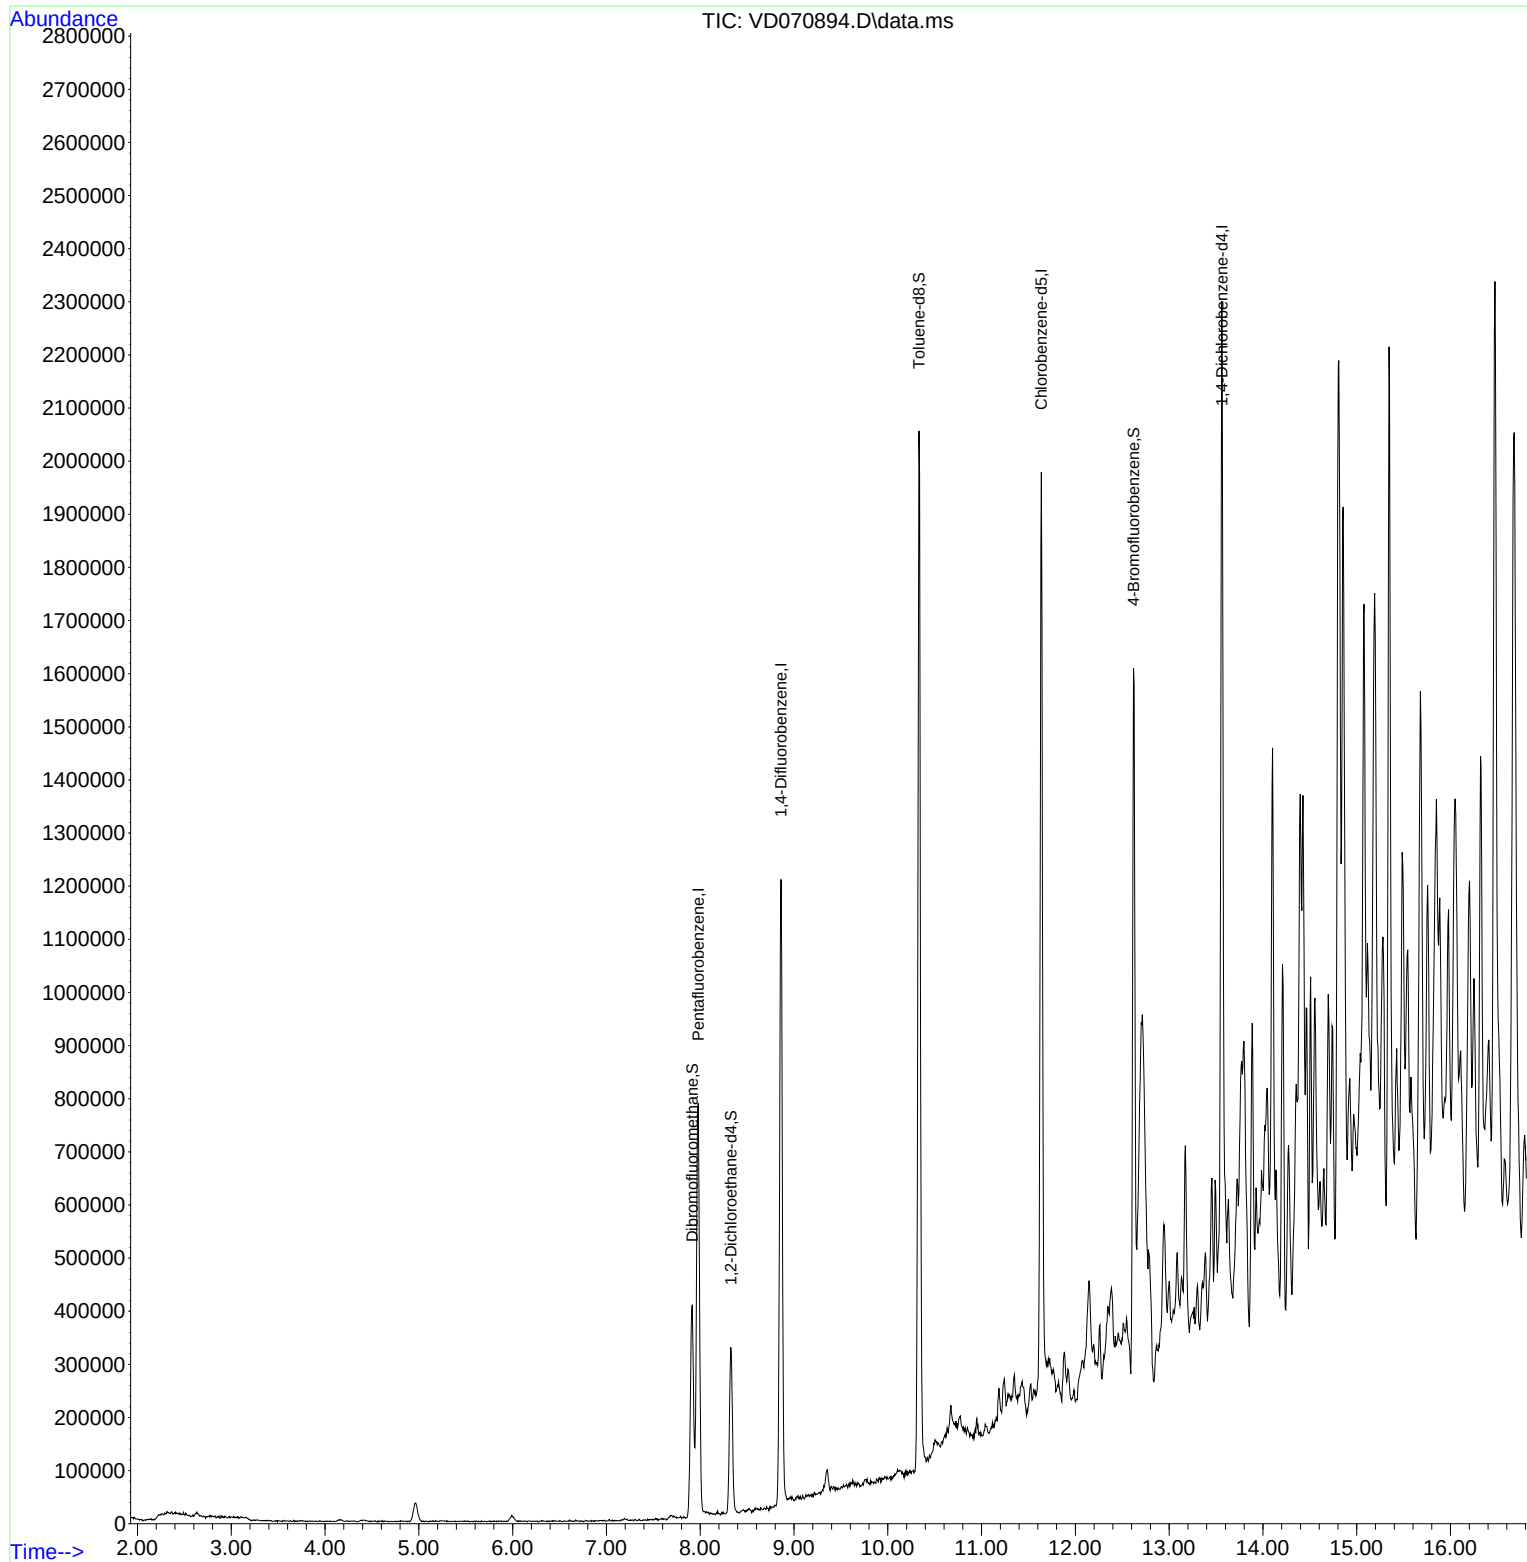


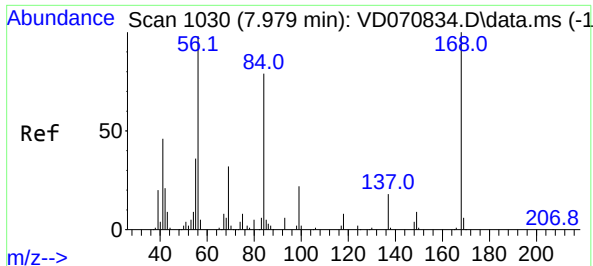

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.979 min Scan# 1030
Delta R.T. 0.000 min
Lab File: VD070894.D
Acq: 28 Oct 2021 15:55




Instrument :
MSVOA_D
ClientSampled :
SB-4


Tgt Ion:168 Resp: 608834
Ion Ratio Lower Upper
168 100
99 56.3 46.6 69.8

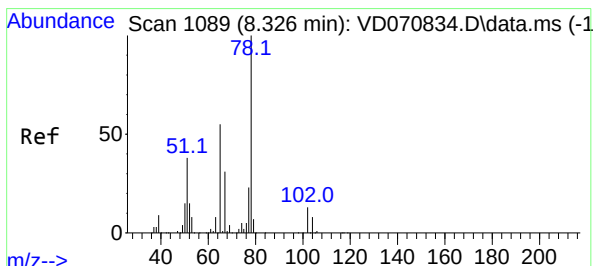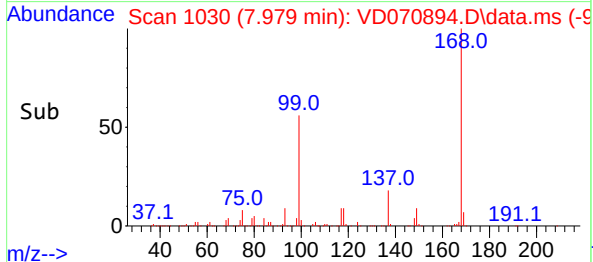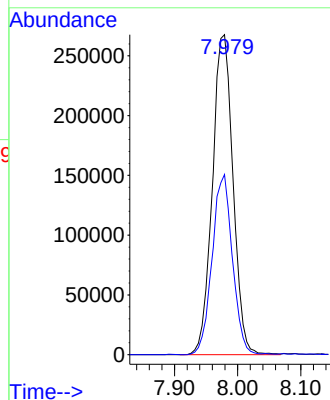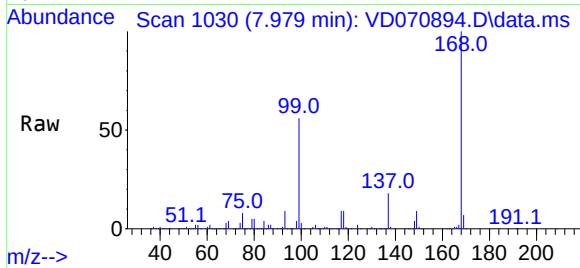

#33
1,2-Dichloroethane-d4
Concen: 40.163 ug/l
RT: 8.326 min Scan# 1089
Delta R.T. 0.000 min
Lab File: VD070894.D
Acq: 28 Oct 2021 15:55

Tgt Ion: 65 Resp: 245933
Ion Ratio Lower Upper
65 100
67 56.0 0.0 112.2

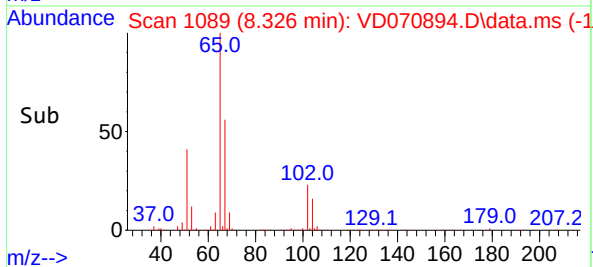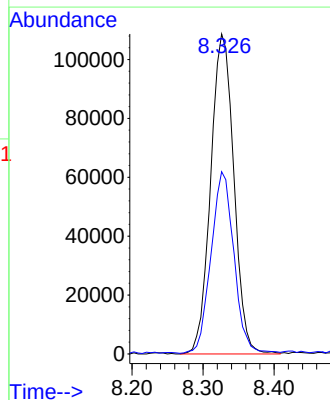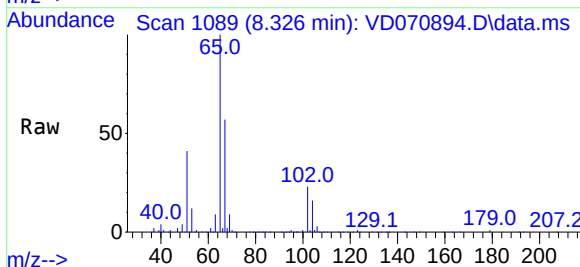




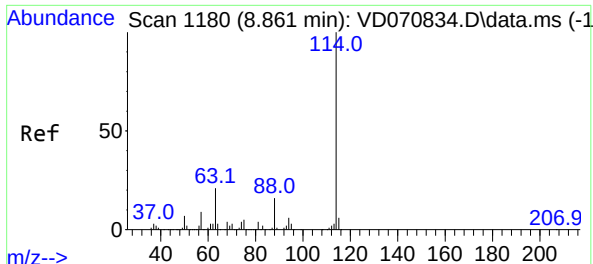


#34

1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.861 min Scan# 1180
Delta R.T. 0.000 min
Lab File: VD070894.D
Acq: 28 Oct 2021 15:55

Instrument :
MSVOA_D
ClientSampled :
SB-4




Tgt Ion:114 Resp: 1043053
Ion Ratio Lower Upper
114 100
63 20.4 0.0 41.8
88 15.3 0.0 32.8

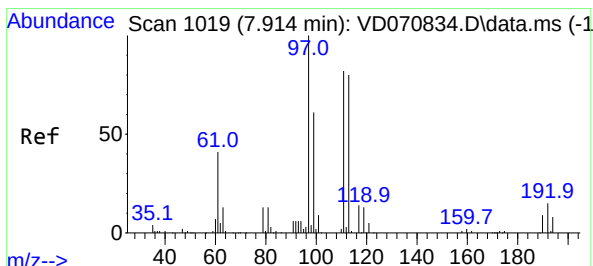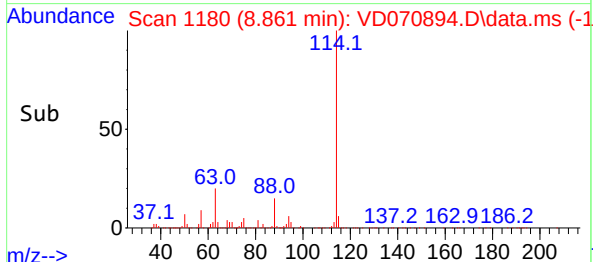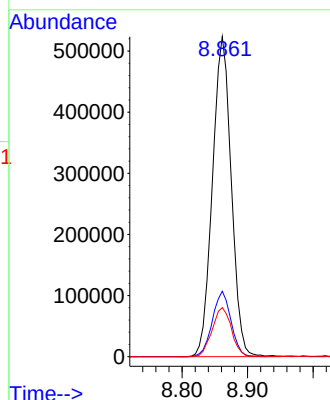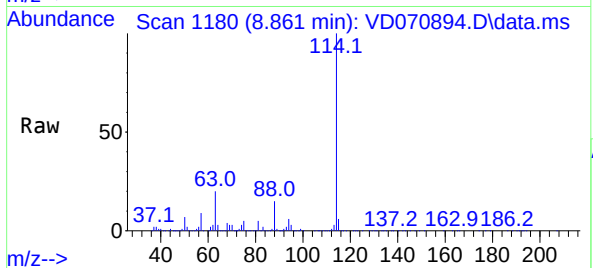


#35

Dibromofluoromethane
Concen: 43.736 ug/l
RT: 7.914 min Scan# 1019
Delta R.T. 0.000 min
Lab File: VD070894.D
Acq: 28 Oct 2021 15:55

Tgt Ion:113 Resp: 300785
Ion Ratio Lower Upper
113 100
111 102.9 82.0 123.0
192 19.4 15.2 22.8


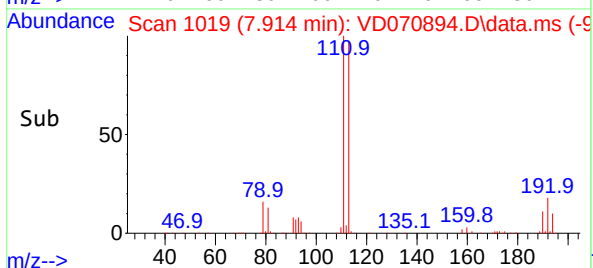
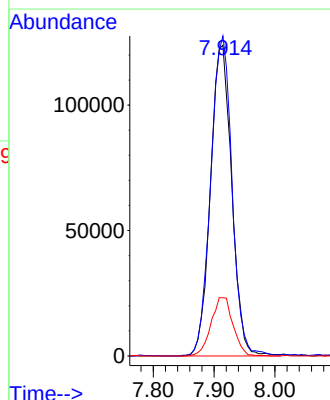
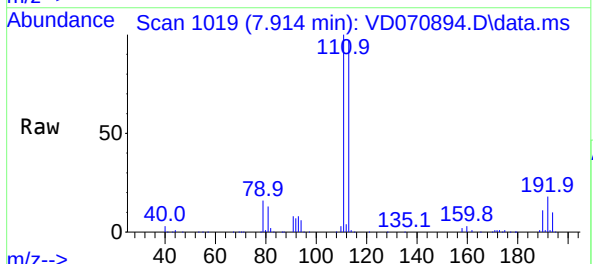


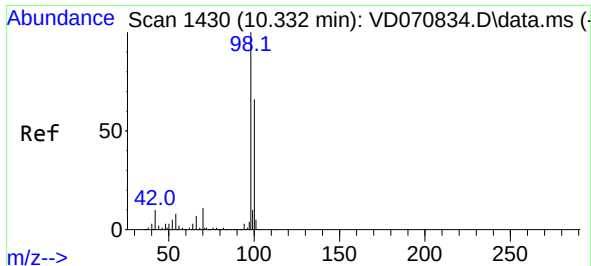

#50
Toluene-d8
Concen: 53.368 ug/l
RT: 10.332 min Scan# 1430
Delta R.T. 0.000 min
Lab File: VD070894.D
Acq: 28 Oct 2021 15:55




Instrument :
MSVOA_D
ClientSampled :
SB-4


Tgt Ion: 98 Resp: 1380824
Ion Ratio Lower Upper
98 100
100 64.4 51.8 77.6

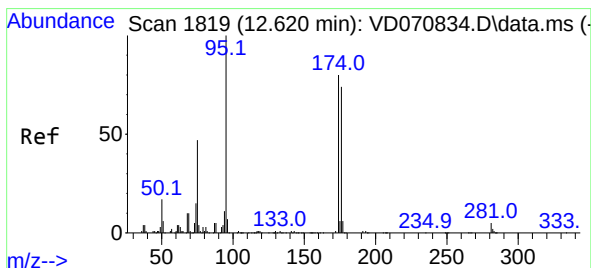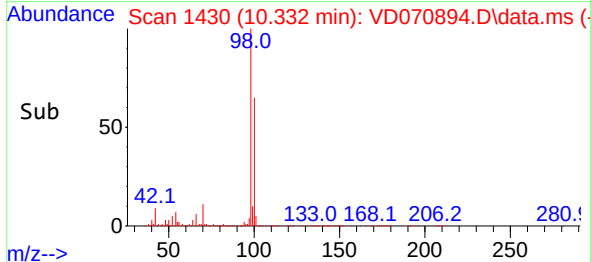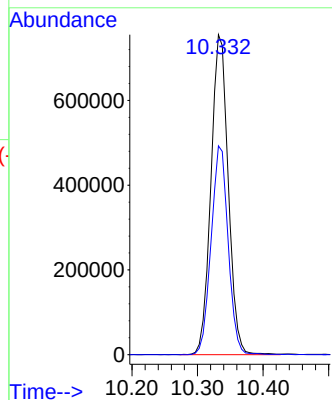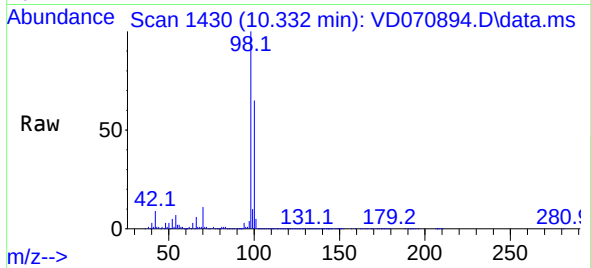

#62
4-Bromofluorobenzene
Concen: 58.152 ug/l
RT: 12.620 min Scan# 1819
Delta R.T. 0.000 min
Lab File: VD070894.D
Acq: 28 Oct 2021 15:55

Tgt Ion: 95 Resp: 496443
Ion Ratio Lower Upper
95 100
174 75.9 0.0 159.4
176 74.7 0.0 154.0


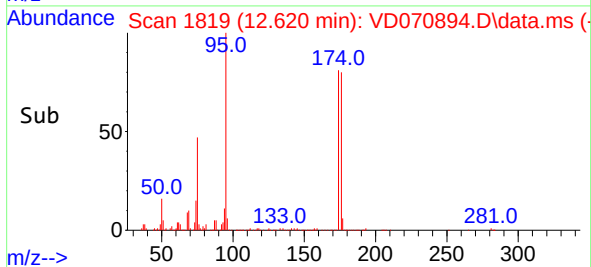
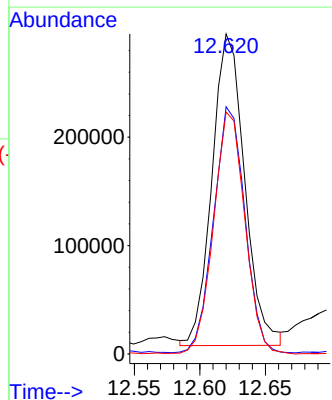
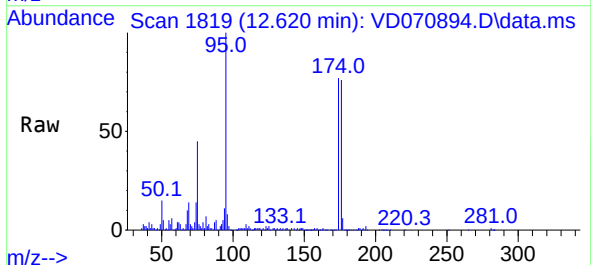


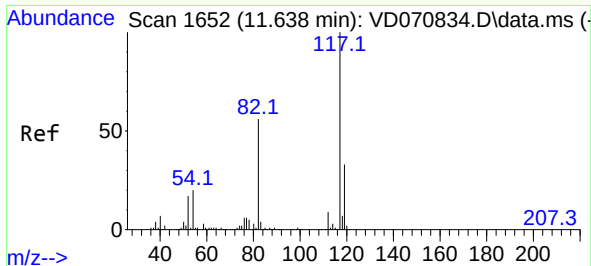

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.638 min Scan# 1652
Delta R.T. 0.000 min
Lab File: VD070894.D
Acq: 28 Oct 2021 15:55

Instrument :
MSVOA_D
ClientSampled :
SB-4

Tgt Ion:117 Resp: 1044895
Ion Ratio Lower Upper
117 100
82 56.4 44.7 67.1
119 31.0 26.2 39.4

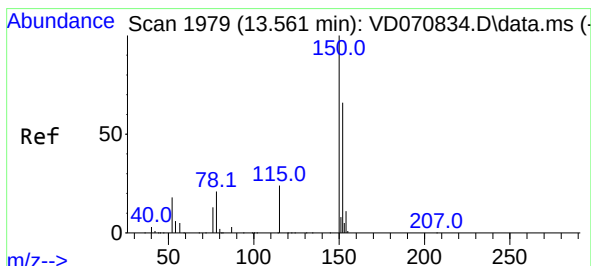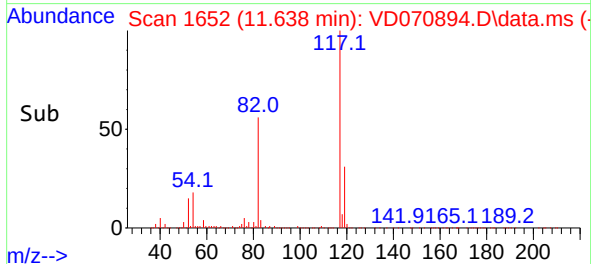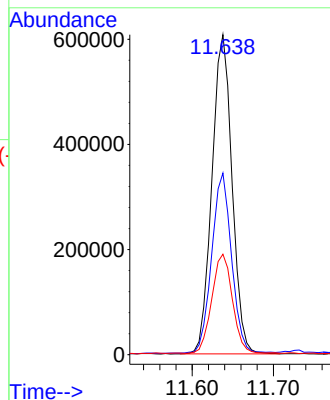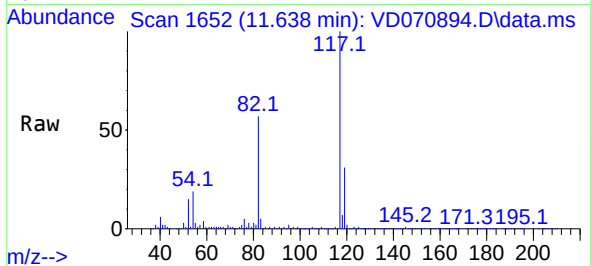

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.561 min Scan# 1979
Delta R.T. 0.000 min
Lab File: VD070894.D
Acq: 28 Oct 2021 15:55

Tgt Ion:152 Resp: 494349
Ion Ratio Lower Upper
152 100
115 57.0 29.8 89.3
150 155.5 0.0 349.2

