


Ethyl methacrylate

Response Ratio

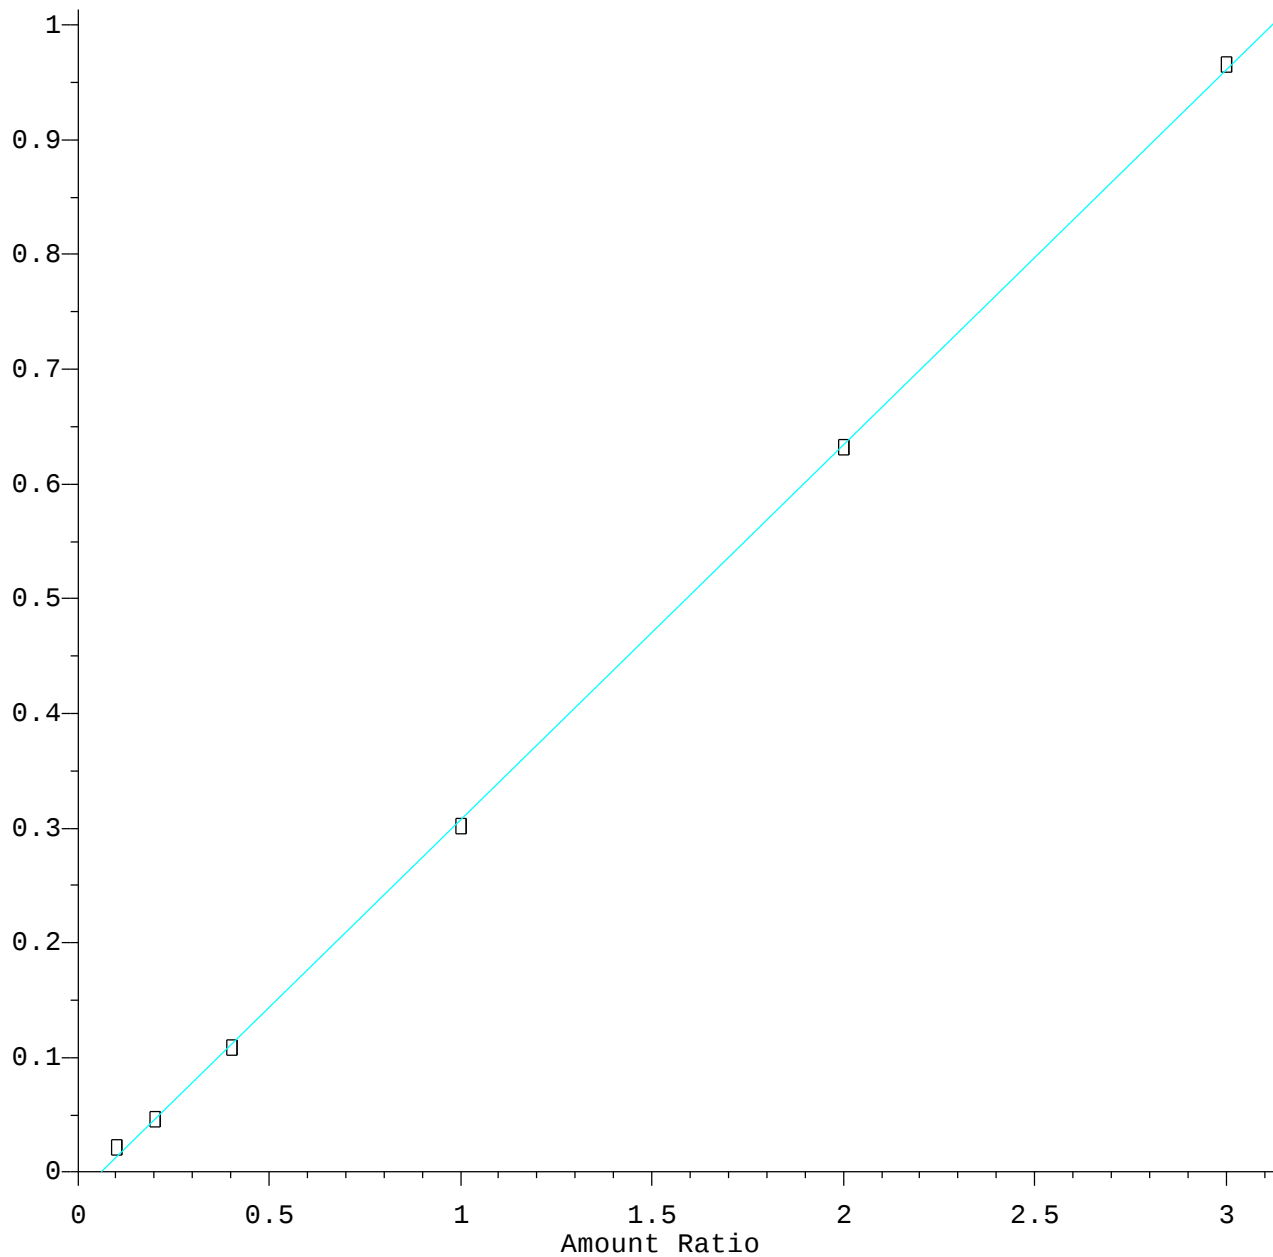


Resp Ratio = $3.27 \times 10^{-1} \times \text{Amt} - 1.97 \times 10^{-2}$
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D102919S.M
Calibration Table Last Updated: Wed Oct 30 08:00:10 2019


2-Hexanone

Response Ratio

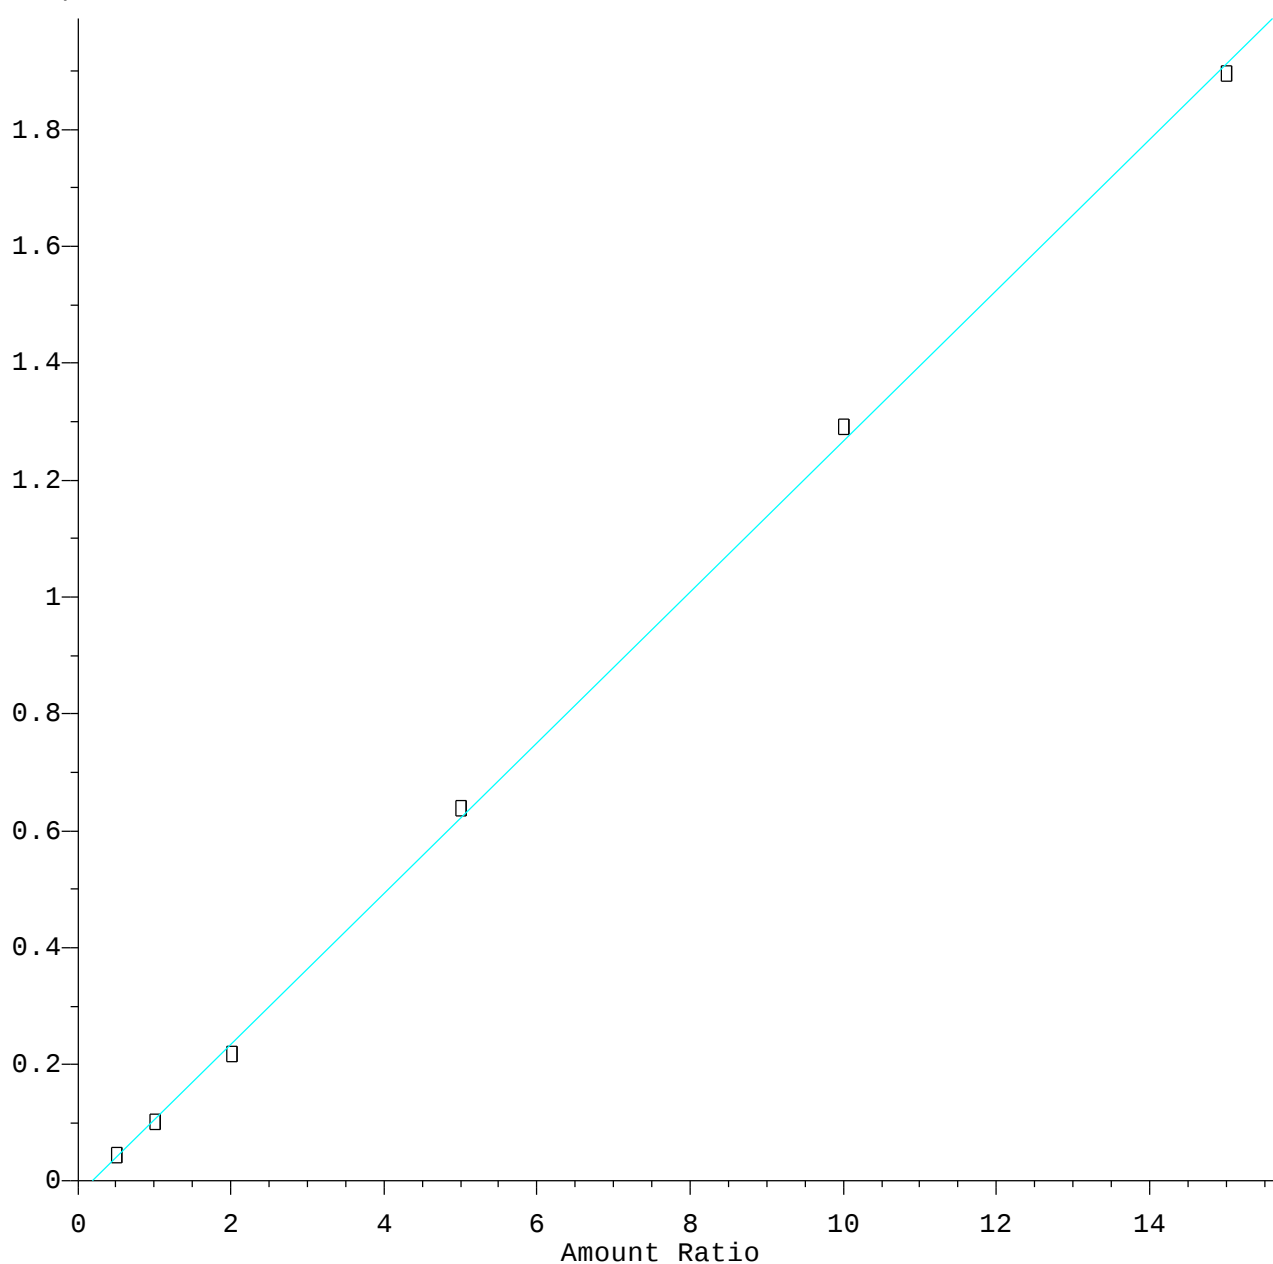

Resp Ratio = $1.29 \times 10^{-1} \times \text{Amt} - 2.33 \times 10^{-2}$
Coef of Det (r^2) = 1.000 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D102919S.M
Calibration Table Last Updated: Wed Oct 30 08:00:10 2019

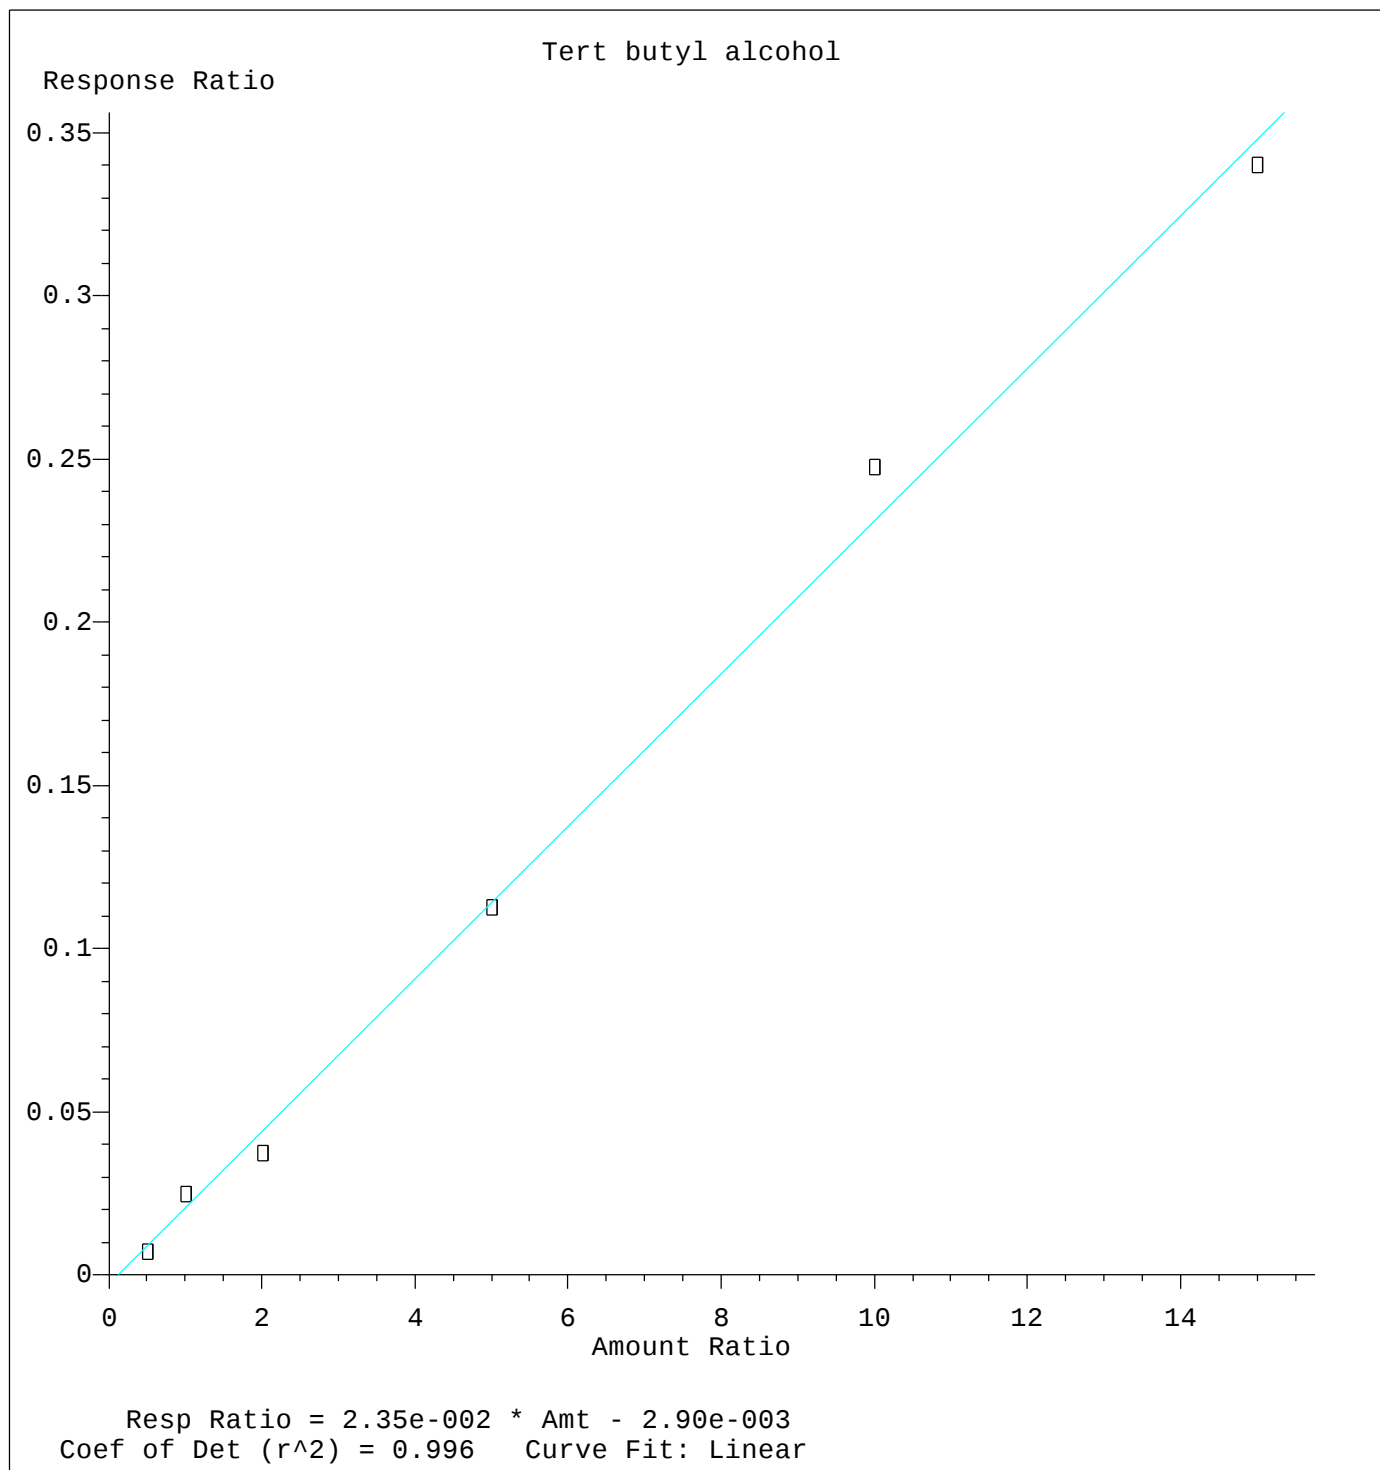

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D102919S.M
Calibration Table Last Updated: Wed Oct 30 08:00:10 2019


Methylene Chloride

Response Ratio

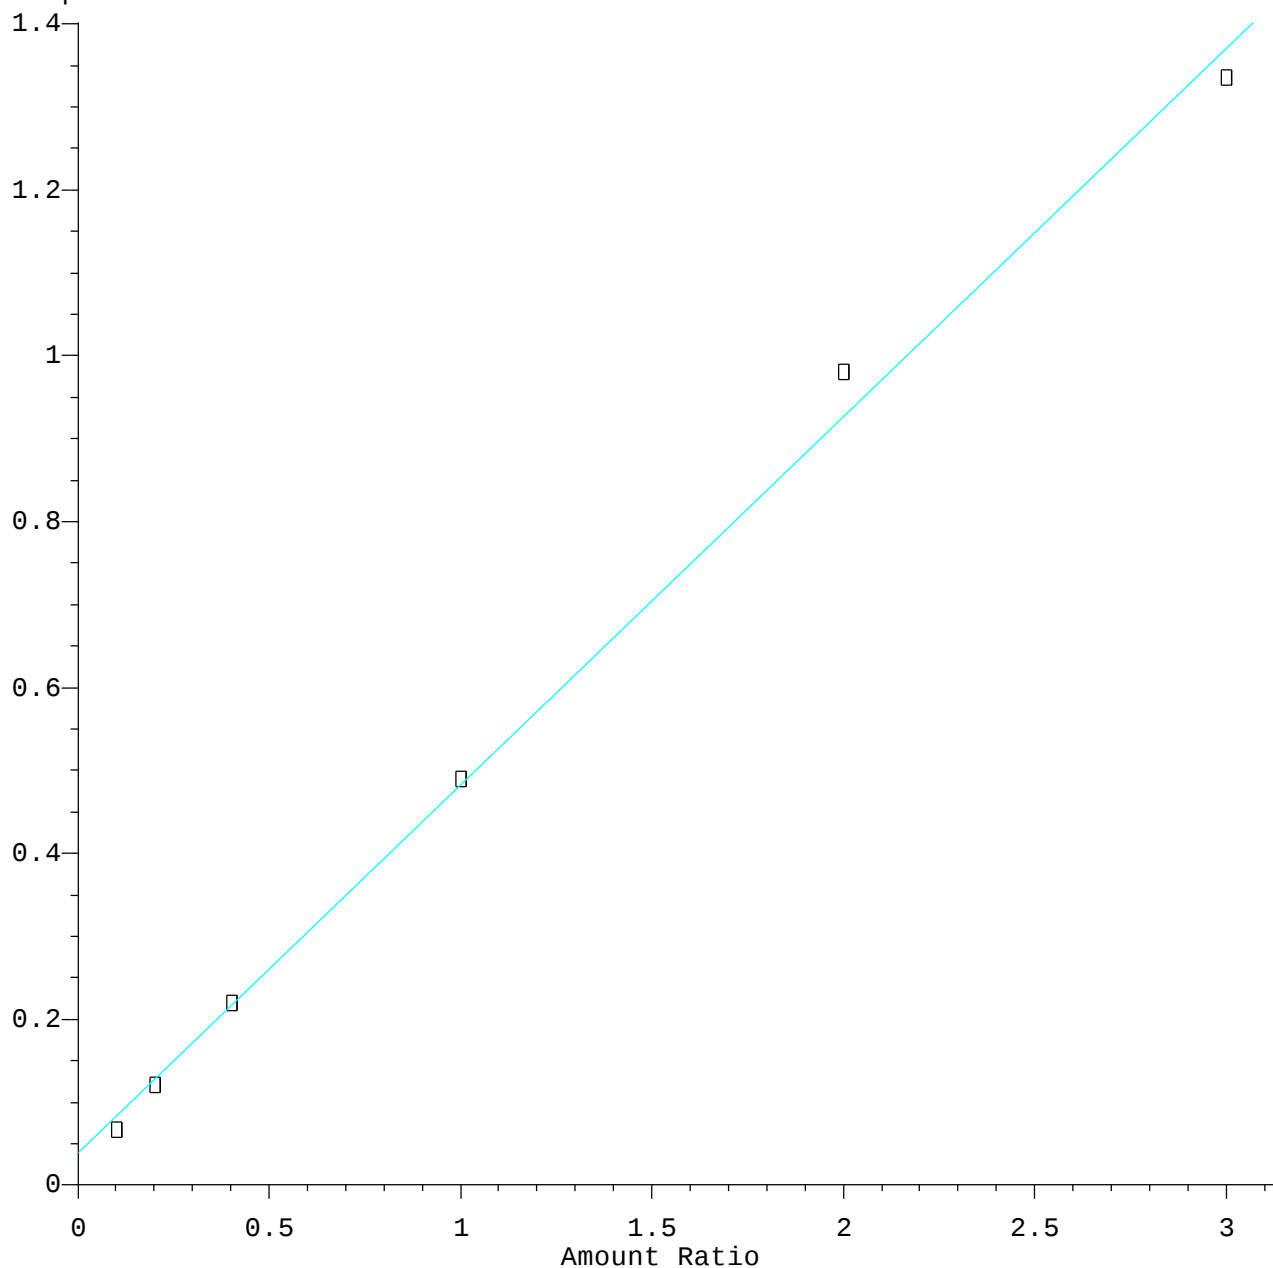

Resp Ratio = $4.44 \times 10^{-1} \times \text{Amt} + 3.94 \times 10^{-2}$
Coef of Det (r^2) = 0.997 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D102919S.M
Calibration Table Last Updated: Wed Oct 30 08:00:10 2019

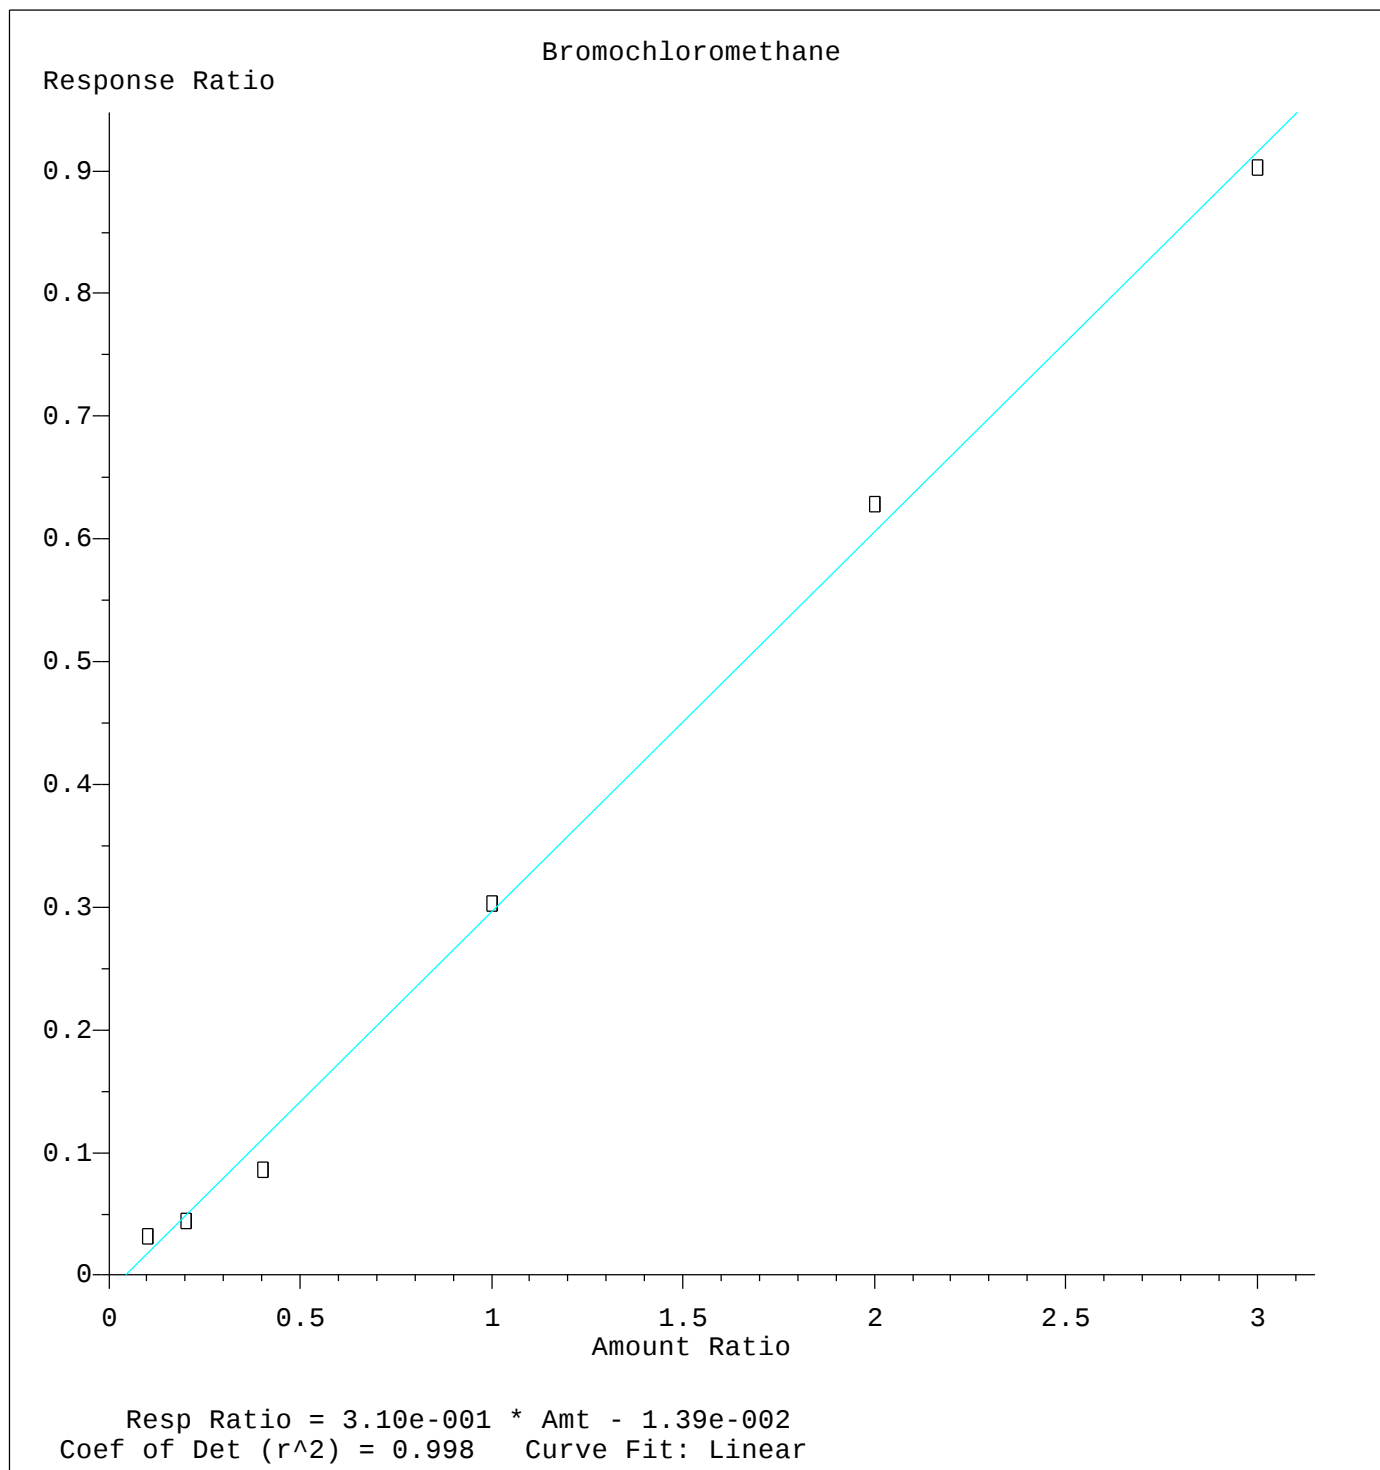

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D102919S.M
Calibration Table Last Updated: Wed Oct 30 08:00:10 2019