


Data Path : \\74.0.250.170\terastorage\voasrv\HPCHEM1\MSVOA_D\Data\VD102919\
Data File : VD064082.D
Acq On : 29 Oct 2019 11:10
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D102919S.M
Title : SW846 8260
Last Update : Wed Oct 30 08:00:10 2019

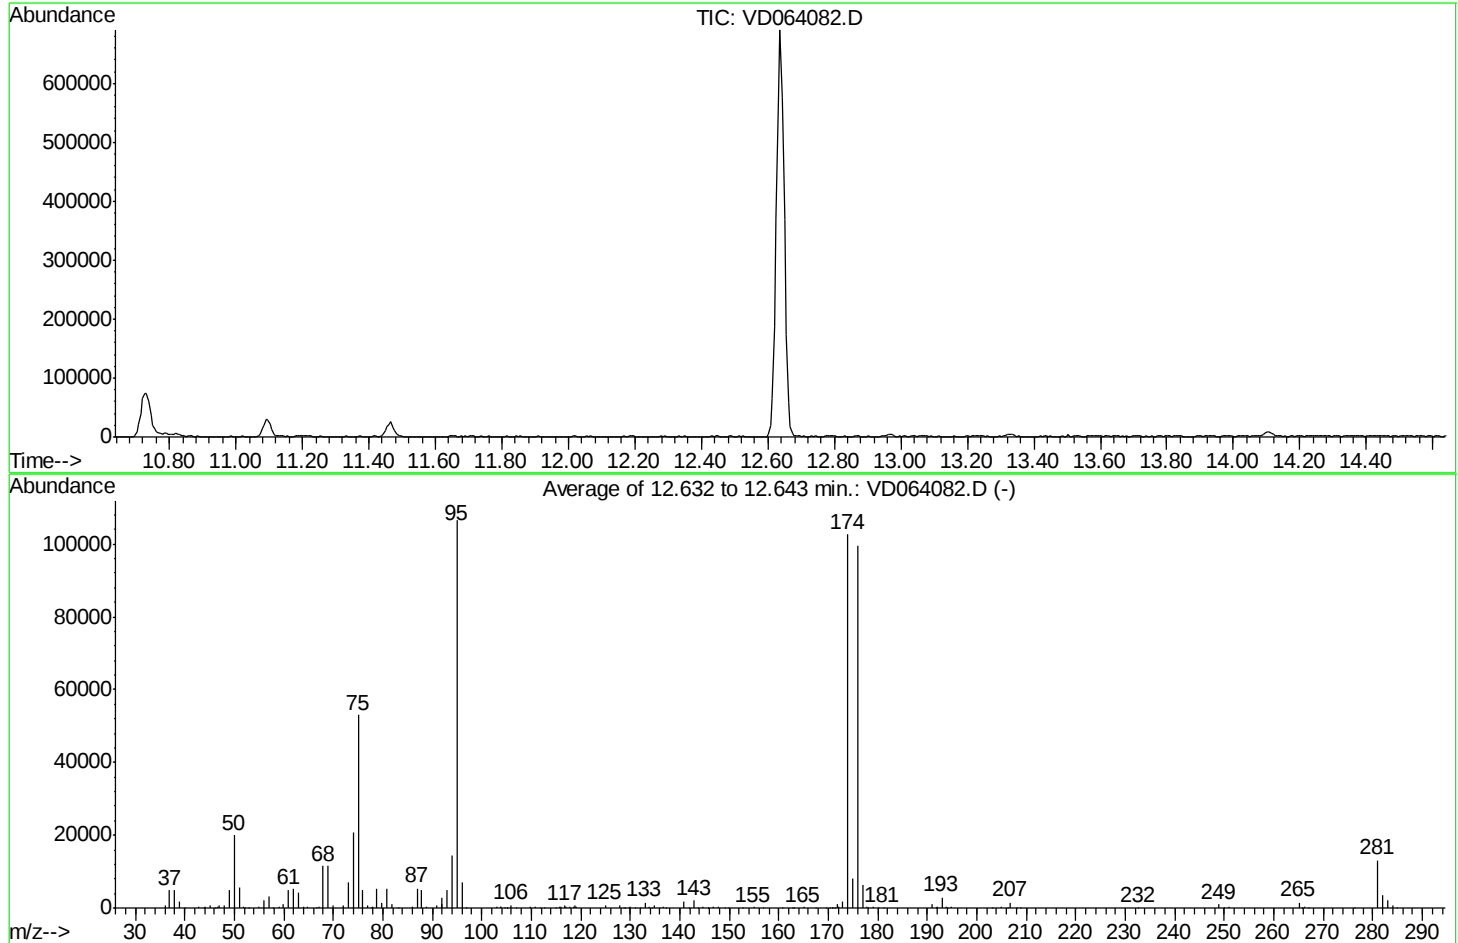

AutoFind: Scans 1821, 1822, 1823; Background Corrected with Scan 1813

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	20048	PASS
75	95	30	60	49.8	53026	PASS
95	95	100	100	100.0	106538	PASS
96	95	5	9	6.5	6897	PASS
173	174	0.00	2	1.8	1809	PASS
174	95	50	100	96.3	102602	PASS
175	174	5	9	7.9	8106	PASS
176	174	95	101	97.0	99536	PASS
177	176	5	9	6.5	6485	PASS