

Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD102920\
 Data File : VD067454.D
 Acq On : 29 Oct 2020 16:14
 Operator : VA/SY
 Sample : L4560-03
 Misc : 7.57G/5.00ml/MSVOA D/SOIL
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 B308-B309-LOC2-SO-0003

Quant Time: Oct 30 03:23:36 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D101320S.M
 Quant Title : SW846 8260
 QLast Update : Mon Oct 19 19:13:29 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.99	168	18113	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.87	114	28131	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.65	117	30184	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.57	152	14893	50.00	ug/l	-0.01

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.34	65	12795	70.51	ug/l	0.00
Spiked Amount	50.000		Recovery	=	141.02%	
35) Dibromofluoromethane	7.91	113	10126	54.09	ug/l	0.00
Spiked Amount	50.000		Recovery	=	108.18%	
50) Toluene-d8	10.34	98	32311	47.69	ug/l	0.00
Spiked Amount	50.000		Recovery	=	95.38%	
62) 4-Bromofluorobenzene	12.64	95	11494	48.79	ug/l	0.00
Spiked Amount	50.000		Recovery	=	97.58%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD102920\
Data File : VD067454.D
Acq On : 29 Oct 2020 16:14
Operator : VA/SY
Sample : L4560-03
Misc : 7.57G/5.00ml/MSVOA D/SOIL
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
B308-B309-LOC2-SO-0003

Quant Time: Oct 30 03:23:36 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D101320S.M
Quant Title : SW846 8260
QLast Update : Mon Oct 19 19:13:29 2020
Response via : Initial Calibration

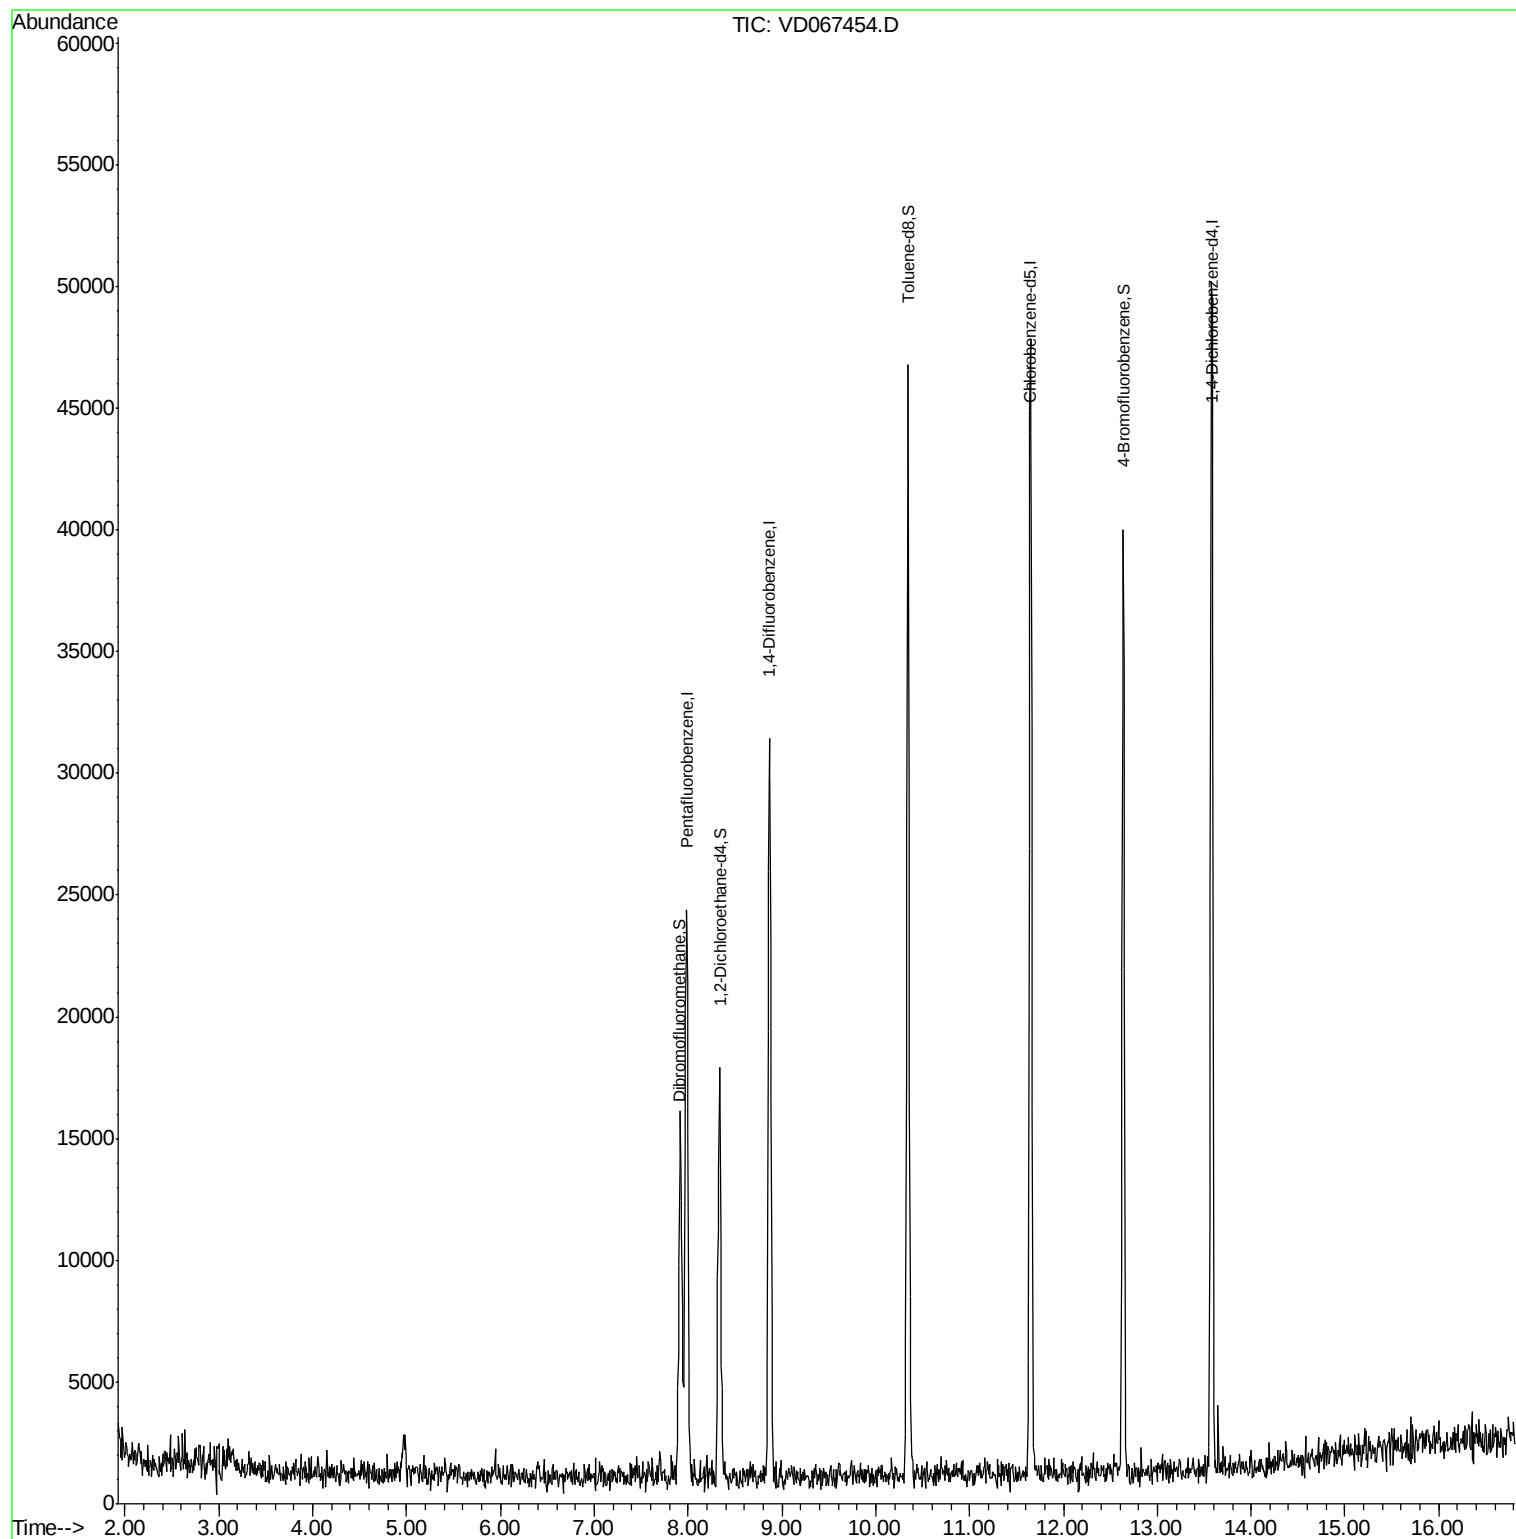

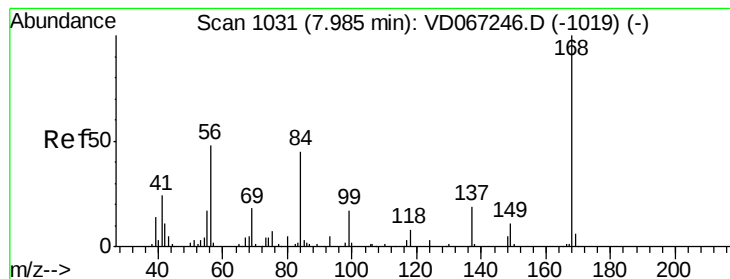

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.99 min Scan# 1031

Delta R.T. 0.00 min

Lab File: VD067454.D

Acq: 29 Oct 2020 16:14

Instrument :

MSVOA_D

ClientSampleId :


B308-B309-LOC2-SO-0003

Tot Ion:168 Resp: 18113

Ion Ratio Lower Upper




168 100

99 48.2 45.9 68.9

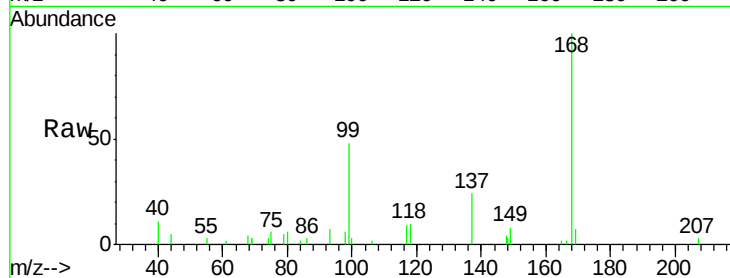

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VDC

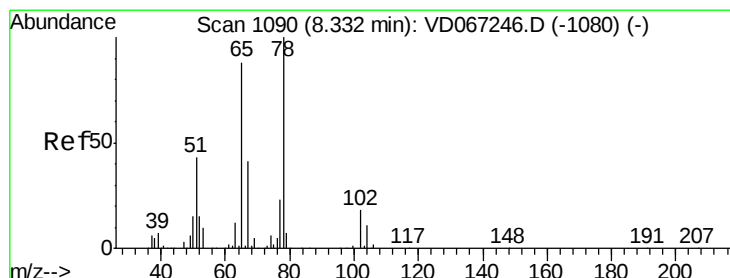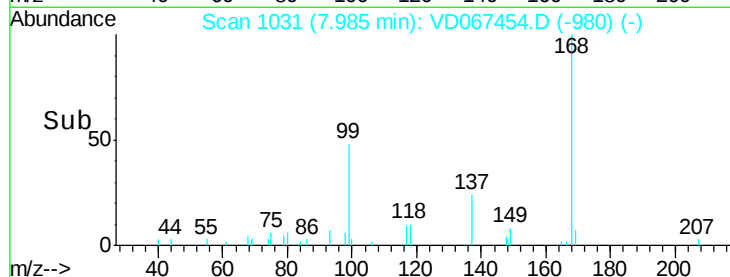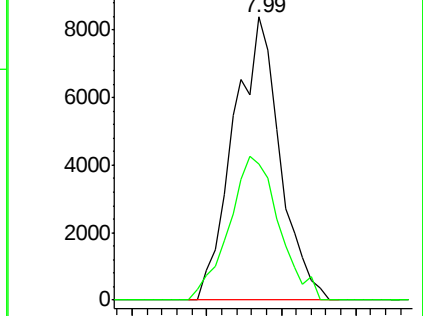

#33

1,2-Dichloroethane-d4

Concen: 70.509 ug/l

RT: 8.34 min Scan# 1091

Delta R.T. 0.01 min

Lab File: VD067454.D


Acq: 29 Oct 2020 16:14

Tgt Ion: 65 Resp: 12795

Ion Ratio Lower Upper



65 100


67 63.2 0.0 103.8

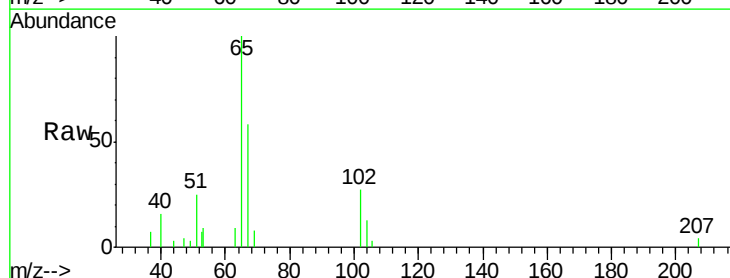

Abundance Ion 64.90 (64.60 to 65.60): VDC

Ion 66.90 (66.60 to 67.60): VDC

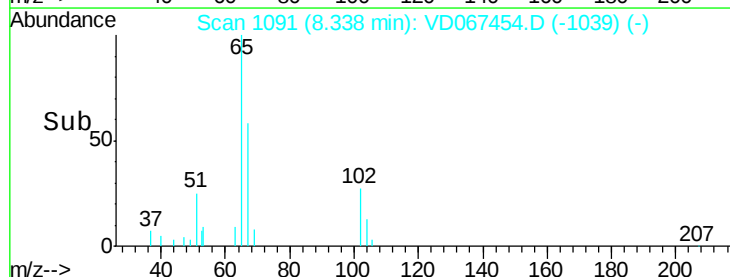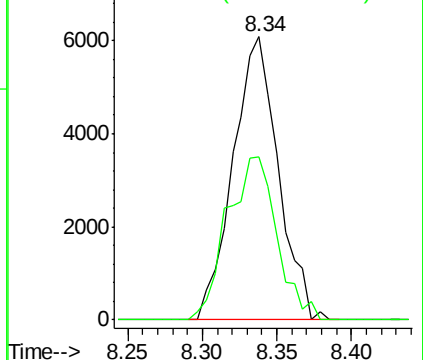

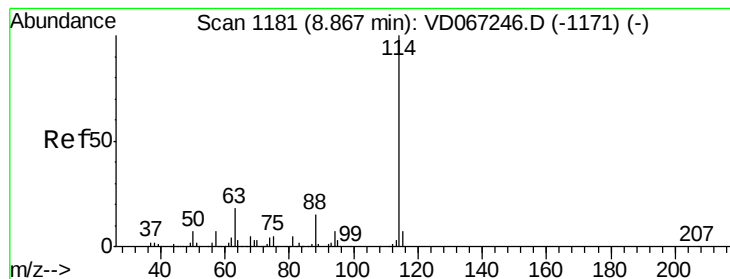

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.87 min Scan# 1181

Delta R.T. 0.00 min

Lab File: VD067454.D

Acq: 29 Oct 2020 16:14

Instrument :

MSVOA_D

ClientSampleId :

B308-B309-LOC2-SO-0003


Tot Ion:114 Resp: 28131

Ion Ratio Lower Upper

114 100

63 16.4 0.0 35.0




88 9.2 0.0 30.6

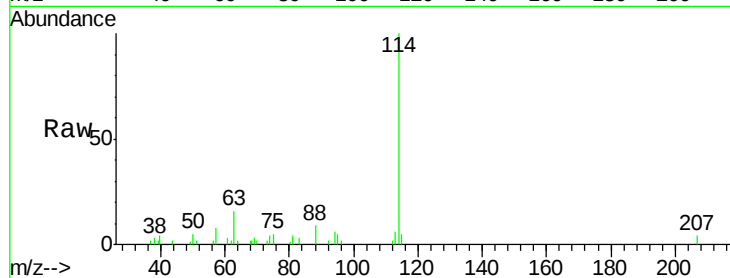

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): V

Ion 87.90 (87.60 to 88.60): V

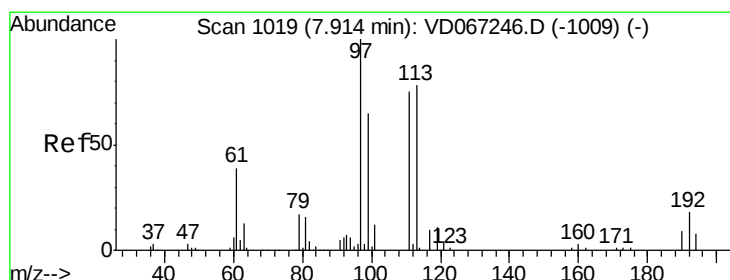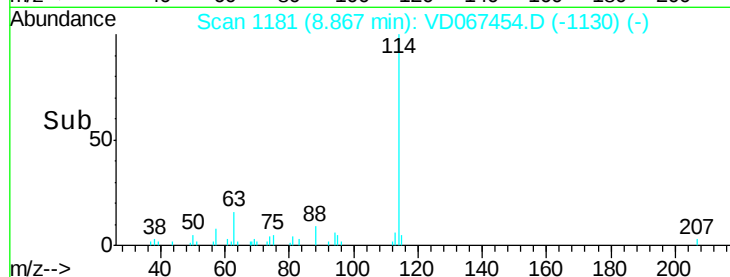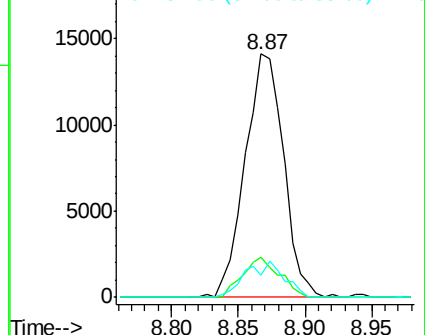

#35

Dibromofluoromethane

Concen: 54.088 ug/l

RT: 7.91 min Scan# 1018

Delta R.T. -0.01 min

Lab File: VD067454.D

Acq: 29 Oct 2020 16:14


Tgt Ion:113 Resp: 10126

Ion Ratio Lower Upper

113 100

111 101.2 81.6 122.4



192 20.1 17.0 25.4

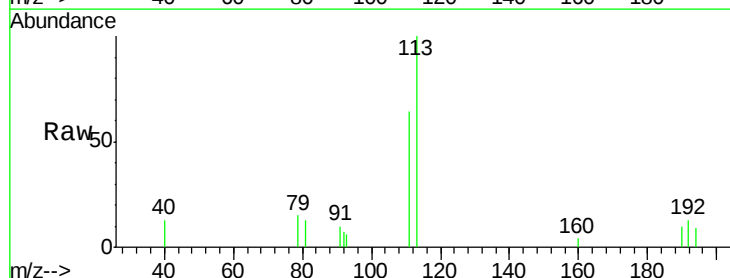


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V



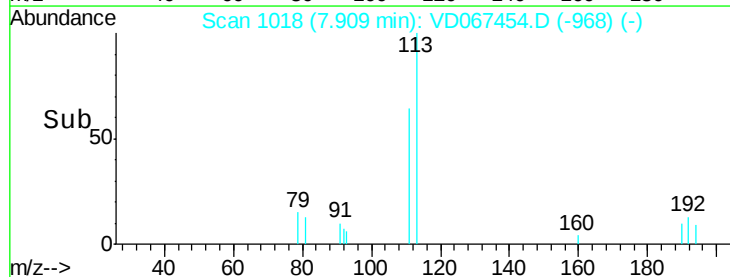
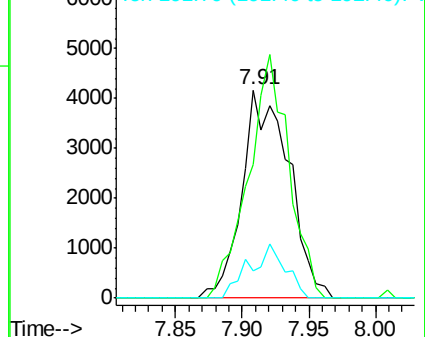


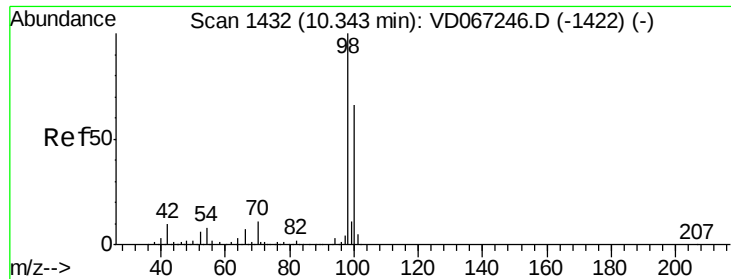

#50
Toluene-d8
Concen: 47.691 ug/l
RT: 10.34 min Scan# 1432
Delta R.T. 0.00 min
Lab File: VD067454.D
Acq: 29 Oct 2020 16:14




Instrument :
MSVOA_D
ClientSampleId :
B308-B309-LOC2-SO-0003


Tot Ion: 98 Resp: 32311
Ion Ratio Lower Upper
98 100
100 64.7 53.1 79.7

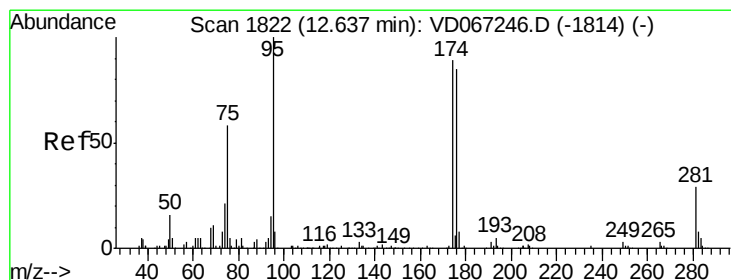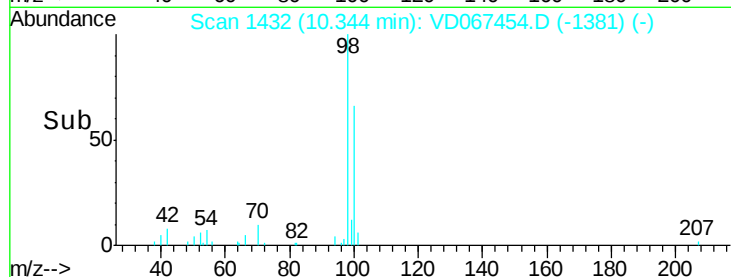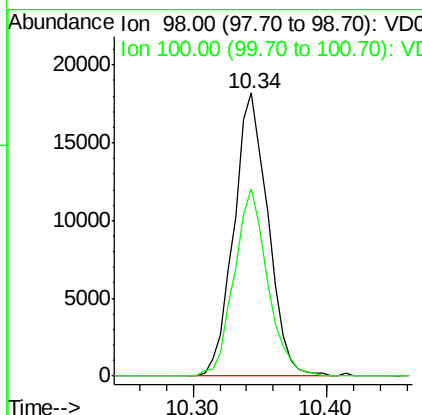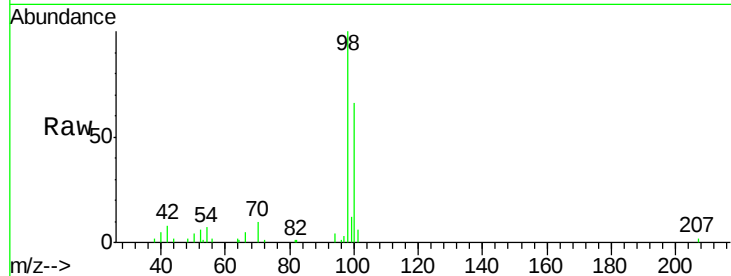

#62
4-Bromofluorobenzene
Concen: 48.790 ug/l
RT: 12.64 min Scan# 1822
Delta R.T. 0.00 min
Lab File: VD067454.D
Acq: 29 Oct 2020 16:14

Tgt Ion: 95 Resp: 11494
Ion Ratio Lower Upper
95 100
174 96.0 0.0 175.2
176 99.1 0.0 168.6


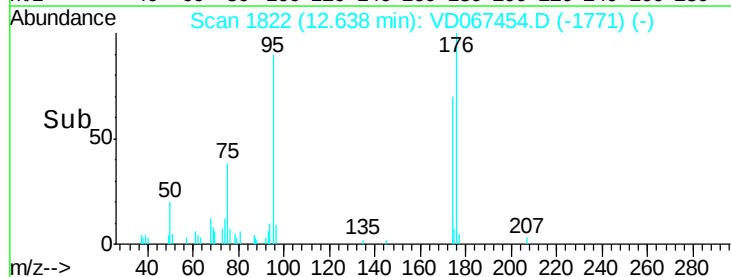
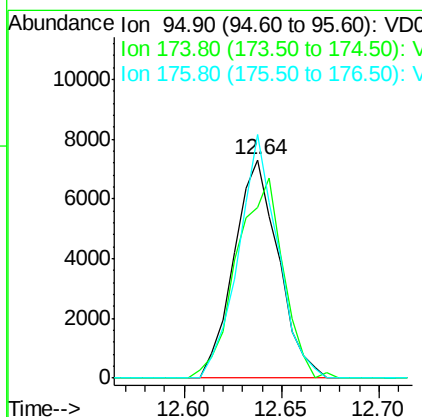
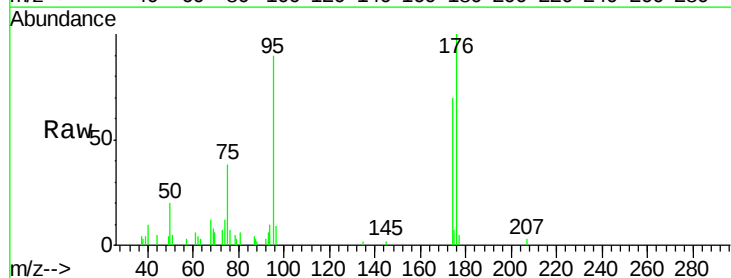


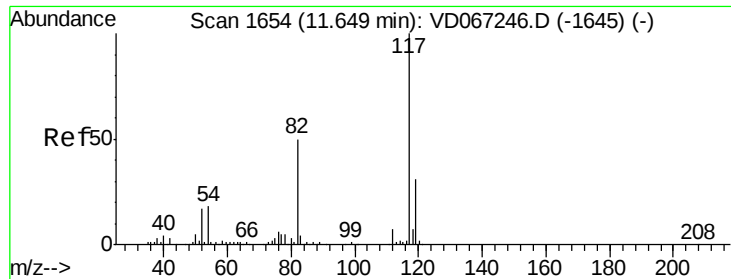

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.65 min Scan# 1654
Delta R.T. 0.00 min
Lab File: VD067454.D
Acq: 29 Oct 2020 16:14

Instrument :
MSVOA_D
ClientSampleId :
B308-B309-LOC2-SO-0003

Tot Ion:117 Resp: 30184
Ion Ratio Lower Upper
117 100
82 56.3 39.9 59.9
119 36.2 24.9 37.3

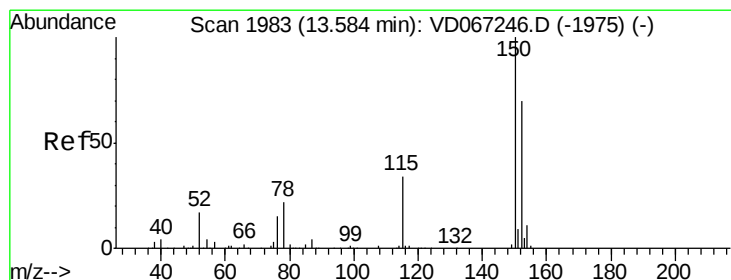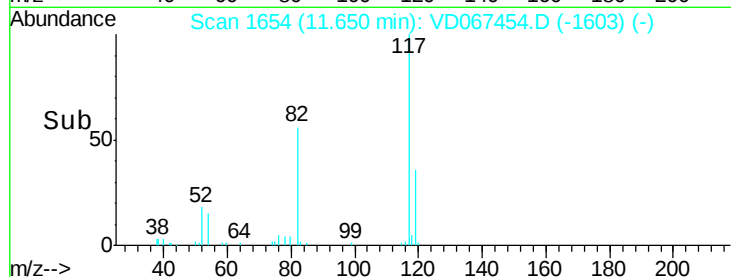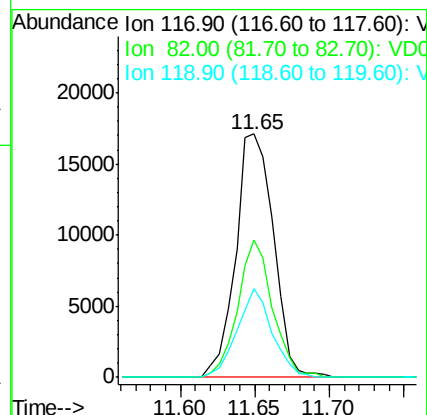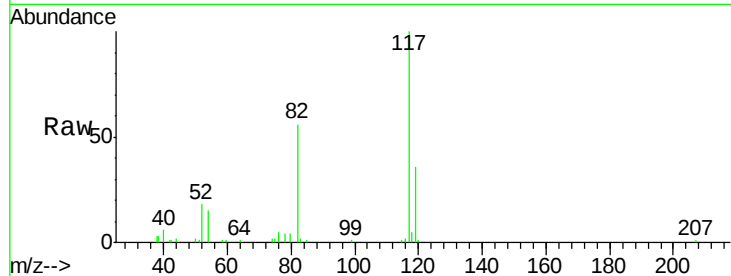

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.57 min Scan# 1981
Delta R.T. -0.01 min
Lab File: VD067454.D
Acq: 29 Oct 2020 16:14

Tgt Ion:152 Resp: 14893
Ion Ratio Lower Upper
152 100
115 57.5 29.3 87.9
150 161.6 0.0 339.0

