


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD102920\
 Data File : VD067444.D
 Acq On : 29 Oct 2020 10:08
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D101320S.M
 Title : SW846 8260
 Last Update : Mon Oct 19 19:13:29 2020

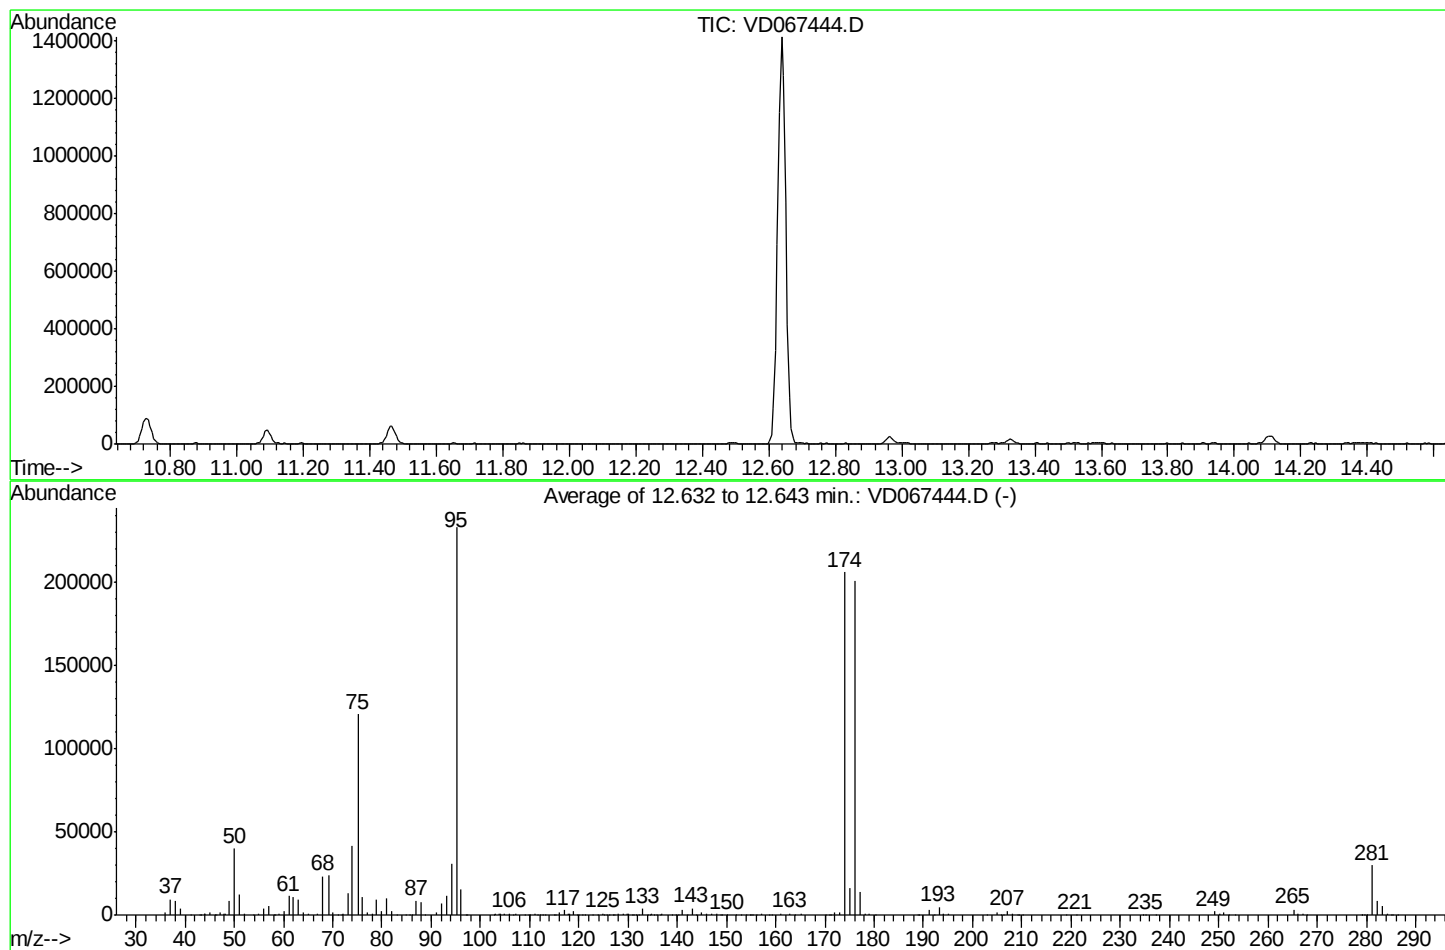

AutoFind: Scans 1821, 1822, 1823; Background Corrected with Scan 1812

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	39952	PASS
75	95	30	60	51.7	120592	PASS
95	95	100	100	100.0	233194	PASS
96	95	5	9	6.7	15612	PASS
173	174	0.00	2	0.9	1912	PASS
174	95	50	100	88.4	206080	PASS
175	174	5	9	7.9	16184	PASS
176	174	95	101	97.6	201194	PASS
177	176	5	9	7.0	14103	PASS