
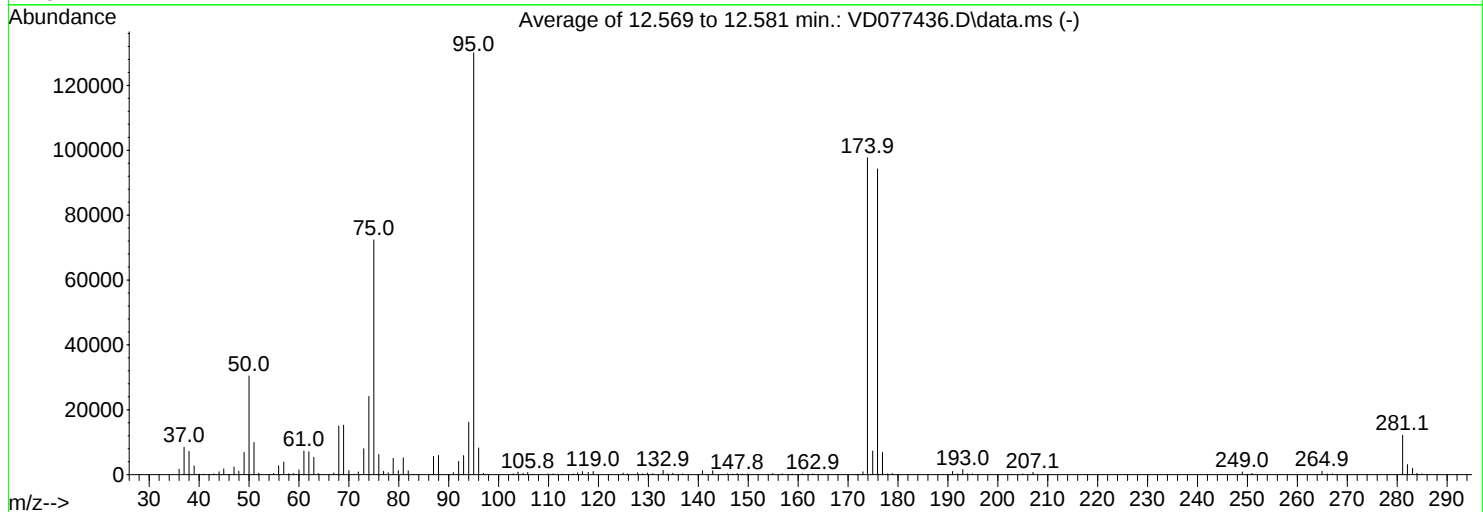


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD103023\
Data File : VD077436.D
Acq On : 30 Oct 2023 08:41
Operator : JC/SY
Sample : BFB
Misc : 5.00G/5.0ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D103023S.M
Title : SW846 8260
Last Update : Tue Oct 31 04:19:17 2023

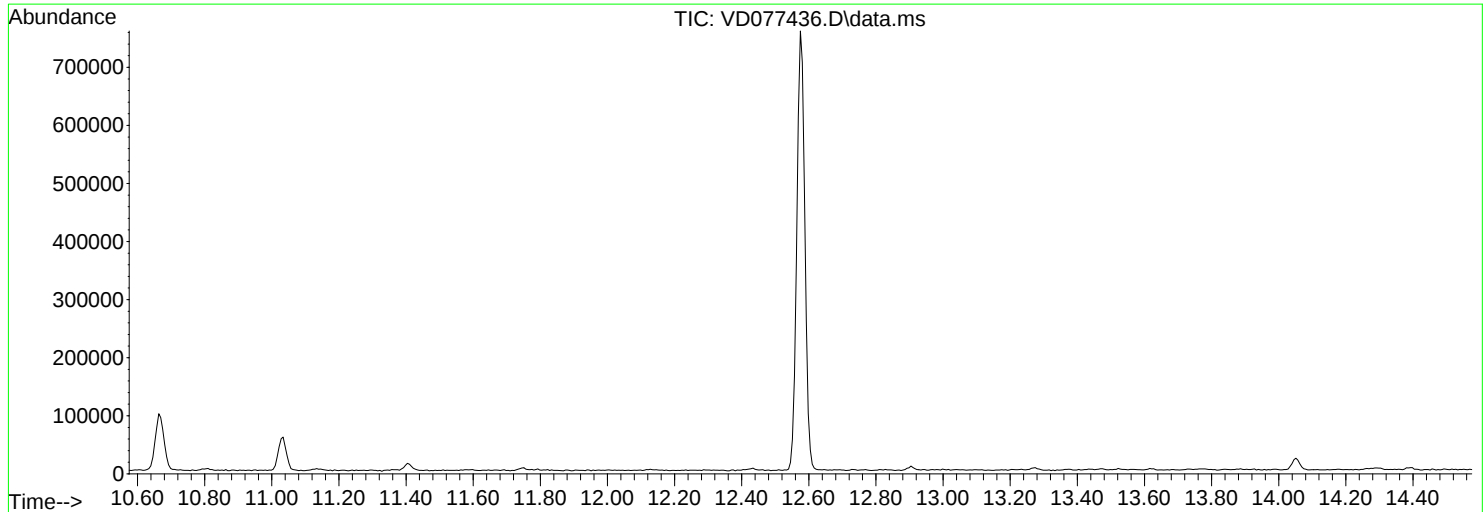

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1859

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	23.4	30443	PASS
75	95	30	60	55.6	72352	PASS
95	95	100	100	100.0	130029	PASS
96	95	5	9	6.3	8254	PASS
173	174	0.00	2	0.9	891	PASS
174	95	50	100	75.2	97733	PASS
175	174	5	9	7.5	7285	PASS
176	174	95	101	96.4	94251	PASS
177	176	5	9	7.3	6852	PASS