


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD103118\
Data File : VD060239.D
Acq On : 31 Oct 2018 11:53
Operator : VA/AP
Sample : BFB
Misc : 5.00µl/5ml/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D100118S.M
Title : SW846 8260
Last Update : Tue Oct 02 06:56:35 2018

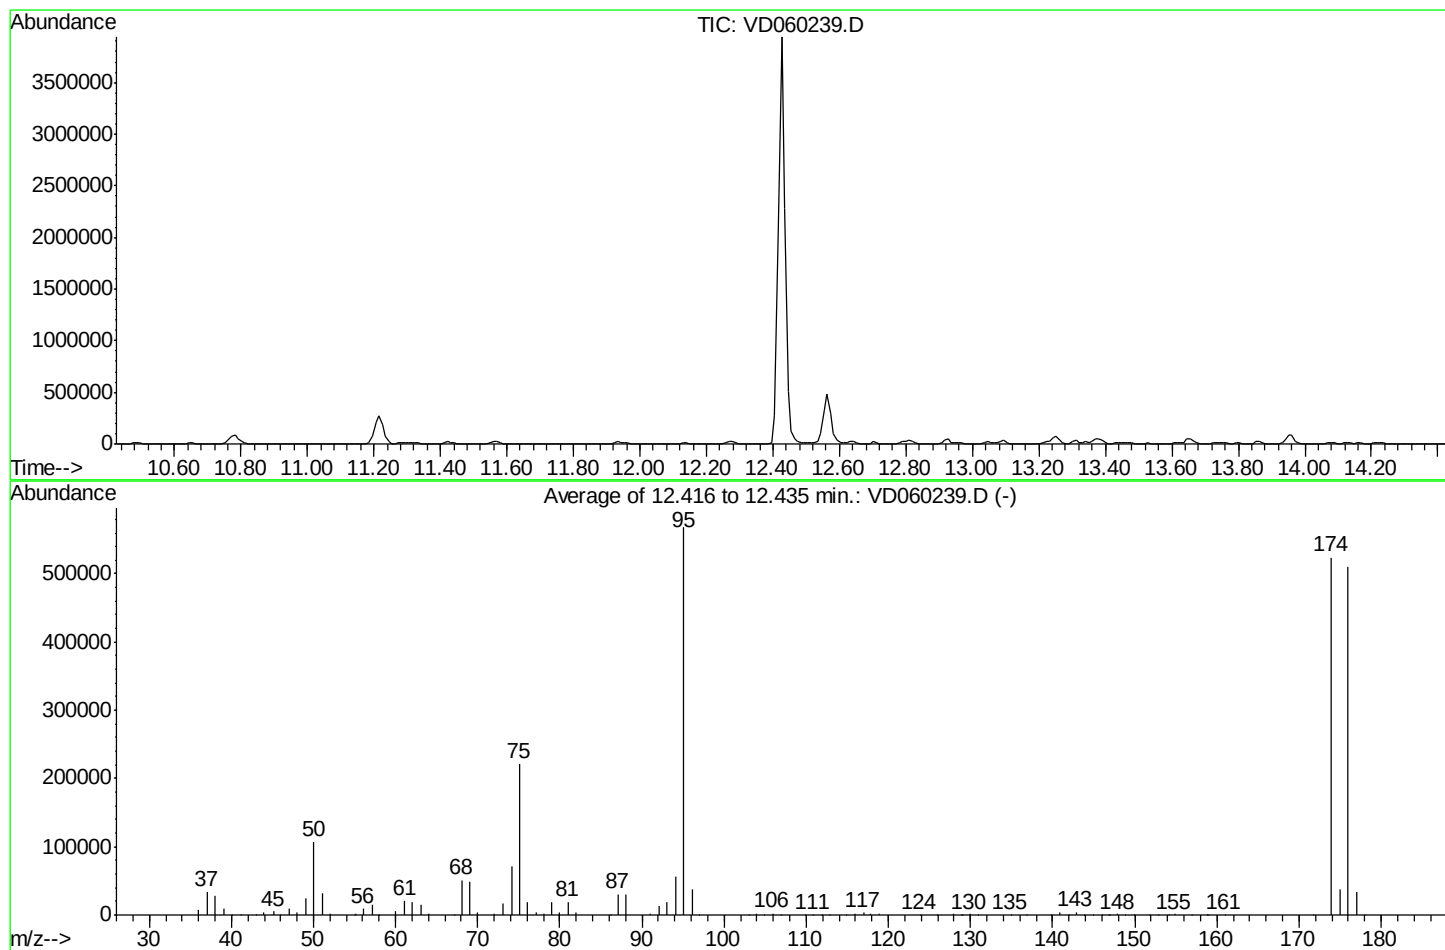

AutoFind: Scans 1107, 1108, 1109; Background Corrected with Scan 1102

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	107688	PASS
75	95	30	60	39.1	222144	PASS
95	95	100	100	100.0	568149	PASS
96	95	5	9	6.5	37032	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	92.3	524330	PASS
175	174	5	9	7.1	37042	PASS
176	174	95	101	97.4	510890	PASS
177	176	5	9	6.7	34360	PASS