
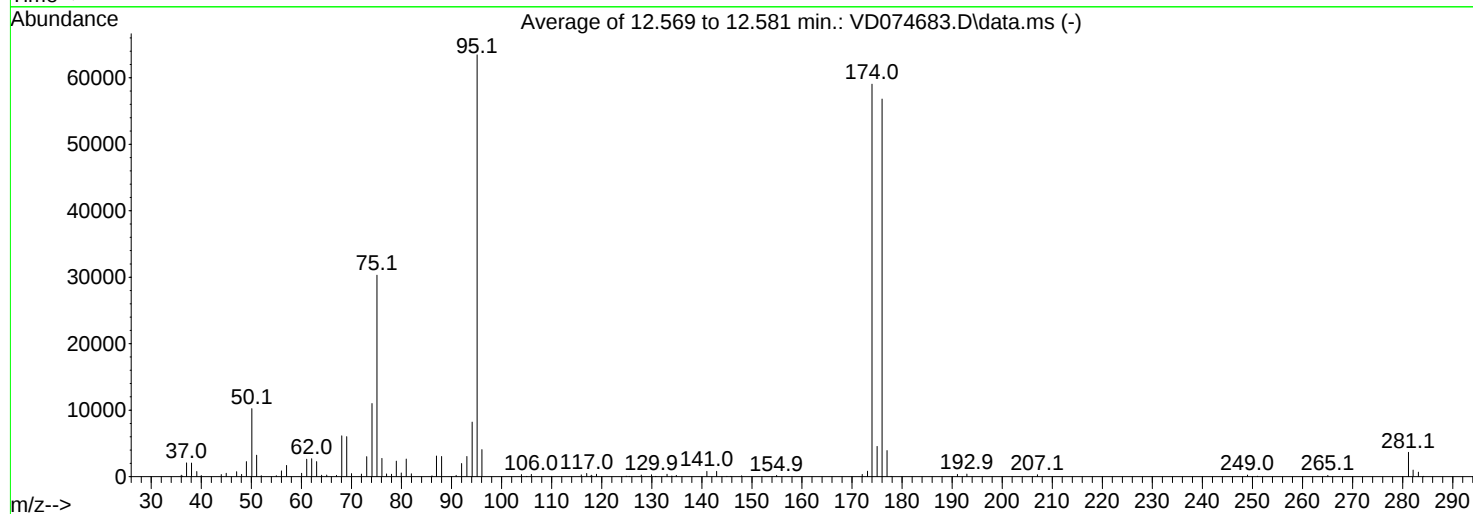


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD103122\
Data File : VD074683.D
Acq On : 31 Oct 2022 09:17
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D102722S.M
Title : SW846 8260
Last Update : Fri Oct 28 00:18:17 2022

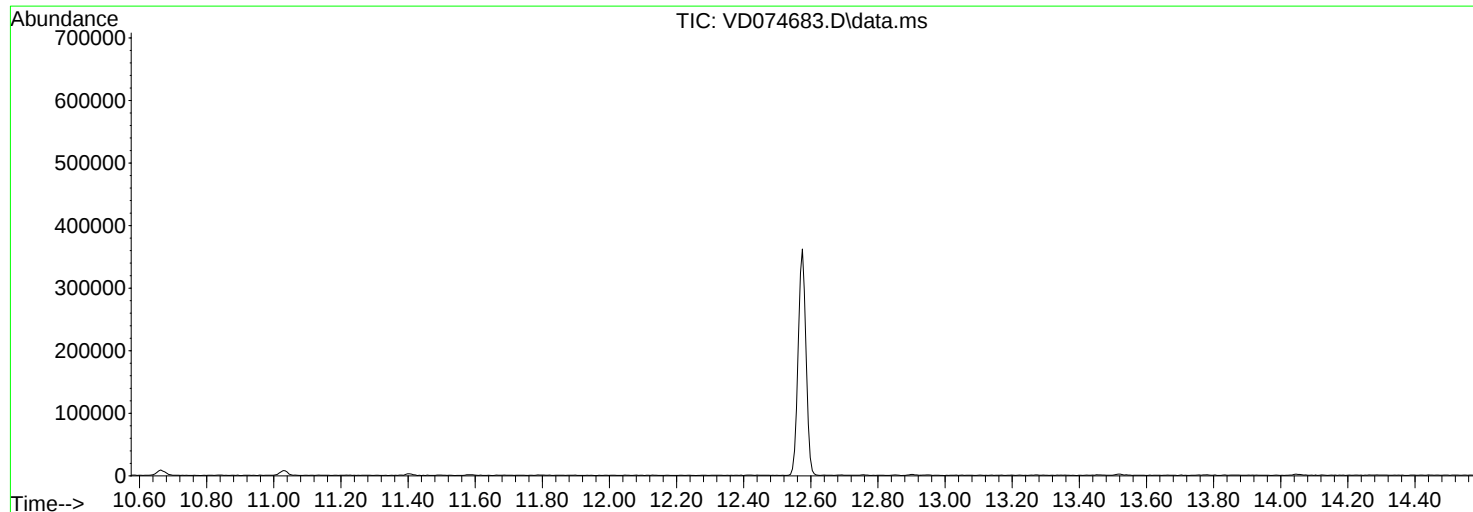

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1859

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.1	10223	PASS
75	95	30	60	47.8	30304	PASS
95	95	100	100	100.0	63451	PASS
96	95	5	9	6.4	4065	PASS
173	174	0.00	2	1.4	829	PASS
174	95	50	100	93.1	59043	PASS
175	174	5	9	7.7	4541	PASS
176	174	95	101	96.2	56819	PASS
177	176	5	9	6.9	3938	PASS