


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD110118\
 Data File : VD060258.D
 Acq On : 1 Nov 2018 12:37
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00µl/5ml/MSVOA D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D100118S.M
 Title : SW846 8260
 Last Update : Tue Oct 02 06:56:35 2018

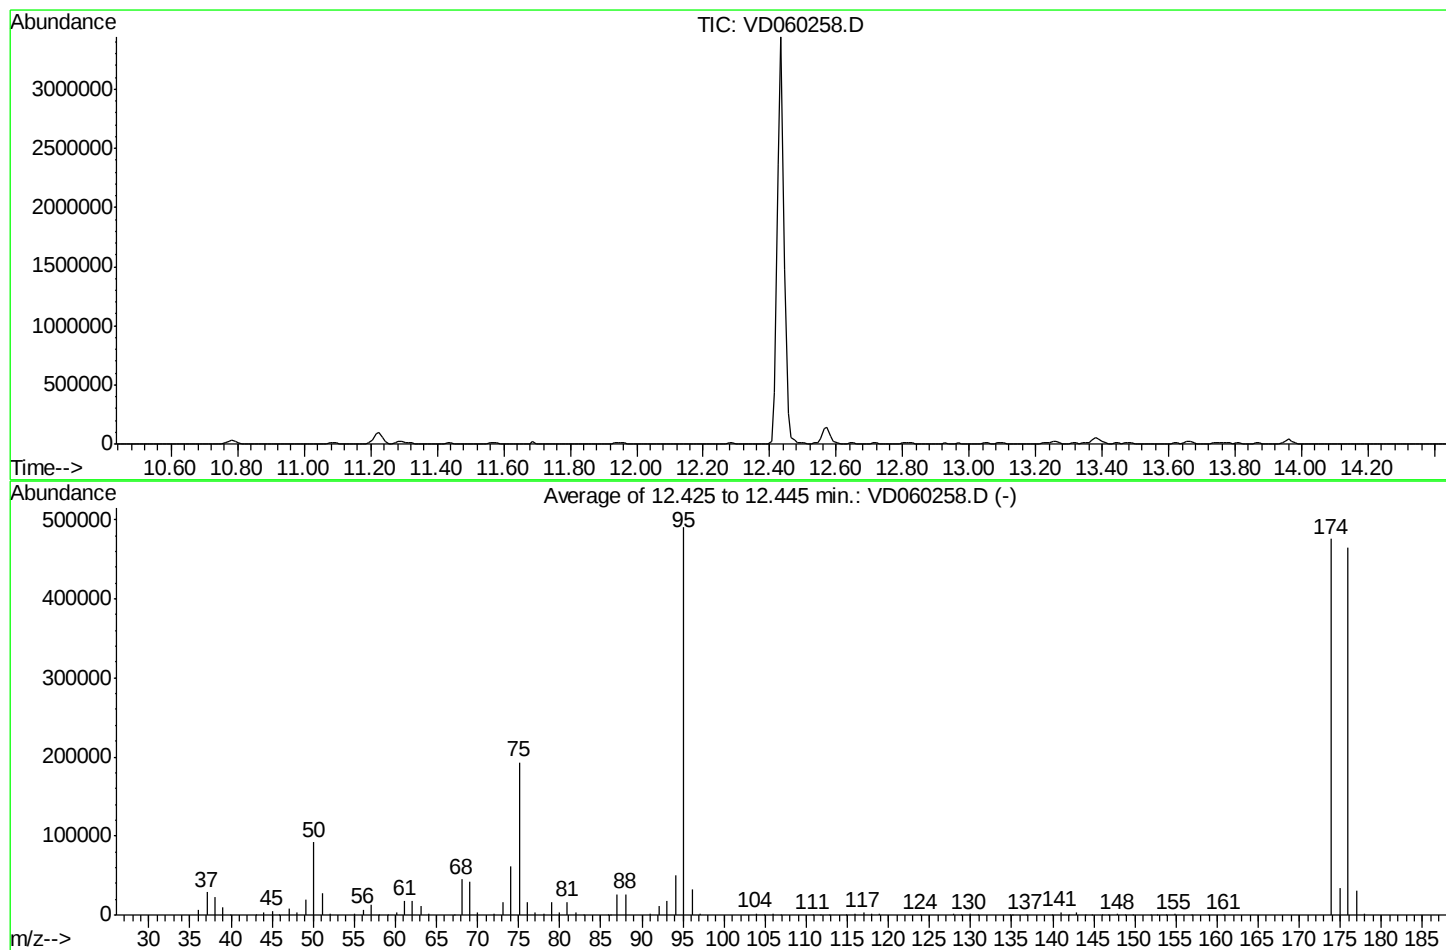

AutoFind: Scans 1108, 1109, 1110; Background Corrected with Scan 1103

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.7	91808	PASS
75	95	30	60	39.4	193109	PASS
95	95	100	100	100.0	490453	PASS
96	95	5	9	6.6	32154	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	97.0	475562	PASS
175	174	5	9	7.1	33581	PASS
176	174	95	101	97.6	464213	PASS
177	176	5	9	6.5	30312	PASS