



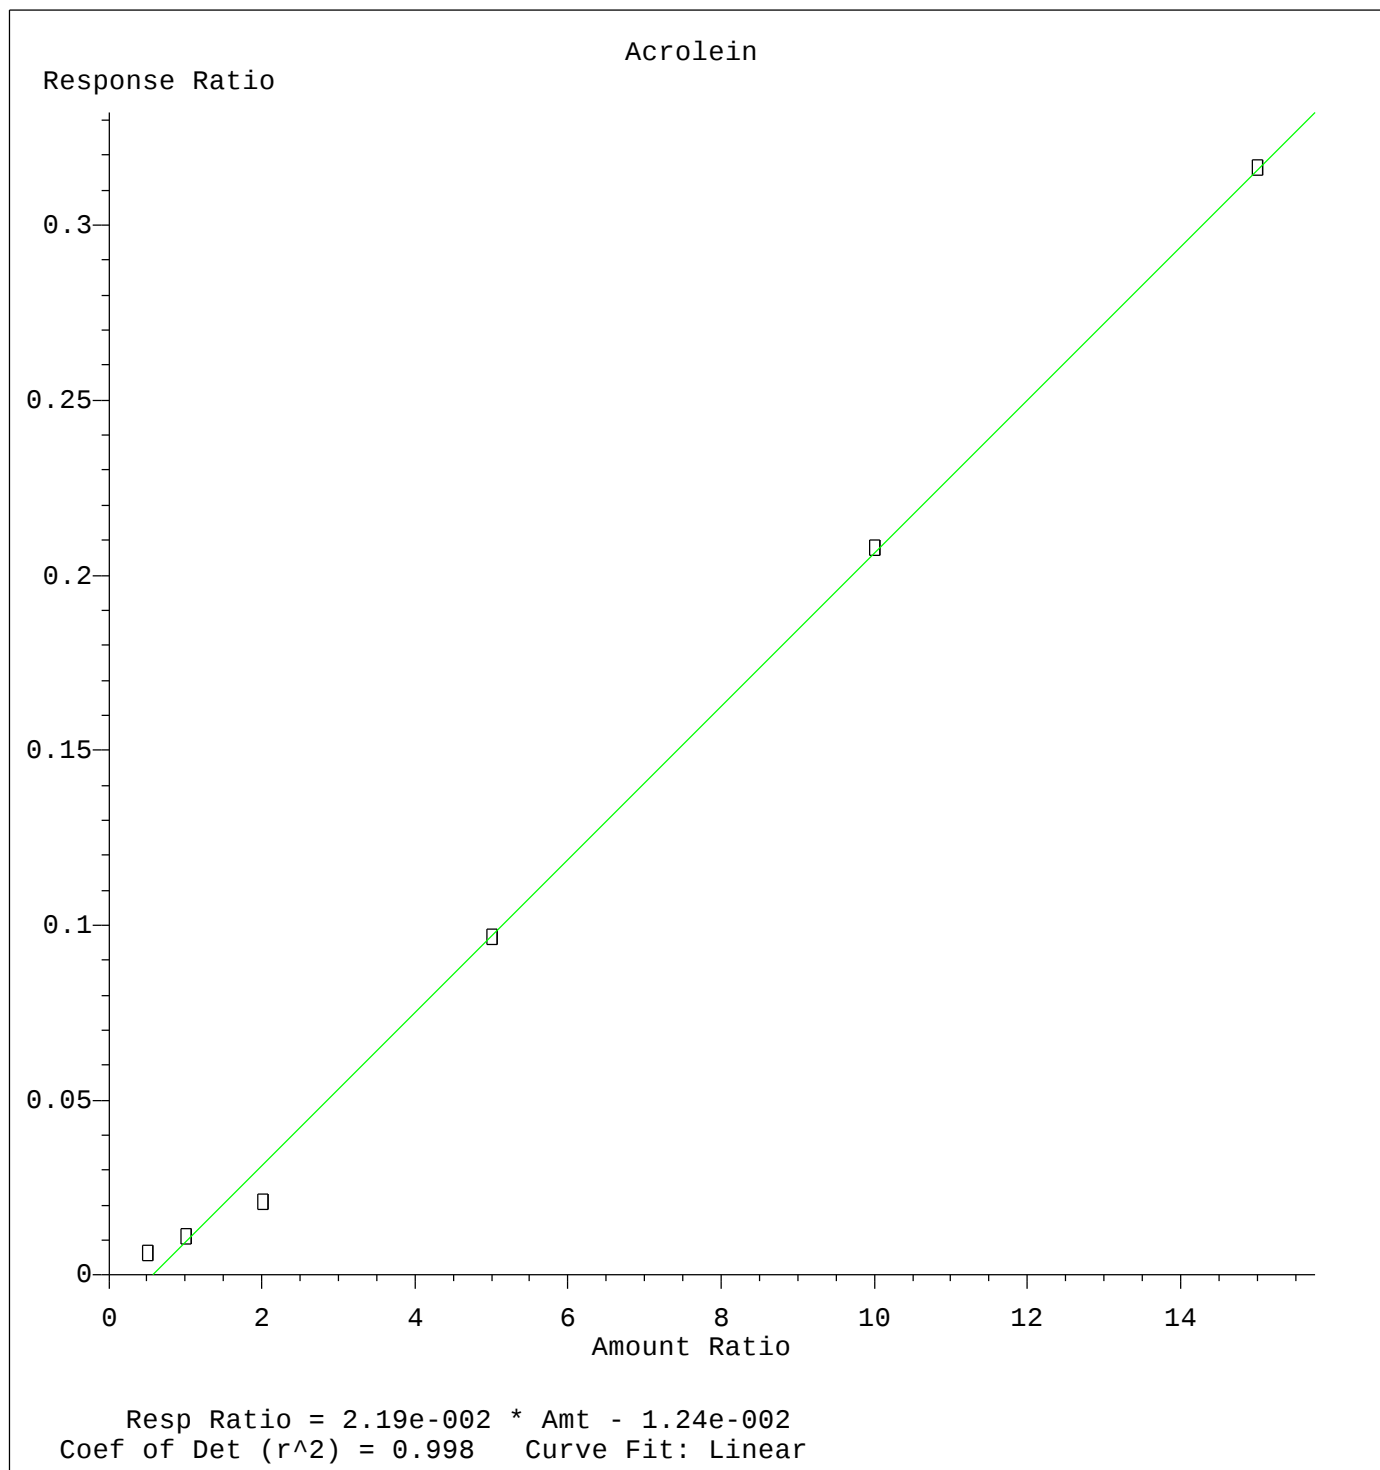


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D110320S.M
Calibration Table Last Updated: Wed Nov 04 00:56:28 2020

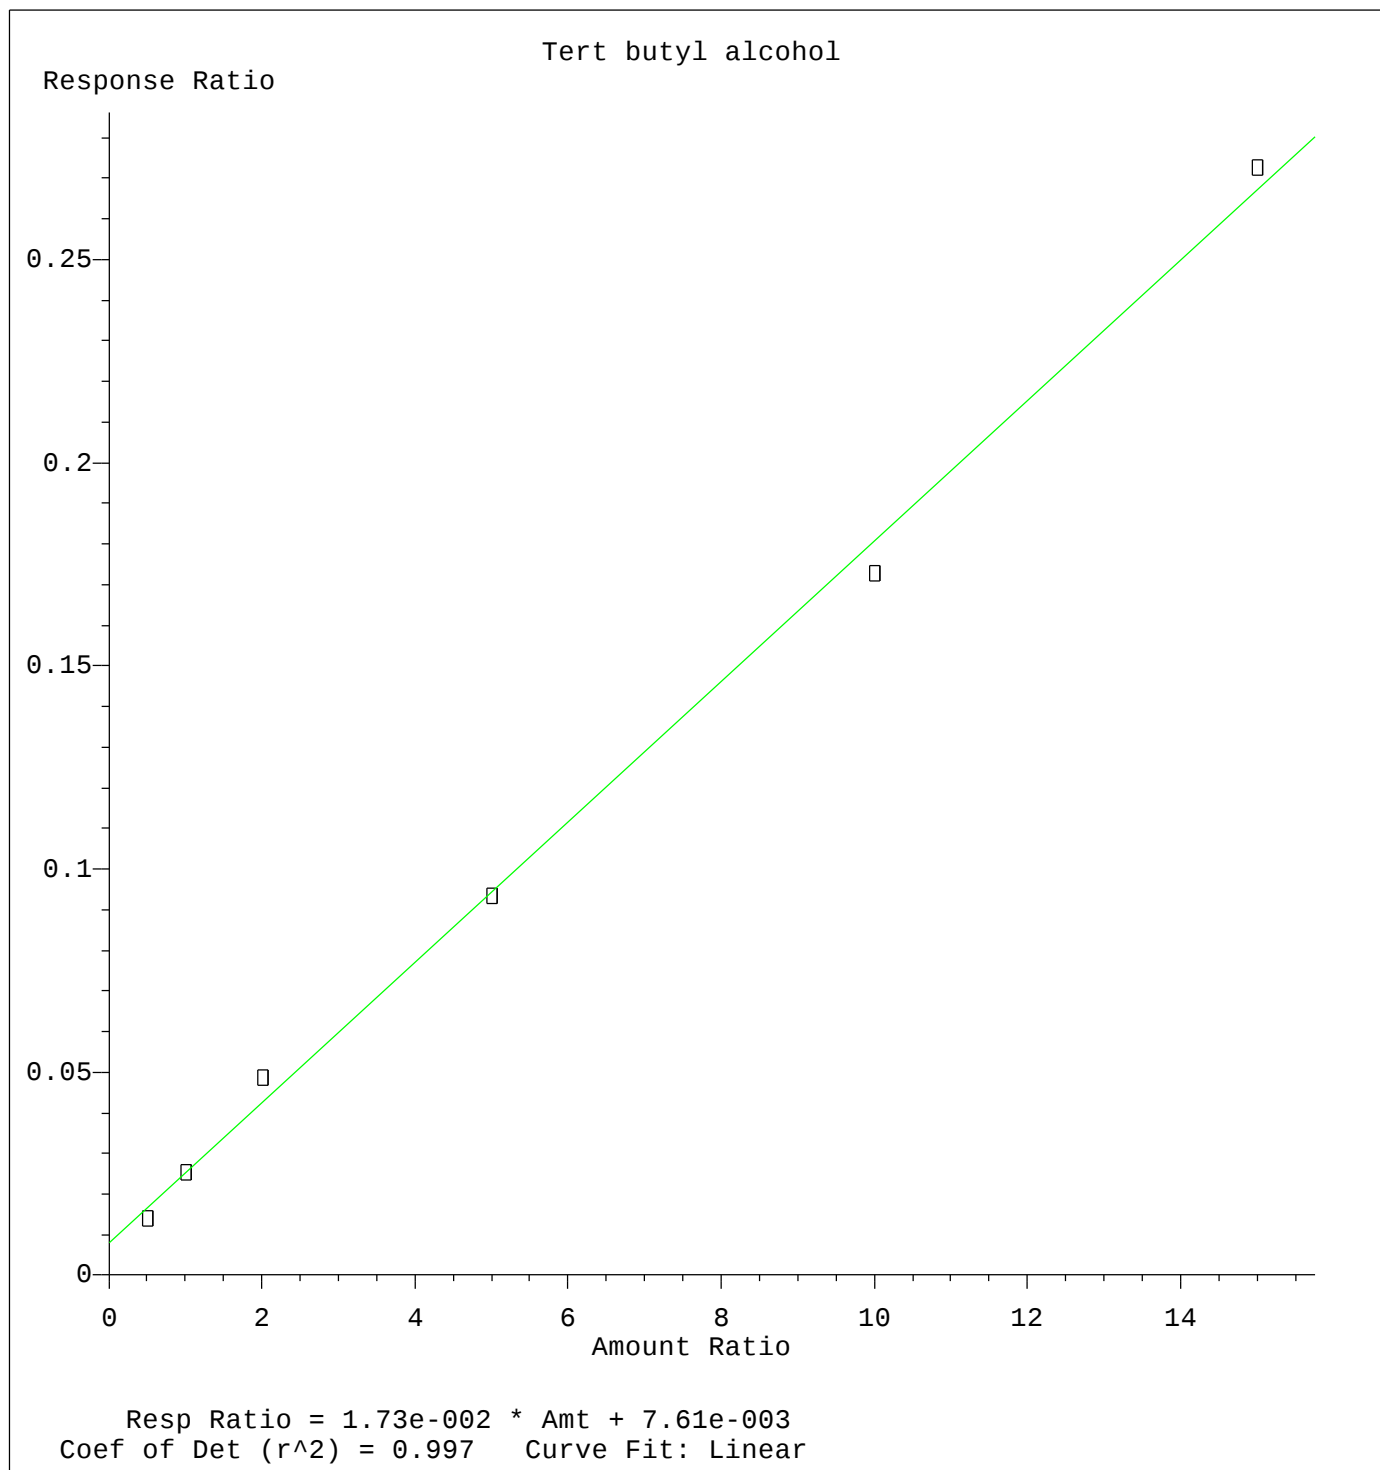

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D110320S.M
Calibration Table Last Updated: Wed Nov 04 00:56:28 2020

Dichlorodifluoromethane

Response Ratio

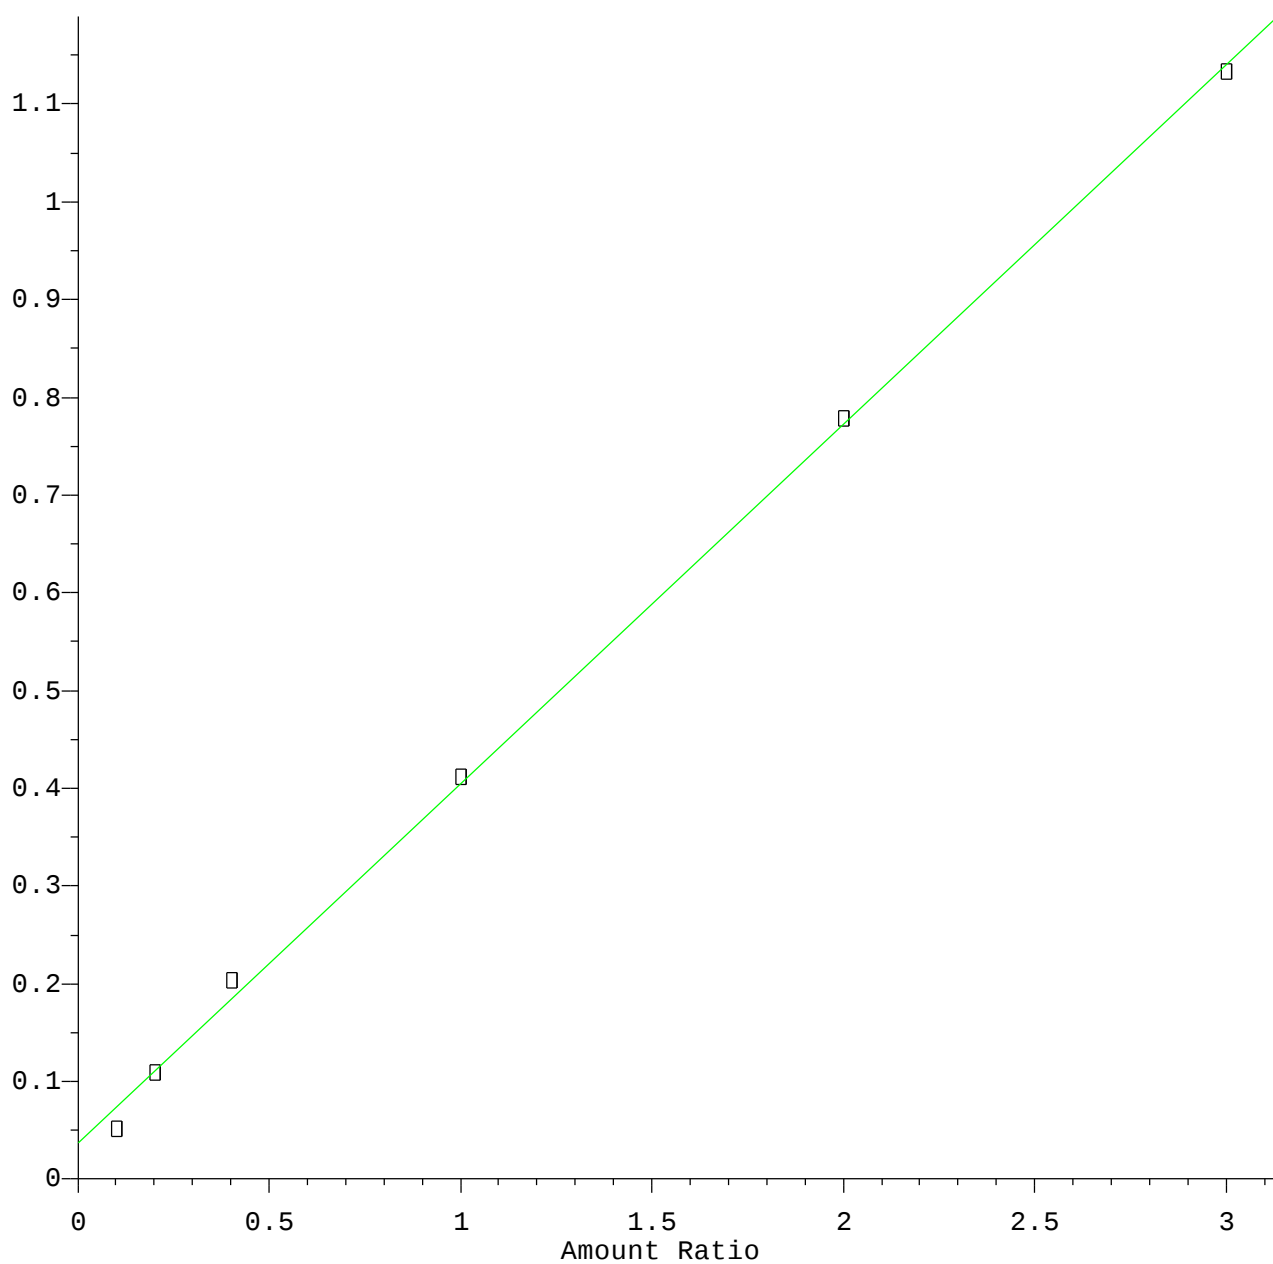

Resp Ratio = 3.68e-001 * Amt + 3.68e-002
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D110320S.M
Calibration Table Last Updated: Wed Nov 04 00:56:28 2020