
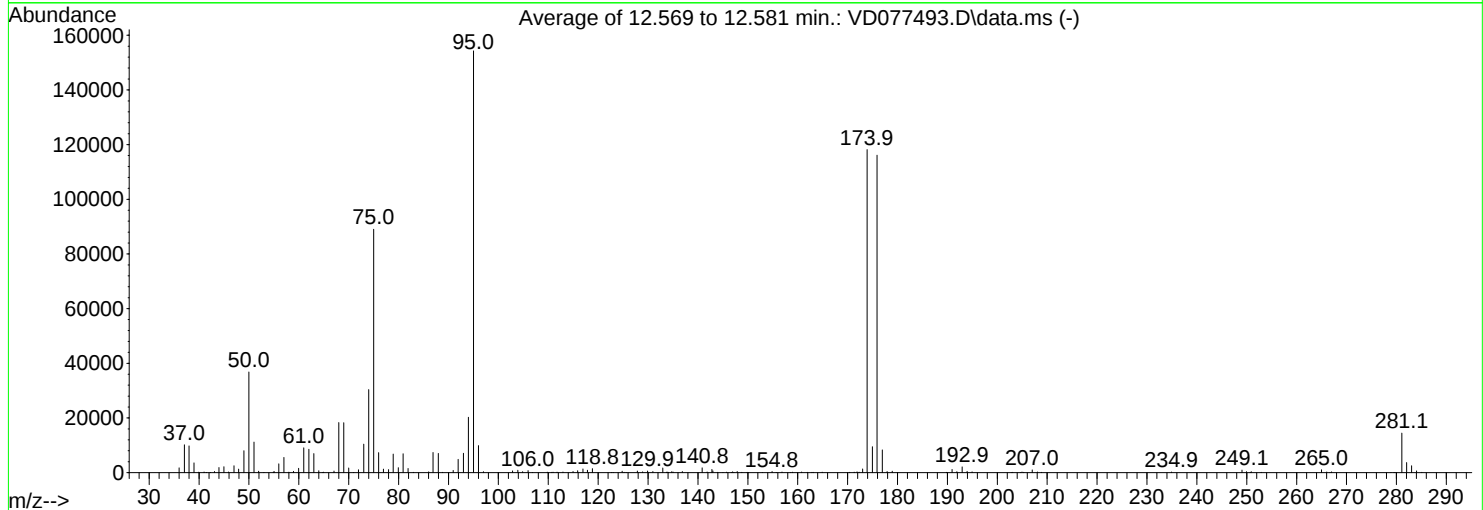


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD110323\
Data File : VD077493.D
Acq On : 03 Nov 2023 08:21
Operator : JC/SY
Sample : BFB
Misc : 5.00G/5.0ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D103023S.M
Title : SW846 8260
Last Update : Tue Oct 31 04:19:17 2023

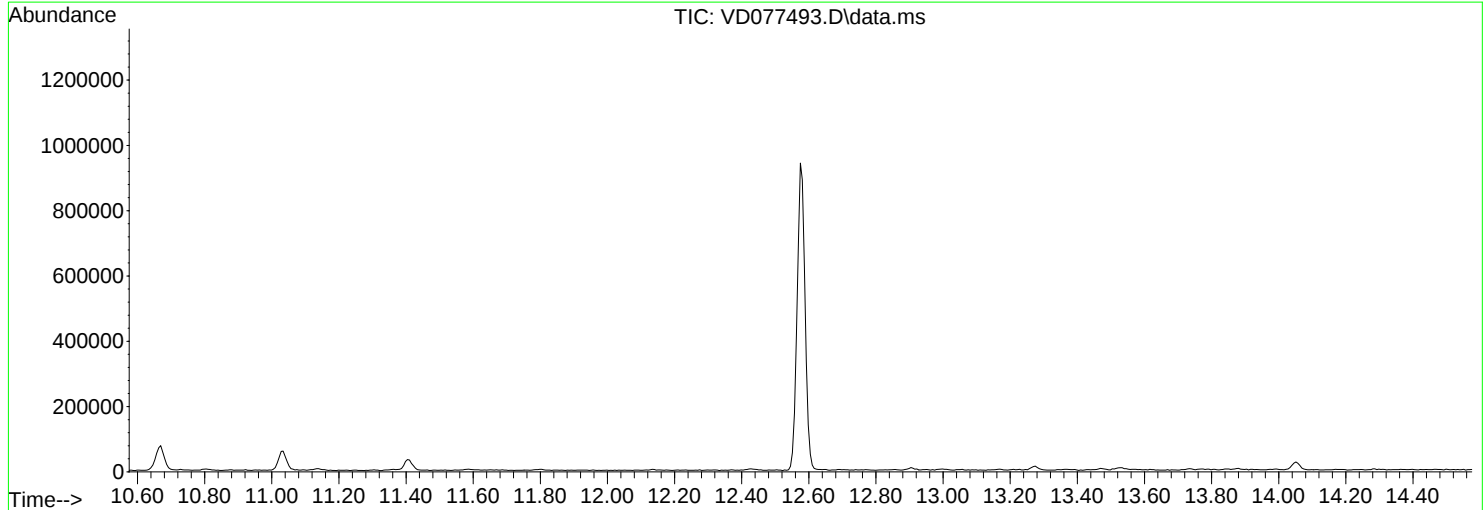

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1859

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	23.8	36792	PASS
75	95	30	60	57.7	89037	PASS
95	95	100	100	100.0	154301	PASS
96	95	5	9	6.4	9919	PASS
173	174	0.00	2	1.1	1321	PASS
174	95	50	100	76.6	118189	PASS
175	174	5	9	8.0	9484	PASS
176	174	95	101	98.3	116123	PASS
177	176	5	9	7.2	8320	PASS