
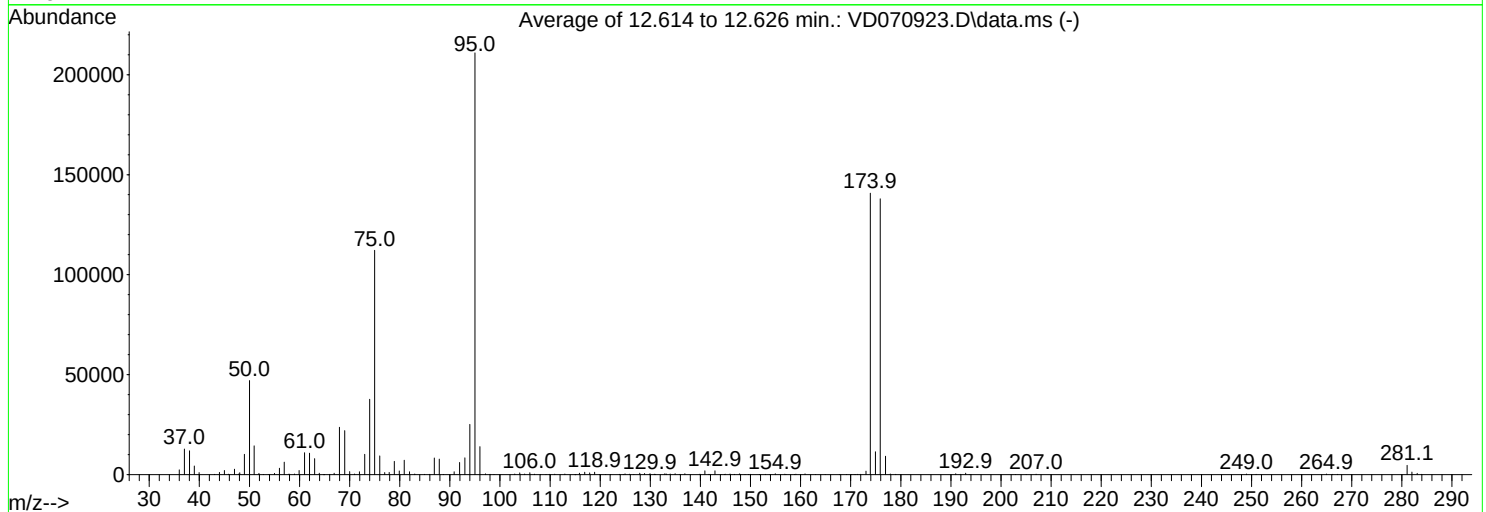


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD110521\
Data File : VD070923.D
Acq On : 05 Nov 2021 11:30
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D110521S.M
Title : SW846 8260
Last Update : Mon Nov 08 13:56:36 2021

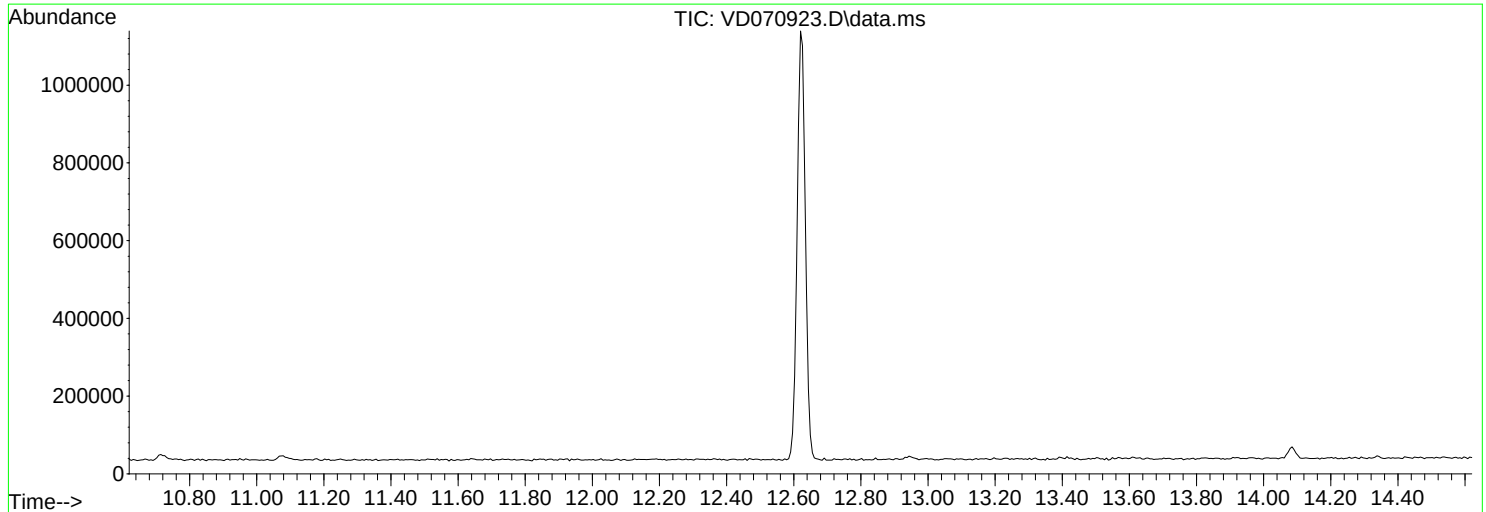

AutoFind: Scans 1818, 1819, 1820; Background Corrected with Scan 1809

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.3	47048	PASS
75	95	30	60	53.2	112184	PASS
95	95	100	100	100.0	210954	PASS
96	95	5	9	6.6	14027	PASS
173	174	0.00	2	1.2	1754	PASS
174	95	50	100	66.7	140739	PASS
175	174	5	9	8.1	11410	PASS
176	174	95	101	98.0	137923	PASS
177	176	5	9	6.7	9219	PASS