


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD110618\
 Data File : VD060283.D
 Acq On : 6 Nov 2018 10:26
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D110618S.M
 Title : SW846 8260
 Last Update : Tue Nov 06 13:56:04 2018

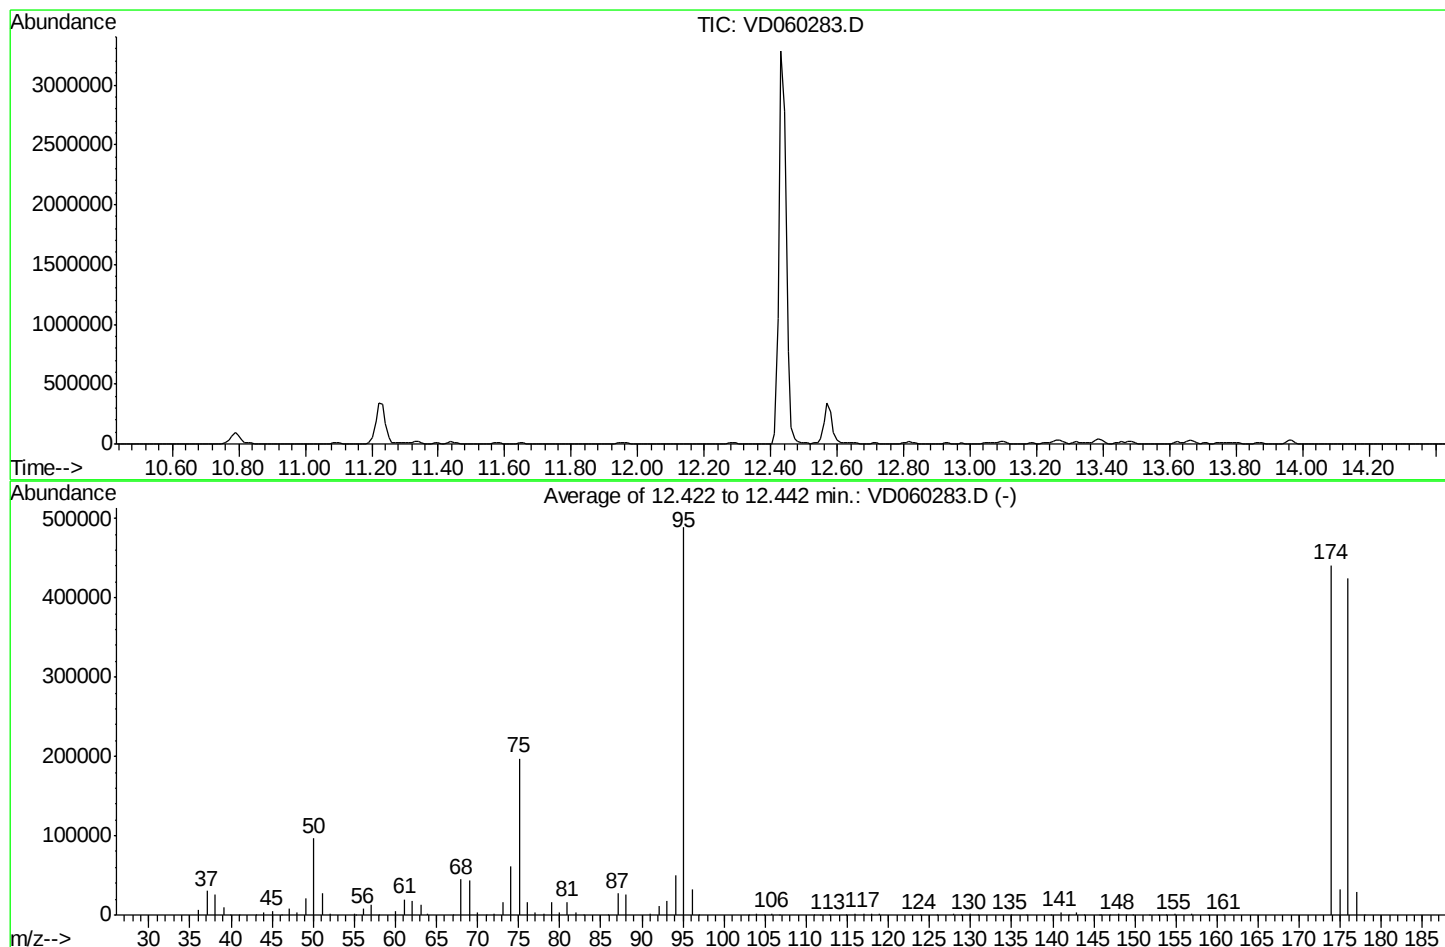

AutoFind: Scans 1107, 1108, 1109; Background Corrected with Scan 1103

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	96584	PASS
75	95	30	60	40.4	197704	PASS
95	95	100	100	100.0	488938	PASS
96	95	5	9	6.8	33045	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	90.3	441416	PASS
175	174	5	9	7.2	31906	PASS
176	174	95	101	96.1	424213	PASS
177	176	5	9	6.8	28649	PASS